Quantitation Report (QT Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121025\
Data File : PD091537.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Dec 2025 15:43
Operator : AR\AJ
Sample : Q3814-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
TP-5

Manual Integrations APPROVED

Reviewed By :Abdul Mirza 12/11/2025
Supervised By :Yogesh Patel 12/11/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 01:54:29 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120825.M
Quant Title : GC Extractables
QLast Update : Tue Dec 09 04:29:17 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
	System Monitoring Compounds						
1)	SA Tetrachlo...	3.539	2.869	76707341	1011.5E6	22.085m	25.671m
28)	SA Decachlor...	9.065	8.058	99304409	827.3E6	19.104	19.978
	Target Compounds						

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121025\
Data File : PD091537.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Dec 2025 15:43
Operator : AR\AJ
Sample : Q3814-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
TP-5

Manual Integrations APPROVED

Reviewed By :Abdul Mirza 12/11/2025
Supervised By :Yogesh Patel 12/11/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 01:54:29 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120825.M
Quant Title : GC Extractables
QLast Update : Tue Dec 09 04:29:17 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

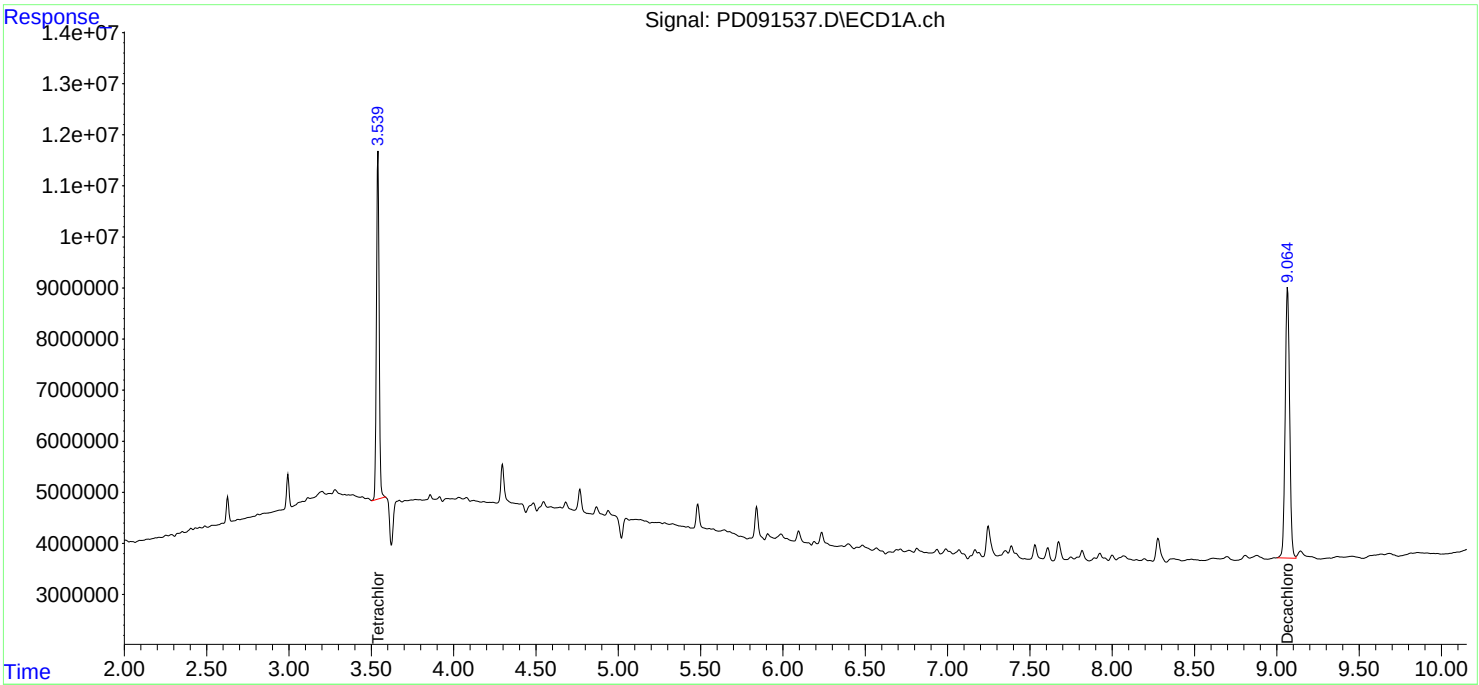

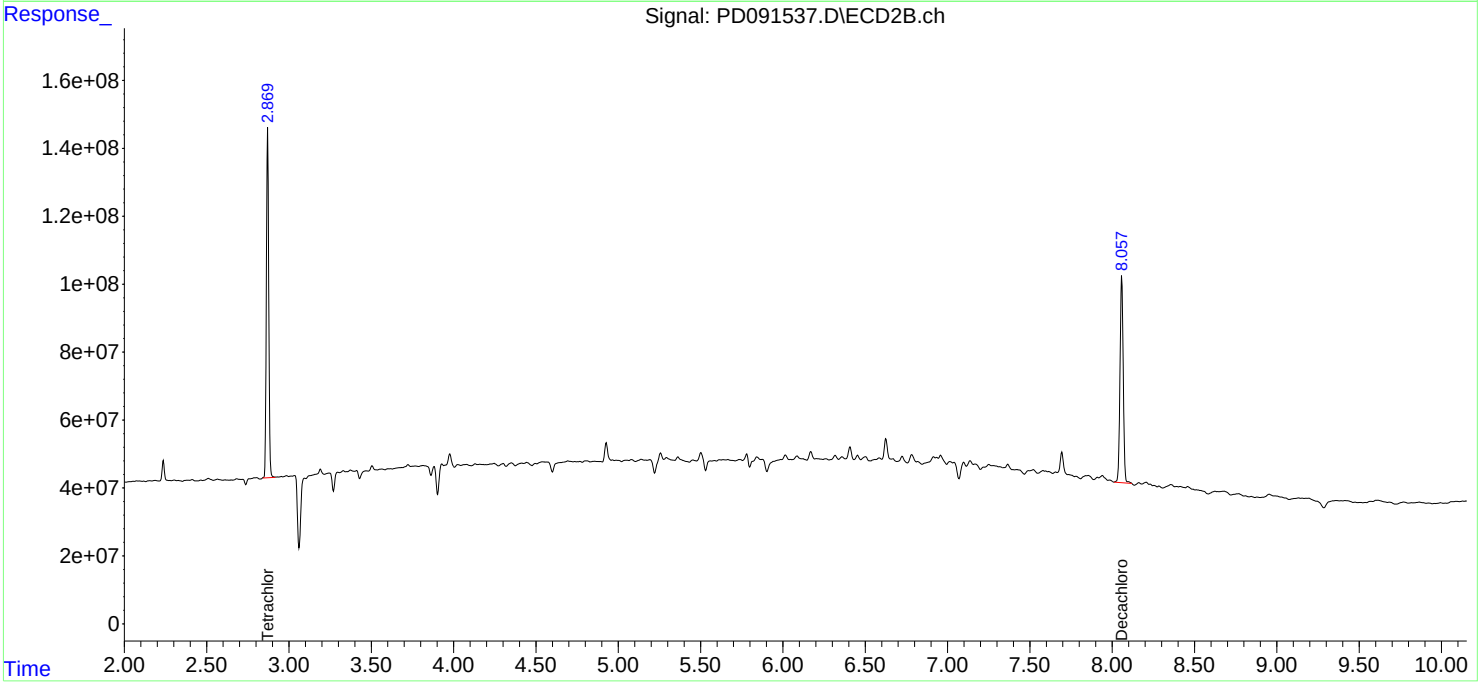

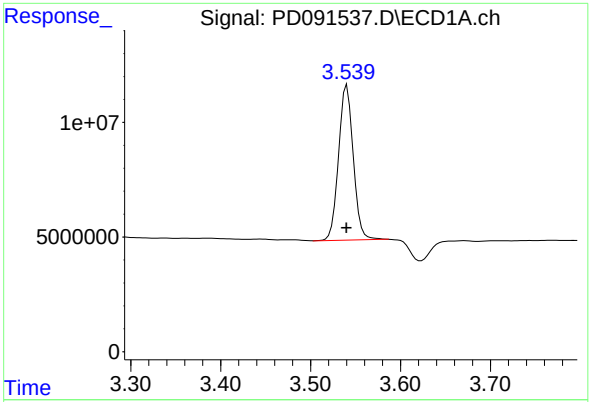

#1 Tetrachloro-m-xylene

R.T.: 3.539 min
Delta R.T.: 0.000 min
Response: 76707341
Conc: 22.08 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-5

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/11/2025
Supervised By :Yogesh Patel 12/11/2025

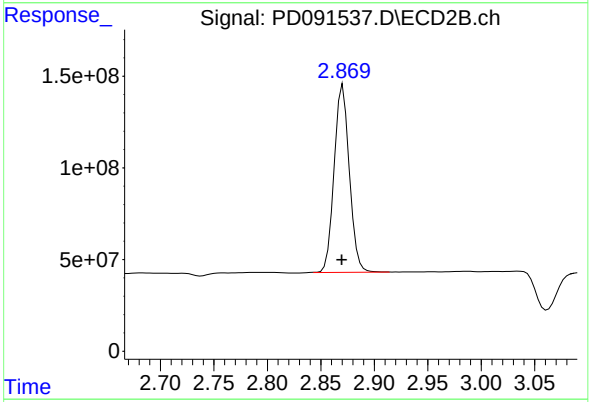

#1 Tetrachloro-m-xylene

R.T.: 2.869 min
Delta R.T.: 0.000 min
Response: 1011517760
Conc: 25.67 ng/ml m

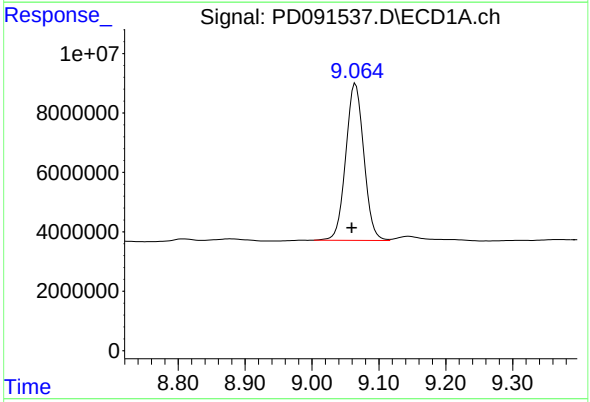

#28 Decachlorobiphenyl

R.T.: 9.065 min
Delta R.T.: 0.006 min
Response: 99304409
Conc: 19.10 ng/ml

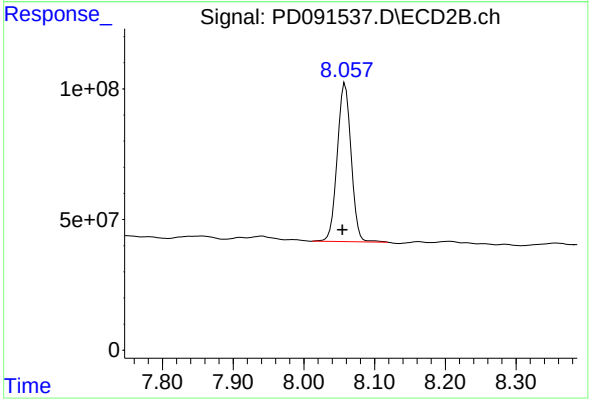

#28 Decachlorobiphenyl

R.T.: 8.058 min
Delta R.T.: 0.004 min
Response: 827285482
Conc: 19.98 ng/ml