

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121025\
 Data File : PD091540.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Dec 2025 16:24
 Operator : AR\AJ
 Sample : Q3814-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TP-6

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/11/2025
 Supervised By :Yogesh Patel 12/11/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 01:54:58 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120825.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 09 04:29:17 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.540	2.870	77053342	1044.6E6	22.184m	26.511m
28)	SA Decachlor...	9.066	8.059	97144431	880.7E6	18.689	21.269

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121025\
Data File : PD091540.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Dec 2025 16:24
Operator : AR\AJ
Sample : Q3814-03
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
TP-6


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/11/2025
Supervised By : Yogesh Patel 12/11/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 01:54:58 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120825.M
Quant Title : GC Extractables
QLast Update : Tue Dec 09 04:29:17 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

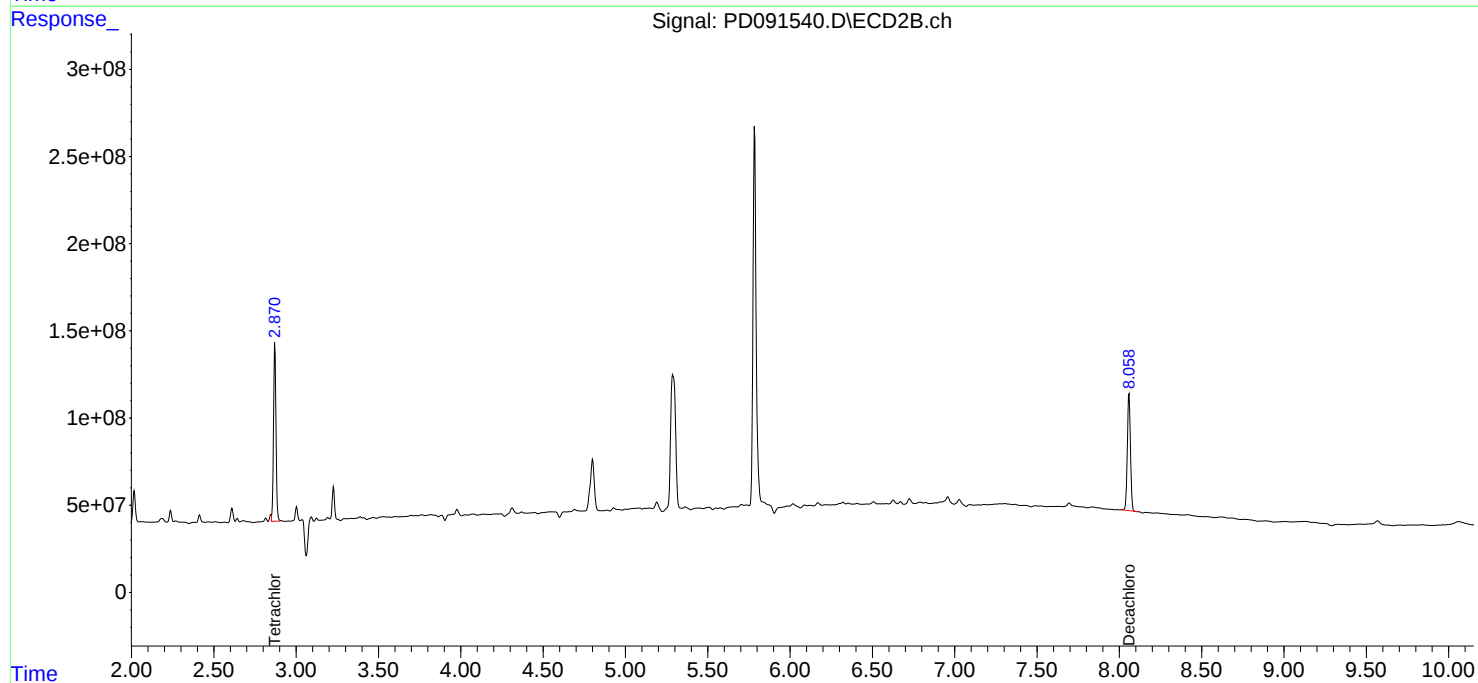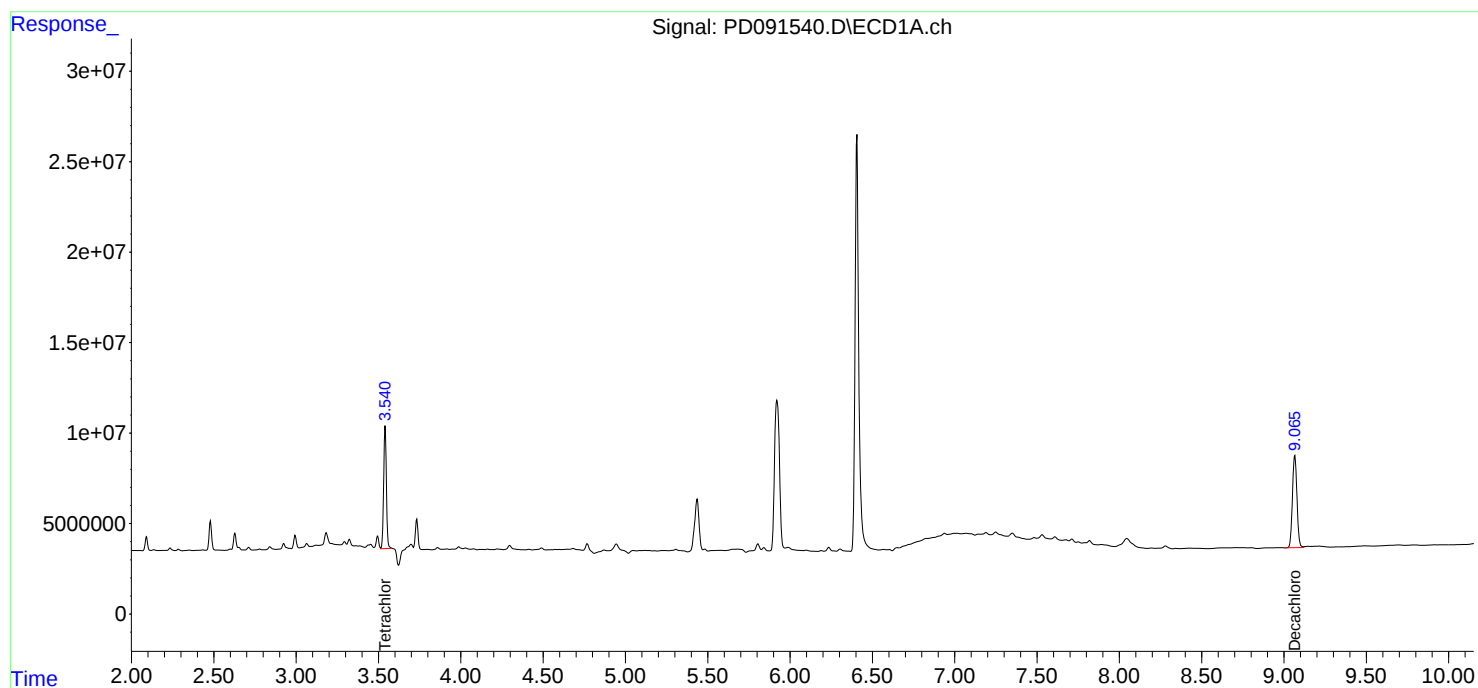

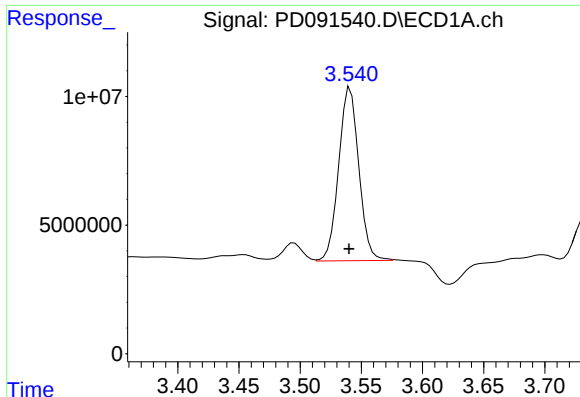


#1 Tetrachloro-m-xylene

R.T.: 3.540 min
Delta R.T.: 0.000 min
Response: 77053342
Conc: 22.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-6


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/11/2025
Supervised By :Yogesh Patel 12/11/2025

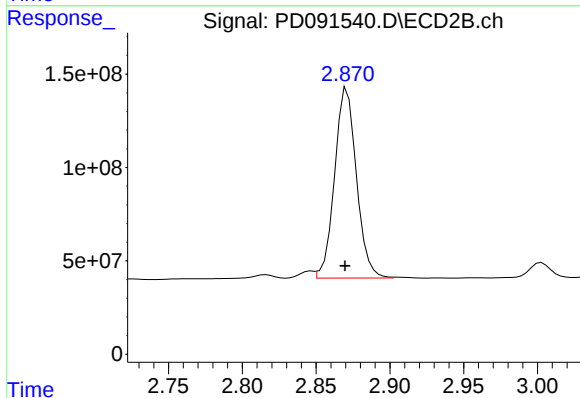


#1 Tetrachloro-m-xylene

R.T.: 2.870 min
Delta R.T.: 0.000 min
Response: 1044631946
Conc: 26.51 ng/ml m

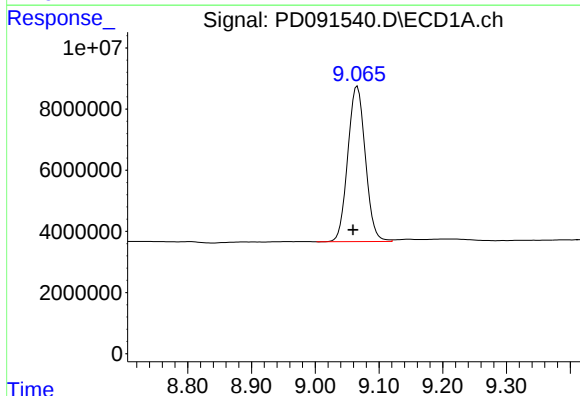

#28 Decachlorobiphenyl

R.T.: 9.066 min
Delta R.T.: 0.007 min
Response: 97144431
Conc: 18.69 ng/ml

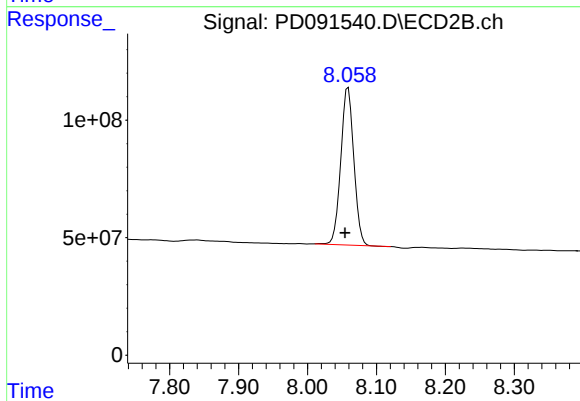

#28 Decachlorobiphenyl

R.T.: 8.059 min
Delta R.T.: 0.004 min
Response: 880747495
Conc: 21.27 ng/ml