

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121025\
 Data File : PD091546.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Dec 2025 17:46
 Operator : AR\AJ
 Sample : Q3814-15
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TP-4

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/11/2025
 Supervised By :Yogesh Patel 12/11/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 01:55:52 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120825.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 09 04:29:17 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.539	2.871	81957147	1102.5E6	23.596m	27.981
28) SA Decachlor...	9.065	8.057	110.9E6	1054.2E6	21.327	25.456m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121025\
Data File : PD091546.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Dec 2025 17:46
Operator : AR\AJ
Sample : Q3814-15
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
TP-4


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/11/2025
Supervised By : Yogesh Patel 12/11/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 01:55:52 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120825.M
Quant Title : GC Extractables
QLast Update : Tue Dec 09 04:29:17 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

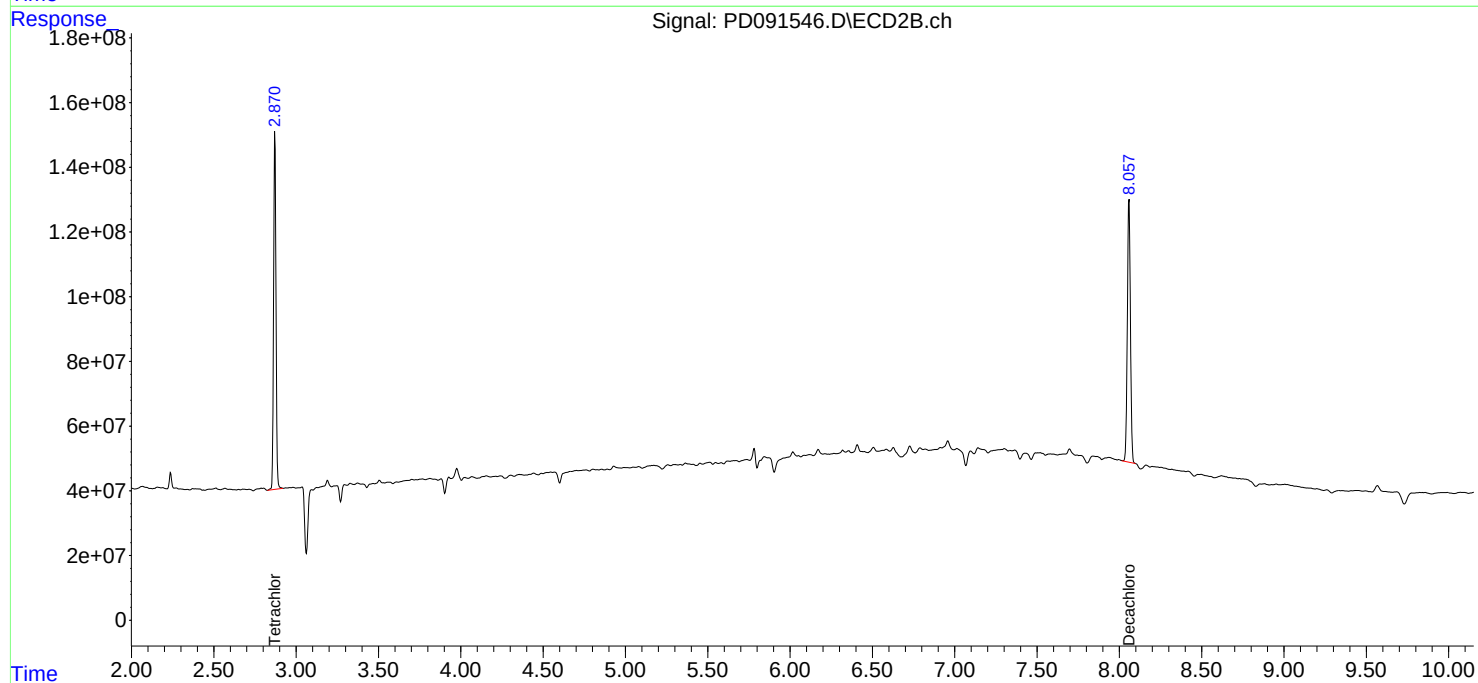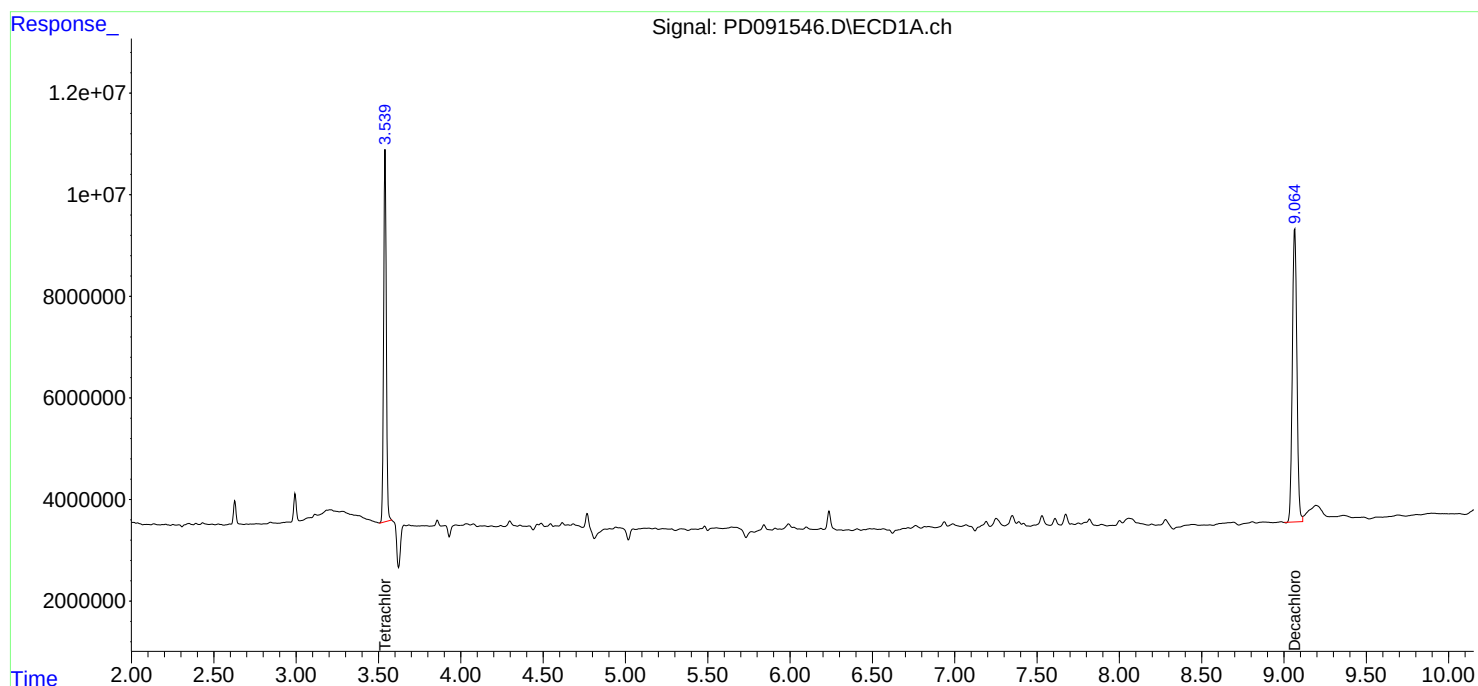

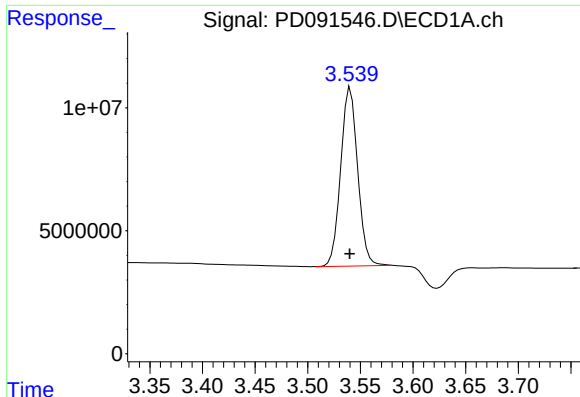


#1 Tetrachloro-m-xylene

R.T.: 3.539 min
Delta R.T.: 0.000 min
Response: 81957147
Conc: 23.60 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-4


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/11/2025
Supervised By :Yogesh Patel 12/11/2025

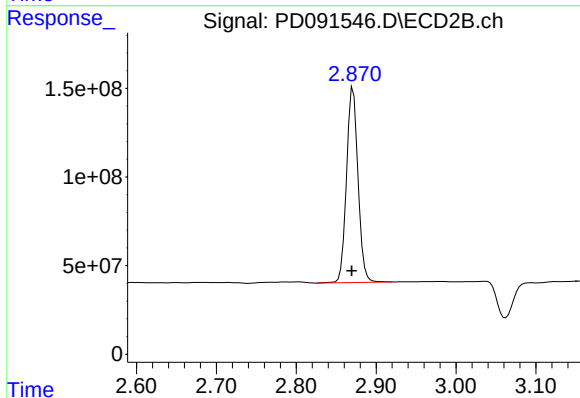


#1 Tetrachloro-m-xylene

R.T.: 2.871 min
Delta R.T.: 0.002 min
Response: 1102543434
Conc: 27.98 ng/ml

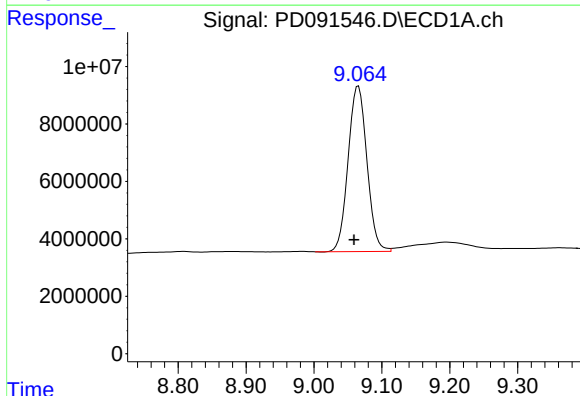

#28 Decachlorobiphenyl

R.T.: 9.065 min
Delta R.T.: 0.006 min
Response: 110855772
Conc: 21.33 ng/ml

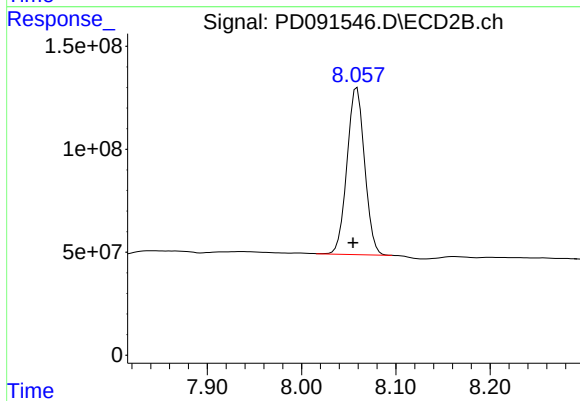

#28 Decachlorobiphenyl

R.T.: 8.057 min
Delta R.T.: 0.003 min
Response: 1054169890
Conc: 25.46 ng/ml m