

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121119\
 Data File : PD056371.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Dec 2019 11:57
 Operator : SG\AJ
 Sample : K6167-14
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BFQT6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 01:12:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.288	3.961	19106862	26606879	23.070	22.131
27)	SA Decachlor...	7.960	8.995	31350079	39734489	34.719	33.025
Target Compounds							
3)	MA gamma-BHC...	0.000	4.591f	0	393409	N.D.	0.244
4)	MA Heptachlor	0.000	5.166f	0	363289	N.D.	0.223
6)	B beta-BHC	0.000	4.848f	0	398705	N.D.	0.484
7)	B delta-BHC	0.000	4.989f	0	3187556	N.D.	1.914
8)	B Heptachlo...	0.000	5.854	0	1321826	N.D.	0.853
15)	B Endosulfa...	0.000	6.840	0	5761074	N.D.	3.932
16)	A 4,4'-DDD	0.000	6.733f	0	2596655	N.D.	2.207
19)	B Endosulfa...	0.000	7.231	0	4022840	N.D.	3.009


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121119\
Data File : PD056371.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Dec 2019 11:57
Operator : SG\AJ
Sample : K6167-14
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
BFQT6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 01:12:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

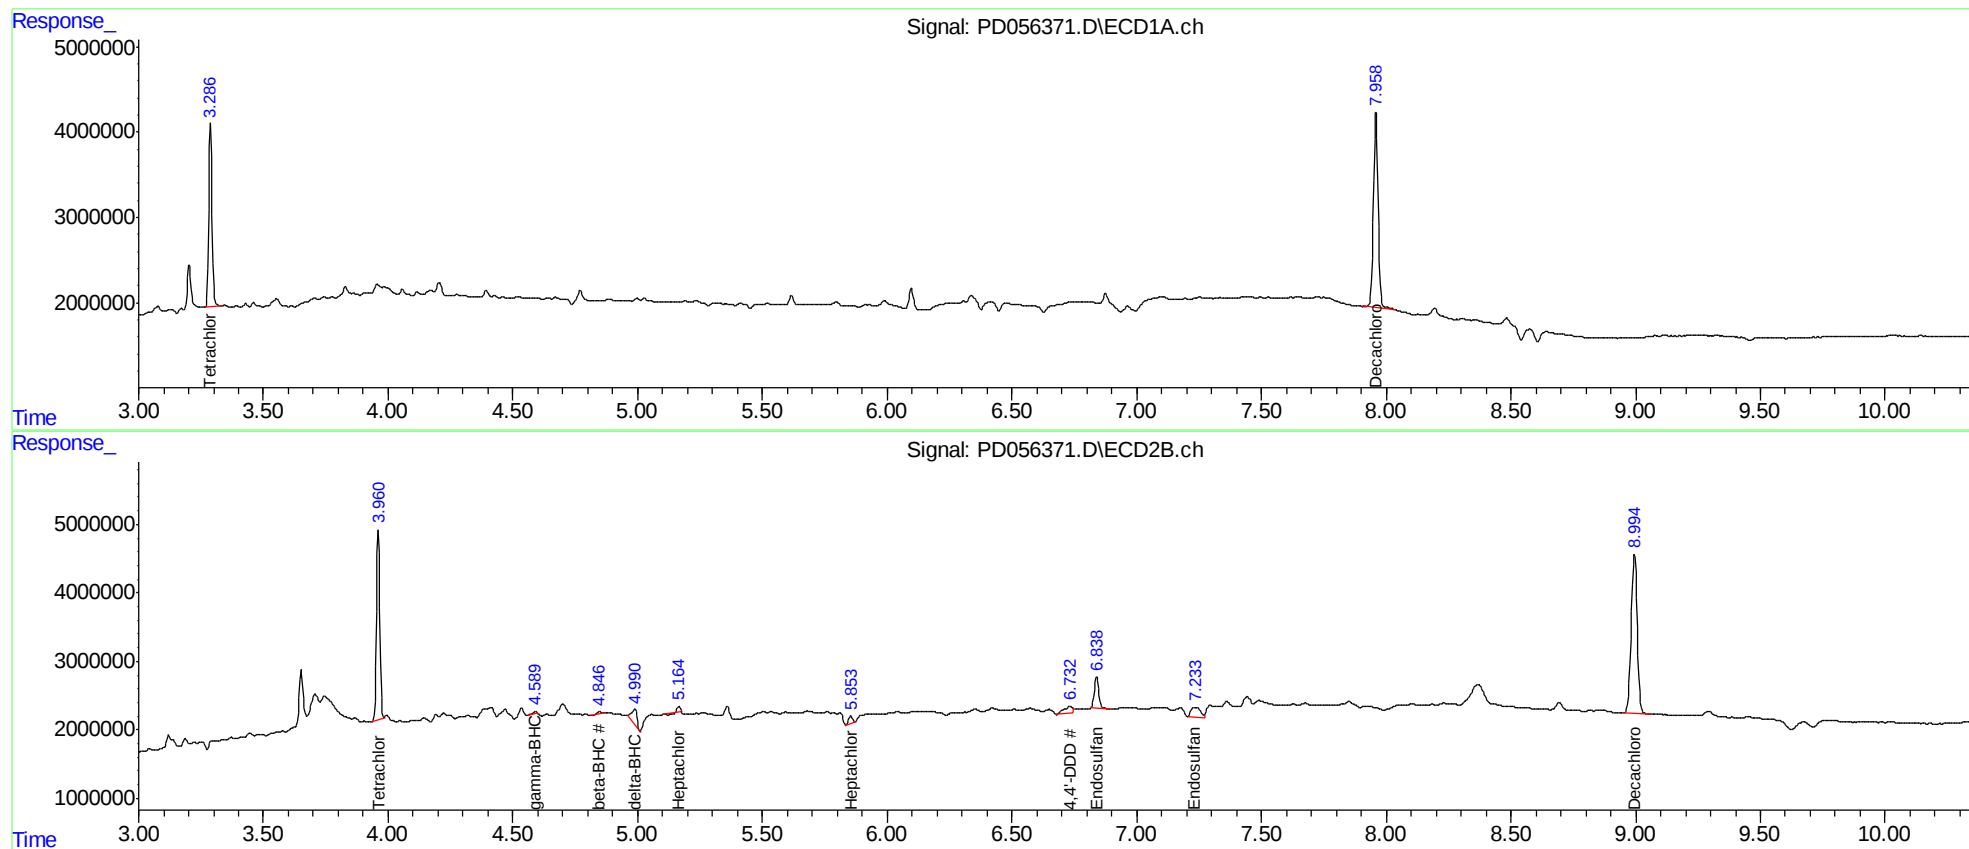


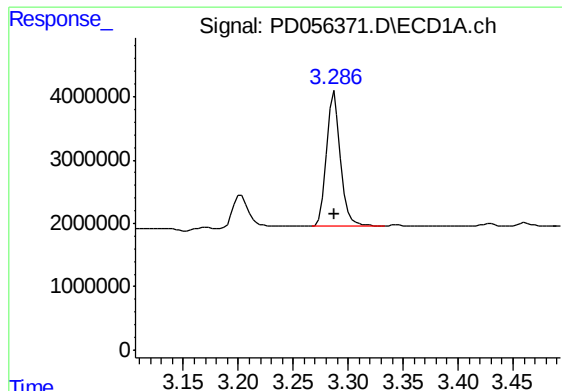

#1 Tetrachloro-m-xylene


R.T.: 3.288 min
Delta R.T.: 0.000 min
Response: 19106862
Conc: 23.07 ng/ml

Instrument :
ECD_D
ClientSampleId :
BFQT6

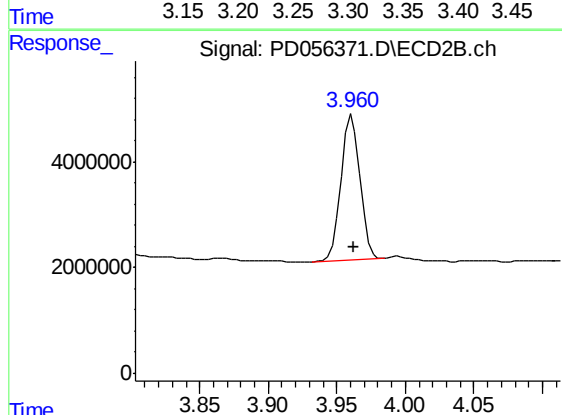


#1 Tetrachloro-m-xylene

R.T.: 3.961 min
Delta R.T.: -0.001 min
Response: 26606879
Conc: 22.13 ng/ml

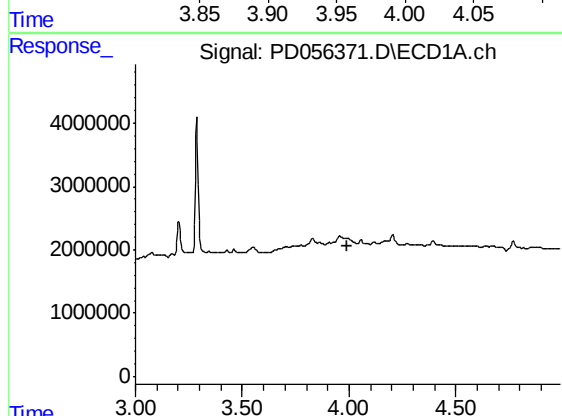


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 3.991 min
Response: 0
Conc: N.D.

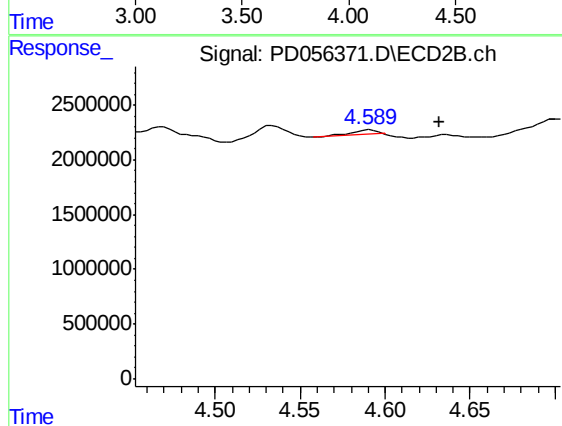

#3 gamma-BHC (Lindane)


R.T.: 4.591 min
Delta R.T.: -0.041 min
Response: 393409
Conc: 0.24 ng/ml

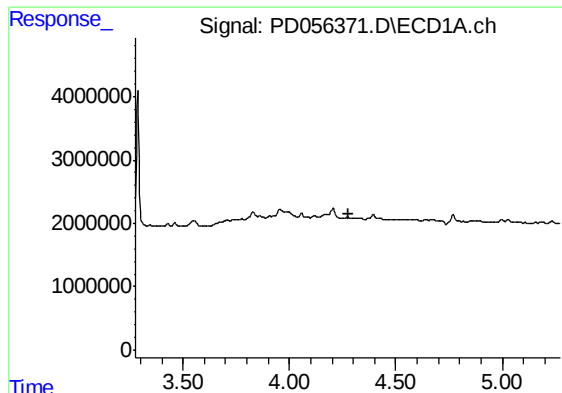

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 4.276 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BFQT6

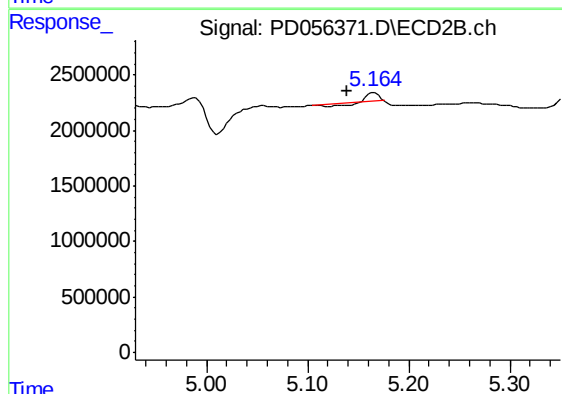


#4 Heptachlor

R.T.: 5.166 min
Delta R.T.: 0.027 min
Response: 363289
Conc: 0.22 ng/ml

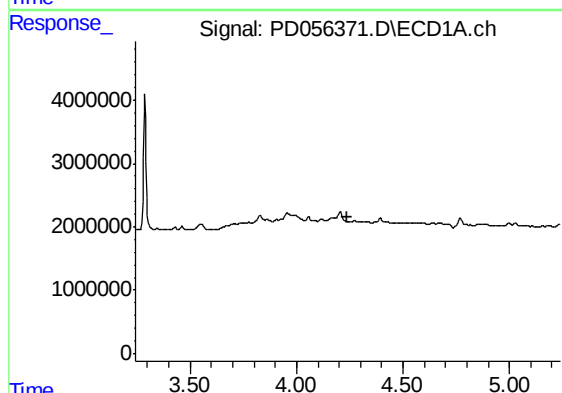


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.240 min
Response: 0
Conc: N.D.

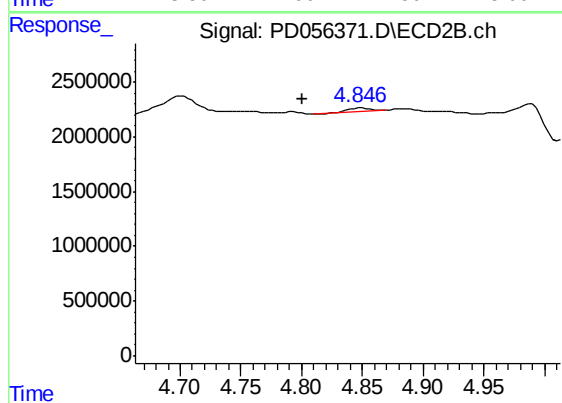

#6 beta-BHC


R.T.: 4.848 min
Delta R.T.: 0.047 min
Response: 398705
Conc: 0.48 ng/ml

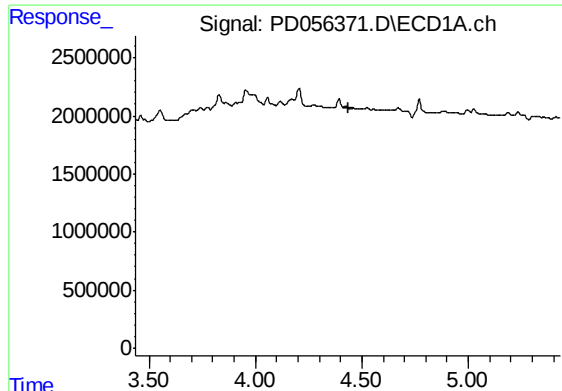

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.436 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BFQT6

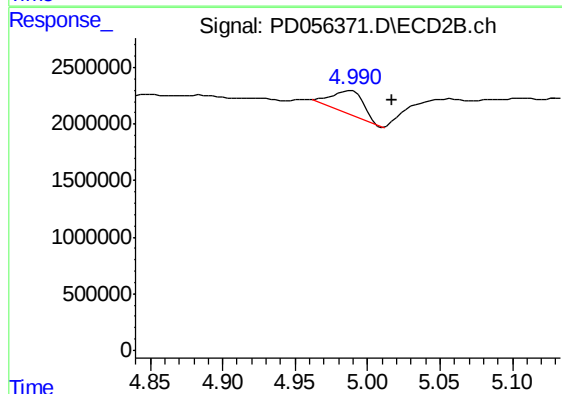


#7 delta-BHC

R.T.: 4.989 min
Delta R.T.: -0.028 min
Response: 3187556
Conc: 1.91 ng/ml

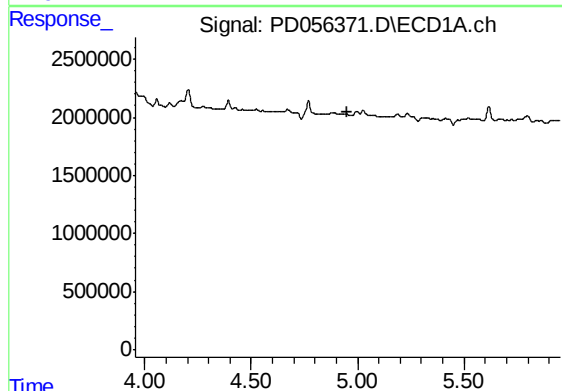


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 4.953 min
Response: 0
Conc: N.D.

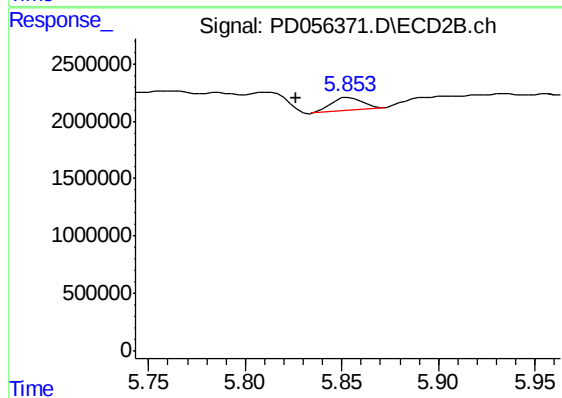

#8 Heptachlor epoxide


R.T.: 5.854 min
Delta R.T.: 0.028 min
Response: 1321826
Conc: 0.85 ng/ml

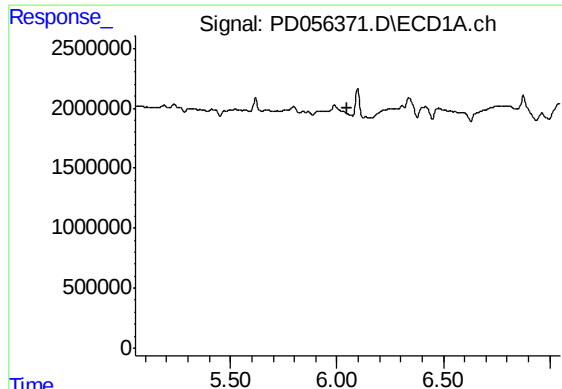

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.051 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BFQT6

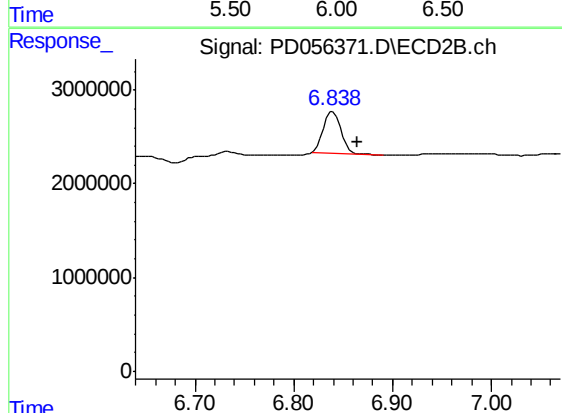


#15 Endosulfan II

R.T.: 6.840 min
Delta R.T.: -0.024 min
Response: 5761074
Conc: 3.93 ng/ml

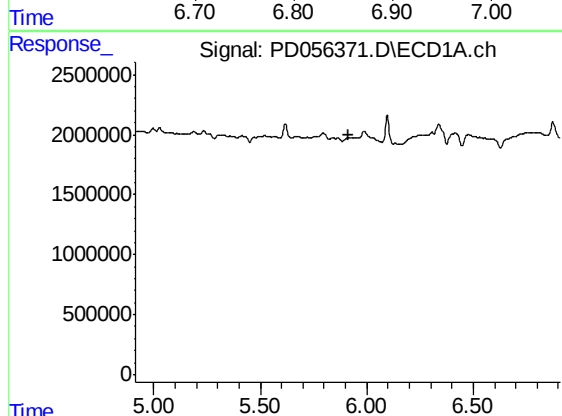


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 5.912 min
Response: 0
Conc: N.D.

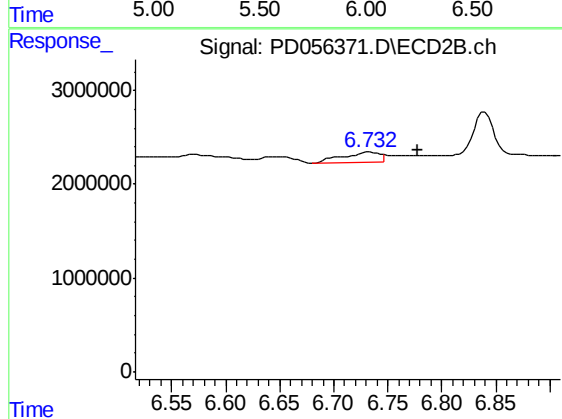

#16 4,4'-DDD


R.T.: 6.733 min
Delta R.T.: -0.044 min
Response: 2596655
Conc: 2.21 ng/ml

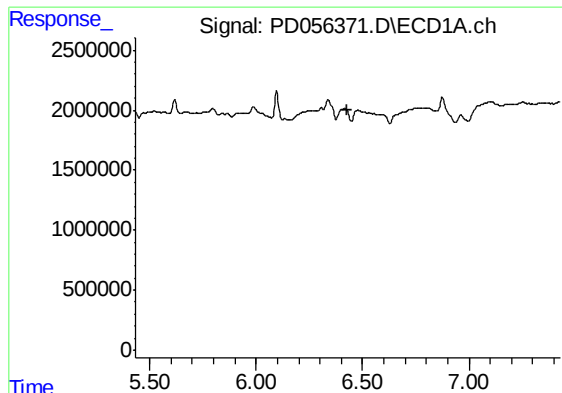

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 6.430 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BFQT6

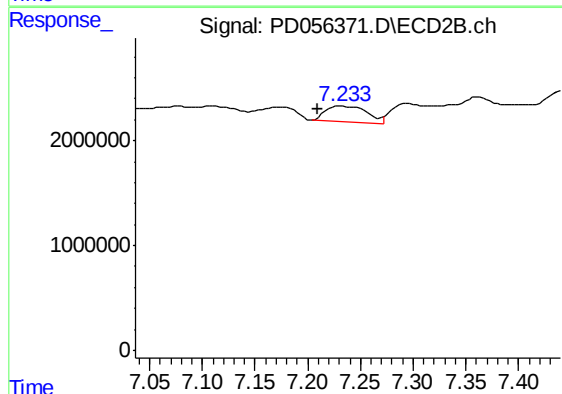


#19 Endosulfan Sulfate

R.T.: 7.231 min
Delta R.T.: 0.021 min
Response: 4022840
Conc: 3.01 ng/ml

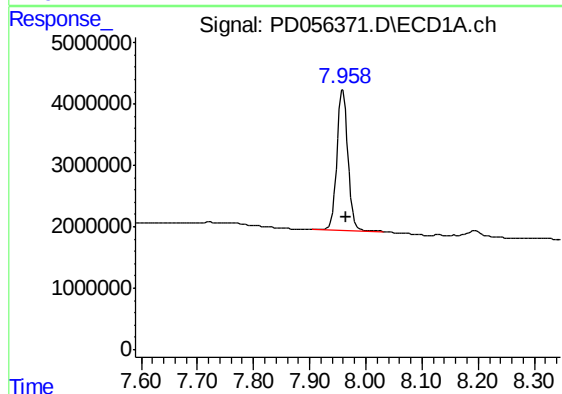

#27 Decachlorobiphenyl

R.T.: 7.960 min
Delta R.T.: -0.006 min
Response: 31350079
Conc: 34.72 ng/ml

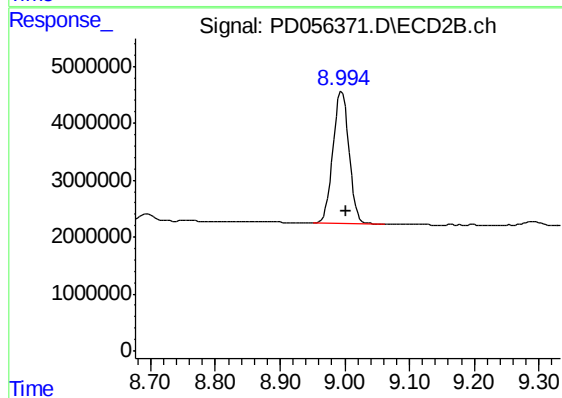

#27 Decachlorobiphenyl

R.T.: 8.995 min
Delta R.T.: -0.007 min
Response: 39734489
Conc: 33.03 ng/ml