

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121119\
 Data File : PD056381.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Dec 2019 14:32
 Operator : SG\AJ
 Sample : K6170-04
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0BS3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 01:15:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.287	3.961	18660109	27630650	22.531	22.982
27)	SA Decachlor...	7.959	8.994	30888162	40713902	34.207	33.840
Target Compounds							
5)	MB Aldrin	0.000	5.458	0	477836	N.D.	0.291
8)	B Heptachlo...	0.000	5.814	0	3839990	N.D.	2.479
10)	B trans-Chl...	0.000	6.052	0	997764	N.D.	0.603
16)	A 4,4'-DDD	0.000	6.733f	0	3127394	N.D.	2.658
19)	B Endosulfa...	0.000	7.241	0	2295252	N.D.	1.717
20)	A Methoxychlor	0.000	7.481f	0	390504	N.D.	0.645


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121119\
Data File : PD056381.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Dec 2019 14:32
Operator : SG\AJ
Sample : K6170-04
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
C0BS3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 01:15:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

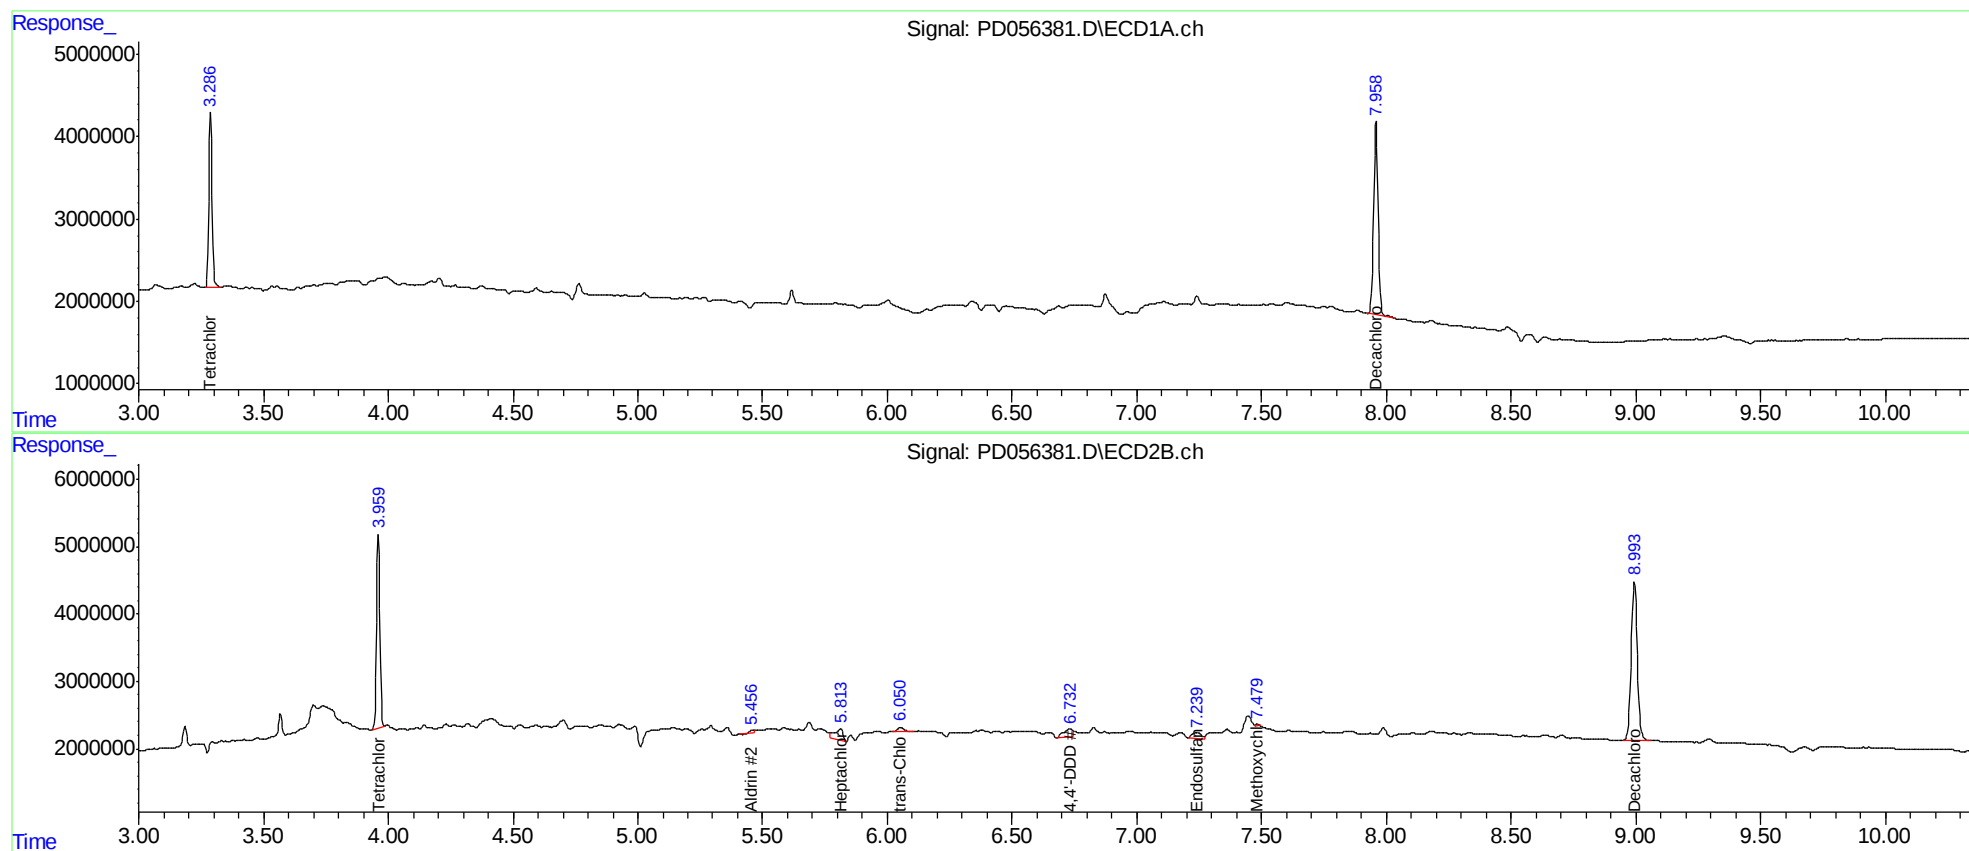


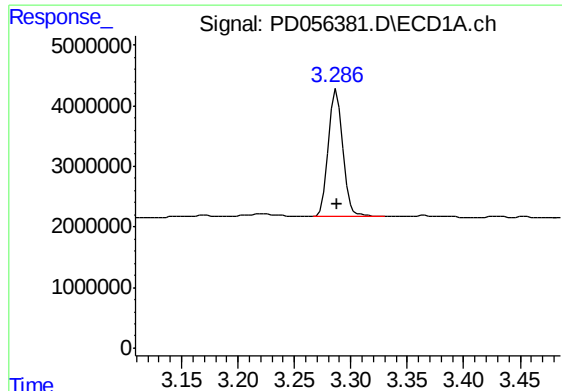

#1 Tetrachloro-m-xylene


R.T.: 3.287 min
Delta R.T.: 0.000 min
Response: 18660109
Conc: 22.53 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0BS3

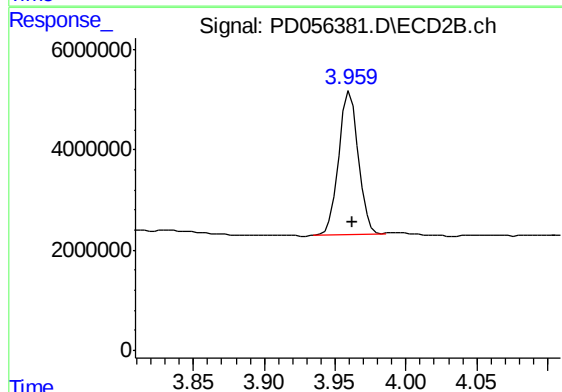


#1 Tetrachloro-m-xylene

R.T.: 3.961 min
Delta R.T.: -0.002 min
Response: 27630650
Conc: 22.98 ng/ml

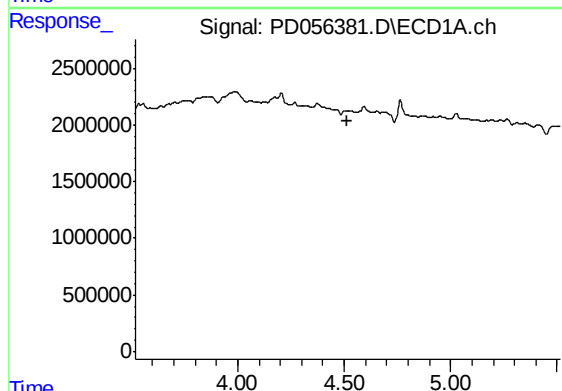


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.516 min
Response: 0
Conc: N.D.

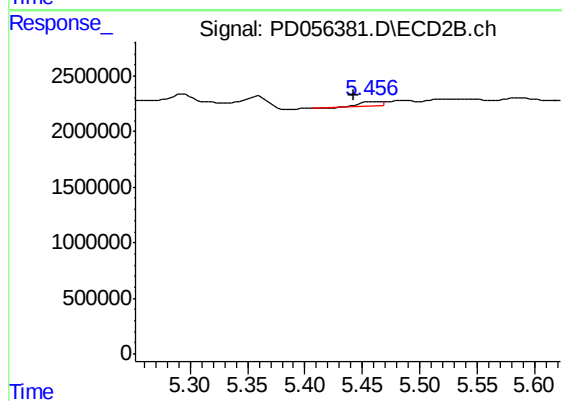

#5 Aldrin


R.T.: 5.458 min
Delta R.T.: 0.016 min
Response: 477836
Conc: 0.29 ng/ml

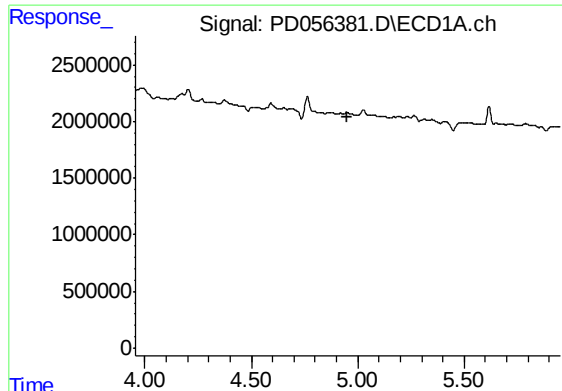

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.953 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C0BS3

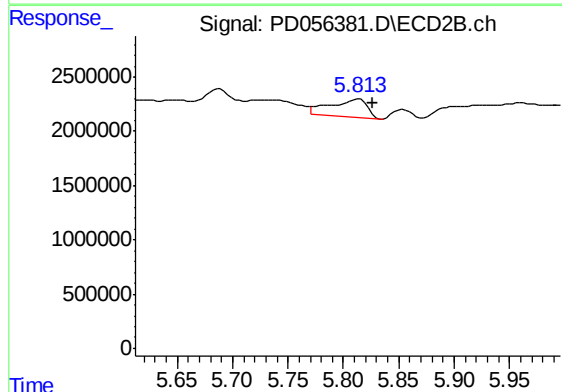


#8 Heptachlor epoxide

R.T.: 5.814 min
Delta R.T.: -0.013 min
Response: 3839990
Conc: 2.48 ng/ml

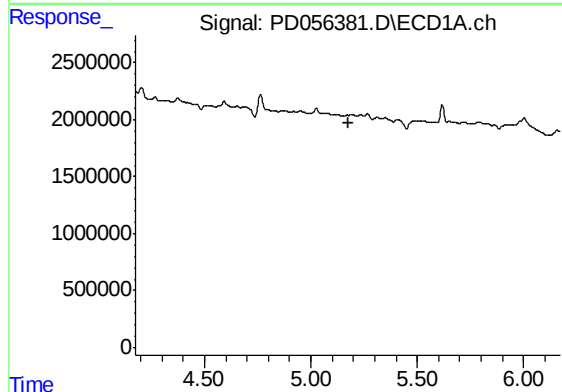


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.175 min
Response: 0
Conc: N.D.

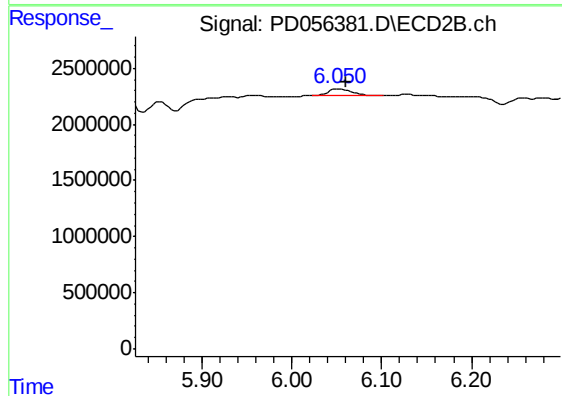

#10 trans-Chlordane


R.T.: 6.052 min
Delta R.T.: -0.008 min
Response: 997764
Conc: 0.60 ng/ml

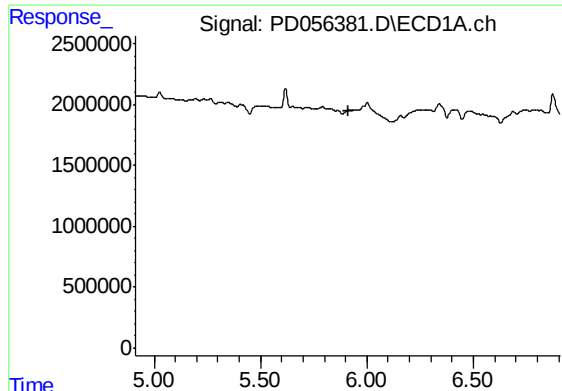

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.912 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C0BS3

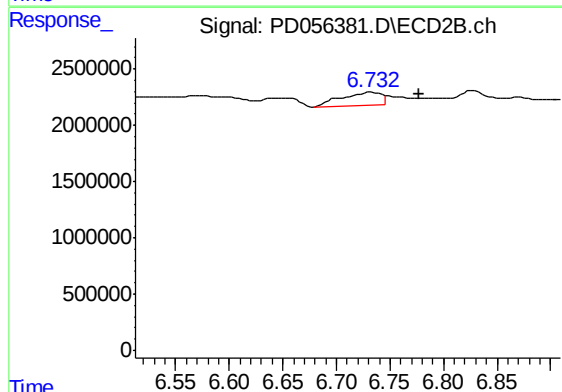


#16 4,4'-DDD

R.T.: 6.733 min
Delta R.T.: -0.045 min
Response: 3127394
Conc: 2.66 ng/ml

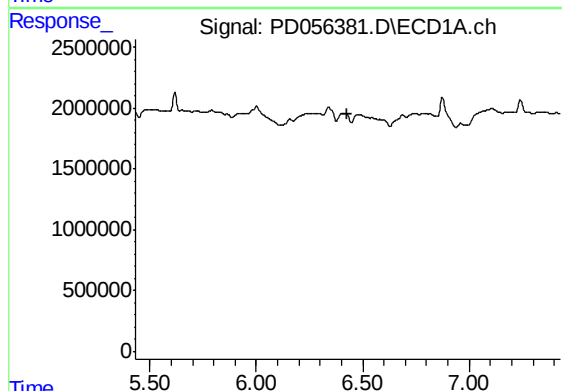


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 6.430 min
Response: 0
Conc: N.D.

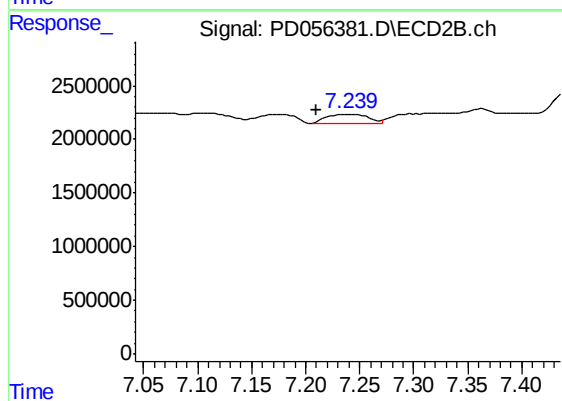

#19 Endosulfan Sulfate


R.T.: 7.241 min
Delta R.T.: 0.031 min
Response: 2295252
Conc: 1.72 ng/ml

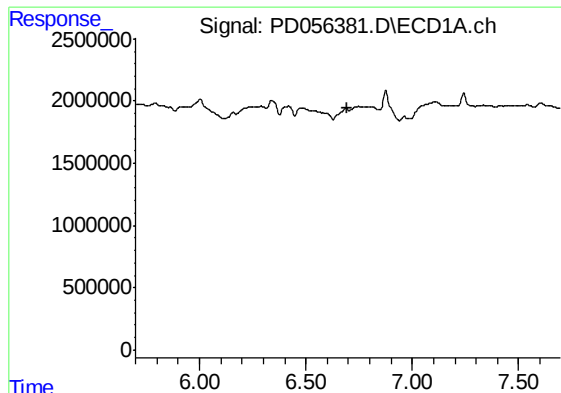

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.696 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C0BS3

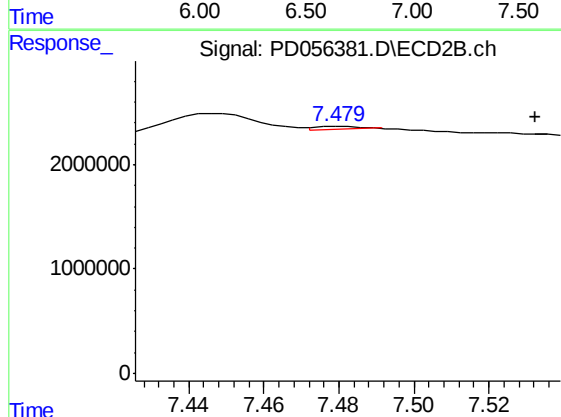


#20 Methoxychlor

R.T.: 7.481 min
Delta R.T.: -0.051 min
Response: 390504
Conc: 0.64 ng/ml

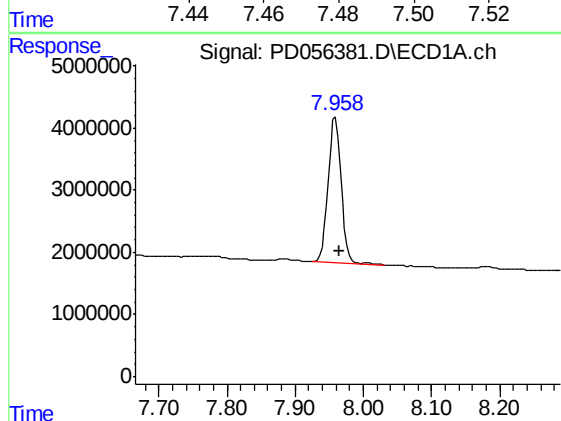

#27 Decachlorobiphenyl

R.T.: 7.959 min
Delta R.T.: -0.006 min
Response: 30888162
Conc: 34.21 ng/ml

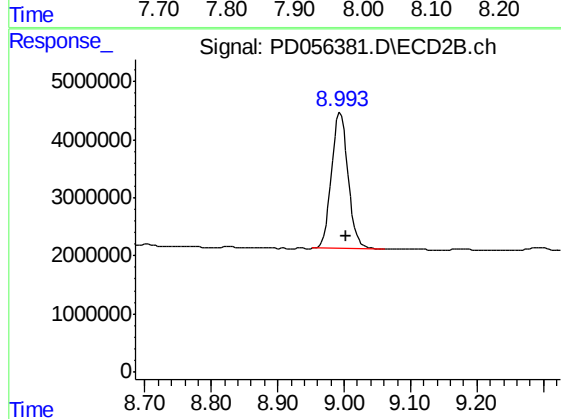

#27 Decachlorobiphenyl

R.T.: 8.994 min
Delta R.T.: -0.008 min
Response: 40713902
Conc: 33.84 ng/ml