

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121119\
 Data File : PD056388.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Dec 2019 16:42
 Operator : SG\AJ
 Sample : K6170-16
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0BW6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 01:17:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.288	3.961	19117797	28427913	23.084	23.645
27)	SA Decachlor...	7.960	8.993	35467134	46607102	39.278	38.738
Target Compounds							
3)	MA gamma-BHC...	0.000	4.593f	0	485918	N.D.	0.301
5)	MB Aldrin	0.000	5.489f	0	942510	N.D.	0.574
6)	B beta-BHC	4.209f	4.765f	3032621	480051	5.634	0.583 #
7)	B delta-BHC	0.000	4.989f	0	2772660	N.D.	1.665
8)	B Heptachlo...	0.000	5.815	0	2967551	N.D.	1.915
10)	B trans-Chl...	0.000	6.051	0	1066367	N.D.	0.645
16)	A 4,4'-DDD	0.000	6.733f	0	2386230	N.D.	2.028
19)	B Endosulfa...	0.000	7.239	0	4578467	N.D.	3.424


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121119\
Data File : PD056388.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Dec 2019 16:42
Operator : SG\AJ
Sample : K6170-16
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
C0BW6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 01:17:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

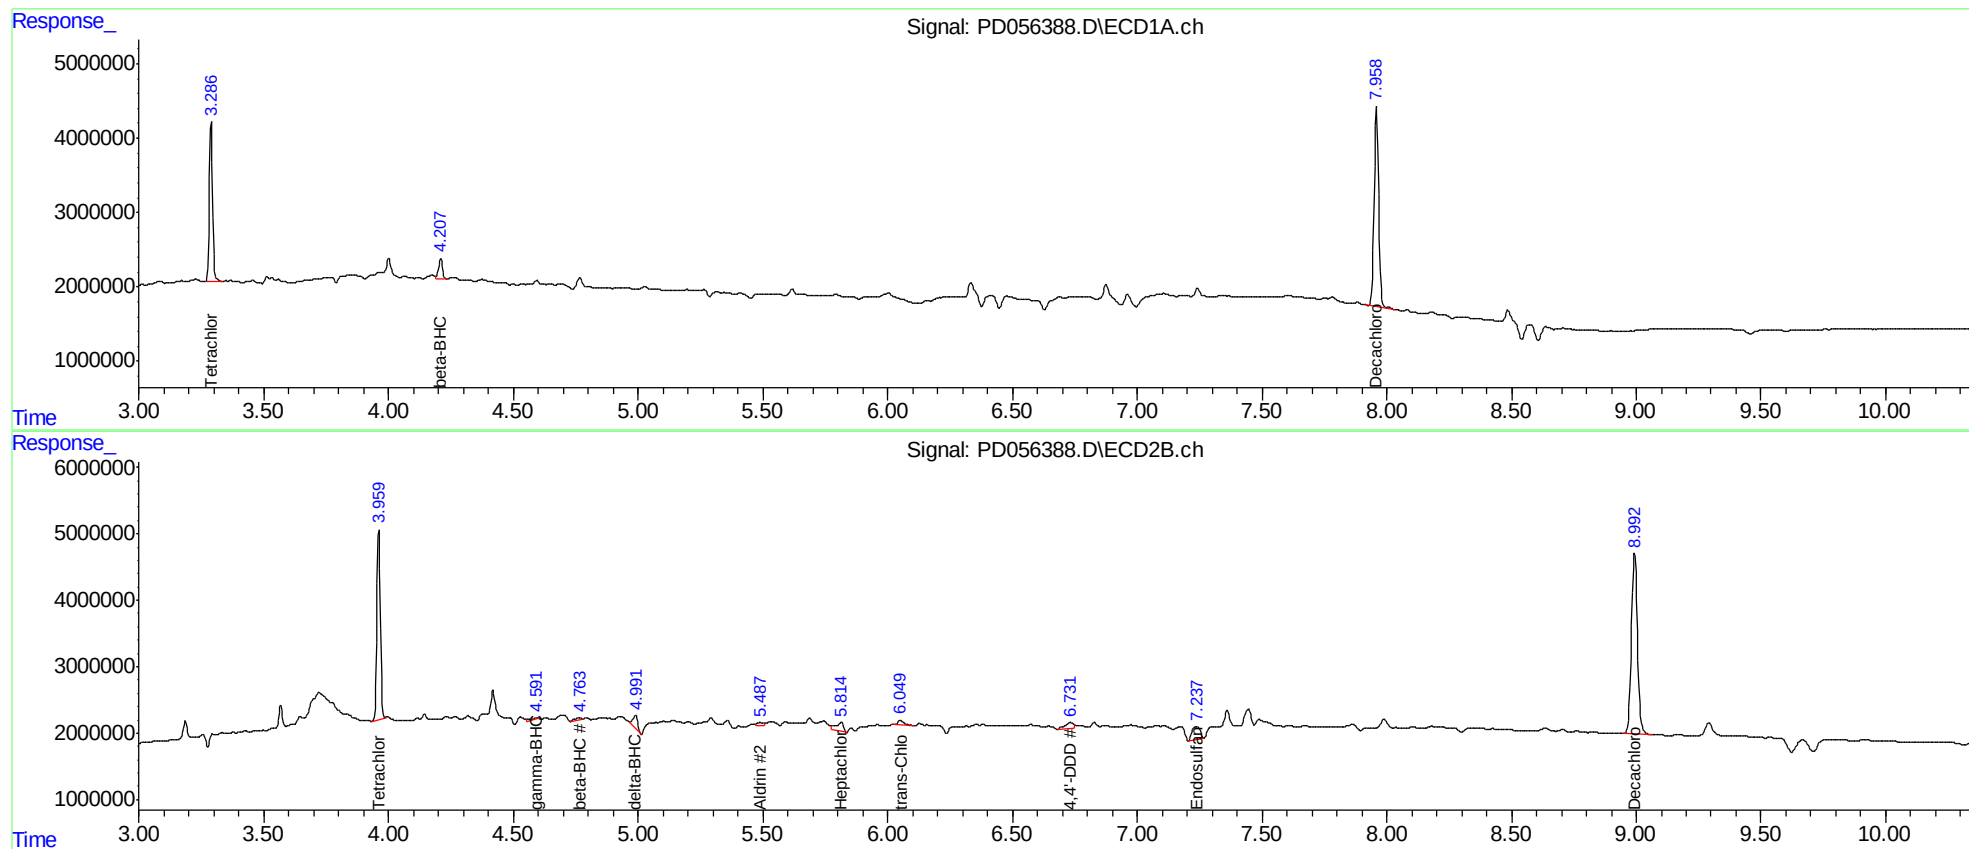


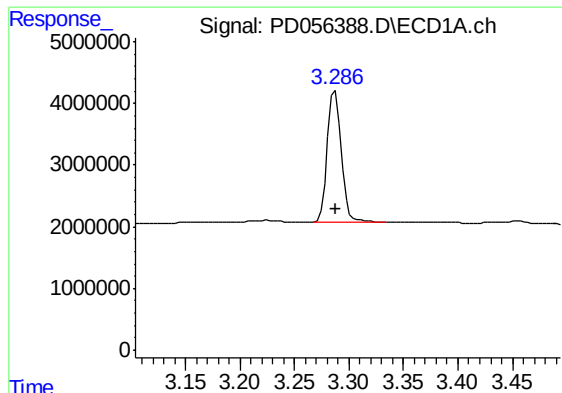

#1 Tetrachloro-m-xylene


R.T.: 3.288 min
Delta R.T.: 0.000 min
Response: 19117797
Conc: 23.08 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0BW6

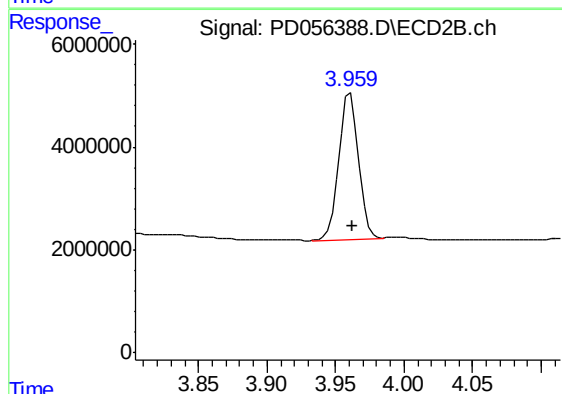


#1 Tetrachloro-m-xylene

R.T.: 3.961 min
Delta R.T.: -0.002 min
Response: 28427913
Conc: 23.65 ng/ml

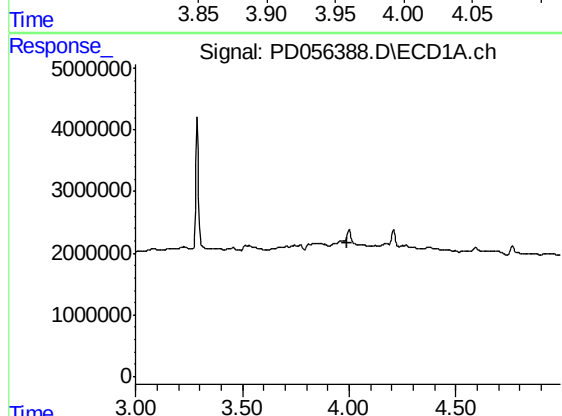


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 3.991 min
Response: 0
Conc: N.D.

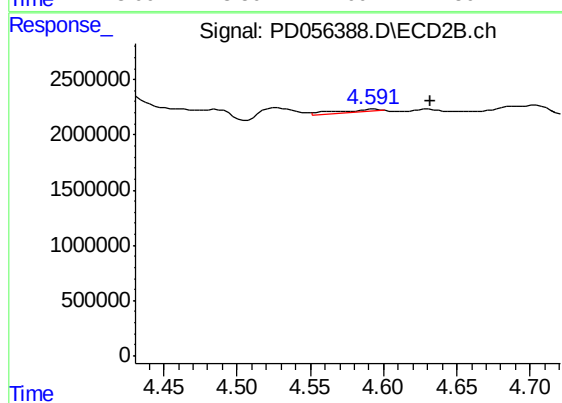

#3 gamma-BHC (Lindane)


R.T.: 4.593 min
Delta R.T.: -0.039 min
Response: 485918
Conc: 0.30 ng/ml

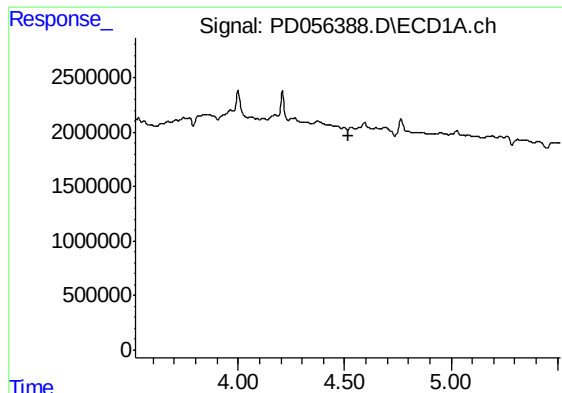

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 4.516 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C0BW6

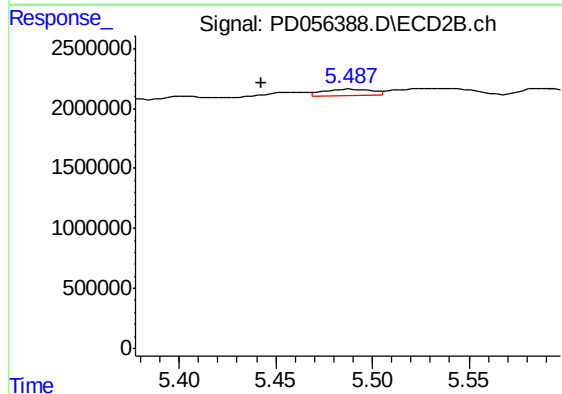


#5 Aldrin

R.T.: 5.489 min
Delta R.T.: 0.046 min
Response: 942510
Conc: 0.57 ng/ml

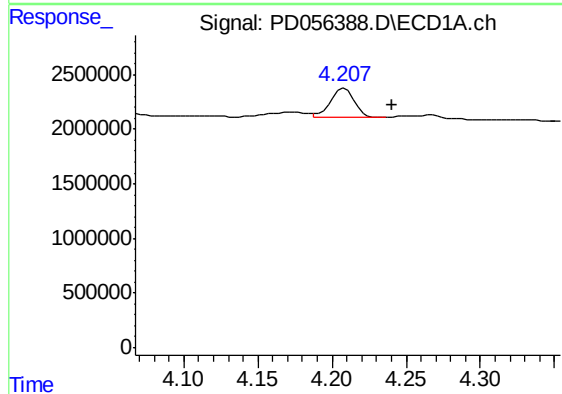


#6 beta-BHC

R.T.: 4.209 min
Delta R.T.: -0.032 min
Response: 3032621
Conc: 5.63 ng/ml

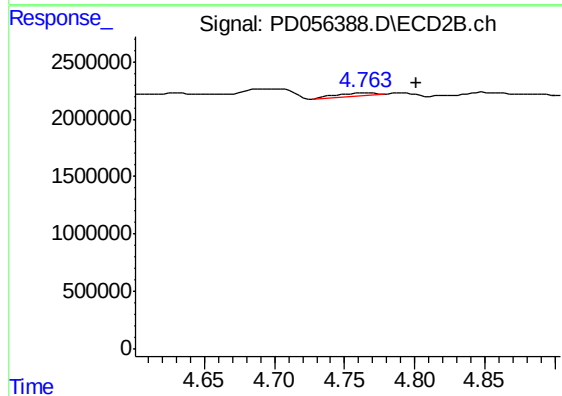

#6 beta-BHC


R.T.: 4.765 min
Delta R.T.: -0.036 min
Response: 480051
Conc: 0.58 ng/ml

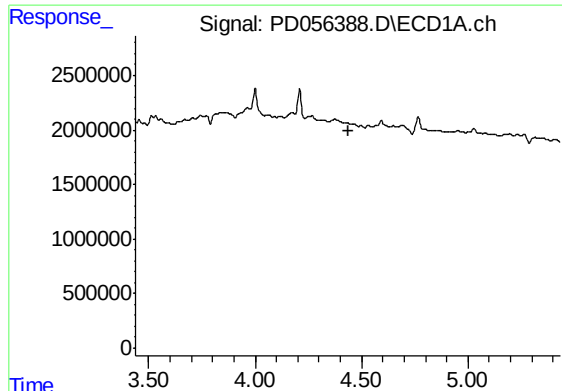

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.436 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C0BW6

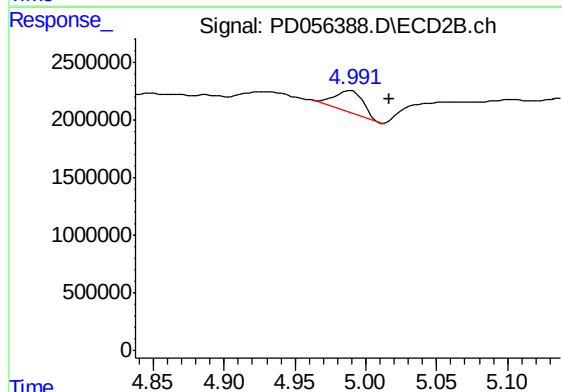


#7 delta-BHC

R.T.: 4.989 min
Delta R.T.: -0.028 min
Response: 2772660
Conc: 1.66 ng/ml

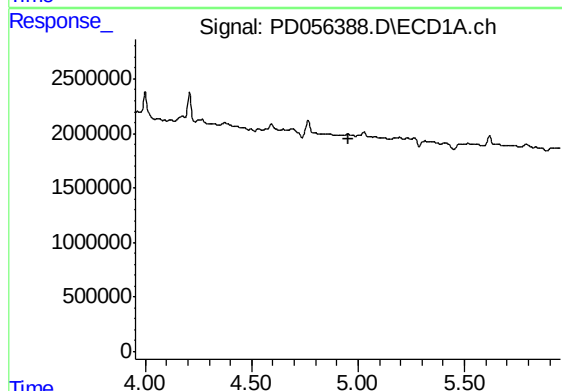


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.953 min
Response: 0
Conc: N.D.

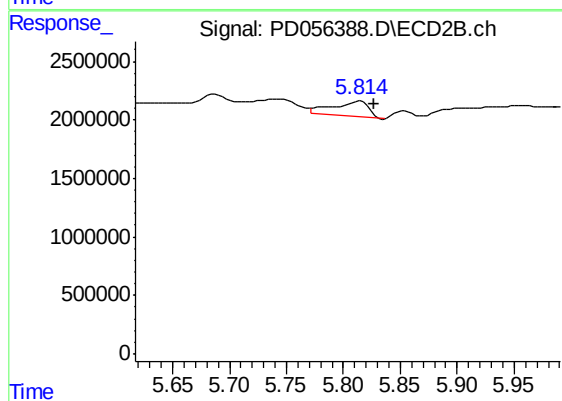

#8 Heptachlor epoxide


R.T.: 5.815 min
Delta R.T.: -0.012 min
Response: 2967551
Conc: 1.92 ng/ml

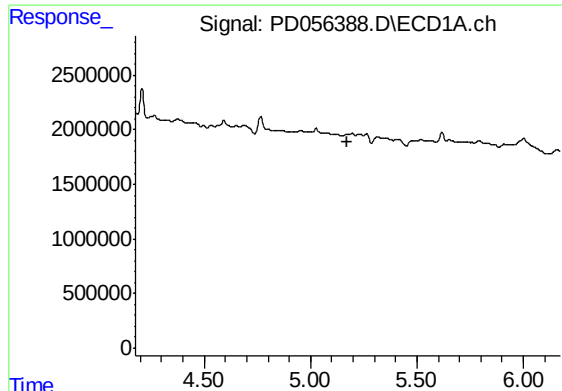

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.175 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C0BW6

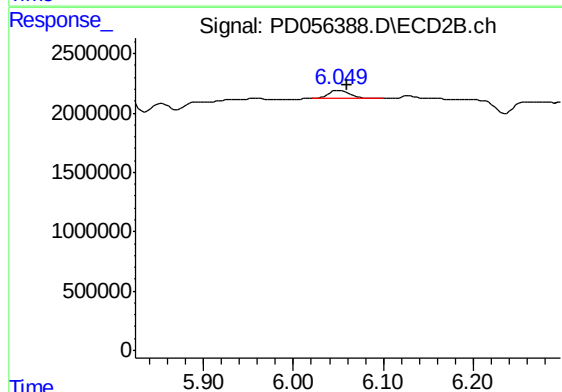


#10 trans-Chlordane

R.T.: 6.051 min
Delta R.T.: -0.009 min
Response: 1066367
Conc: 0.64 ng/ml

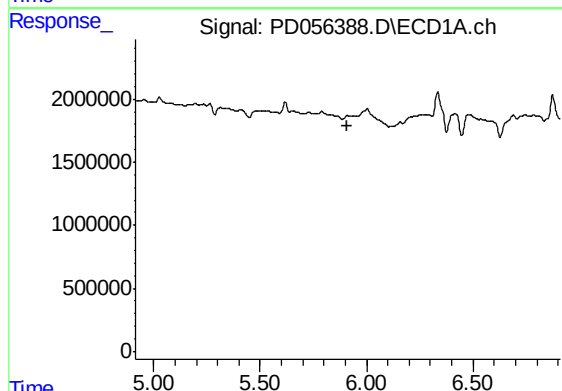


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 5.912 min
Response: 0
Conc: N.D.

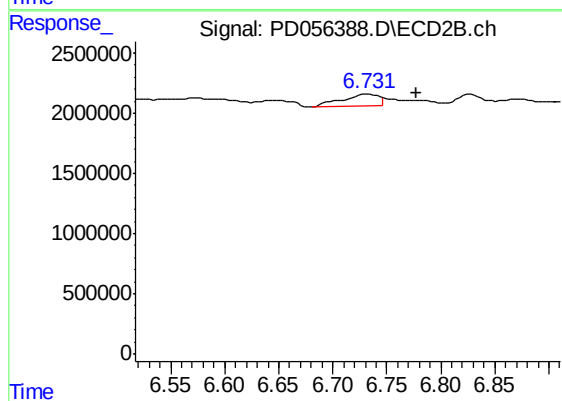

#16 4,4'-DDD


R.T.: 6.733 min
Delta R.T.: -0.045 min
Response: 2386230
Conc: 2.03 ng/ml

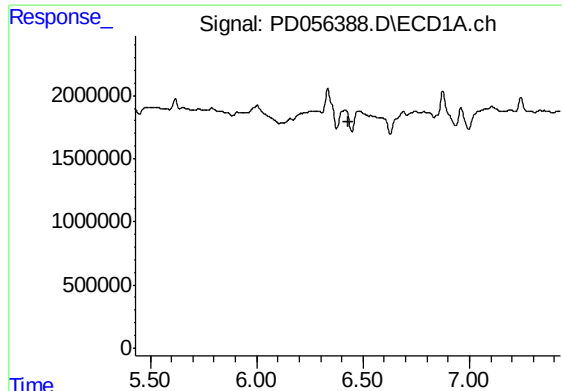

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 6.430 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C0BW6

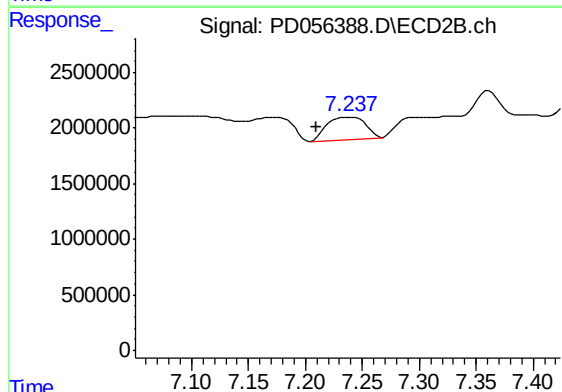


#19 Endosulfan Sulfate

R.T.: 7.239 min
Delta R.T.: 0.029 min
Response: 4578467
Conc: 3.42 ng/ml

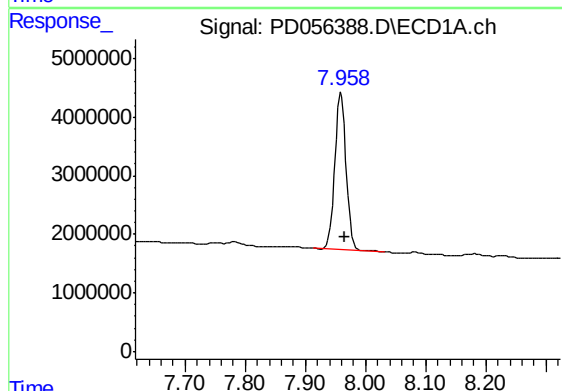

#27 Decachlorobiphenyl

R.T.: 7.960 min
Delta R.T.: -0.006 min
Response: 35467134
Conc: 39.28 ng/ml

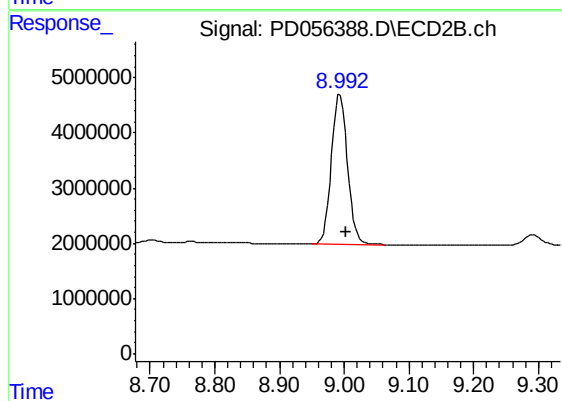

#27 Decachlorobiphenyl

R.T.: 8.993 min
Delta R.T.: -0.009 min
Response: 46607102
Conc: 38.74 ng/ml