

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121119\
 Data File : PD056391.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Dec 2019 17:24
 Operator : SG\AJ
 Sample : K6170-19
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0BT3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 01:18:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.287	3.961	18041772	26708372	21.784	22.215
27)	SA Decachlor...	7.959	8.995	31234735	41601780	34.591	34.577
Target Compounds							
3)	MA gamma-BHC...	0.000	4.591f	0	422621	N.D.	0.262
5)	MB Aldrin	0.000	5.456	0	525783	N.D.	0.320
7)	B delta-BHC	0.000	4.989f	0	3074130	N.D.	1.846
8)	B Heptachlo...	0.000	5.857	0	1106349	N.D.	0.714
10)	B trans-Chl...	0.000	6.052	0	1675969	N.D.	1.014
15)	B Endosulfa...	0.000	6.875	0	339368	N.D.	0.232
16)	A 4,4'-DDD	0.000	6.733f	0	1851683	N.D.	1.574
19)	B Endosulfa...	0.000	7.240	0	5523122	N.D.	4.131


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121119\
Data File : PD056391.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Dec 2019 17:24
Operator : SG\AJ
Sample : K6170-19
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
C0BT3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 01:18:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

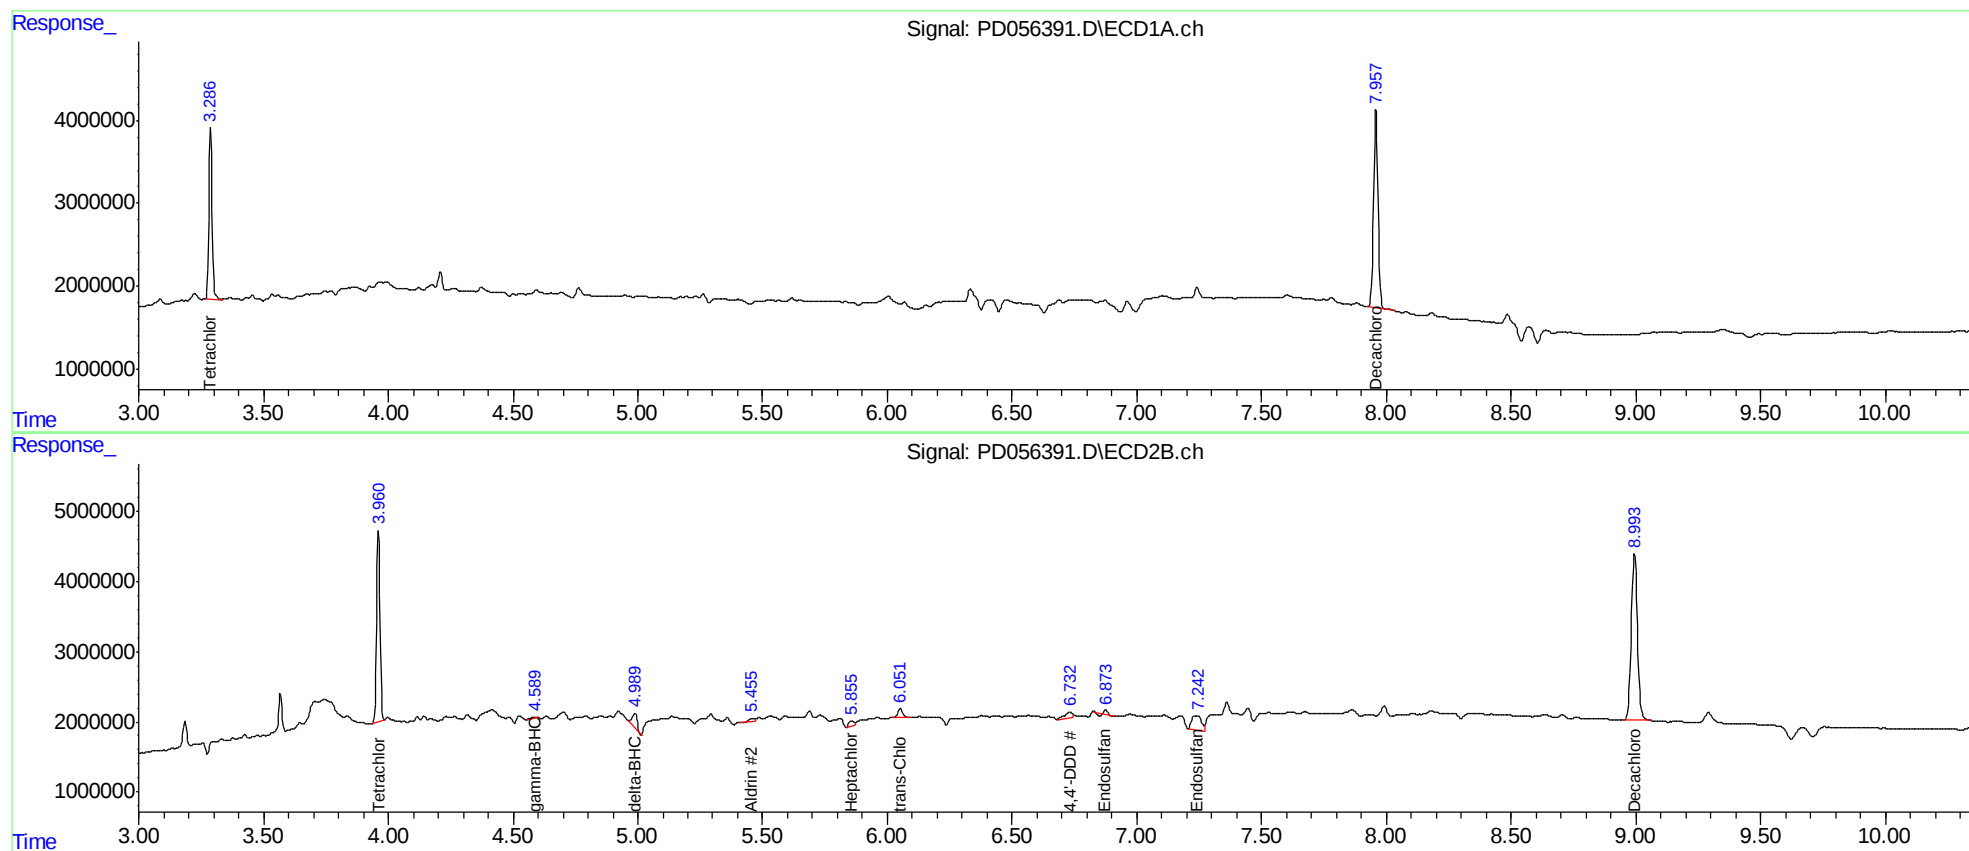


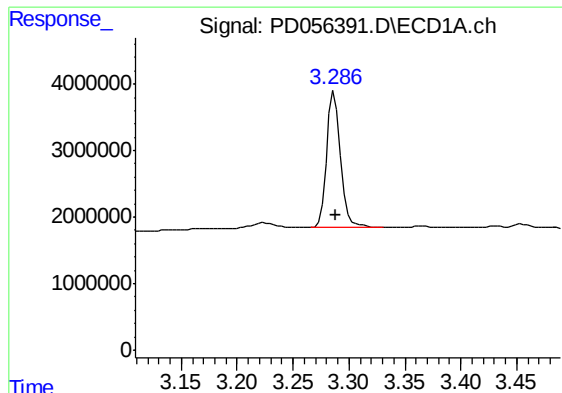

#1 Tetrachloro-m-xylene


R.T.: 3.287 min
Delta R.T.: 0.000 min
Response: 18041772
Conc: 21.78 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0BT3

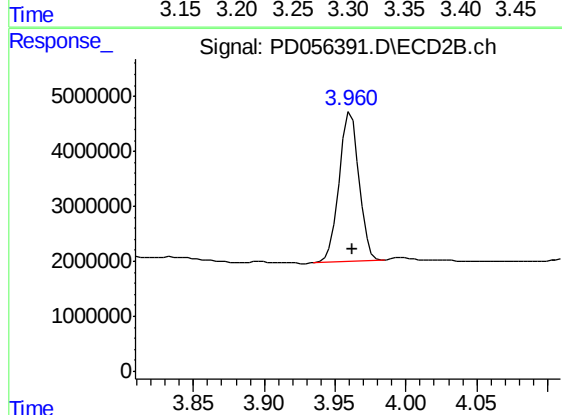


#1 Tetrachloro-m-xylene

R.T.: 3.961 min
Delta R.T.: -0.001 min
Response: 26708372
Conc: 22.22 ng/ml

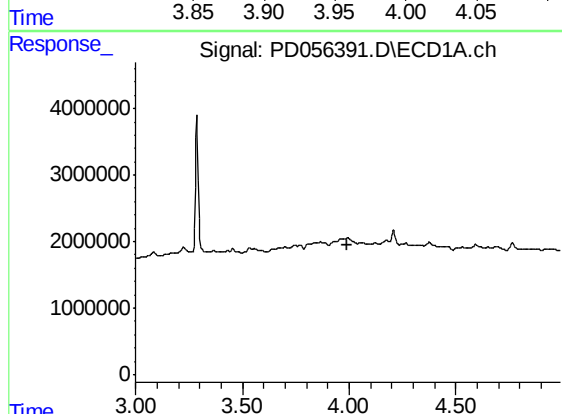


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 3.991 min
Response: 0
Conc: N.D.

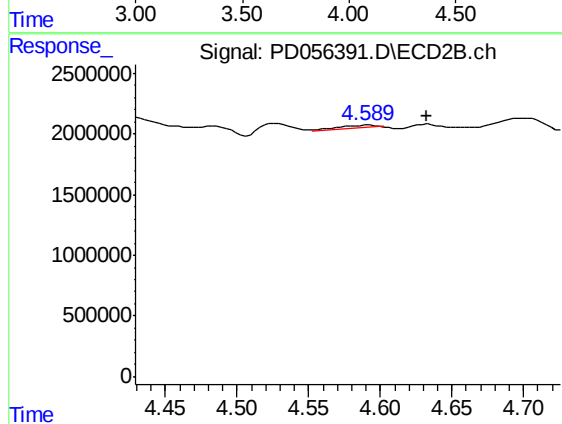

#3 gamma-BHC (Lindane)


R.T.: 4.591 min
Delta R.T.: -0.041 min
Response: 422621
Conc: 0.26 ng/ml

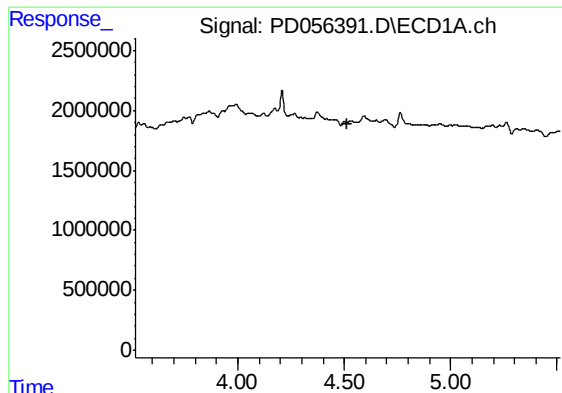

#5 Aldrin


R.T.: 0.000 min
Exp R.T. : 4.516 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C0BT3

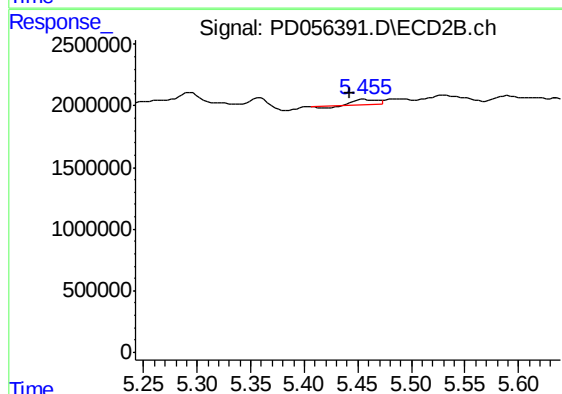


#5 Aldrin

R.T.: 5.456 min
Delta R.T.: 0.014 min
Response: 525783
Conc: 0.32 ng/ml

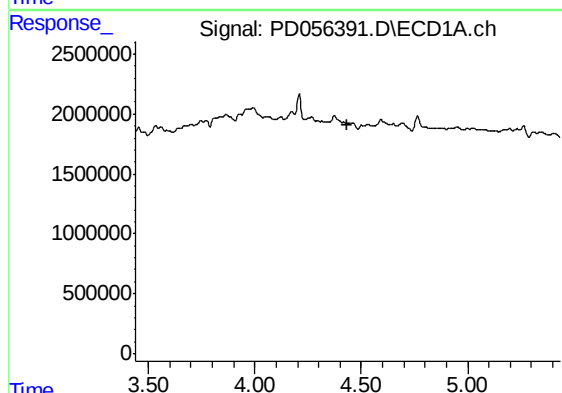


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.436 min
Response: 0
Conc: N.D.

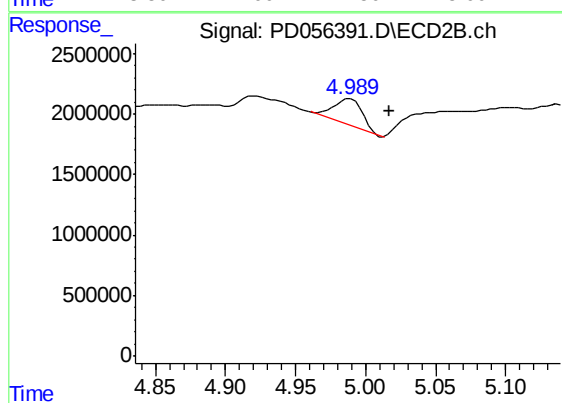

#7 delta-BHC


R.T.: 4.989 min
Delta R.T.: -0.028 min
Response: 3074130
Conc: 1.85 ng/ml

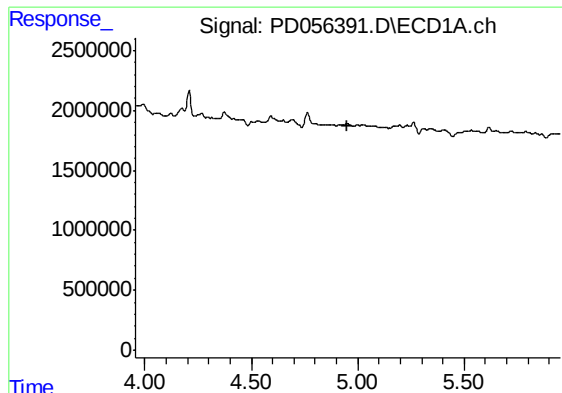

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.953 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C0BT3

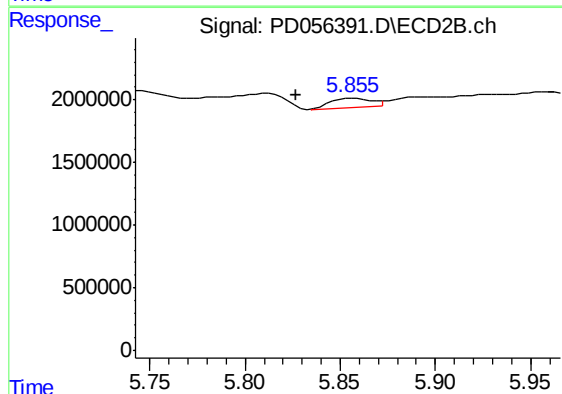


#8 Heptachlor epoxide

R.T.: 5.857 min
Delta R.T.: 0.030 min
Response: 1106349
Conc: 0.71 ng/ml

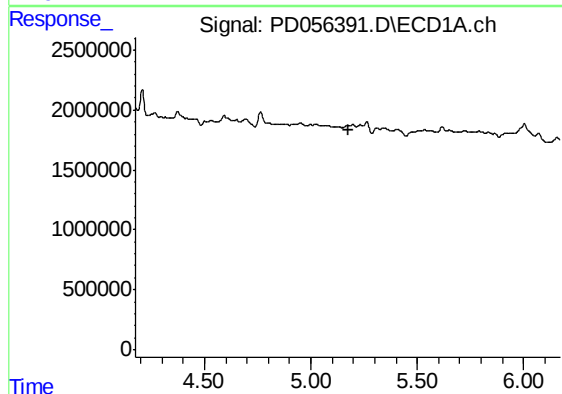


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.175 min
Response: 0
Conc: N.D.

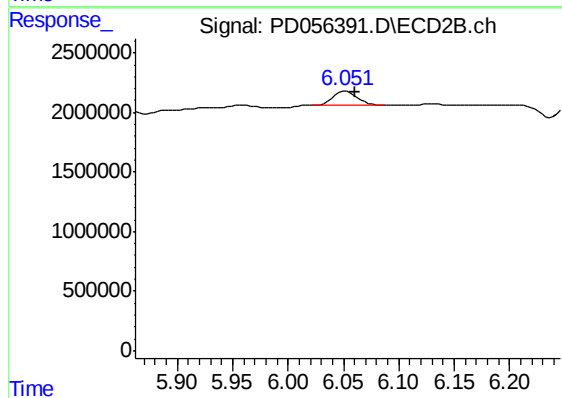

#10 trans-Chlordane


R.T.: 6.052 min
Delta R.T.: -0.008 min
Response: 1675969
Conc: 1.01 ng/ml

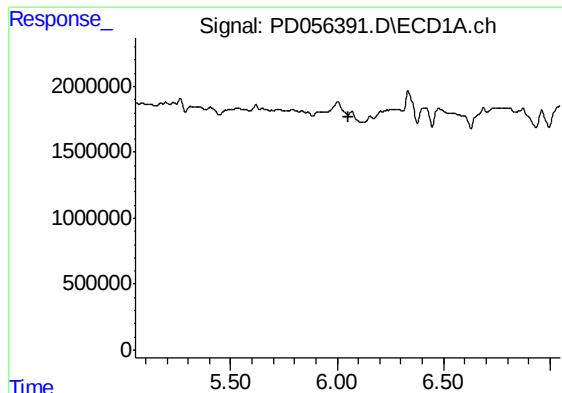

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.051 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C0BT3

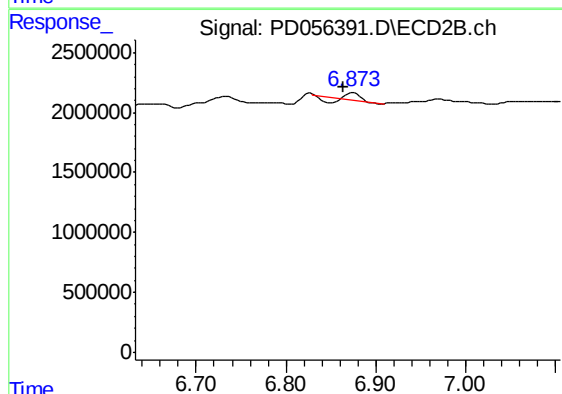


#15 Endosulfan II

R.T.: 6.875 min
Delta R.T.: 0.011 min
Response: 339368
Conc: 0.23 ng/ml

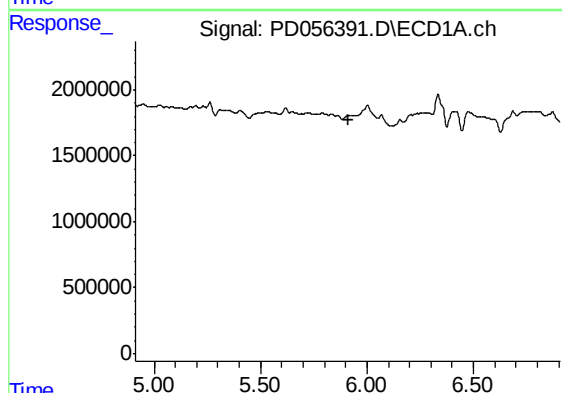


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 5.912 min
Response: 0
Conc: N.D.

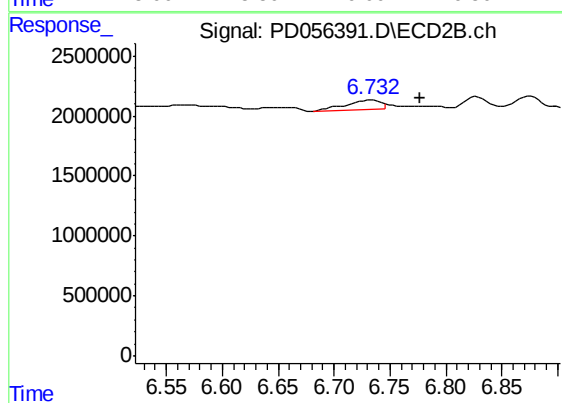

#16 4,4'-DDD


R.T.: 6.733 min
Delta R.T.: -0.044 min
Response: 1851683
Conc: 1.57 ng/ml

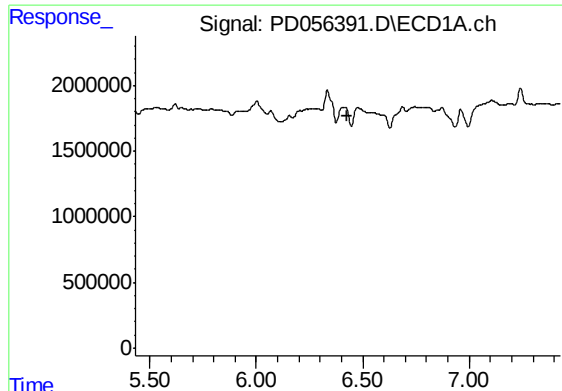

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 6.430 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C0BT3

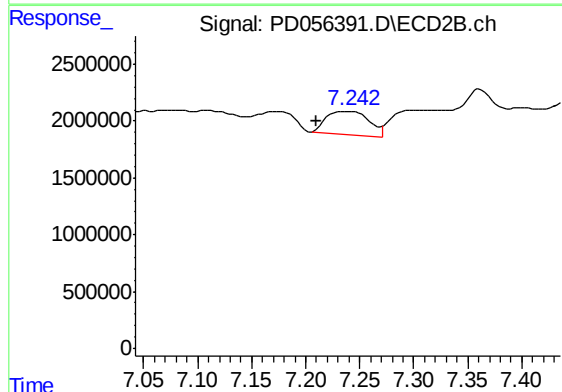


#19 Endosulfan Sulfate

R.T.: 7.240 min
Delta R.T.: 0.030 min
Response: 5523122
Conc: 4.13 ng/ml

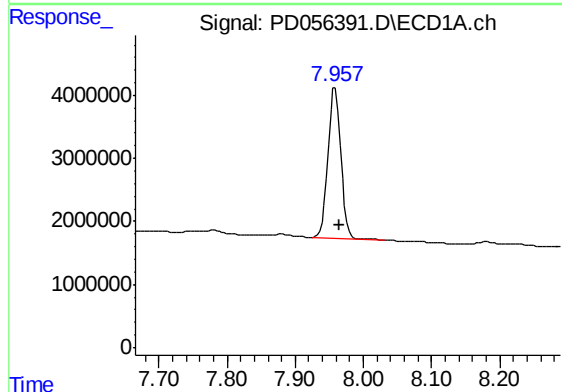

#27 Decachlorobiphenyl

R.T.: 7.959 min
Delta R.T.: -0.007 min
Response: 31234735
Conc: 34.59 ng/ml

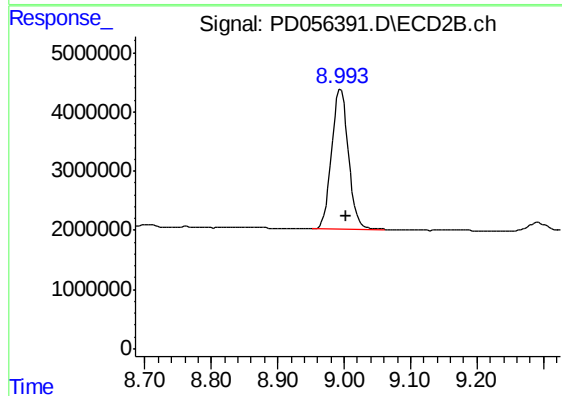

#27 Decachlorobiphenyl

R.T.: 8.995 min
Delta R.T.: -0.008 min
Response: 41601780
Conc: 34.58 ng/ml