

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121119\
 Data File : PD056392.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Dec 2019 17:38
 Operator : SG\AJ
 Sample : K6170-23MS
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0BW3MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 01:18:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.288	3.961	19650965	29231997	23.727	24.314
27)	SA Decachlor...	7.958	8.994	33614487	43832246	37.227	36.431
Target Compounds							
3)	MA gamma-BHC...	3.990	4.630	70903597	103.6E6	63.141	64.200
4)	MA Heptachlor	4.275	5.136	61069373	94903820	60.590	58.230
5)	MB Aldrin	4.514	5.440	57807108	89597326	53.230	54.527
13)	MA Dieldrin	5.520	6.434	127.8E6	191.0E6	125.777	121.575
14)	MA Endrin	5.773	6.651	108.7E6	154.6E6	130.127	122.141
17)	MA 4,4'-DDT	6.143	7.071	87564611	133.8E6	124.445	113.185

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121119\
Data File : PD056392.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Dec 2019 17:38
Operator : SG\AJ
Sample : K6170-23MS
Misc :
ALS Vial : 40 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 01:18:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

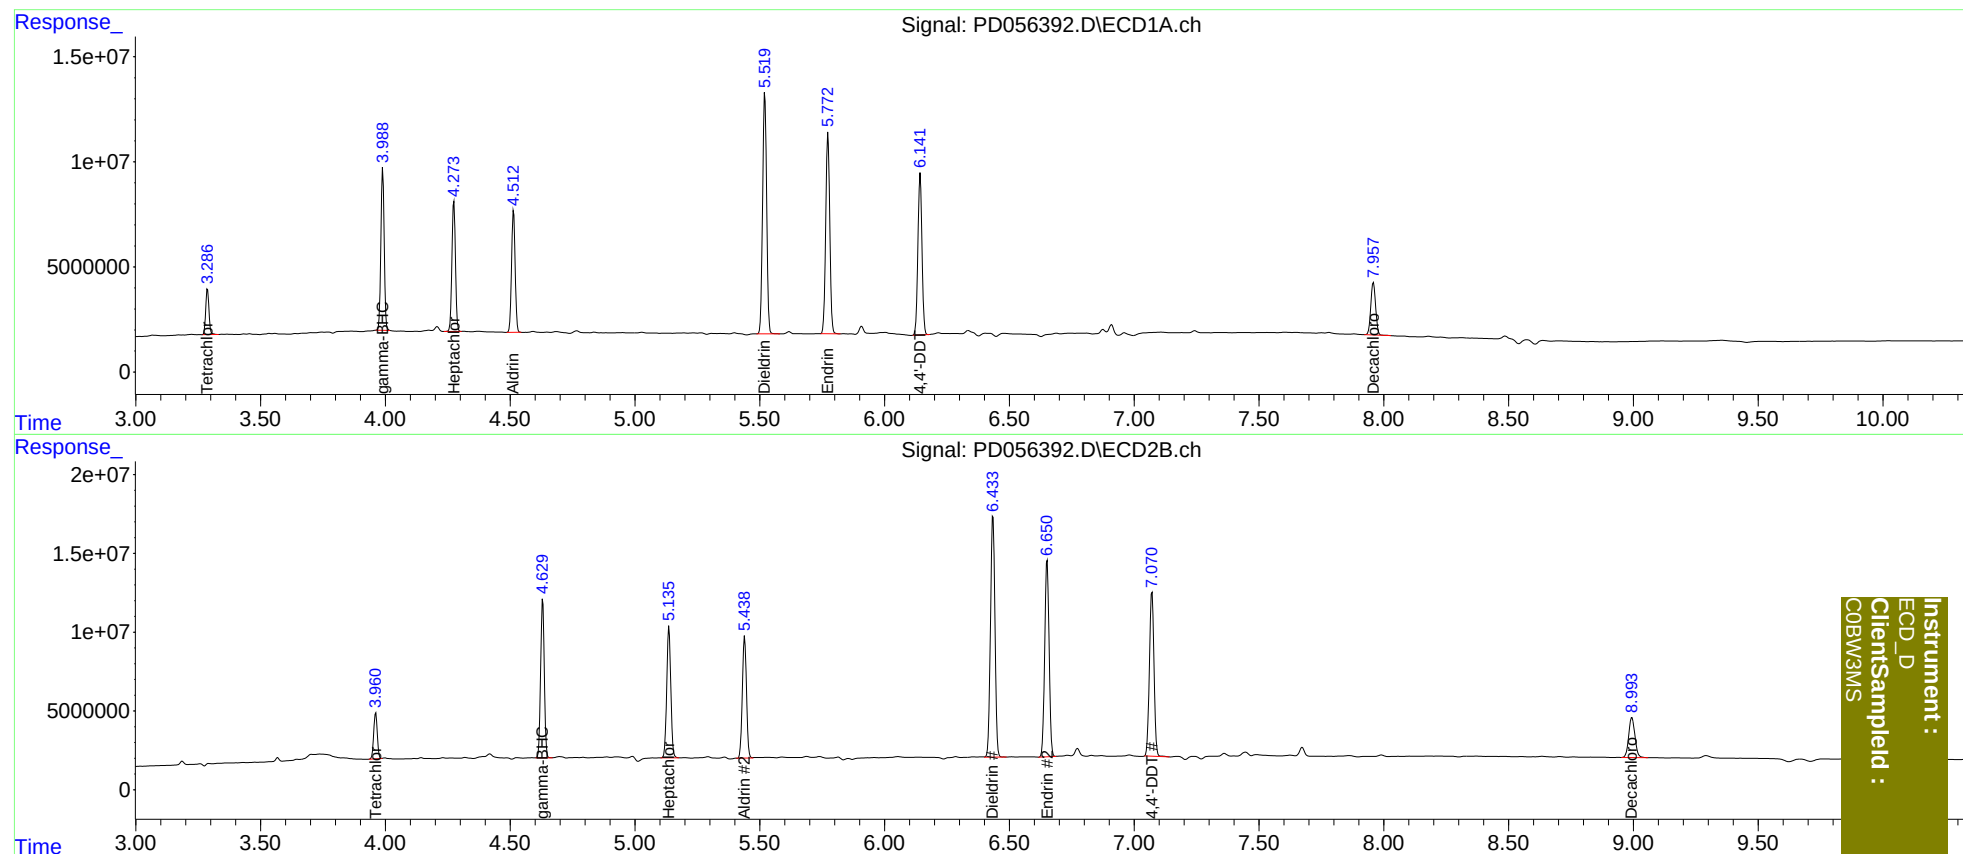

Instrument :
ECD_D
ClientSampled :
C08W3MS