

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121119\
 Data File : PD056393.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Dec 2019 17:52
 Operator : SG\AJ
 Sample : K6170-24MSD
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0BW3MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 01:18:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.288	3.961	19825155	29387358	23.938	24.444
27)	SA Decachlor...	7.958	8.995	33710595	43959151	37.333	36.537
Target Compounds							
3)	MA gamma-BHC...	3.989	4.631	71151366	103.9E6	63.362	64.373
4)	MA Heptachlor	4.274	5.136	61102530	94863151	60.622	58.205
5)	MB Aldrin	4.513	5.440	57867766	90238810	53.286	54.917
13)	MA Dieldrin	5.520	6.434	128.1E6	191.5E6	126.095	121.859
14)	MA Endrin	5.773	6.651	108.7E6	154.9E6	130.111	122.401
17)	MA 4,4'-DDT	6.142	7.071	87227154	133.6E6	123.965	113.053

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121119\
Data File : PD056393.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Dec 2019 17:52
Operator : SG\AJ
Sample : K6170-24MSD
Misc :
ALS Vial : 41 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 01:18:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

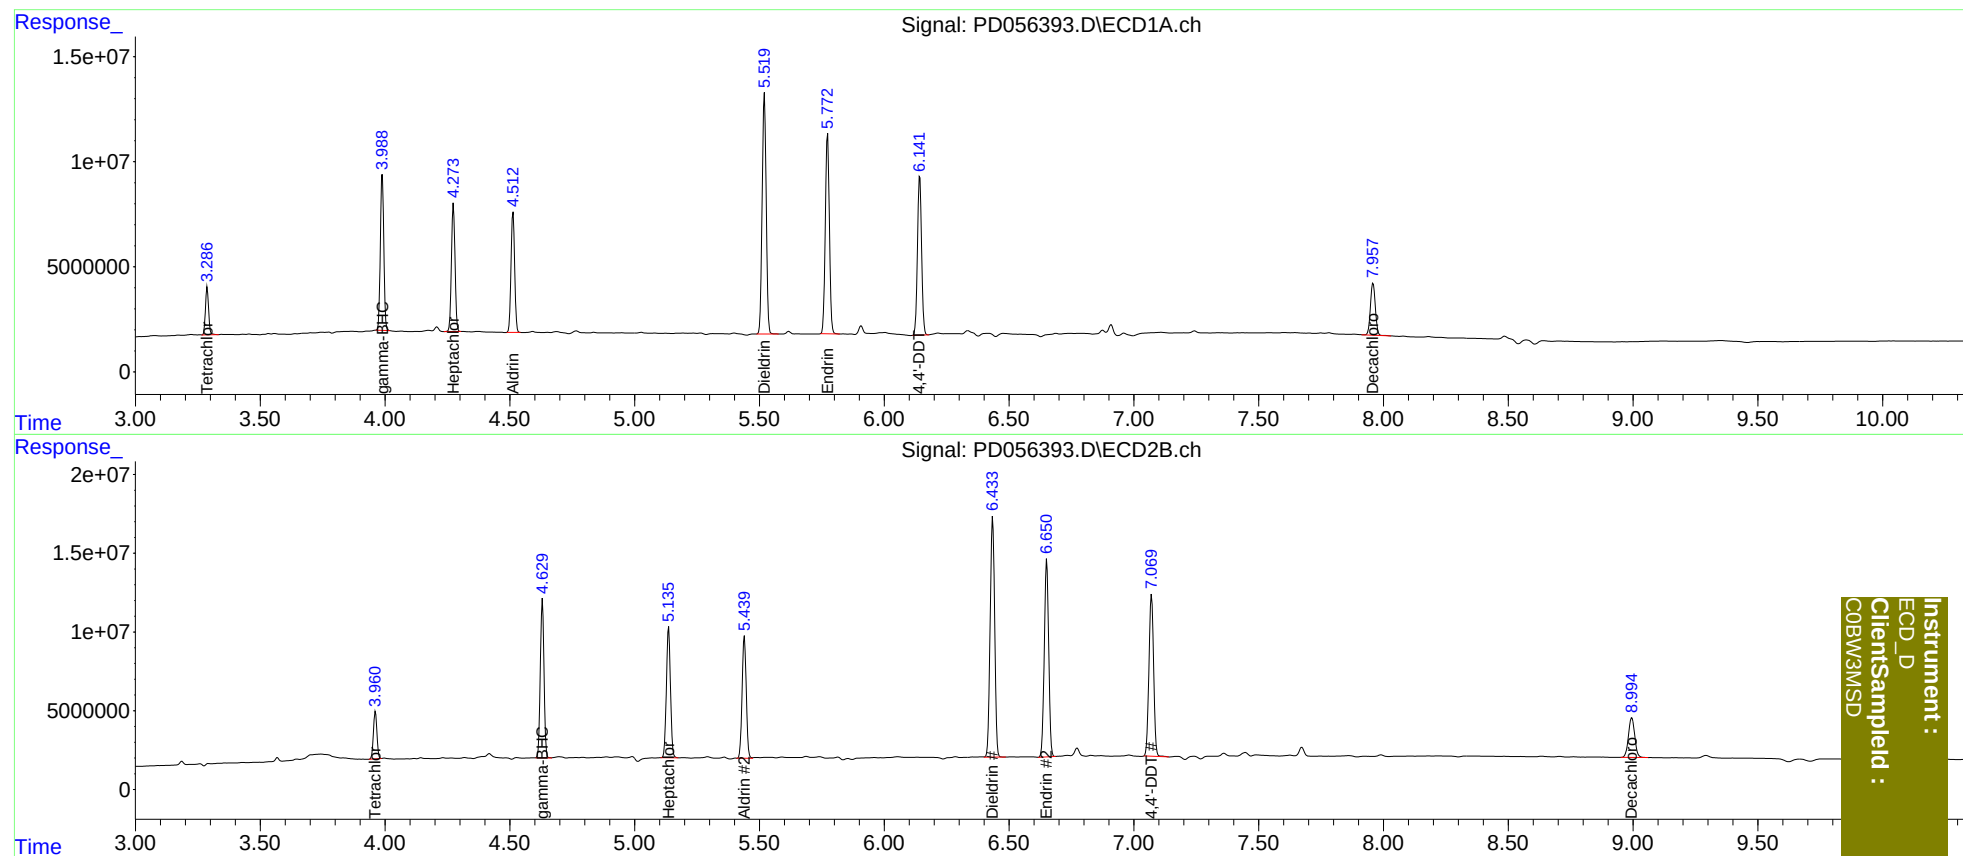

Instrument :
ECD_D
ClientSampled :
C08W3MSD