

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121123\
 Data File : PD080016.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Dec 2023 10:44
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 21:38:20 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120523CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 05 17:09:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	0.000	2.795	0	256191	N.D.	0.112
27)	SA Decachlor...	0.000	7.942	0	241303	N.D.	<MDL
Target Compounds							
5)	MB Aldrin	0.000	4.238	0	1367935	N.D.	0.405
6)	B beta-BHC	0.000	3.891f	0	290141	N.D.	0.182
7)	B delta-BHC	0.000	4.156	0	132302	N.D.	<MDL
9)	A Endosulfan I	0.000	5.095	0	1154984	N.D.	0.406
10)	B trans-Chl...	0.000	5.017	0	666554	N.D.	0.217
11)	B cis-Chlor...	0.000	5.095	0	1154984	N.D.	0.366
14)	MA Endrin	0.000	5.686	0	273997	N.D.	<MDL
15)	B Endosulfa...	0.000	5.921f	0	1503277	N.D.	0.550
18)	B Endrin al...	0.000	6.154	0	1201412	N.D.	0.568
22)	Toxaphene-1	0.000	5.044	0	284586	N.D.	16.323
25)	Toxaphene-4	0.000	6.794f	0	144056	N.D.	1.701

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121123\
Data File : PD080016.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Dec 2023 10:44
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 21:38:20 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 05 17:09:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

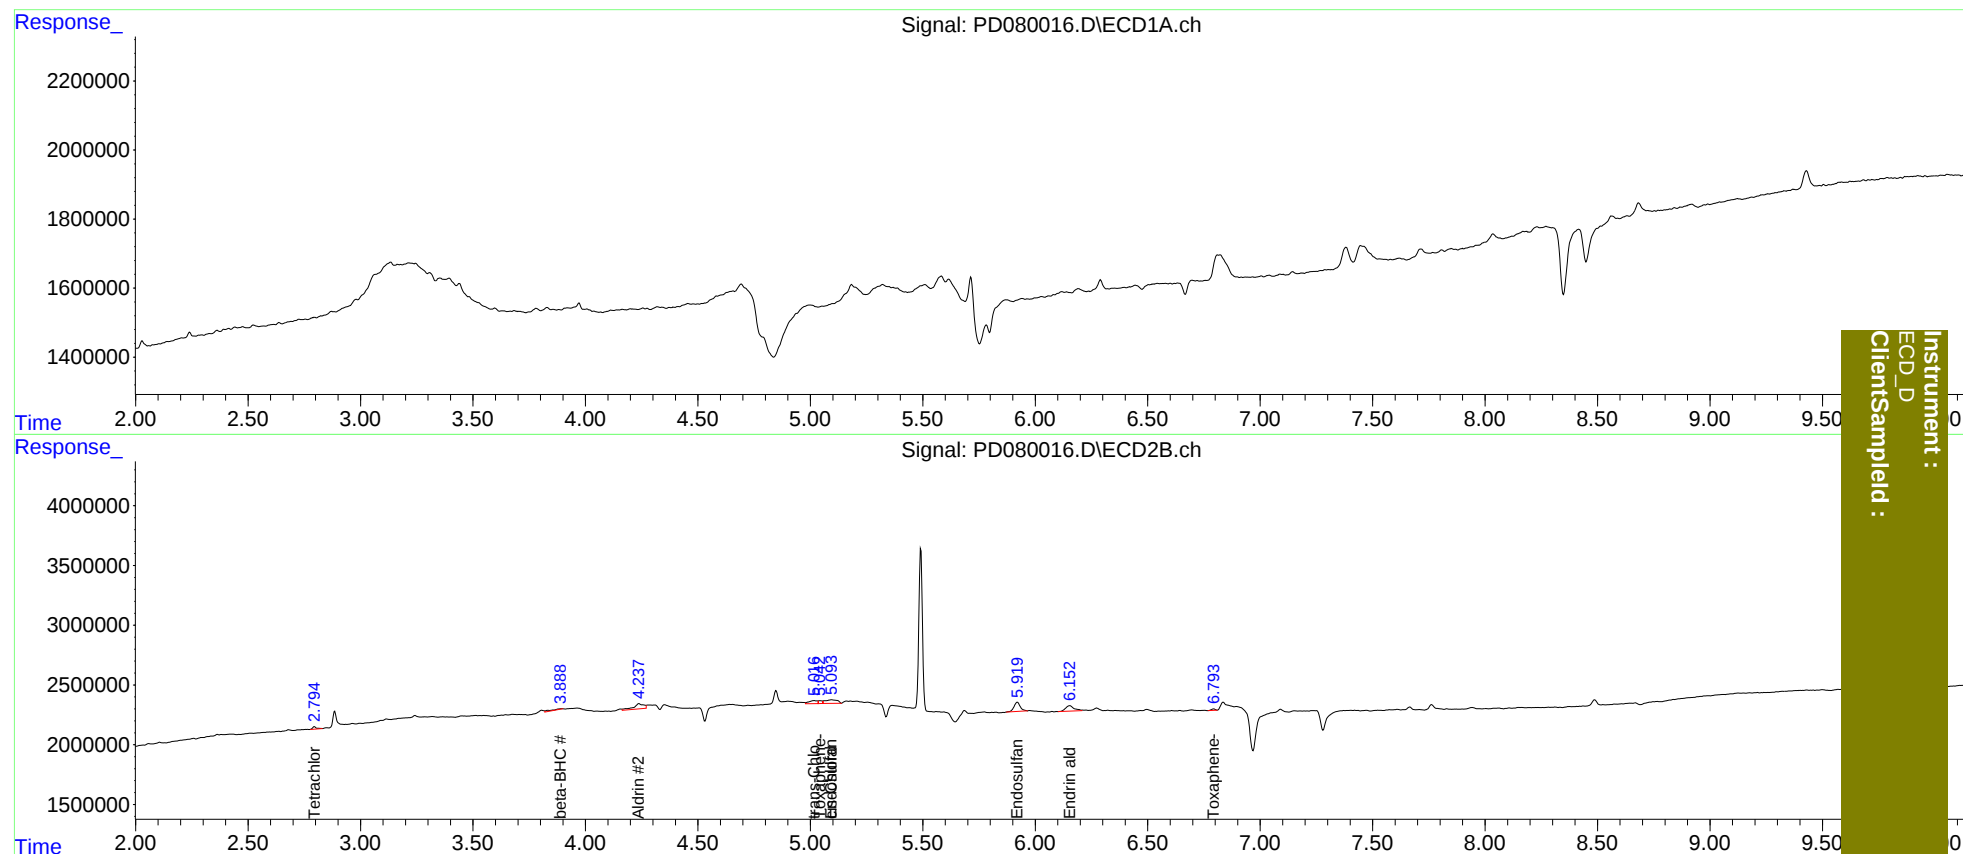


Instrument :
ECD_D
ClientSampled :
0

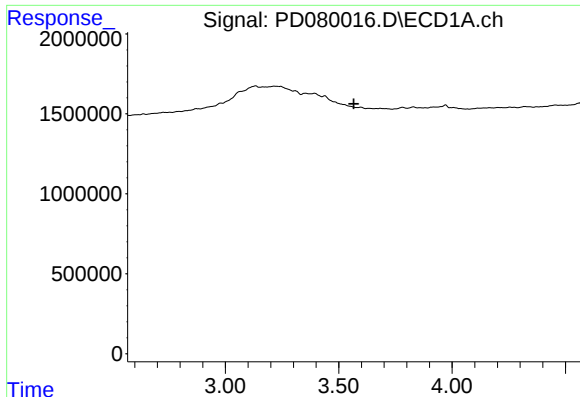

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.567 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

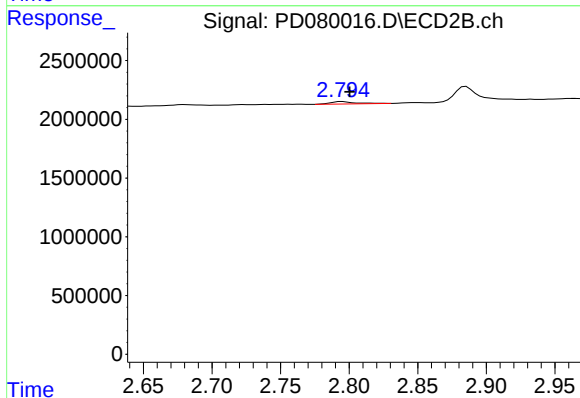


#1 Tetrachloro-m-xylene

R.T.: 2.795 min
Delta R.T.: -0.005 min
Response: 256191
Conc: 0.11 ng/ml

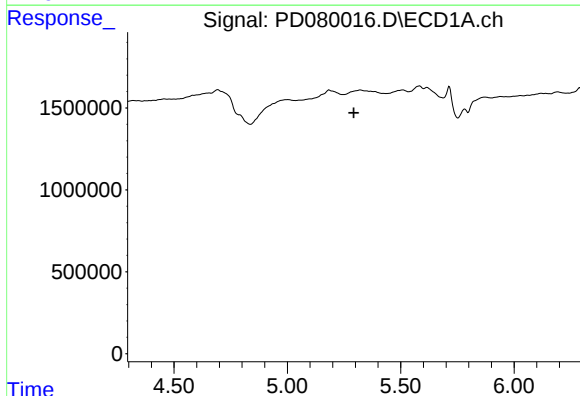


#5 Aldrin

R.T.: 0.000 min
Exp R.T.: 5.293 min
Response: 0
Conc: N.D.

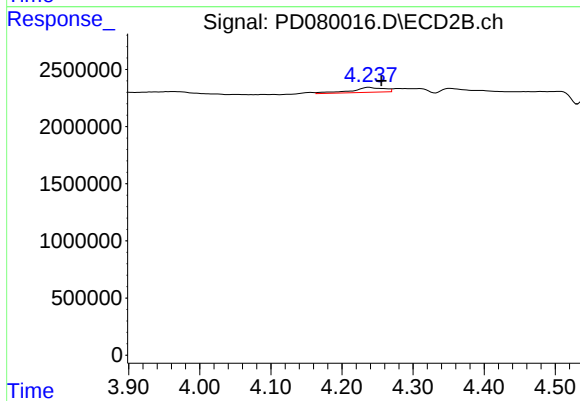

#5 Aldrin


R.T.: 4.238 min
Delta R.T.: -0.017 min
Response: 1367935
Conc: 0.40 ng/ml

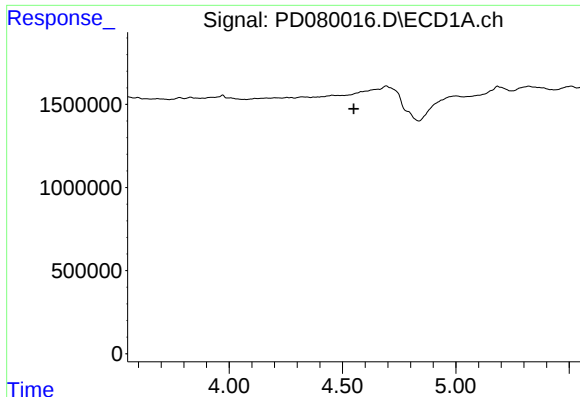

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.550 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

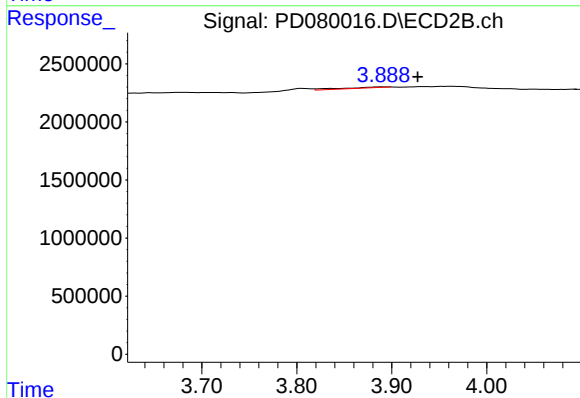


#6 beta-BHC

R.T.: 3.891 min
Delta R.T.: -0.037 min
Response: 290141
Conc: 0.18 ng/ml

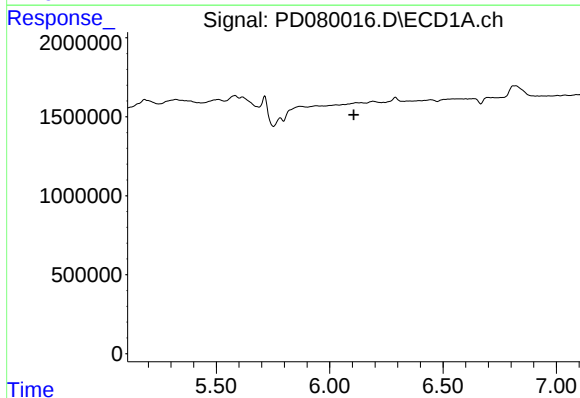


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 6.106 min
Response: 0
Conc: N.D.

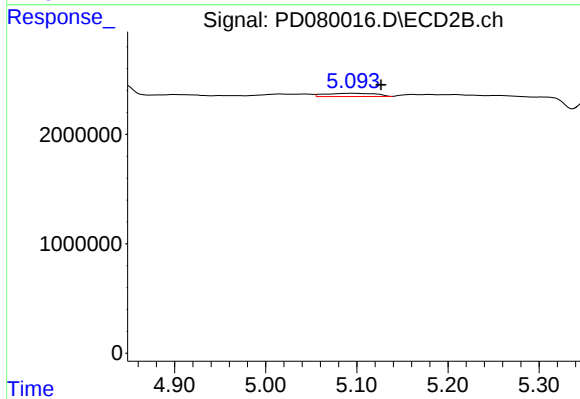

#9 Endosulfan I


R.T.: 5.095 min
Delta R.T.: -0.032 min
Response: 1154984
Conc: 0.41 ng/ml

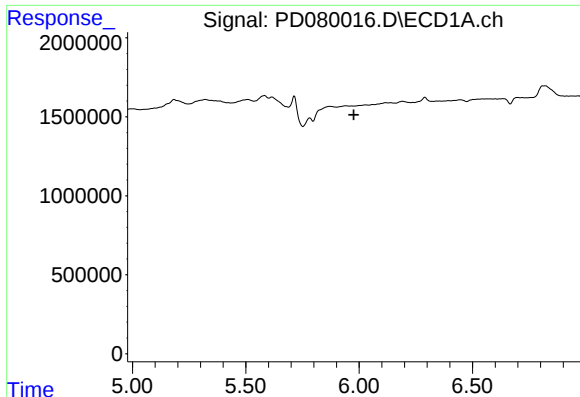

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.976 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

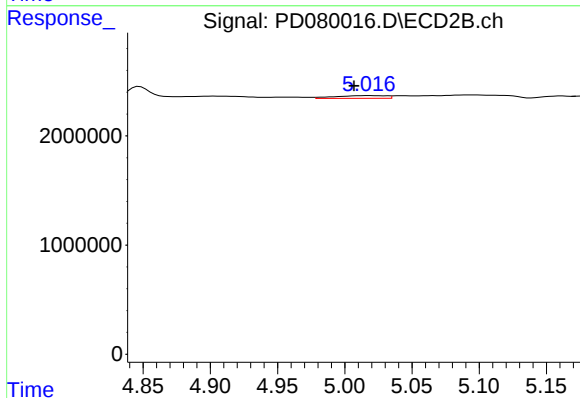


#10 trans-Chlordane

R.T.: 5.017 min
Delta R.T.: 0.010 min
Response: 666554
Conc: 0.22 ng/ml

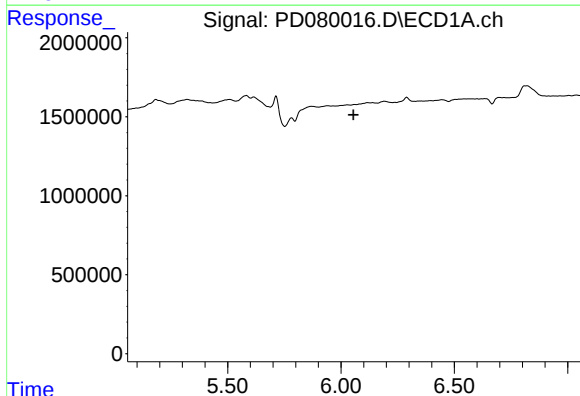


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 6.055 min
Response: 0
Conc: N.D.

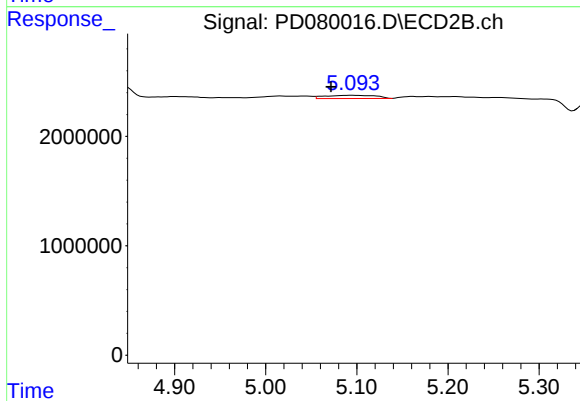

#11 cis-Chlordane


R.T.: 5.095 min
Delta R.T.: 0.023 min
Response: 1154984
Conc: 0.37 ng/ml

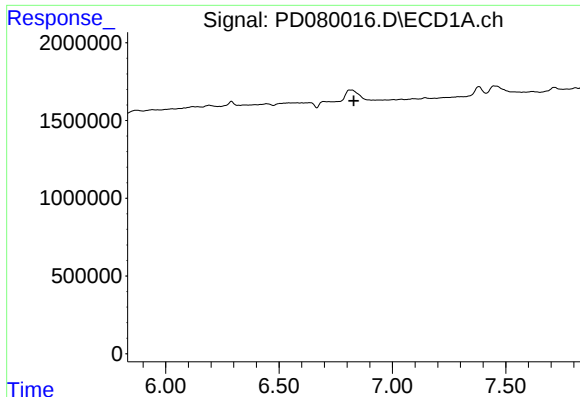

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.830 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

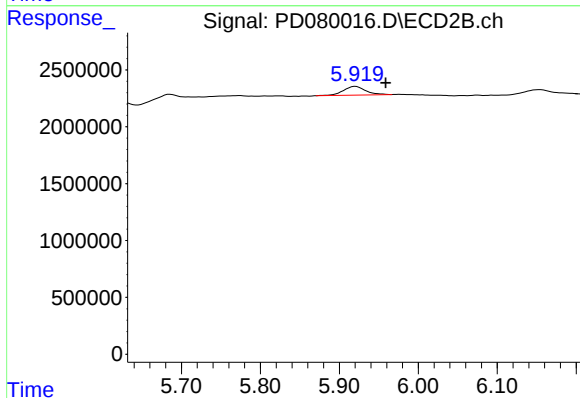


#15 Endosulfan II

R.T.: 5.921 min
Delta R.T.: -0.038 min
Response: 1503277
Conc: 0.55 ng/ml

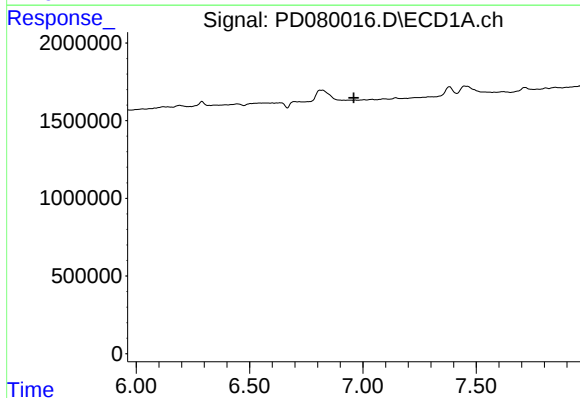


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.960 min
Response: 0
Conc: N.D.

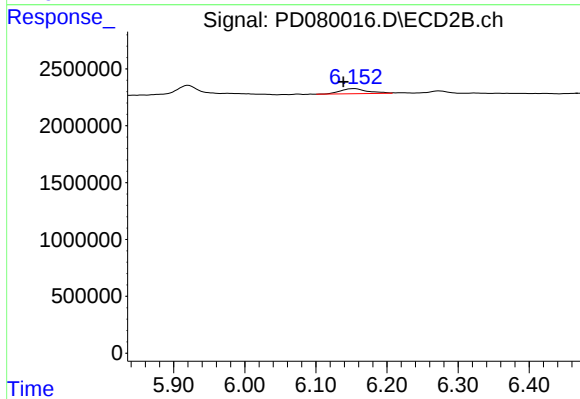

#18 Endrin aldehyde


R.T.: 6.154 min
Delta R.T.: 0.015 min
Response: 1201412
Conc: 0.57 ng/ml

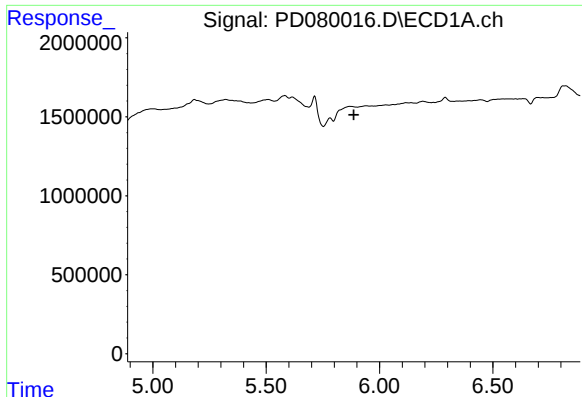

#22 Toxaphene-1


R.T.: 0.000 min
Exp R.T.: 5.886 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

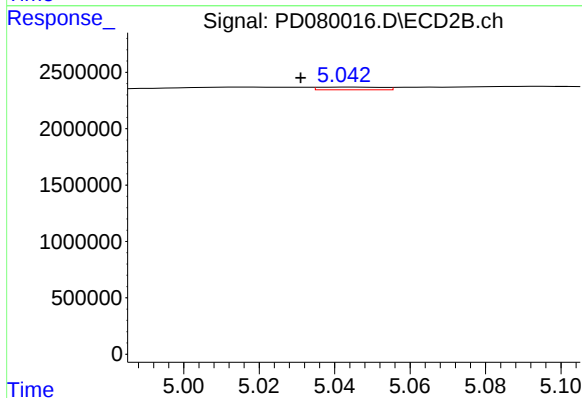


#22 Toxaphene-1

R.T.: 5.044 min
Delta R.T.: 0.013 min
Response: 284586
Conc: 16.32 ng/ml

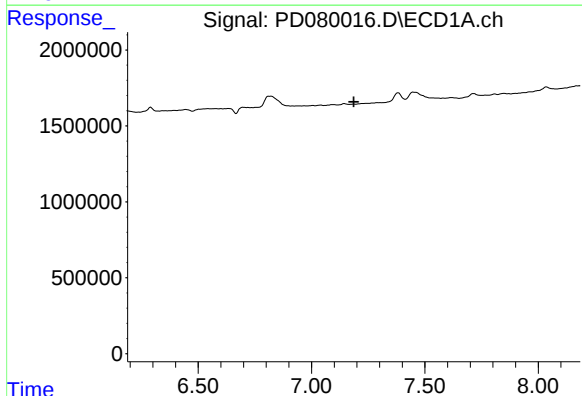


#25 Toxaphene-4

R.T.: 0.000 min
Exp R.T.: 7.187 min
Response: 0
Conc: N.D.

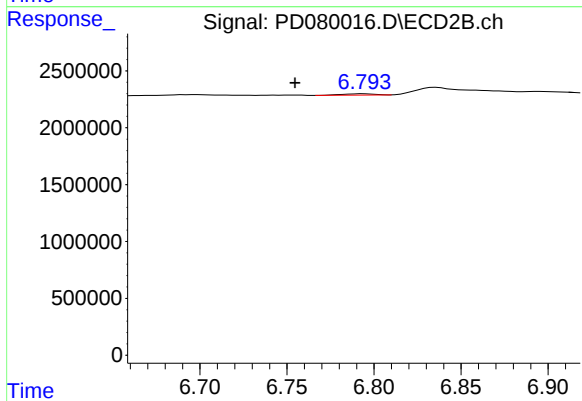

#25 Toxaphene-4


R.T.: 6.794 min
Delta R.T.: 0.040 min
Response: 144056
Conc: 1.70 ng/ml

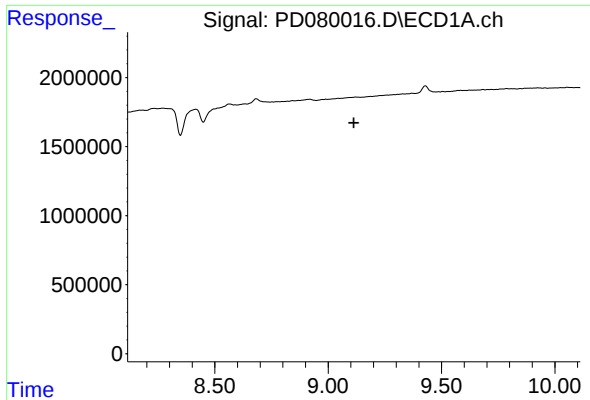

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.114 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

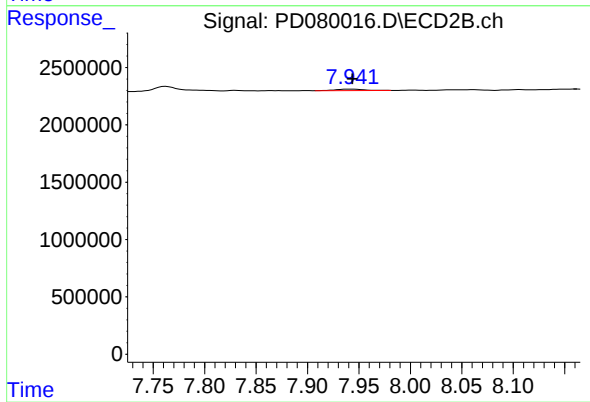

#27 Decachlorobiphenyl

R.T.: 7.942 min
Delta R.T.: -0.001 min
Response: 241303
Conc: N.D.