

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121123\
 Data File : PD080022.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Dec 2023 17:40
 Operator : AR\AJ
 Sample : 05673-02MS
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BHEH8MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 21:41:16 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120523CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 05 17:09:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.568	2.802	30531235	49307581	21.345	21.511
27)	SA Decachlor...	9.116	7.945	34384194	40164795	18.390	15.525
Target Compounds							
2)	A alpha-BHC	4.025	3.304	128.1E6	196.2E6	53.102	53.482
3)	MA gamma-BHC...	4.359	3.634	113.9E6	168.0E6	49.214	49.115
4)	MA Heptachlor	4.952	3.976	108.5E6	158.4E6	44.528	47.207
5)	MB Aldrin	5.295	4.256	101.0E6	149.0E6	43.337	44.050
6)	B beta-BHC	4.552	3.929	46592250	69647472	44.058	43.694
7)	B delta-BHC	4.802	4.160	112.2E6	164.5E6	46.128	44.852
8)	B Heptachlo...	5.722	4.758	93184738	136.3E6	42.346	42.650
9)	A Endosulfan I	6.108	5.129	87472503	126.7E6	42.967	44.538
10)	B trans-Chl...	5.977	5.008	86340791	131.2E6	40.614	42.707
11)	B cis-Chlor...	6.057	5.072	88427121	130.5E6	40.603	41.363
12)	B 4,4'-DDE	6.228	5.262	165.5E6	244.7E6	82.616	83.318
13)	MA Dieldrin	6.384	5.393	188.5E6	267.1E6	86.605	83.249
14)	MA Endrin	6.614	5.668	158.0E6	241.3E6	87.966	86.548
15)	B Endosulfa...	6.832	5.960	155.8E6	222.5E6	80.155	81.359
16)	A 4,4'-DDD	6.745	5.814	132.2E6	199.6E6	81.345	81.281
17)	MA 4,4'-DDT	7.060	6.066	150.4E6	206.2E6	89.829	83.717
18)	B Endrin al...	6.961	6.139	117.9E6	165.6E6	78.829	78.239
19)	B Endosulfa...	7.196	6.362	150.3E6	207.4E6	80.986	80.188
20)	A Methoxychlor	7.535	6.641	391.7E6	540.9E6	431.036	408.062
21)	B Endrin ke...	7.683	6.868	164.0E6	233.9E6	81.829	79.019

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121123\
Data File : PD080022.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Dec 2023 17:40
Operator : AR\AJ
Sample : 05673-02MS
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 21:41:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 05 17:09:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

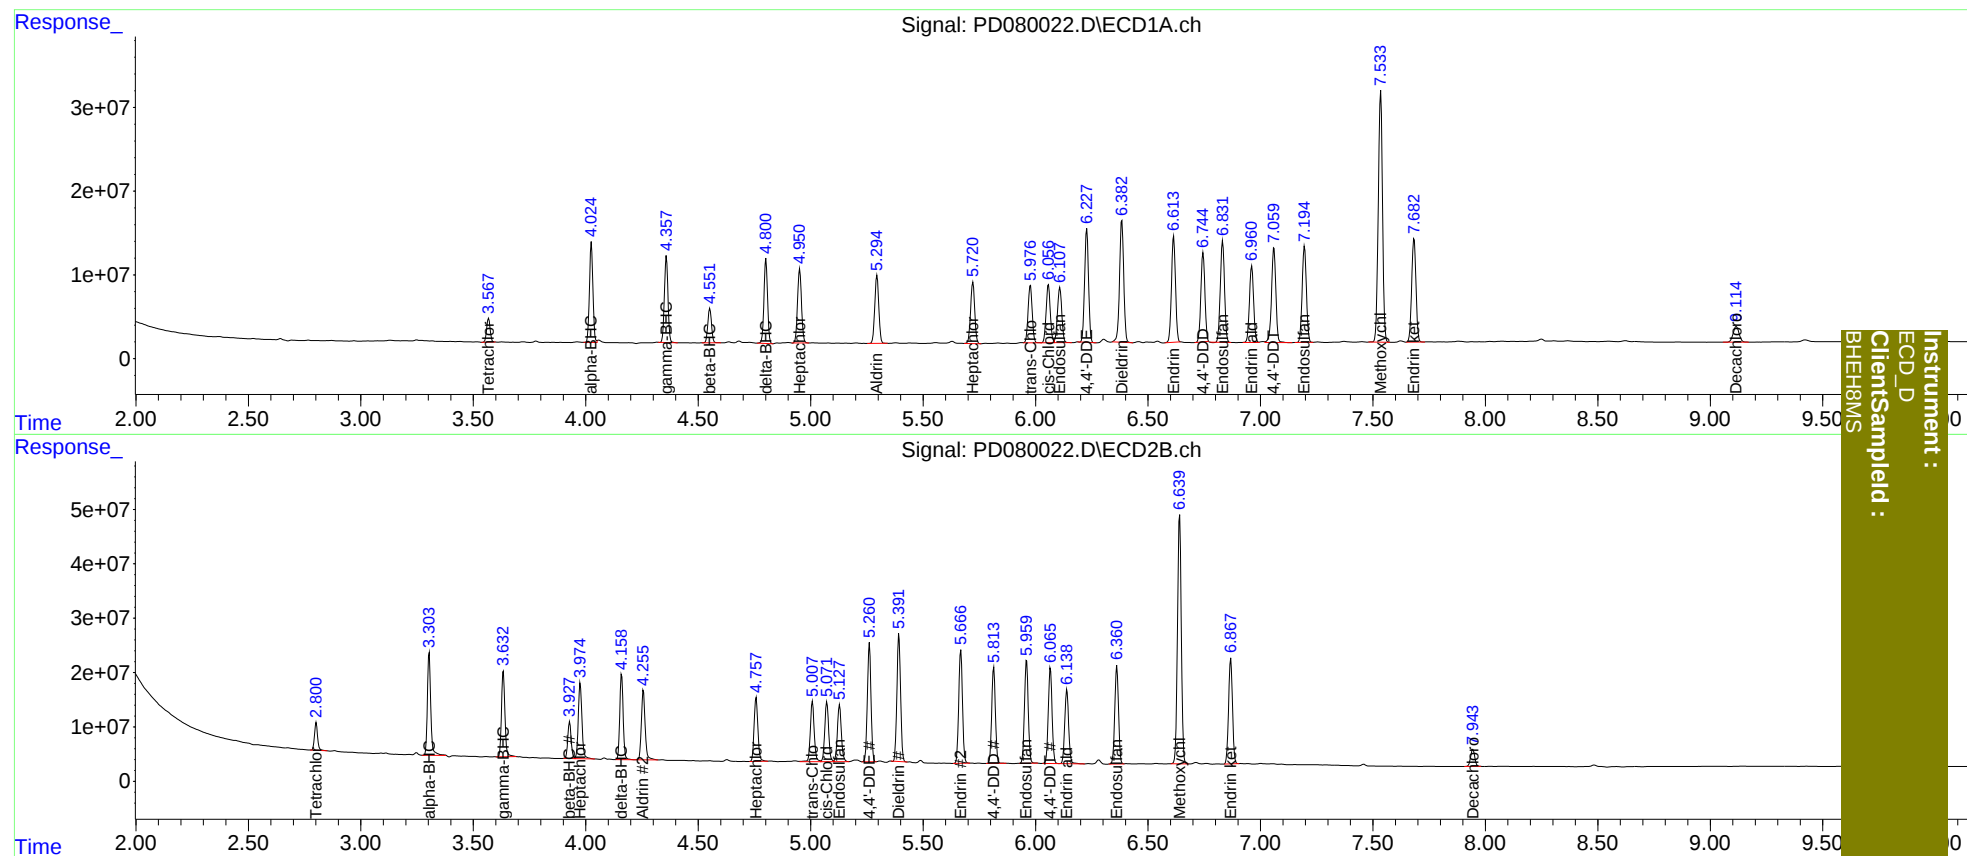

Instrument :
ECD_D
ClientSampled :
BHEH8MS