

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121123\
 Data File : PD080023.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Dec 2023 17:53
 Operator : AR\AJ
 Sample : 05673-03MSD
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BHEH8MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 21:41:57 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120523CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 05 17:09:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.802	29879129	47773173	20.889	20.842
2)	SA Decachlor...	9.116	7.945	31915102	36704256	17.069	14.187
Target Compounds							
2)	A alpha-BHC	4.026	3.305	123.2E6	189.7E6	51.103	51.707
3)	MA gamma-BHC...	4.359	3.634	109.1E6	162.3E6	47.157	47.447
4)	MA Heptachlor	4.952	3.976	103.1E6	151.8E6	42.317	45.251
5)	MB Aldrin	5.296	4.257	95866594	143.3E6	41.127	42.392
6)	B beta-BHC	4.553	3.929	44532535	67709739	42.110	42.478
7)	B delta-BHC	4.802	4.160	107.1E6	158.4E6	44.038	43.180
8)	B Heptachlo...	5.722	4.758	88300990	129.7E6	40.127	40.579
9)	A Endosulfan I	6.108	5.129	82587734	122.6E6	40.567	43.103
10)	B trans-Chl...	5.978	5.008	81420373	124.4E6	38.300	40.470
11)	B cis-Chlor...	6.058	5.073	83397129	125.2E6	38.293	39.696
12)	B 4,4'-DDE	6.228	5.262	155.5E6	232.5E6	77.598	79.160
13)	MA Dieldrin	6.384	5.394	179.3E6	253.9E6	82.371	79.115
14)	MA Endrin	6.615	5.669	148.7E6	229.0E6	82.759	82.165
15)	B Endosulfa...	6.833	5.961	147.2E6	210.4E6	75.746	76.930
16)	A 4,4'-DDD	6.746	5.815	124.5E6	188.3E6	76.646	76.694
17)	MA 4,4'-DDT	7.061	6.067	142.5E6	194.4E6	85.112	78.917
18)	B Endrin al...	6.962	6.140	110.7E6	157.0E6	74.002	74.176
19)	B Endosulfa...	7.196	6.363	142.8E6	196.0E6	76.989	75.746
20)	A Methoxychlor	7.534	6.641	371.1E6	514.0E6	408.281	387.739
21)	B Endrin ke...	7.683	6.869	155.7E6	220.2E6	77.648	74.374

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121123\
Data File : PD080023.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Dec 2023 17:53
Operator : AR\AJ
Sample : 05673-03MSD
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 21:41:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120523CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 05 17:09:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

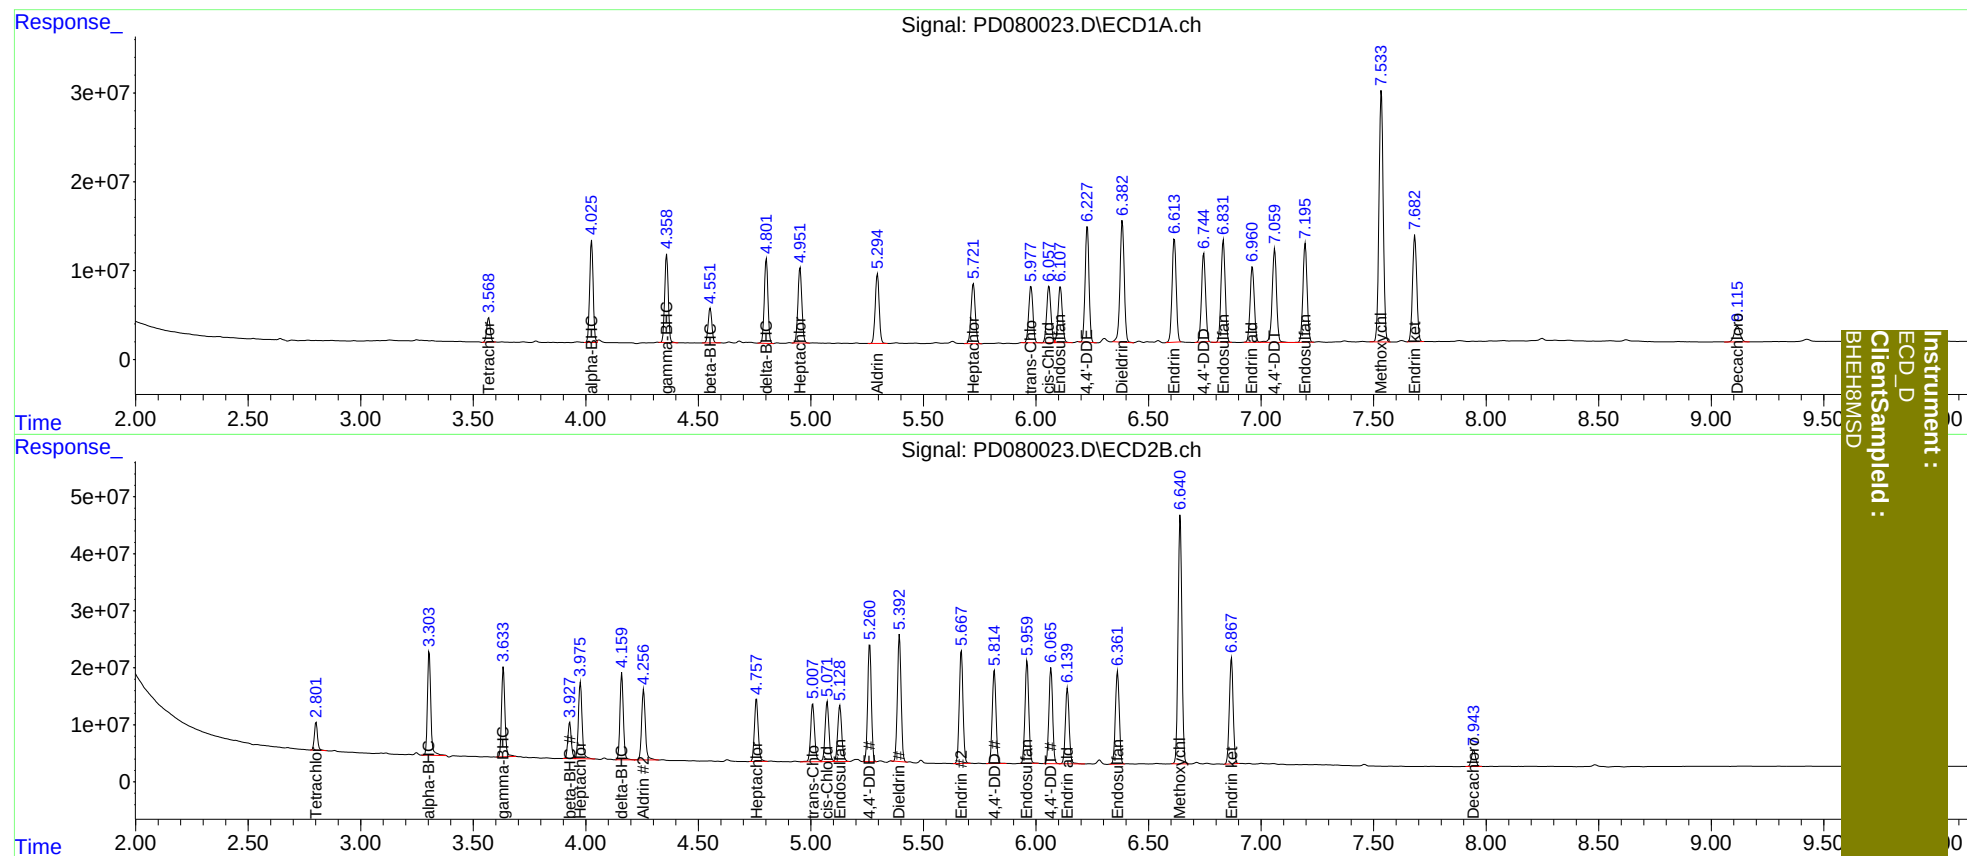

Instrument :
ECD_D
ClientSampled :
BHEH8MSD