

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121124\
 Data File : PD087096.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Dec 2024 17:12
 Operator : AR\AJ
 Sample : P5247-06MSD
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH7T5MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/12/2024
 Supervised By :Ankita Jodhani 12/12/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 00:59:32 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112024CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 20 02:52:29 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.558	2.886	39811993	247.3E6	21.650m	21.431
27)	SA Decachlor...	9.094	8.091	58246731	281.3E6	21.876	22.073
Target Compounds							
2)	A alpha-BHC	4.009	3.400	227.6E6	985.6E6	64.628	55.028
3)	MA gamma-BHC...	4.340	3.737	223.1E6	917.4E6	64.055	55.007
4)	MA Heptachlor	4.941	4.092	212.9E6	858.1E6	61.266	49.882
5)	MB Aldrin	5.283	4.379	206.8E6	850.6E6	58.579	49.794
6)	B beta-BHC	4.524	4.032	85216911	395.8E6	53.759	50.099
7)	B delta-BHC	4.773	4.270	144.7E6	623.5E6	39.754	35.510
8)	B Heptachlo...	5.703	4.883	198.8E6	815.3E6	60.813	51.412
9)	A Endosulfan I	6.086	5.259	182.8E6	766.1E6	61.478	52.930
10)	B trans-Chl...	5.958	5.137	191.4E6	847.7E6	59.834	51.322
11)	B cis-Chlor...	6.039	5.202	196.7E6	838.1E6	60.455	52.297
12)	B 4,4'-DDE	6.207	5.388	379.0E6	1591.8E6	122.888	104.401
13)	MA Dieldrin	6.359	5.525	416.2E6	1609.9E6	126.977	105.368
14)	MA Endrin	6.588	5.801	338.5E6	1418.9E6	125.240	102.710
15)	B Endosulfa...	6.798	6.093	340.1E6	1402.4E6	122.555	100.501
16)	A 4,4'-DDD	6.717	5.943	298.6E6	1328.1E6	125.867	109.934
17)	MA 4,4'-DDT	7.033	6.197	301.8E6	1338.5E6	121.746m	103.532
18)	B Endrin al...	6.927	6.271	251.1E6	1063.4E6	114.236	99.093
19)	B Endosulfa...	7.162	6.495	300.6E6	1293.3E6	111.424	96.380
20)	A Methoxychlor	7.506	6.769	761.0E6	2649.7E6	563.822	458.308
21)	B Endrin ke...	7.643	7.005	350.0E6	1503.5E6	114.743	100.618

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121124\
Data File : PD087096.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Dec 2024 17:12
Operator : AR\AJ
Sample : P5247-06MSD
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 00:59:32 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 20 02:52:29 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

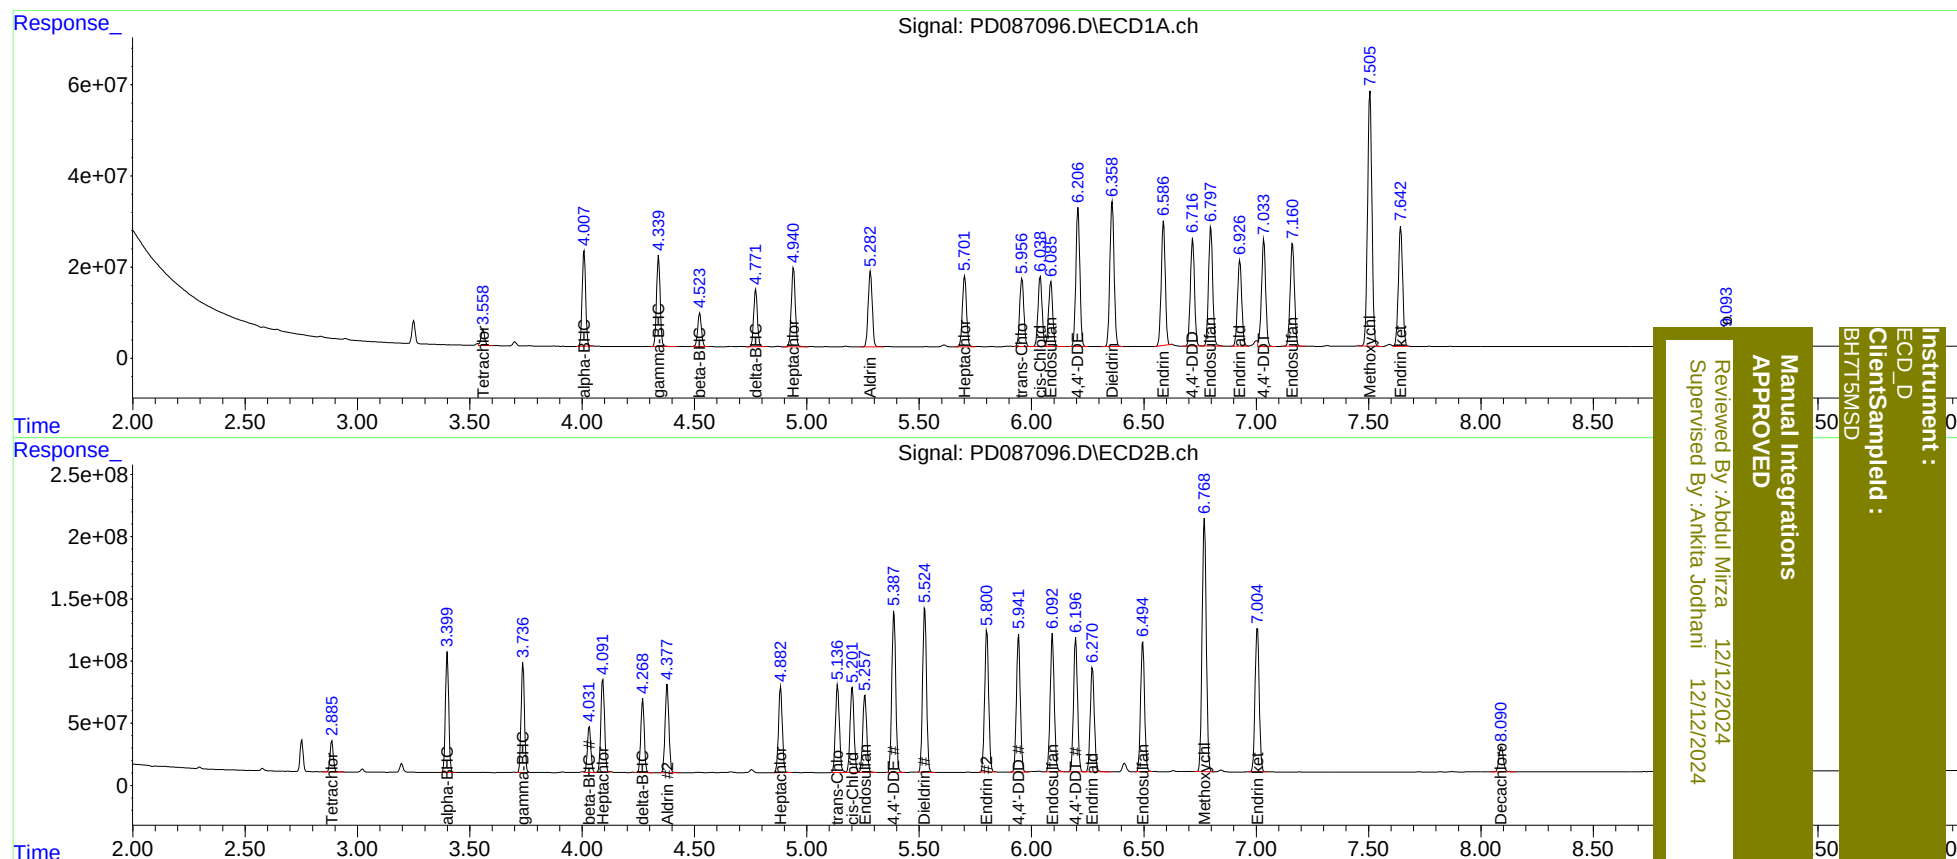

Instrument :
ECD_D
Client Sampled :
BH75MSD

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 12/12/2024
Supervised By: Ankita Jodhani 12/12/2024