

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121219\
 Data File : PD056419.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Dec 2019 18:38
 Operator : SG\AJ
 Sample : K6202-02
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0BX2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 13 00:54:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.287	3.960	17055303	25736104	20.593	21.407
27)	SA Decachlor...	7.959	8.992	35833186	46099671	39.684	38.316
Target Compounds							
6)	B beta-BHC	0.000	4.845f	0	2017677	N.D.	2.448
8)	B Heptachlo...	0.000	5.859	0	659531	N.D.	0.426


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121219\
Data File : PD056419.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Dec 2019 18:38
Operator : SG\AJ
Sample : K6202-02
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
C0BX2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 13 00:54:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

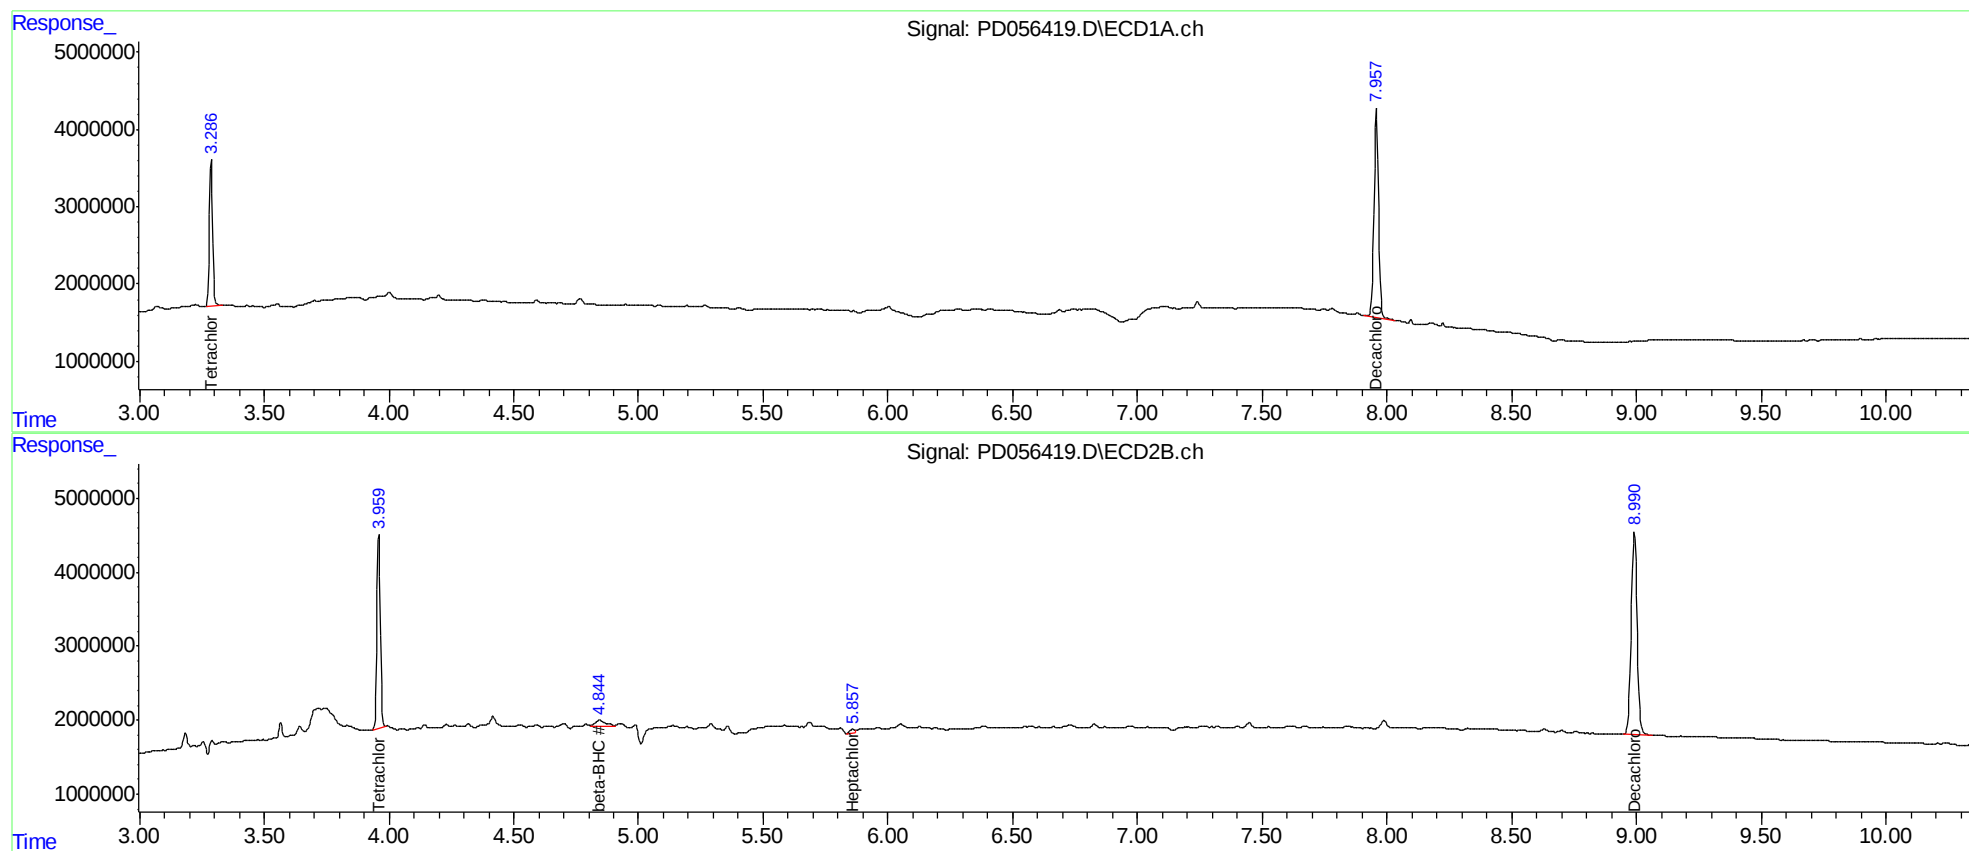


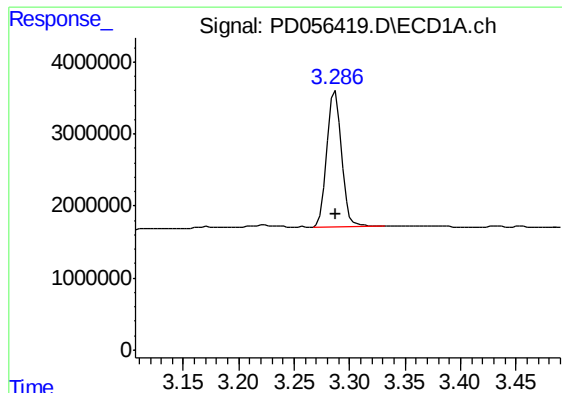

#1 Tetrachloro-m-xylene


R.T.: 3.287 min
Delta R.T.: 0.000 min
Response: 17055303
Conc: 20.59 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0BX2

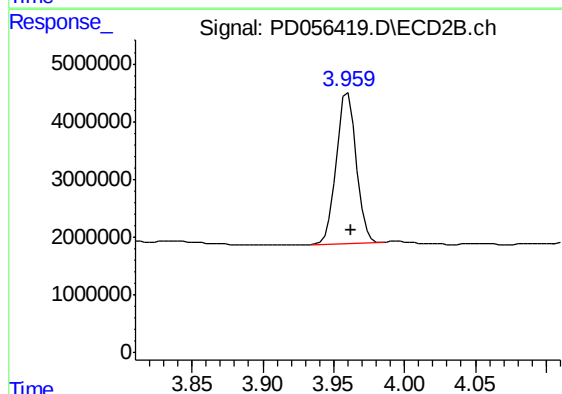


#1 Tetrachloro-m-xylene

R.T.: 3.960 min
Delta R.T.: -0.002 min
Response: 25736104
Conc: 21.41 ng/ml

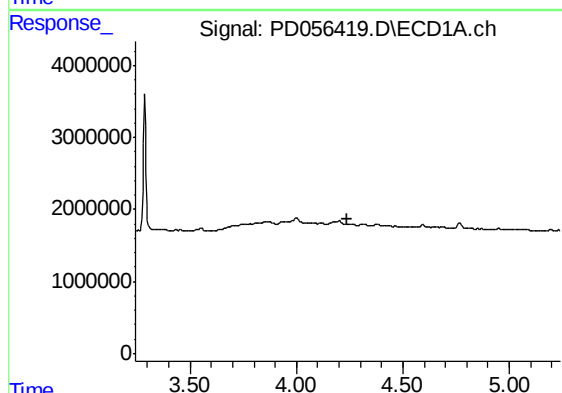


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.240 min
Response: 0
Conc: N.D.

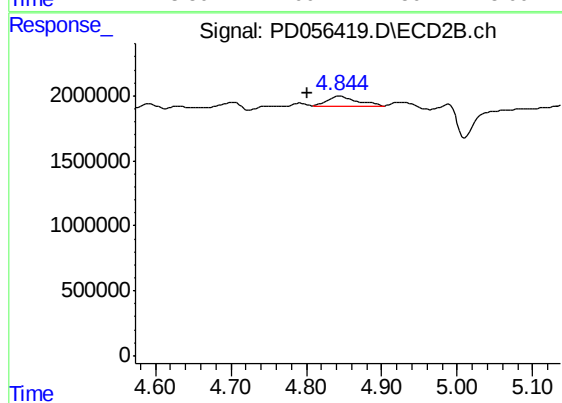

#6 beta-BHC


R.T.: 4.845 min
Delta R.T.: 0.044 min
Response: 2017677
Conc: 2.45 ng/ml

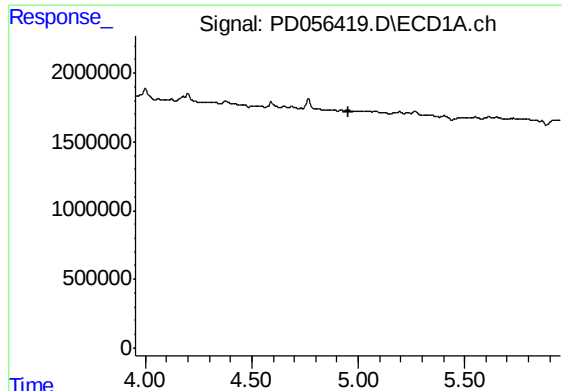

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.953 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C0BX2

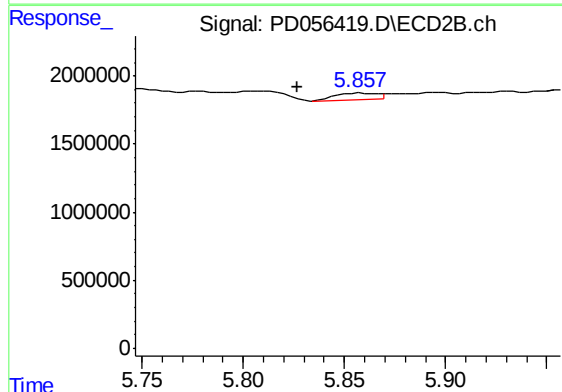


#8 Heptachlor epoxide

R.T.: 5.859 min
Delta R.T.: 0.032 min
Response: 659531
Conc: 0.43 ng/ml

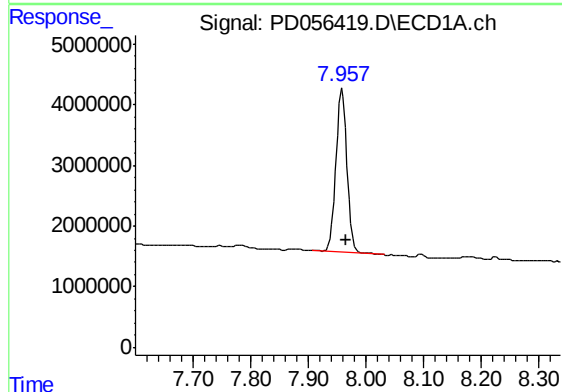

#27 Decachlorobiphenyl

R.T.: 7.959 min
Delta R.T.: -0.007 min
Response: 35833186
Conc: 39.68 ng/ml

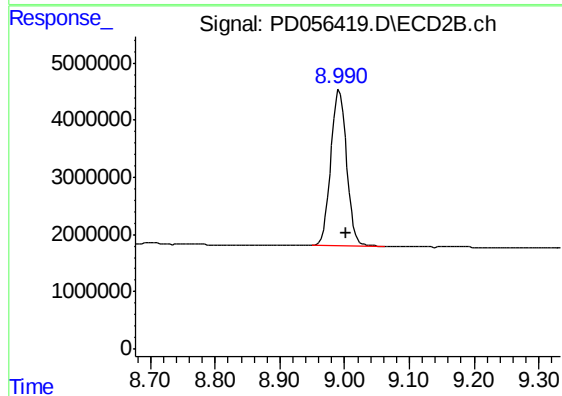

#27 Decachlorobiphenyl

R.T.: 8.992 min
Delta R.T.: -0.011 min
Response: 46099671
Conc: 38.32 ng/ml