

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121219\
 Data File : PD056421.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Dec 2019 19:06
 Operator : SG\AJ
 Sample : K6202-04
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0BZ0

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 13 00:54:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1) SA	Tetrachlo...	3.287	3.960	16014089	24126960	19.336	20.068
27) SA	Decachlor...	7.956	8.992	34856445	44905497	38.602	37.323
Target Compounds							
5) MB	Aldrin	0.000	5.456	0	1750344	N.D.	1.065
6) B	beta-BHC	0.000	4.791	0	1847346	N.D.	2.242
8) B	Heptachlo...	0.000	5.861	0	1316499	N.D.	0.850
10) B	trans-Chl...	0.000	6.049	0	1743049	N.D.	1.054
19) B	Endosulfa...	0.000	7.193	0	993929	N.D.	0.743


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121219\
Data File : PD056421.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Dec 2019 19:06
Operator : SG\AJ
Sample : K6202-04
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
C0BZ0

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 13 00:54:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

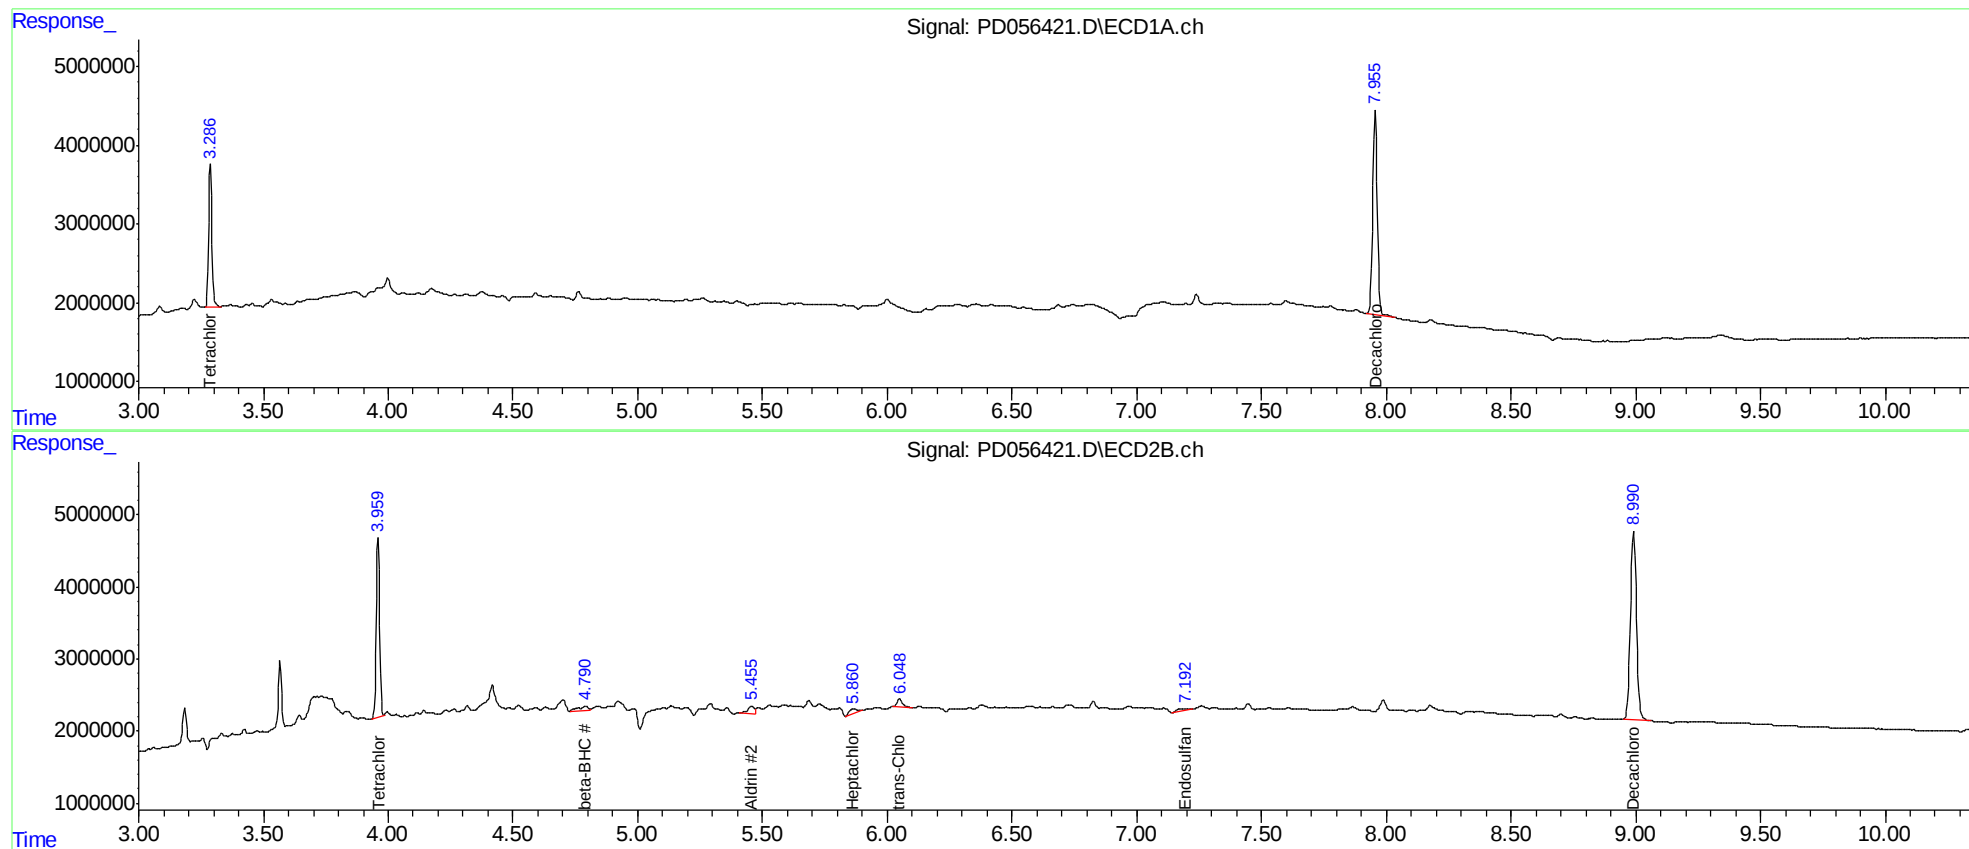


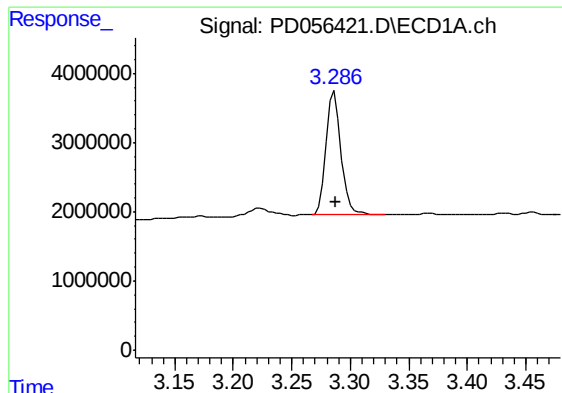

#1 Tetrachloro-m-xylene


R.T.: 3.287 min
Delta R.T.: -0.001 min
Response: 16014089
Conc: 19.34 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0BZ0

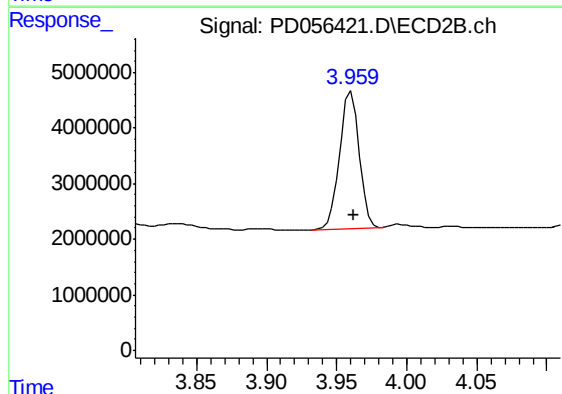


#1 Tetrachloro-m-xylene

R.T.: 3.960 min
Delta R.T.: -0.002 min
Response: 24126960
Conc: 20.07 ng/ml

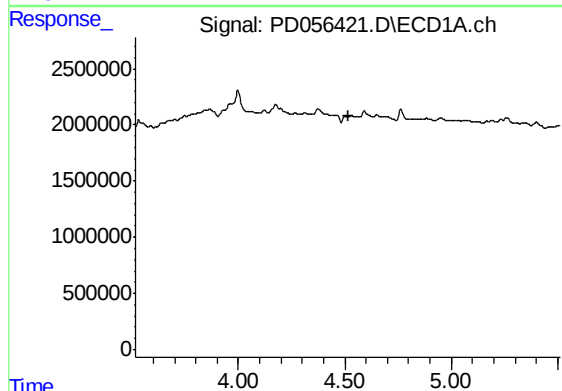


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.516 min
Response: 0
Conc: N.D.

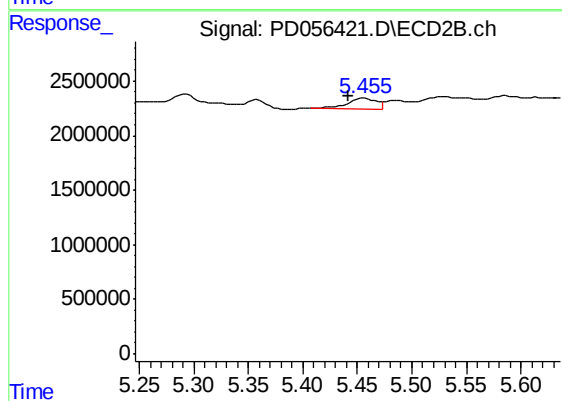

#5 Aldrin


R.T.: 5.456 min
Delta R.T.: 0.014 min
Response: 1750344
Conc: 1.07 ng/ml

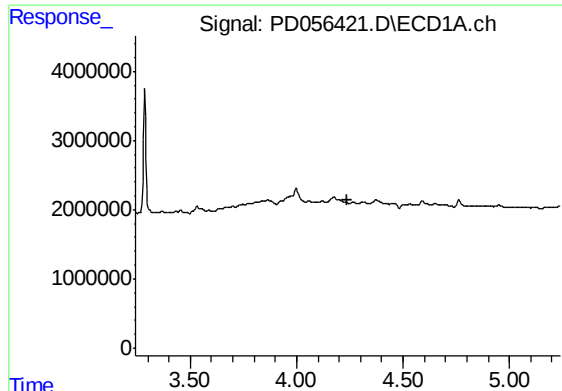

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.240 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C0BZ0

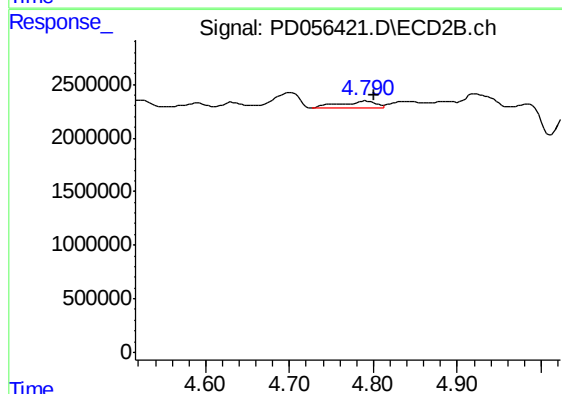


#6 beta-BHC

R.T.: 4.791 min
Delta R.T.: -0.010 min
Response: 1847346
Conc: 2.24 ng/ml

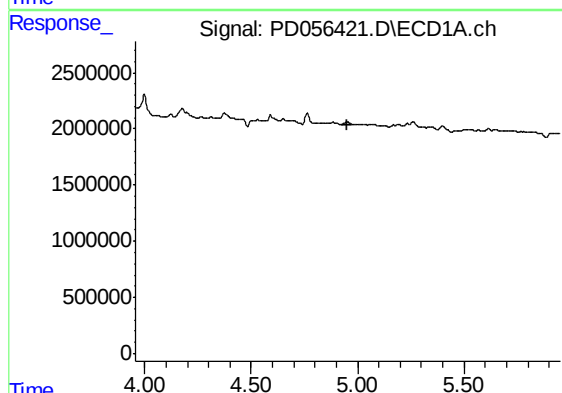


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.953 min
Response: 0
Conc: N.D.

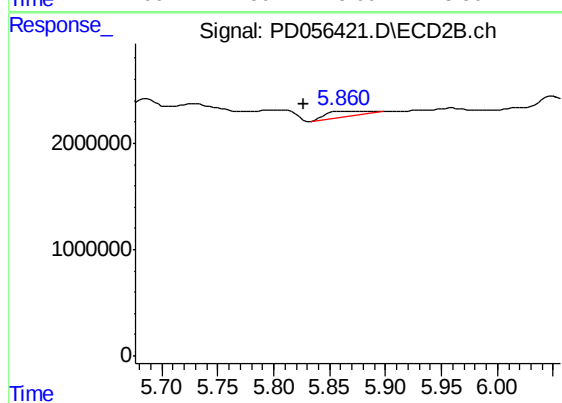

#8 Heptachlor epoxide


R.T.: 5.861 min
Delta R.T.: 0.034 min
Response: 1316499
Conc: 0.85 ng/ml

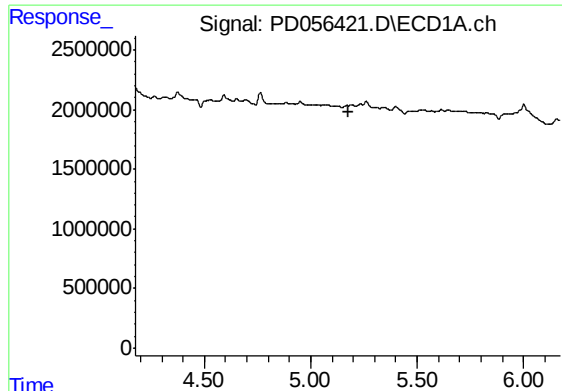

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.175 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C0BZ0

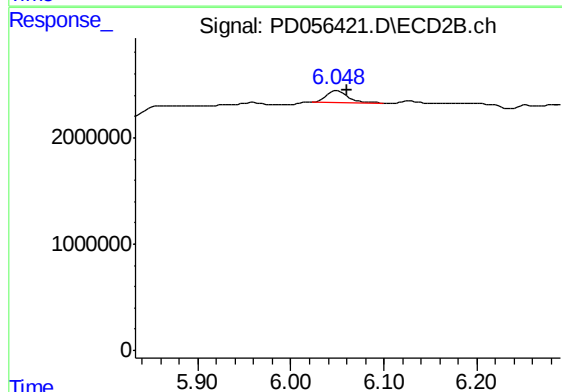


#10 trans-Chlordane

R.T.: 6.049 min
Delta R.T.: -0.011 min
Response: 1743049
Conc: 1.05 ng/ml

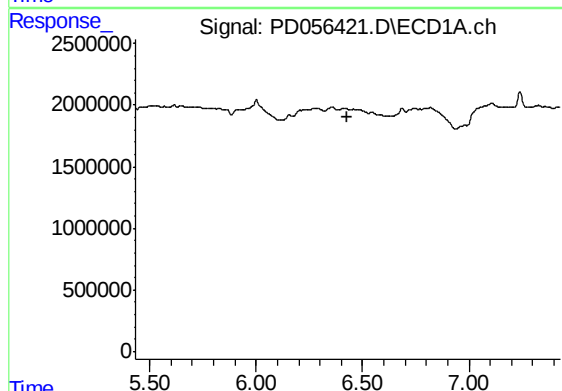


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 6.430 min
Response: 0
Conc: N.D.

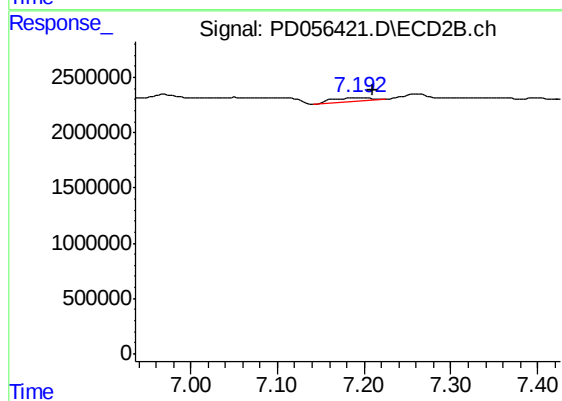

#19 Endosulfan Sulfate


R.T.: 7.193 min
Delta R.T.: -0.016 min
Response: 993929
Conc: 0.74 ng/ml

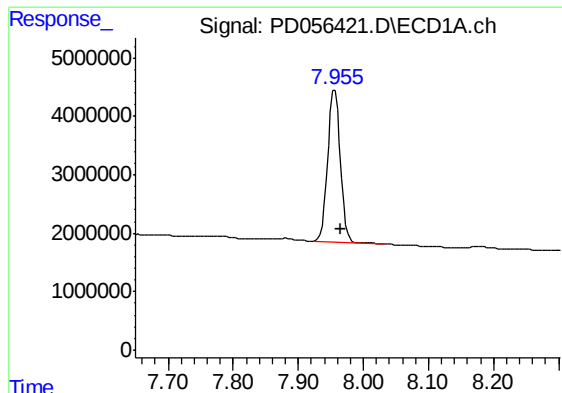

#27 Decachlorobiphenyl

R.T.: 7.956 min
Delta R.T.: -0.009 min
Response: 34856445
Conc: 38.60 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0BZ0

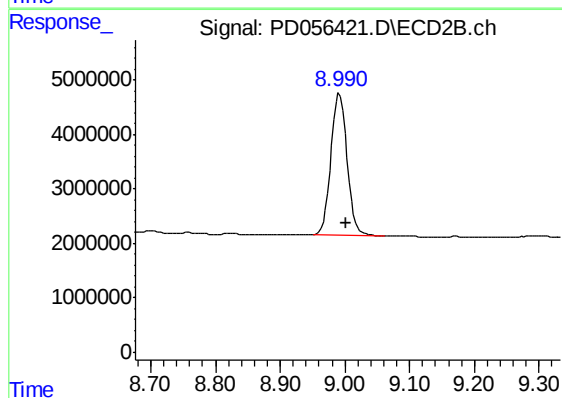

#27 Decachlorobiphenyl

R.T.: 8.992 min
Delta R.T.: -0.011 min
Response: 44905497
Conc: 37.32 ng/ml