

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121319\
 Data File : PD056452.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Dec 2019 20:45
 Operator : SG\AJ
 Sample : K6240-19
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BFQS2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 13 22:14:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.287	3.961	20165000	30686881	24.348	25.524
27)	SA Decachlor...	7.960	8.997	34407144	46126456	38.104	38.338
Target Compounds							
2)	A alpha-BHC	0.000	4.315f	0	150525	N.D.	<MDL
3)	MA gamma-BHC...	0.000	4.592f	0	494705	N.D.	0.307
4)	MA Heptachlor	0.000	5.148	0	652160	N.D.	0.400
6)	B beta-BHC	0.000	4.797	0	422798	N.D.	0.513
7)	B delta-BHC	0.000	4.982f	0	6540418	N.D.	3.927
8)	B Heptachlo...	0.000	5.804	0	11529276	N.D.	7.442
10)	B trans-Chl...	0.000	6.009f	0	1816209	N.D.	1.098
16)	A 4,4'-DDD	0.000	6.736f	0	3076535	N.D.	2.614
19)	B Endosulfa...	0.000	7.196	0	777804	N.D.	0.582


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121319\
Data File : PD056452.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Dec 2019 20:45
Operator : SG\AJ
Sample : K6240-19
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
BFQS2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 13 22:14:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

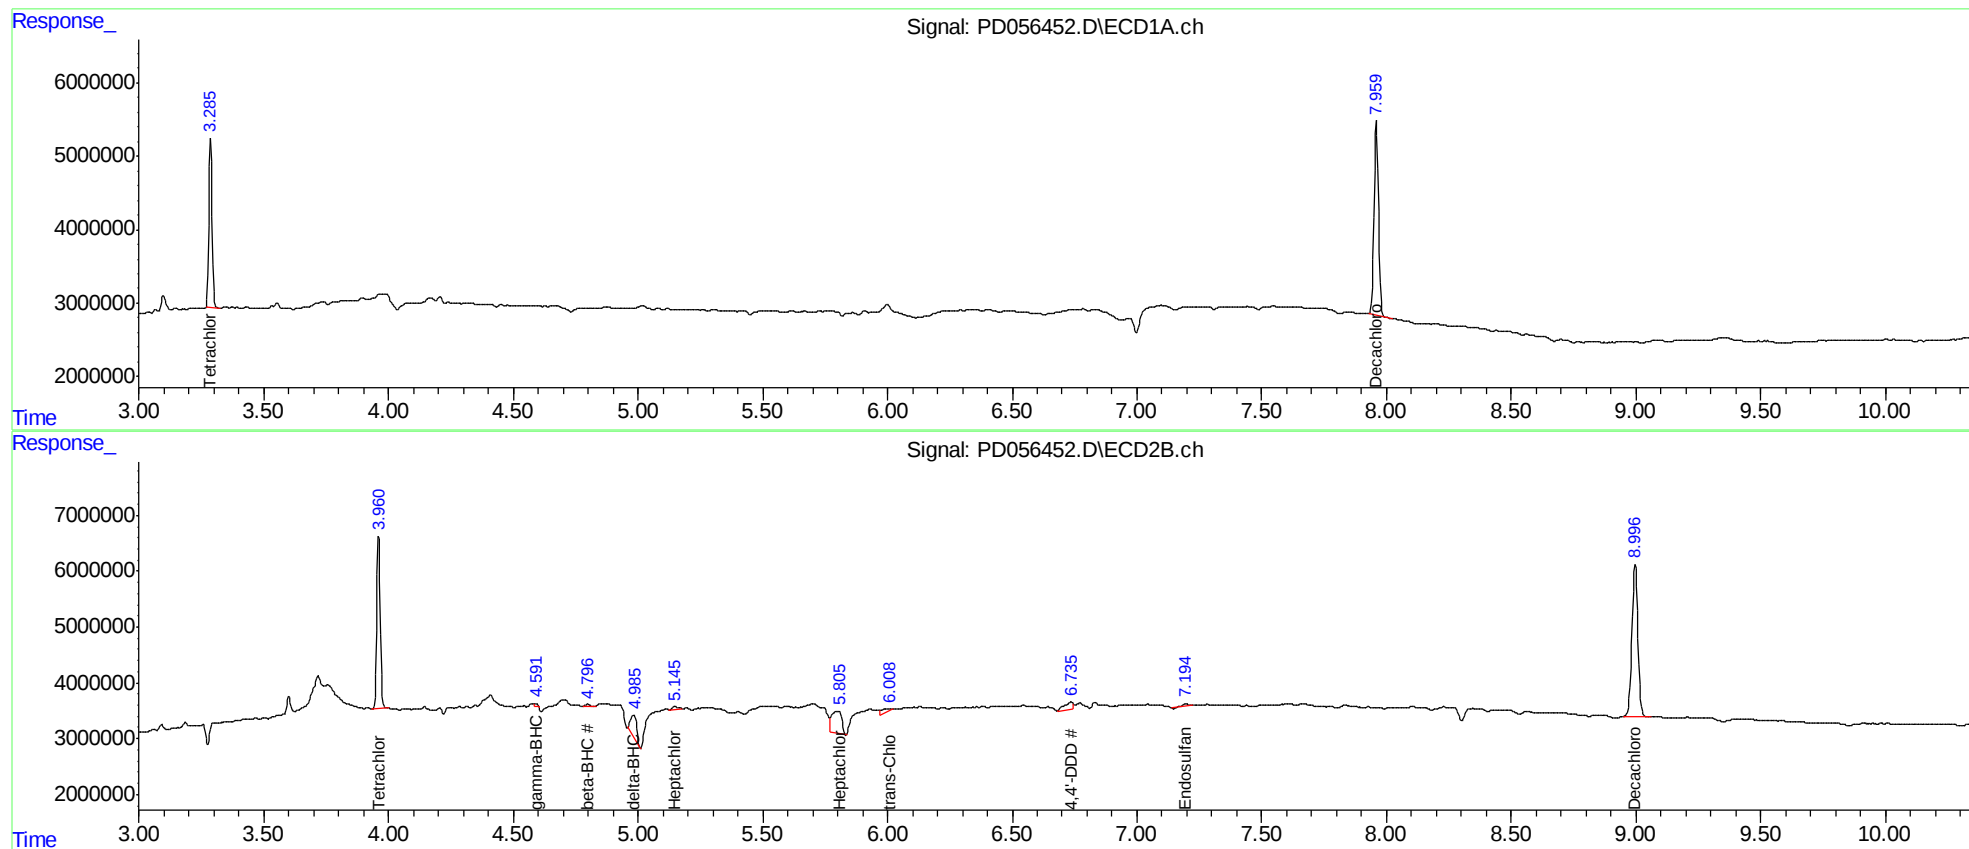


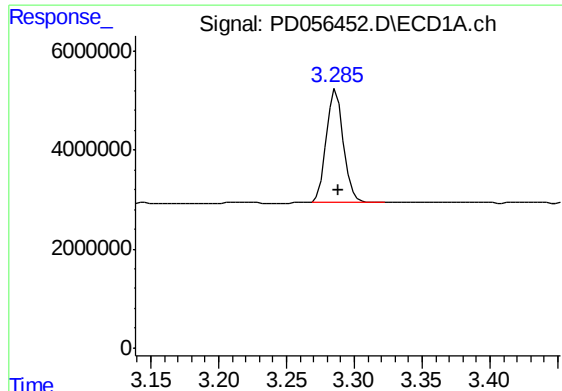

#1 Tetrachloro-m-xylene


R.T.: 3.287 min
Delta R.T.: -0.001 min
Response: 20165000
Conc: 24.35 ng/ml

Instrument :
ECD_D
ClientSampleId :
BFQS2

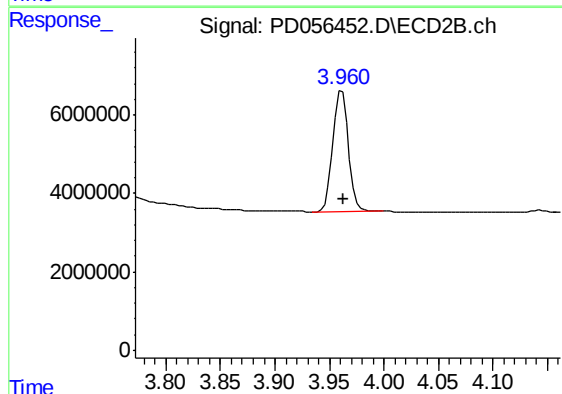


#1 Tetrachloro-m-xylene

R.T.: 3.961 min
Delta R.T.: -0.001 min
Response: 30686881
Conc: 25.52 ng/ml

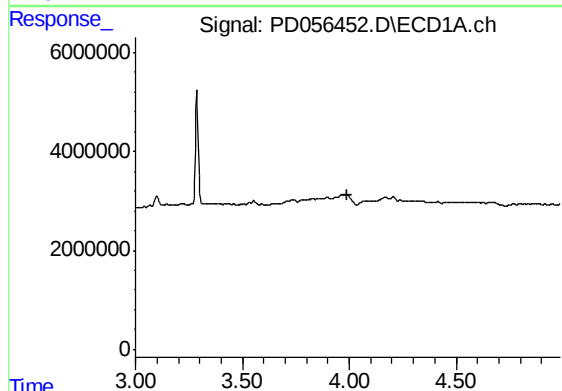


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 3.991 min
Response: 0
Conc: N.D.

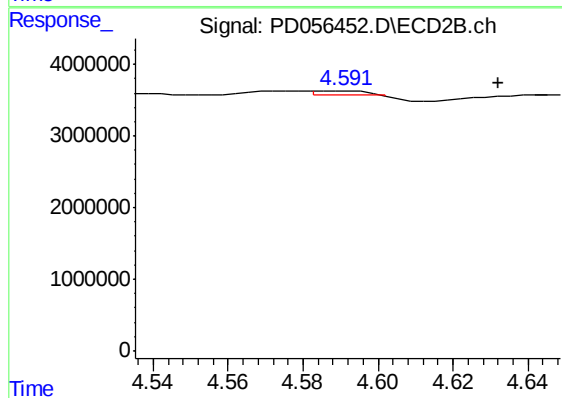

#3 gamma-BHC (Lindane)


R.T.: 4.592 min
Delta R.T.: -0.040 min
Response: 494705
Conc: 0.31 ng/ml

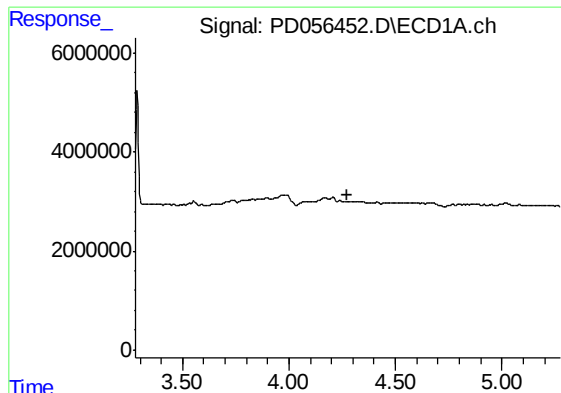

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 4.276 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BFQS2

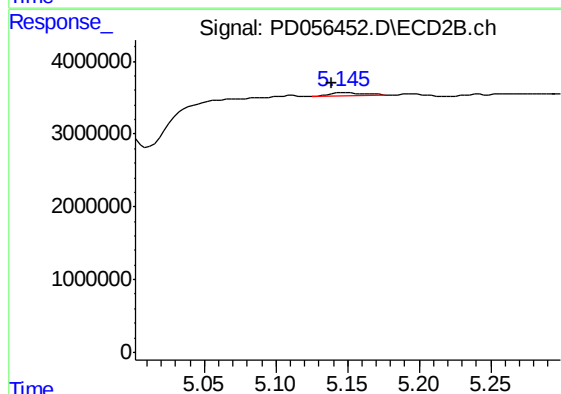


#4 Heptachlor

R.T.: 5.148 min
Delta R.T.: 0.009 min
Response: 652160
Conc: 0.40 ng/ml

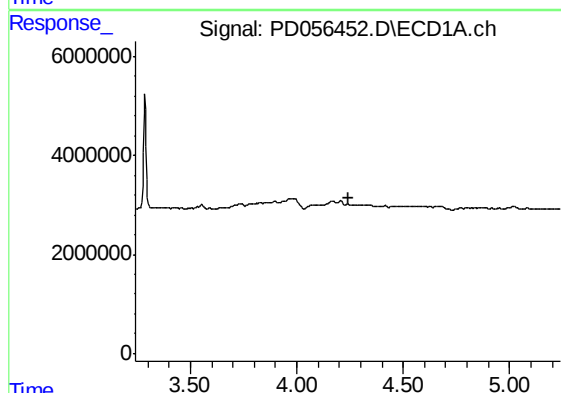


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.240 min
Response: 0
Conc: N.D.

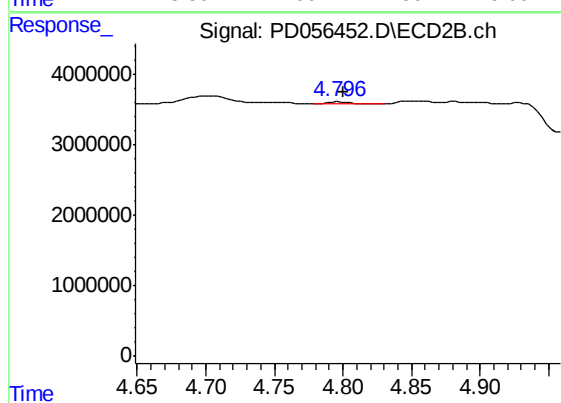

#6 beta-BHC


R.T.: 4.797 min
Delta R.T.: -0.004 min
Response: 422798
Conc: 0.51 ng/ml

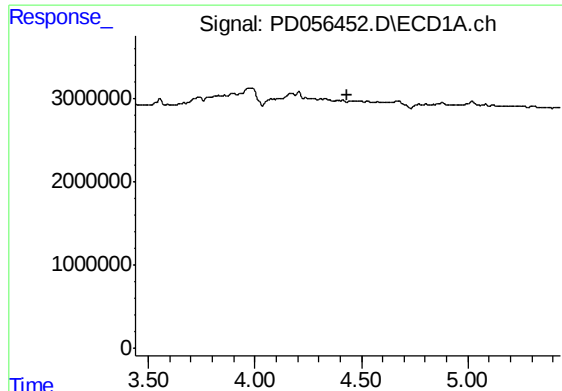

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.436 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BFQS2

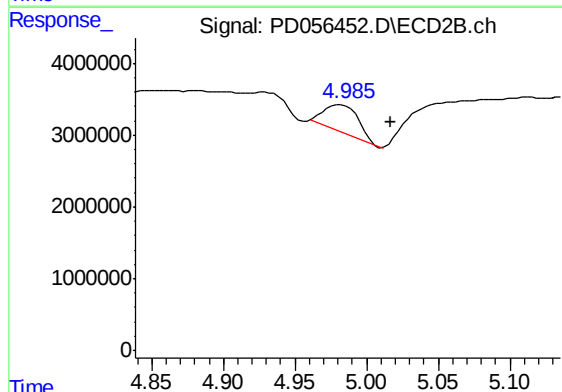


#7 delta-BHC

R.T.: 4.982 min
Delta R.T.: -0.035 min
Response: 6540418
Conc: 3.93 ng/ml

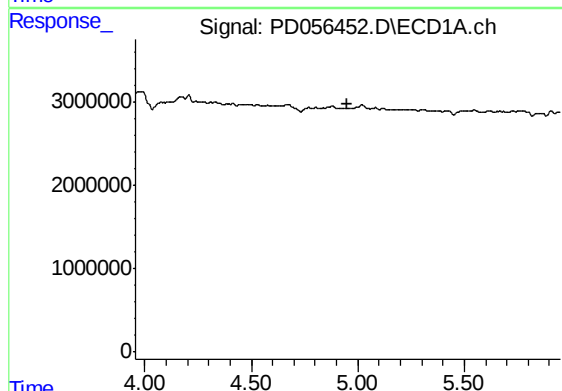


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.953 min
Response: 0
Conc: N.D.

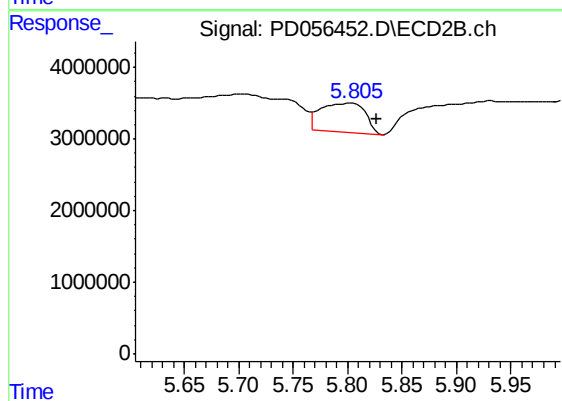

#8 Heptachlor epoxide


R.T.: 5.804 min
Delta R.T.: -0.023 min
Response: 11529276
Conc: 7.44 ng/ml

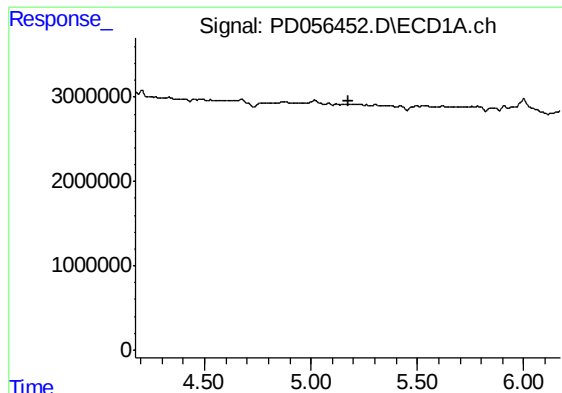

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.175 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BFQS2

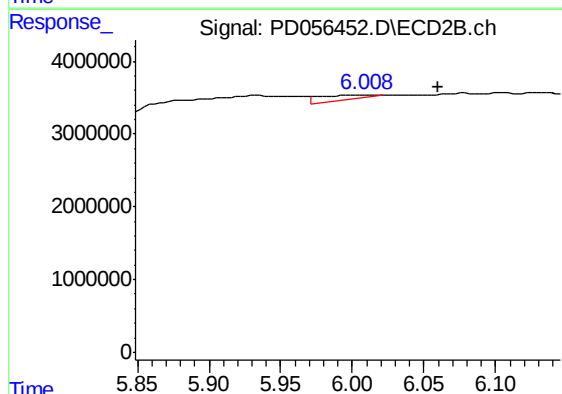


#10 trans-Chlordane

R.T.: 6.009 min
Delta R.T.: -0.051 min
Response: 1816209
Conc: 1.10 ng/ml

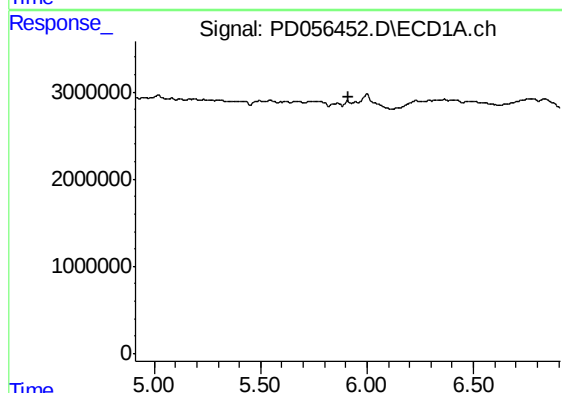


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 5.912 min
Response: 0
Conc: N.D.

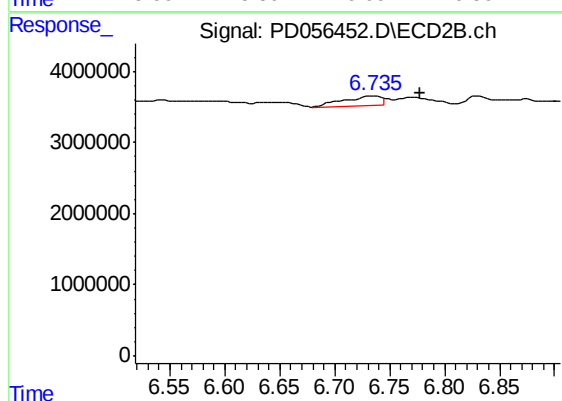

#16 4,4'-DDD


R.T.: 6.736 min
Delta R.T.: -0.042 min
Response: 3076535
Conc: 2.61 ng/ml

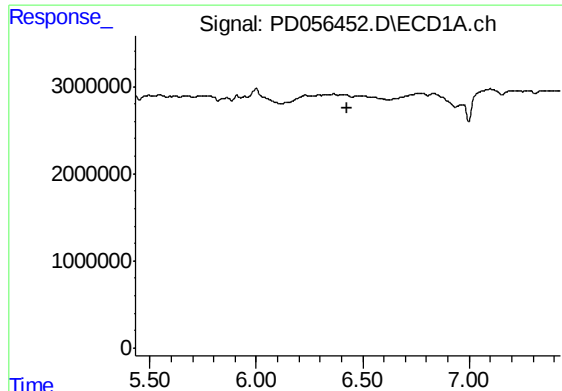

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 6.430 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BFQS2

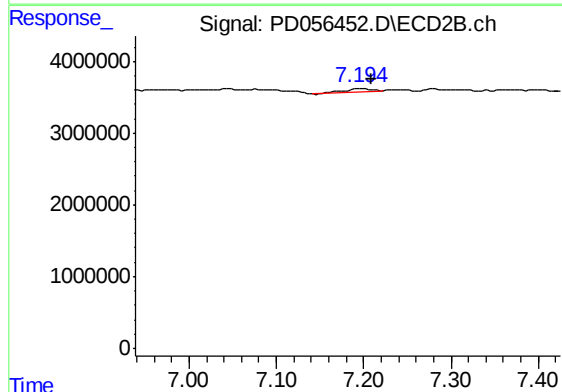


#19 Endosulfan Sulfate

R.T.: 7.196 min
Delta R.T.: -0.014 min
Response: 777804
Conc: 0.58 ng/ml

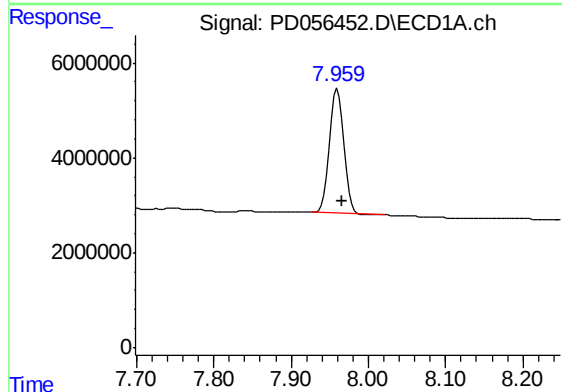

#27 Decachlorobiphenyl

R.T.: 7.960 min
Delta R.T.: -0.005 min
Response: 34407144
Conc: 38.10 ng/ml

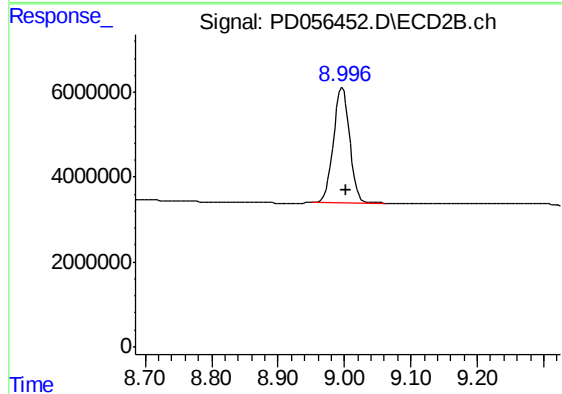

#27 Decachlorobiphenyl

R.T.: 8.997 min
Delta R.T.: -0.005 min
Response: 46126456
Conc: 38.34 ng/ml