

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121319\
 Data File : PD056454.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Dec 2019 21:13
 Operator : SG\AJ
 Sample : K6240-21
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BFQS6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 13 22:15:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 03 08:51:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.287	3.962	20406628	30088759	24.640	25.027
27)	SA Decachlor...	7.961	8.996	36661082	49920166	40.601	41.491
Target Compounds							
3)	MA gamma-BHC...	0.000	4.629	0	519971	N.D.	0.322
4)	MA Heptachlor	0.000	5.148	0	290514	N.D.	0.178
6)	B beta-BHC	0.000	4.847f	0	266611	N.D.	0.324
7)	B delta-BHC	0.000	4.977f	0	6002984	N.D.	3.604
8)	B Heptachlo...	0.000	5.806	0	5654682	N.D.	3.650
15)	B Endosulfa...	0.000	6.839	0	2523967	N.D.	1.723
16)	A 4,4'-DDD	0.000	6.736f	0	978490	N.D.	0.832
19)	B Endosulfa...	0.000	7.182	0	622586	N.D.	0.466


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121319\
Data File : PD056454.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Dec 2019 21:13
Operator : SG\AJ
Sample : K6240-21
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
BFQS6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 13 22:15:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120219CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 03 08:51:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

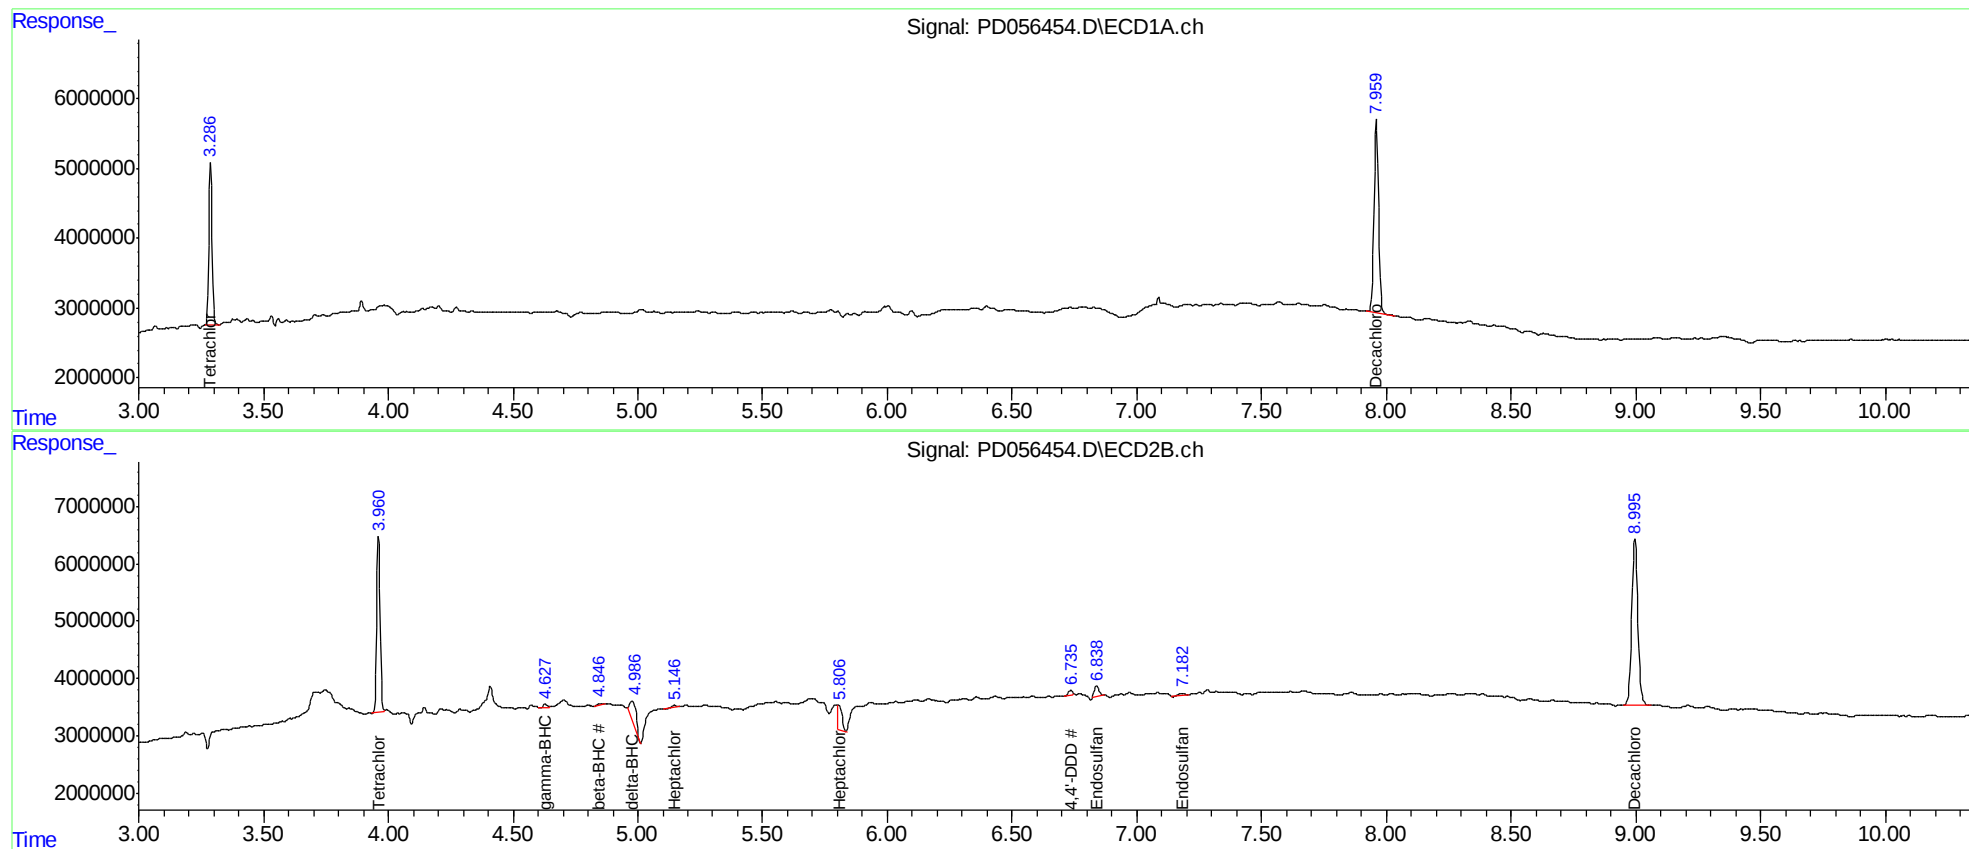


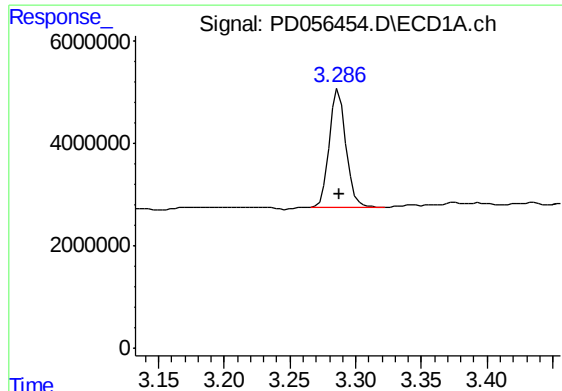

#1 Tetrachloro-m-xylene


R.T.: 3.287 min
Delta R.T.: 0.000 min
Response: 20406628
Conc: 24.64 ng/ml

Instrument :
ECD_D
ClientSampleId :
BFQS6

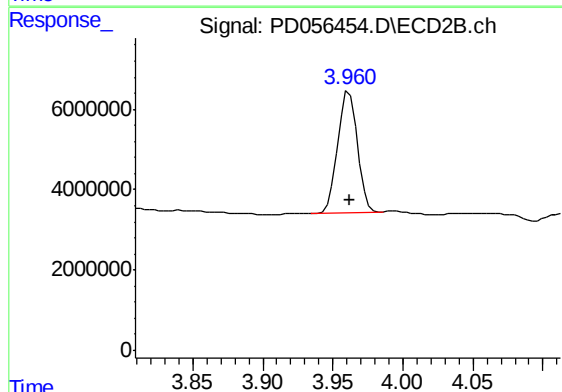


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: 0.000 min
Response: 30088759
Conc: 25.03 ng/ml

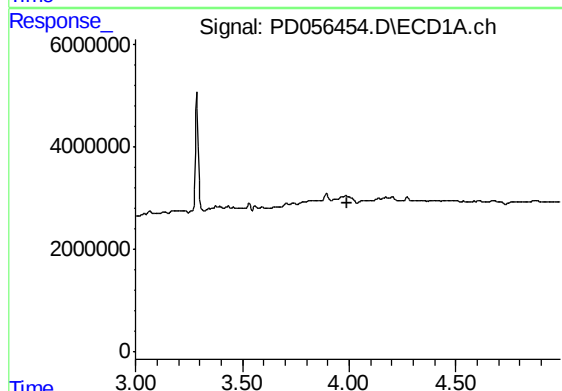


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 3.991 min
Response: 0
Conc: N.D.

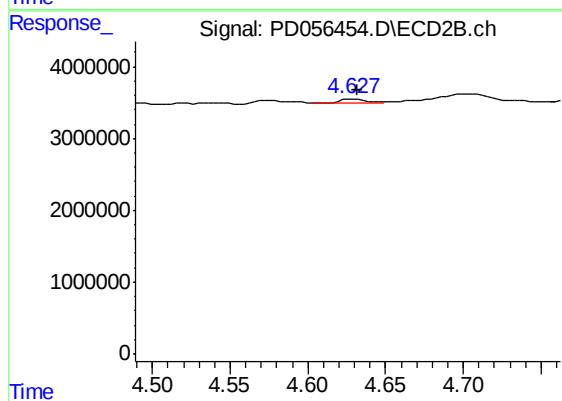

#3 gamma-BHC (Lindane)


R.T.: 4.629 min
Delta R.T.: -0.003 min
Response: 519971
Conc: 0.32 ng/ml

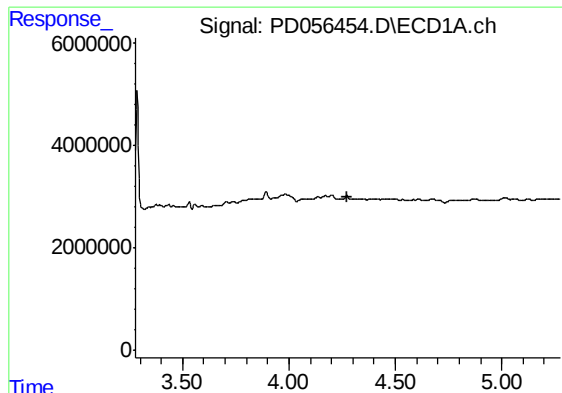

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 4.276 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BFQS6

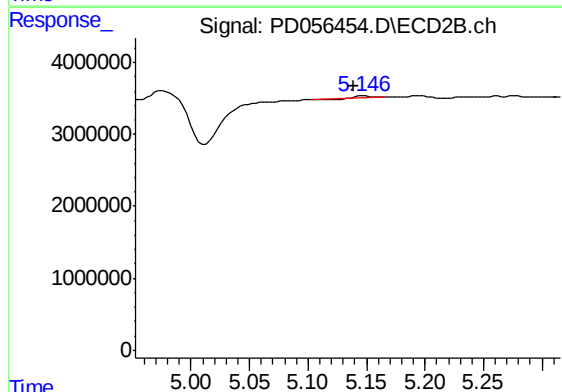


#4 Heptachlor

R.T.: 5.148 min
Delta R.T.: 0.009 min
Response: 290514
Conc: 0.18 ng/ml

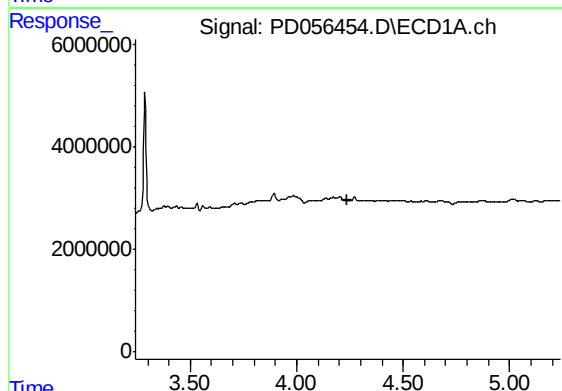


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.240 min
Response: 0
Conc: N.D.

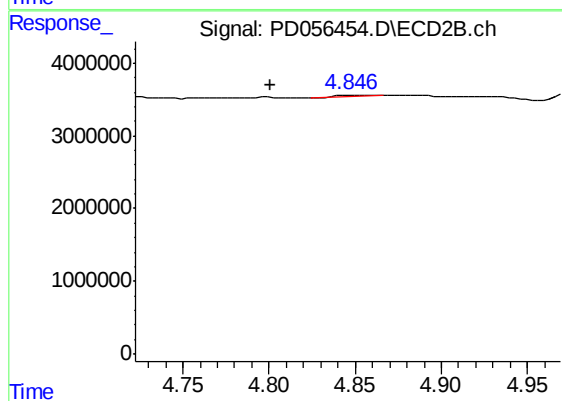

#6 beta-BHC


R.T.: 4.847 min
Delta R.T.: 0.047 min
Response: 266611
Conc: 0.32 ng/ml

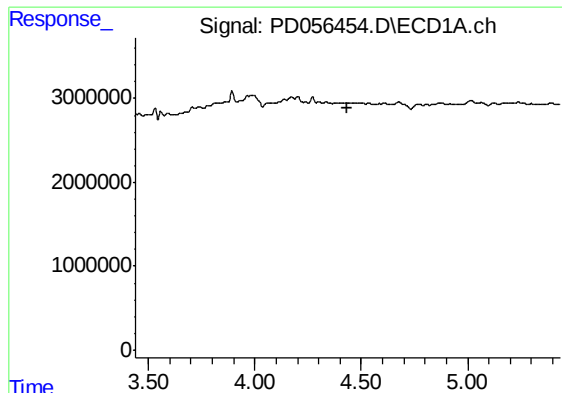

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.436 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BFQS6

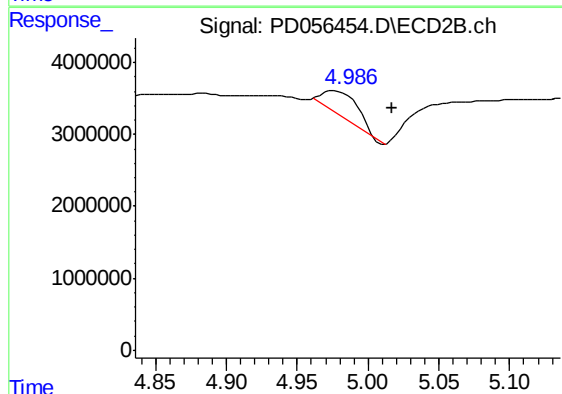


#7 delta-BHC

R.T.: 4.977 min
Delta R.T.: -0.040 min
Response: 6002984
Conc: 3.60 ng/ml

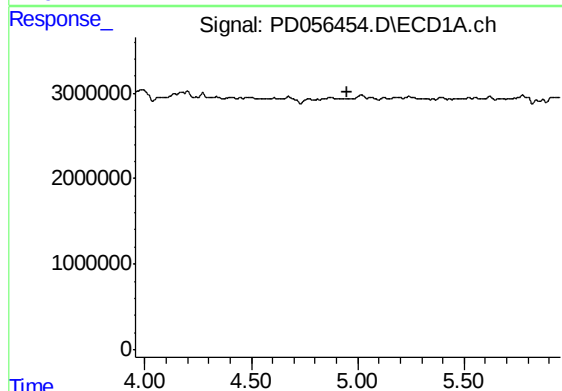


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.953 min
Response: 0
Conc: N.D.

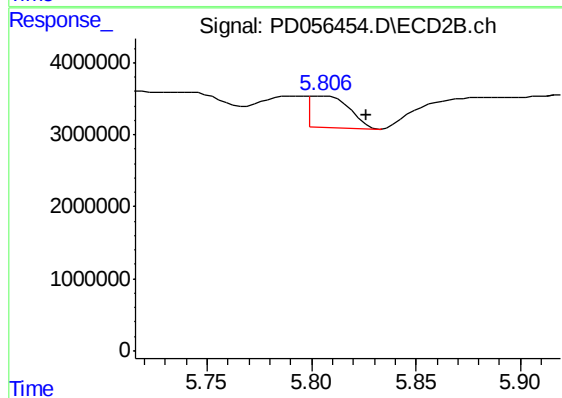

#8 Heptachlor epoxide


R.T.: 5.806 min
Delta R.T.: -0.021 min
Response: 5654682
Conc: 3.65 ng/ml

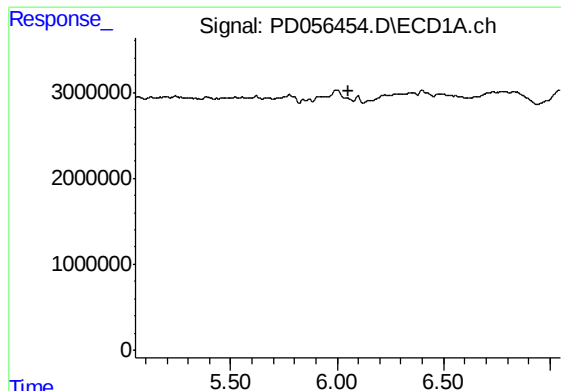

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.051 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BFQS6

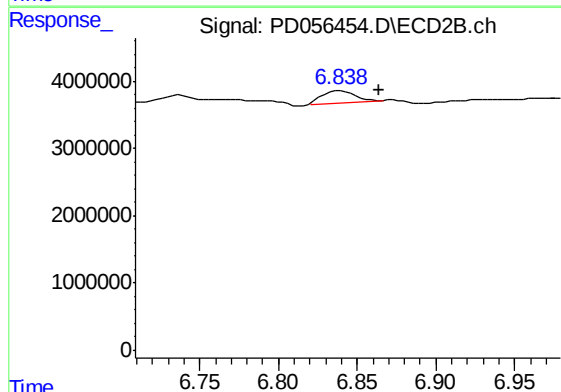


#15 Endosulfan II

R.T.: 6.839 min
Delta R.T.: -0.025 min
Response: 2523967
Conc: 1.72 ng/ml

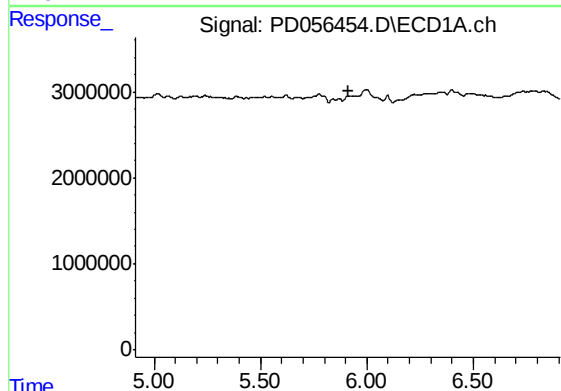


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 5.912 min
Response: 0
Conc: N.D.

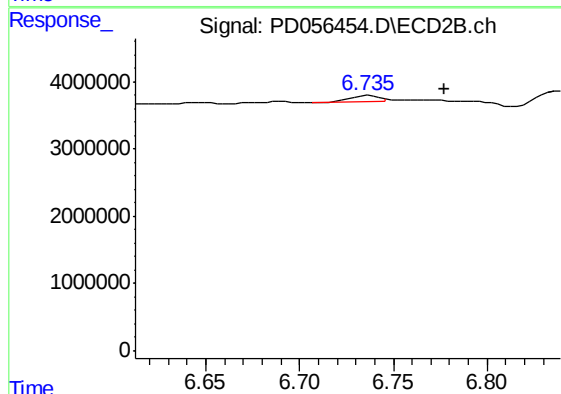

#16 4,4'-DDD


R.T.: 6.736 min
Delta R.T.: -0.041 min
Response: 978490
Conc: 0.83 ng/ml

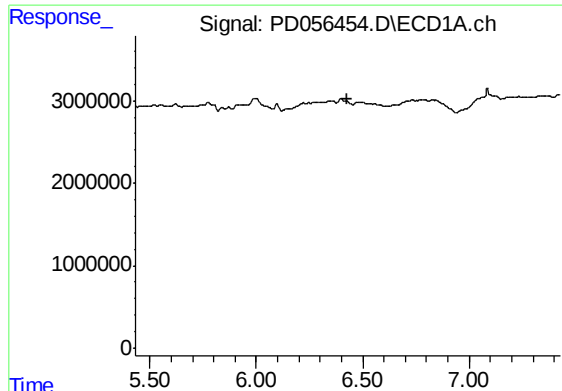

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 6.430 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BFQS6

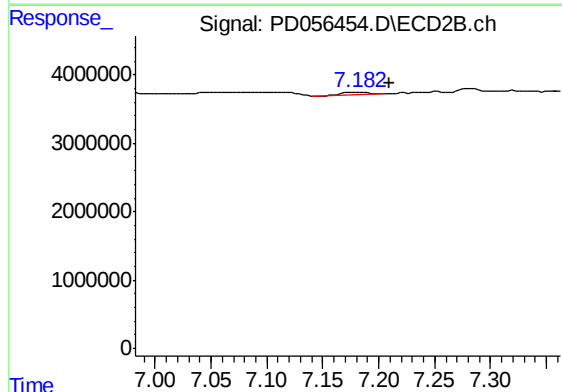


#19 Endosulfan Sulfate

R.T.: 7.182 min
Delta R.T.: -0.028 min
Response: 622586
Conc: 0.47 ng/ml

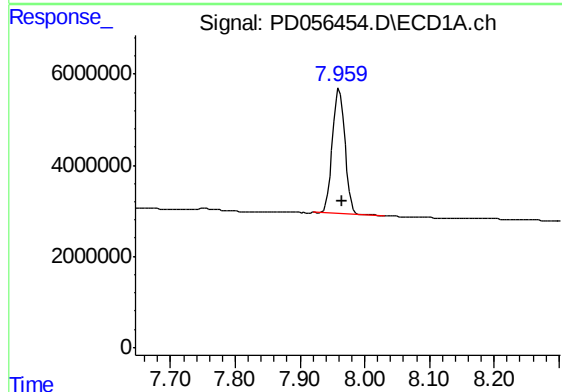

#27 Decachlorobiphenyl

R.T.: 7.961 min
Delta R.T.: -0.005 min
Response: 36661082
Conc: 40.60 ng/ml

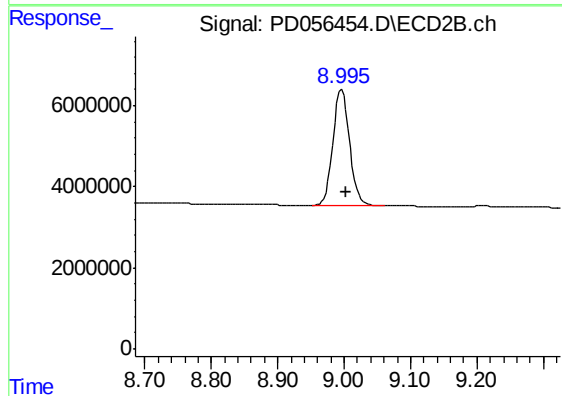

#27 Decachlorobiphenyl

R.T.: 8.996 min
Delta R.T.: -0.006 min
Response: 49920166
Conc: 41.49 ng/ml