

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121321\
 Data File : PD067267.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Dec 2021 08:37
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 14 02:21:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD113021.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 17:33:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
2) A	alpha-BHC	0.000	4.376f	0	1627278	N.D. 0.156 #
4) MA	Heptachlor	4.417f	0.000	234371	0	0.072 N.D. #
6) B	beta-BHC	4.417	0.000	234371	0	0.172 N.D. #
7) B	delta-BHC	0.000	5.052f	0	6471172	N.D. 0.705 #
15) B	Endosulfa...	6.257f	0.000	1934865	0	0.864 N.D. #
20) A	Methoxychlor	0.000	7.562	0	2393948	N.D. 0.743 #
22)	Mirex	0.000	8.146	0	816475	N.D. 0.167 #
27)	Chlordane-5	6.257	6.952	1934865	1904501	21.293 8.785 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121321\
Data File : PD067267.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Dec 2021 08:37
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 14 02:21:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD113021.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 17:33:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

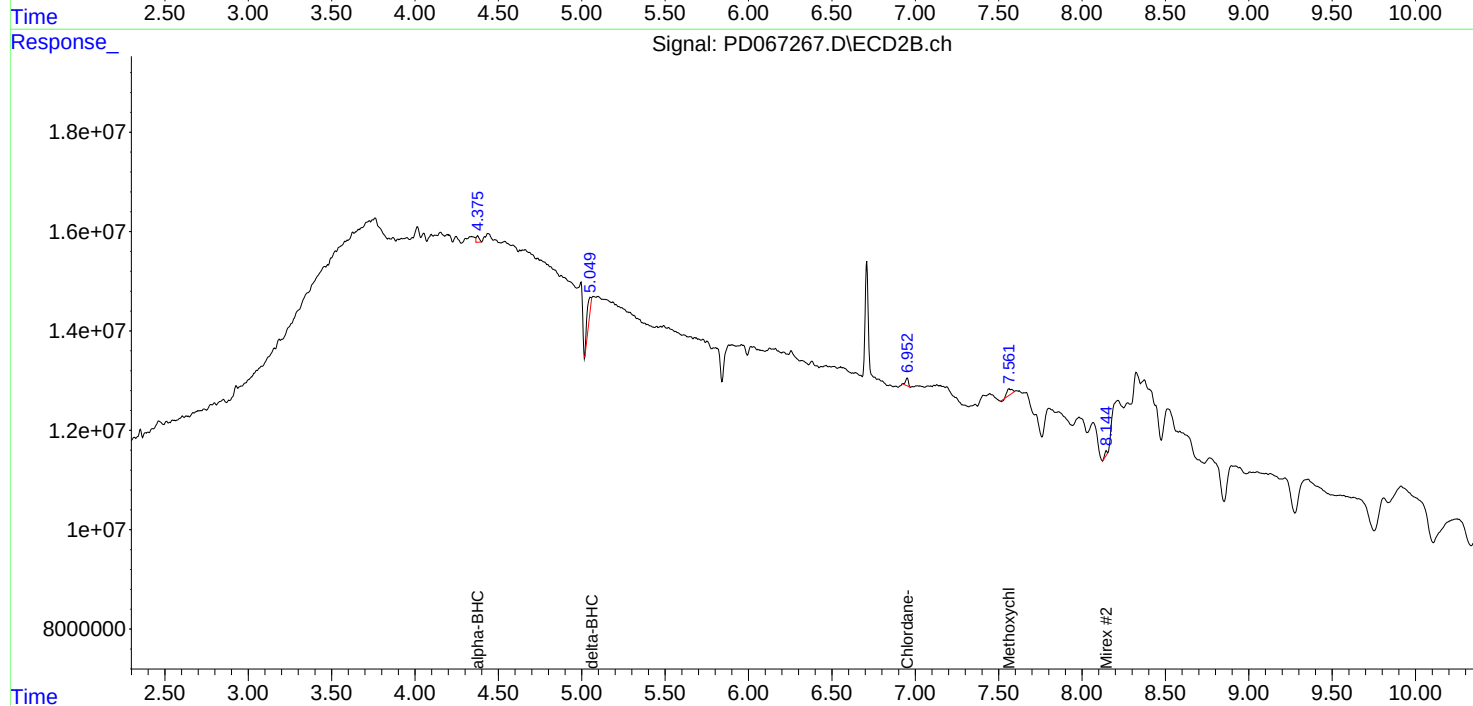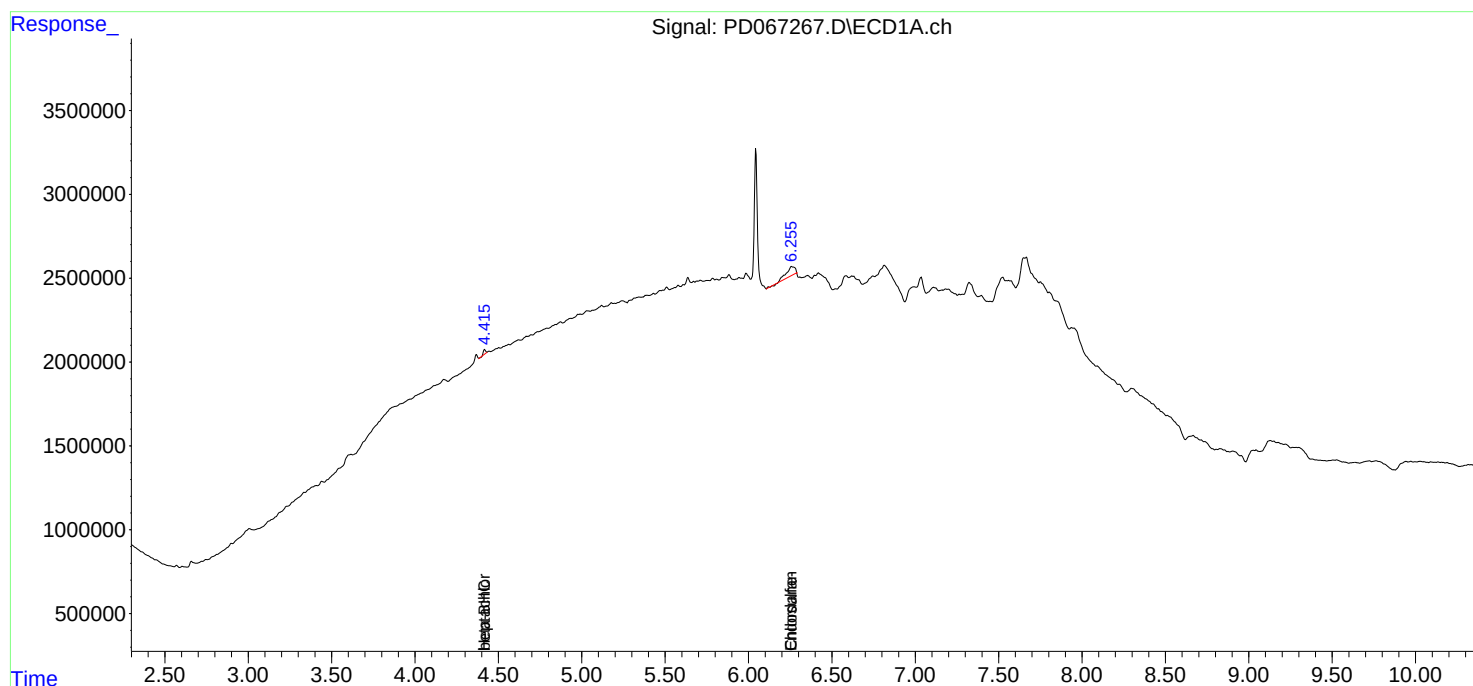


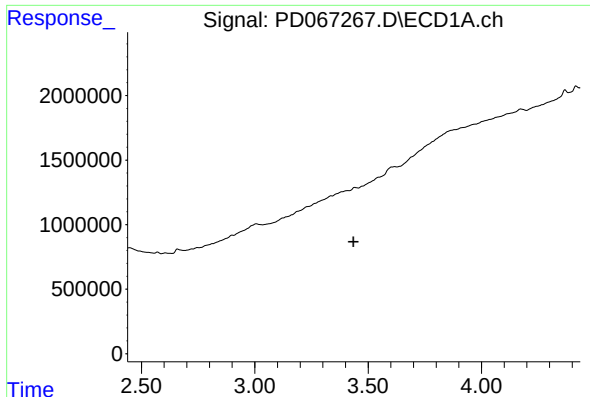

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.436 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

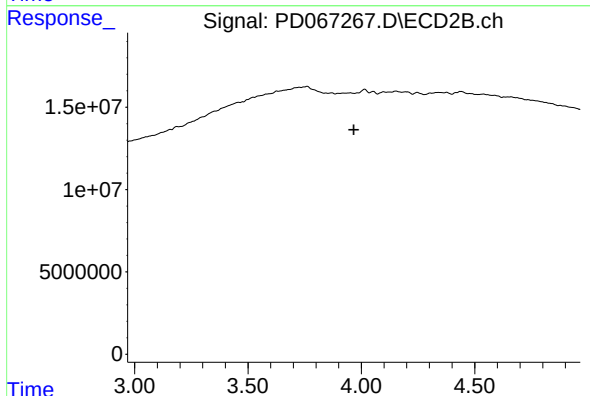


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.966 min
Response: 0
Conc: N.D.

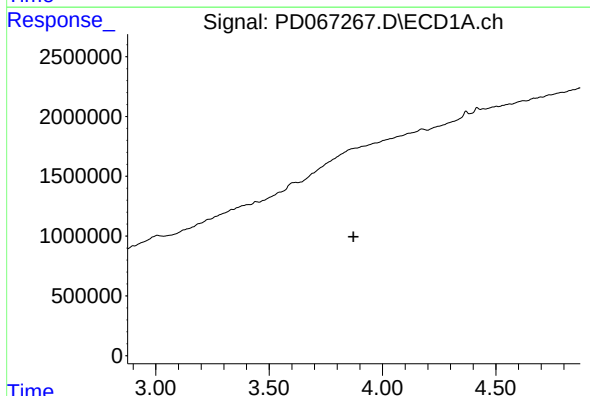




#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 3.873 min
Response: 0
Conc: N.D.

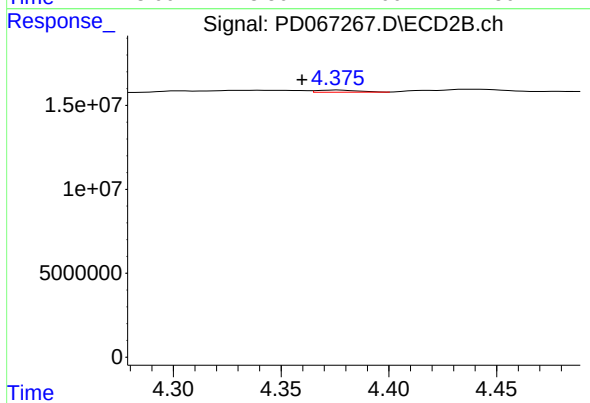

#2 alpha-BHC

R.T.: 4.376 min
Delta R.T.: 0.017 min
Response: 1627278
Conc: 0.16 ng/ml




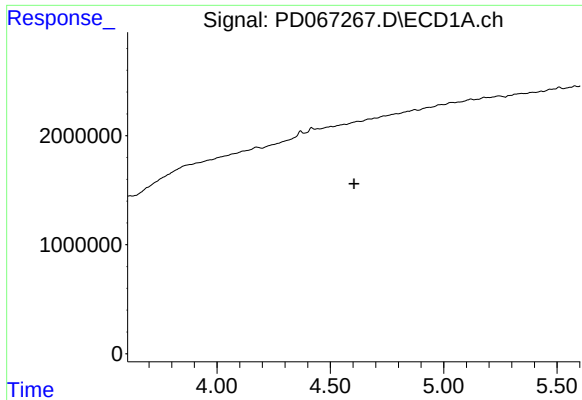

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.604 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

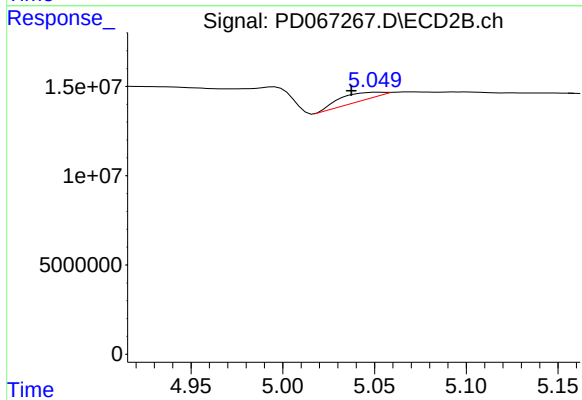


#7 delta-BHC

R.T.: 5.052 min
Delta R.T.: 0.015 min
Response: 6471172
Conc: 0.71 ng/ml

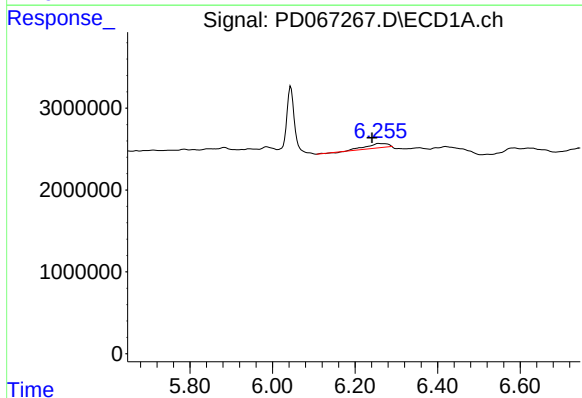


#15 Endosulfan II

R.T.: 6.257 min
Delta R.T.: 0.016 min
Response: 1934865
Conc: 0.86 ng/ml

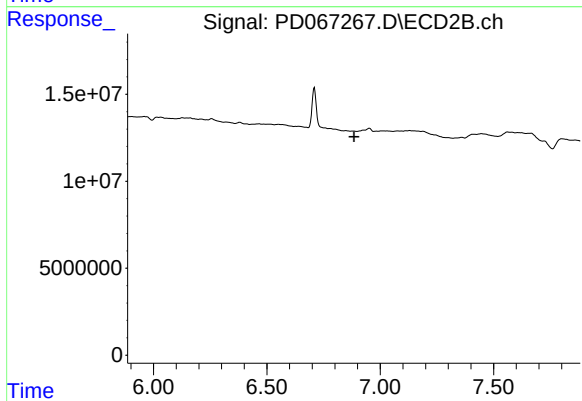

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.885 min
Response: 0
Conc: N.D.

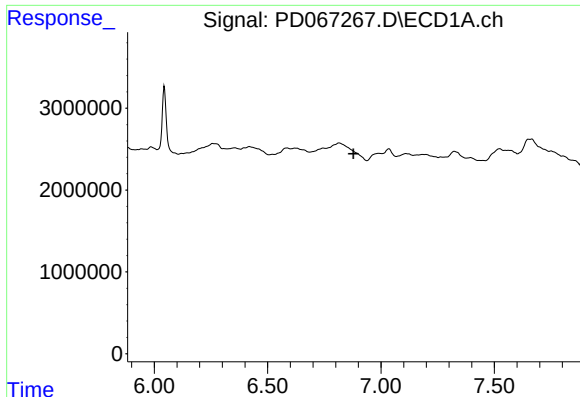

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.879 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

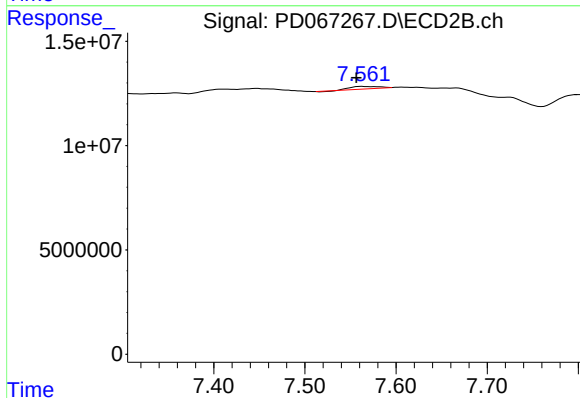


#20 Methoxychlor

R.T.: 7.562 min
Delta R.T.: 0.006 min
Response: 2393948
Conc: 0.74 ng/ml

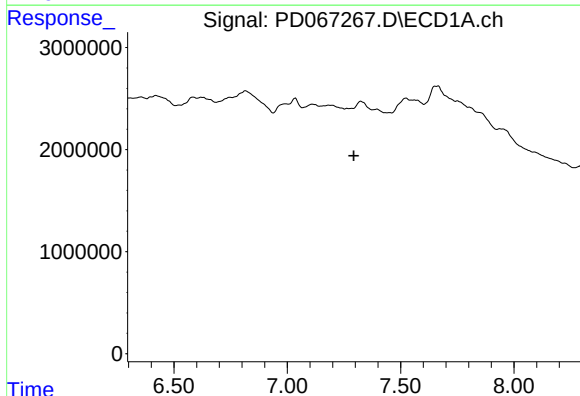


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 7.294 min
Response: 0
Conc: N.D.

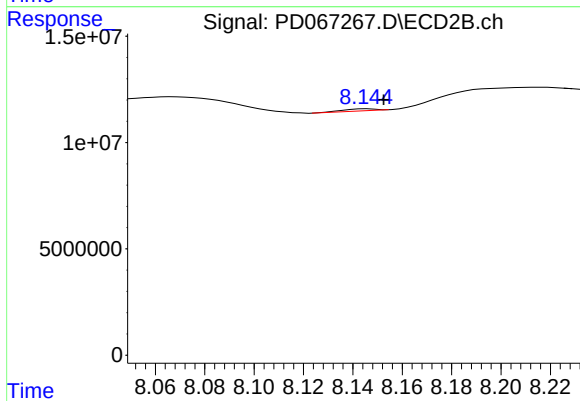

#22 Mirex


R.T.: 8.146 min
Delta R.T.: -0.007 min
Response: 816475
Conc: 0.17 ng/ml

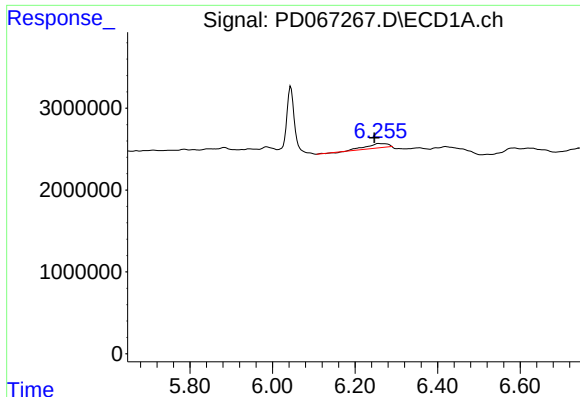

#27 Chlordane-5


R.T.: 6.257 min
Delta R.T.: 0.011 min
Response: 1934865
Conc: 21.29 ng/ml

Instrument :
ECD_D
ClientSampleId :

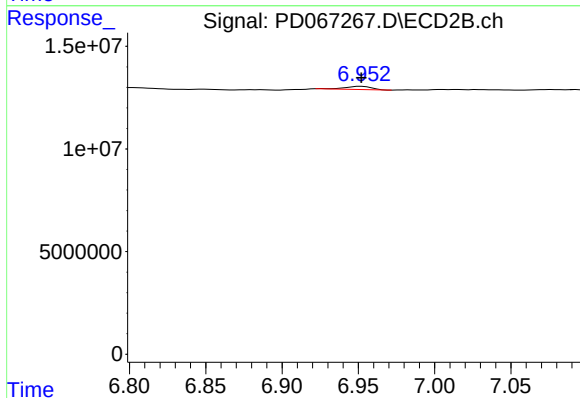


#27 Chlordane-5

R.T.: 6.952 min
Delta R.T.: 0.000 min
Response: 1904501
Conc: 8.78 ng/ml

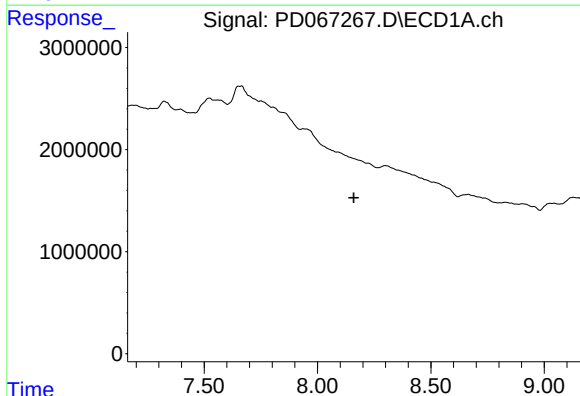

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.160 min
Response: 0
Conc: N.D.

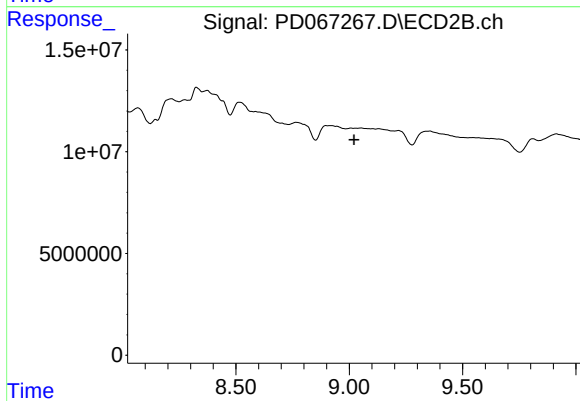

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.021 min
Response: 0
Conc: N.D.