

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121321\
 Data File : PD067268.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Dec 2021 08:51
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 14 02:22:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD113021.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 17:33:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.436	3.965	37859282	177.5E6	18.322	24.460 #
28)	SA Decachlor...	8.160	9.025	17564015	95174189	15.502	18.932
Target Compounds							
2)	A alpha-BHC	0.000	4.366	0	2105587	N.D.	0.202 #
4)	MA Heptachlor	0.000	5.129f	0	969735	N.D.	0.108 #
6)	B beta-BHC	4.411	4.836	1150298	1167250	0.843	0.265 #
15)	B Endosulfa...	6.254	6.887	1256837	606541	0.561	0.101 #
19)	B Endosulfa...	0.000	7.237	0	745333	N.D.	0.124 #
21)	B Endrin ke...	0.000	7.694	0	478518	N.D.	0.066 #
22)	Mirex	0.000	8.153	0	185687	N.D.	0.038 #
27)	Chlordane-5	6.254	0.000	1256837	0	13.832	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121321\
Data File : PD067268.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Dec 2021 08:51
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 14 02:22:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD113021.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 17:33:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

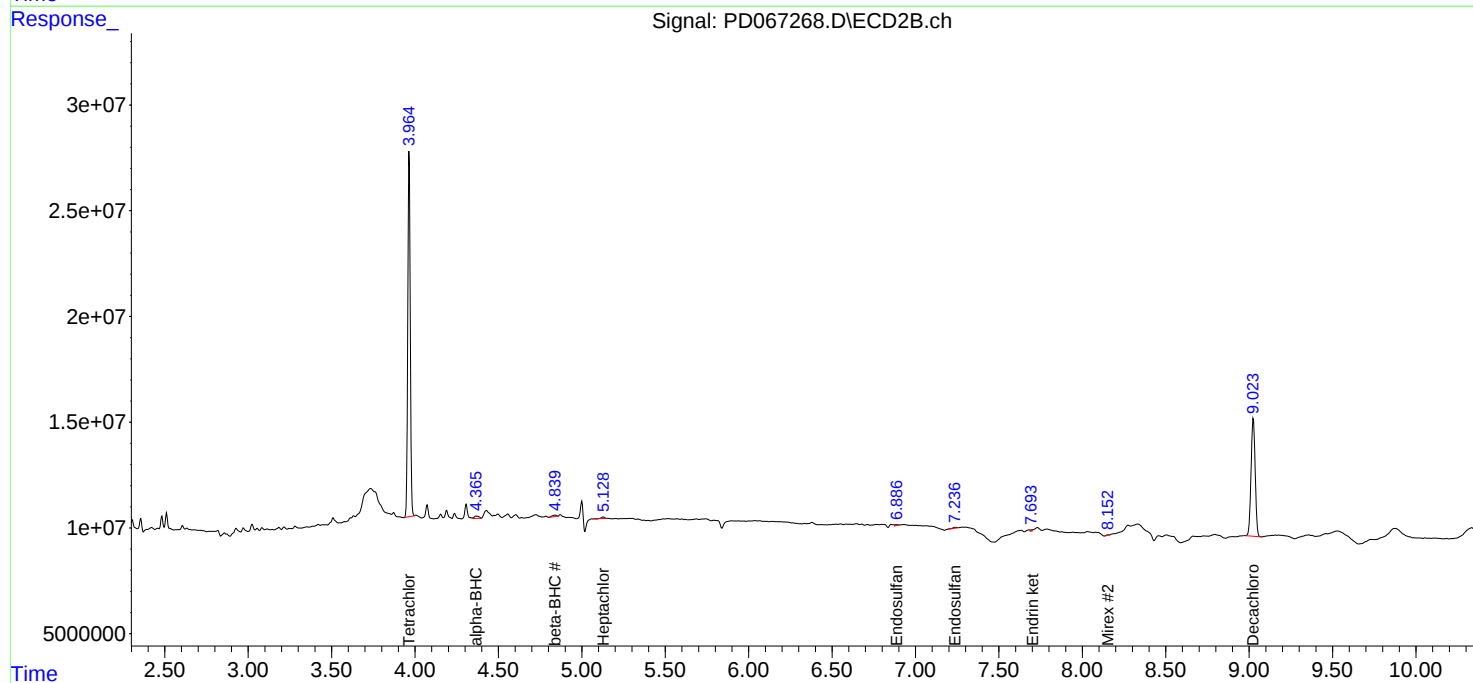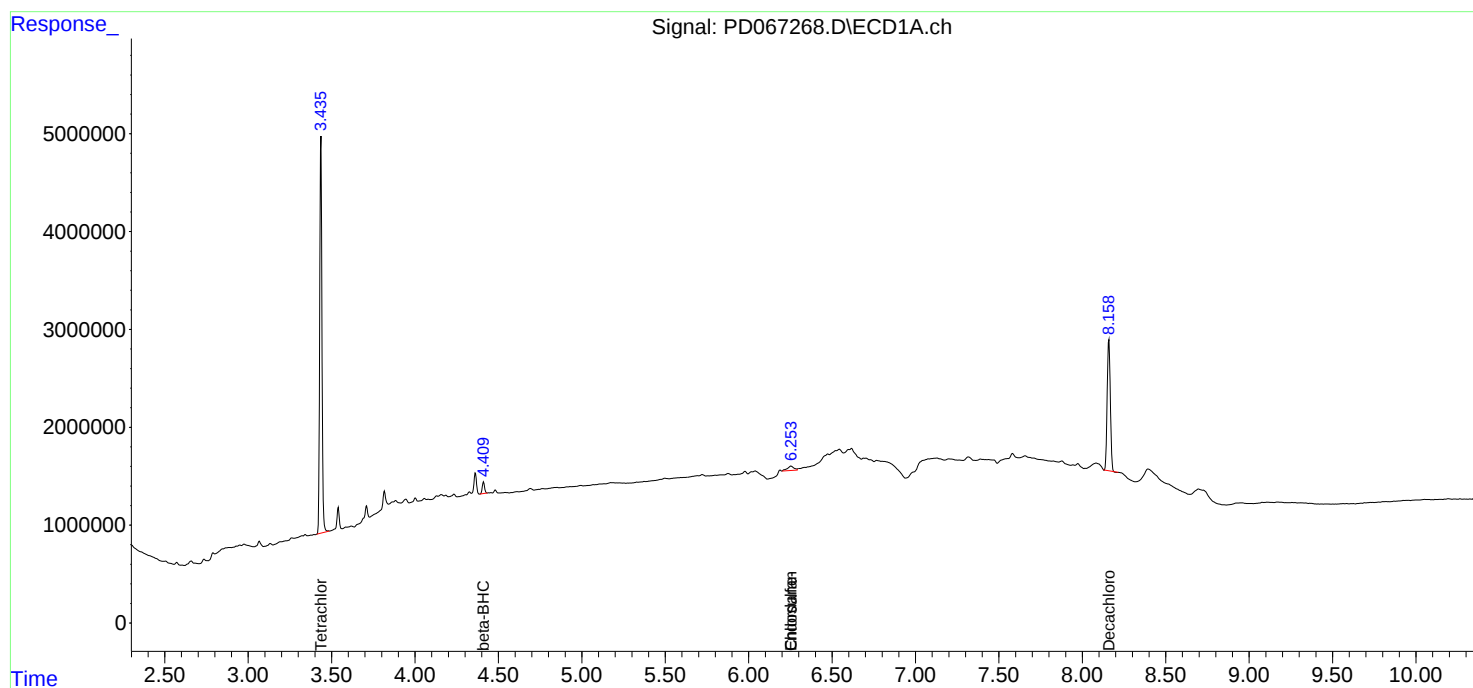


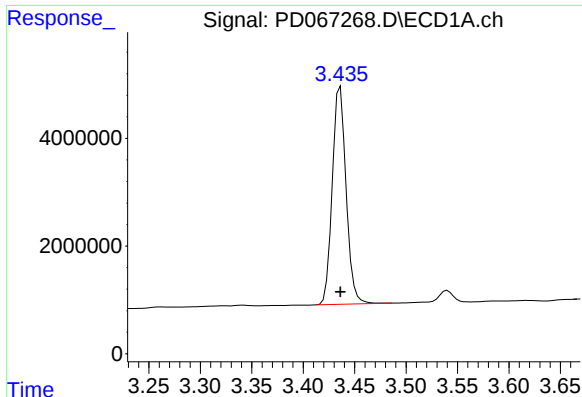

#1 Tetrachloro-m-xylene


R.T.: 3.436 min
Delta R.T.: 0.000 min
Response: 37859282
Conc: 18.32 ng/ml

Instrument :
ECD_D
ClientSampleId :

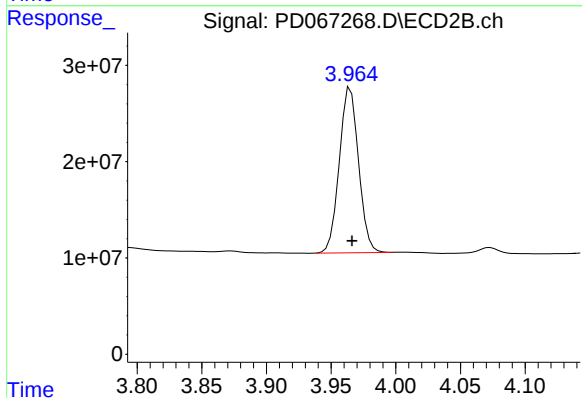


#1 Tetrachloro-m-xylene

R.T.: 3.965 min
Delta R.T.: -0.001 min
Response: 177538731
Conc: 24.46 ng/ml

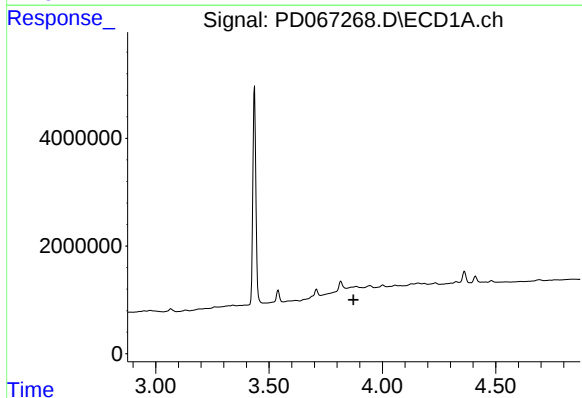


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.873 min
Response: 0
Conc: N.D.

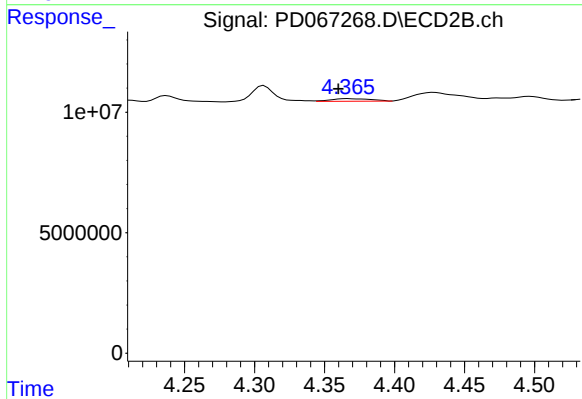

#2 alpha-BHC


R.T.: 4.366 min
Delta R.T.: 0.007 min
Response: 2105587
Conc: 0.20 ng/ml

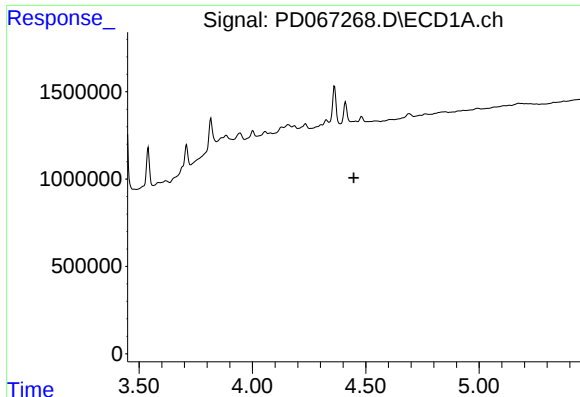

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.448 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

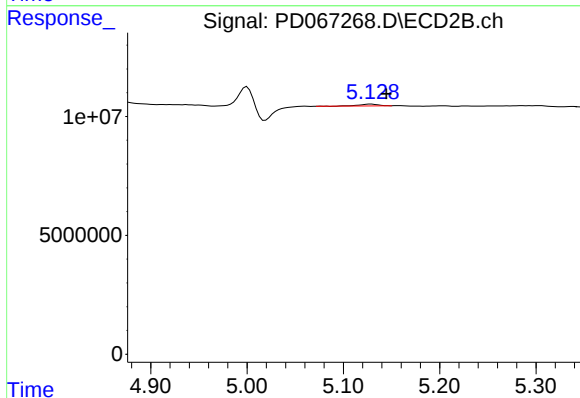


#4 Heptachlor

R.T.: 5.129 min
Delta R.T.: -0.016 min
Response: 969735
Conc: 0.11 ng/ml

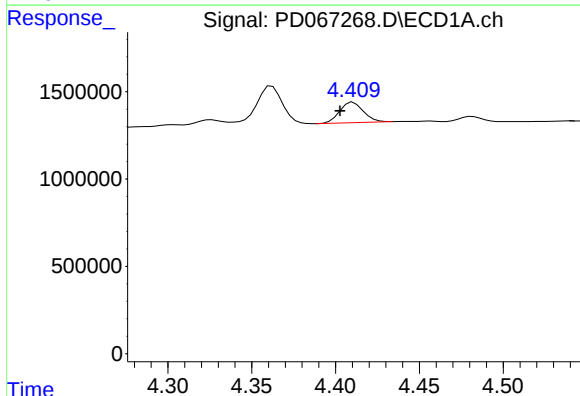


#6 beta-BHC

R.T.: 4.411 min
Delta R.T.: 0.008 min
Response: 1150298
Conc: 0.84 ng/ml

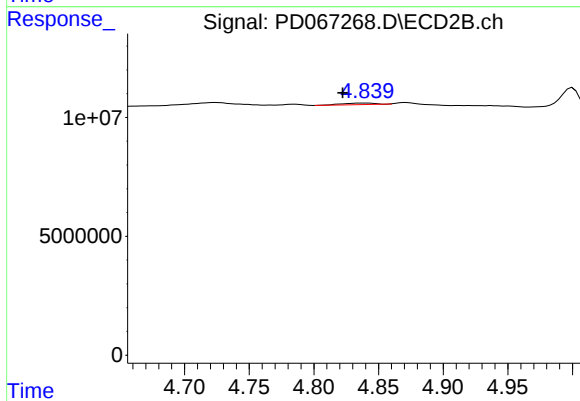

#6 beta-BHC


R.T.: 4.836 min
Delta R.T.: 0.014 min
Response: 1167250
Conc: 0.26 ng/ml

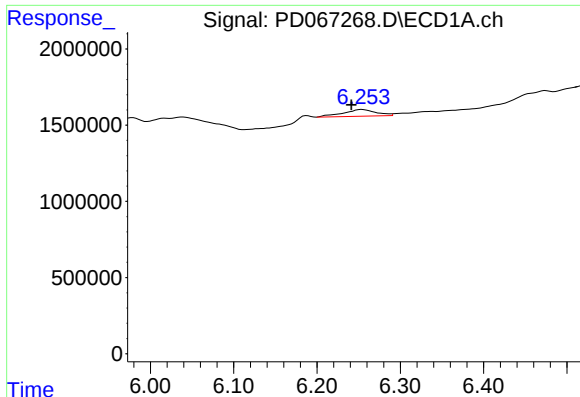

#15 Endosulfan II


R.T.: 6.254 min
Delta R.T.: 0.013 min
Response: 1256837
Conc: 0.56 ng/ml

Instrument :
ECD_D
ClientSampleId :

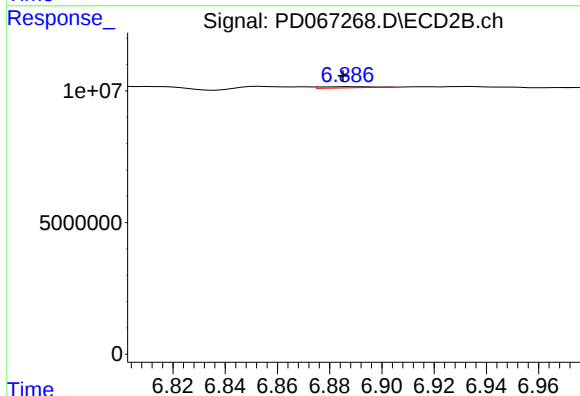


#15 Endosulfan II

R.T.: 6.887 min
Delta R.T.: 0.002 min
Response: 606541
Conc: 0.10 ng/ml

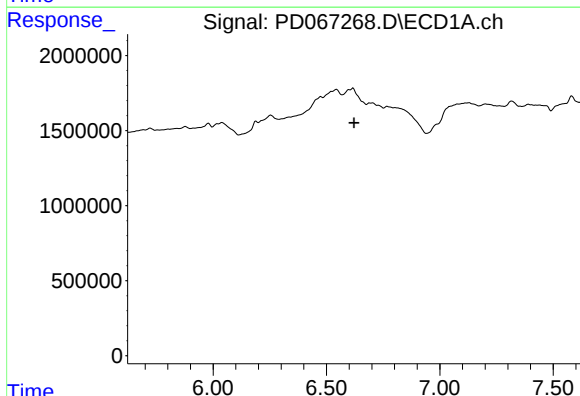


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 6.621 min
Response: 0
Conc: N.D.

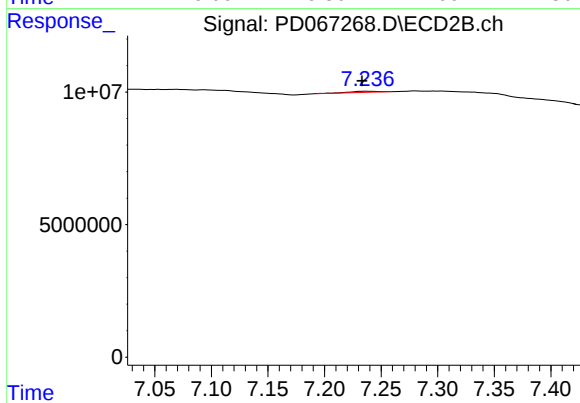

#19 Endosulfan Sulfate


R.T.: 7.237 min
Delta R.T.: 0.004 min
Response: 745333
Conc: 0.12 ng/ml

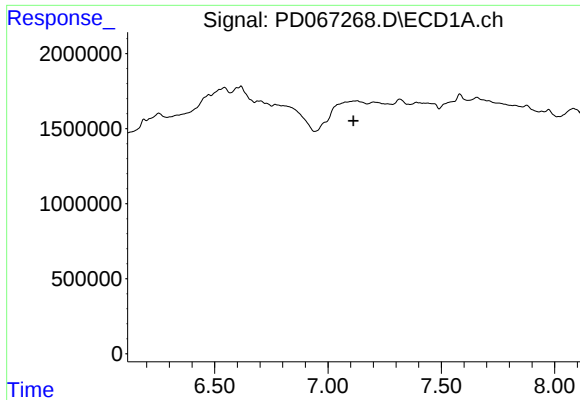

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.113 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

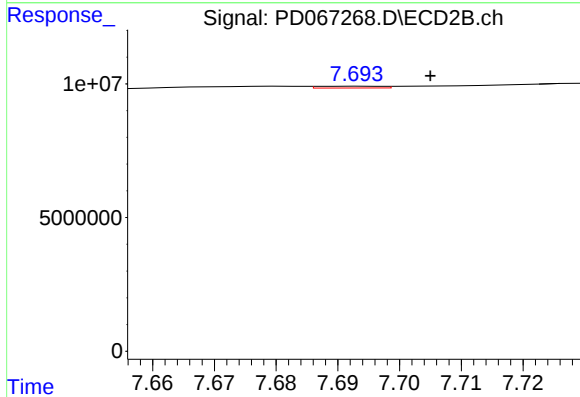


#21 Endrin ketone

R.T.: 7.694 min
Delta R.T.: -0.011 min
Response: 478518
Conc: 0.07 ng/ml

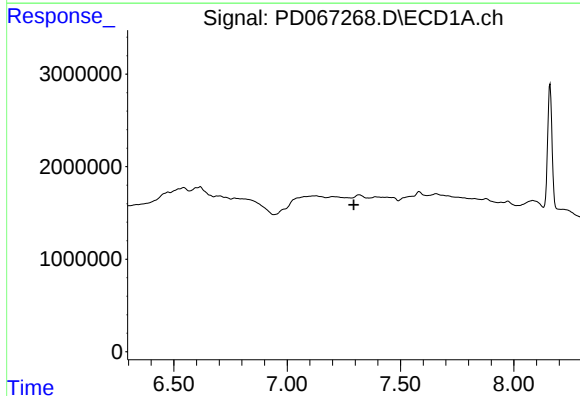


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 7.294 min
Response: 0
Conc: N.D.

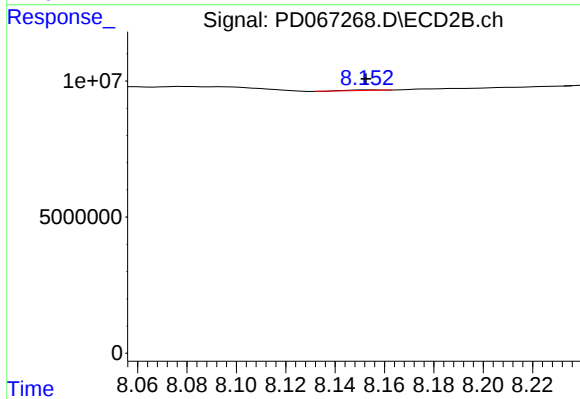

#22 Mirex


R.T.: 8.153 min
Delta R.T.: 0.000 min
Response: 185687
Conc: 0.04 ng/ml

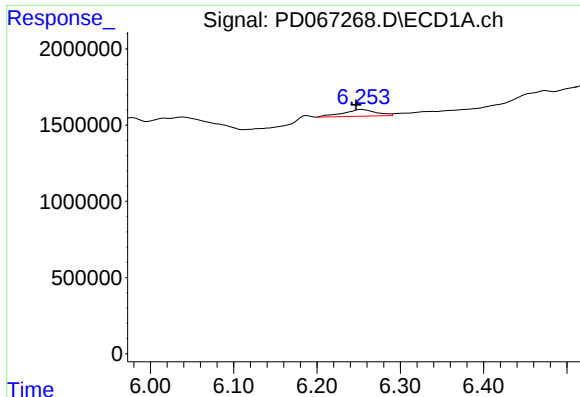

#27 Chlordane-5


R.T.: 6.254 min
Delta R.T.: 0.007 min
Response: 1256837
Conc: 13.83 ng/ml

Instrument :
ECD_D
ClientSampleId :

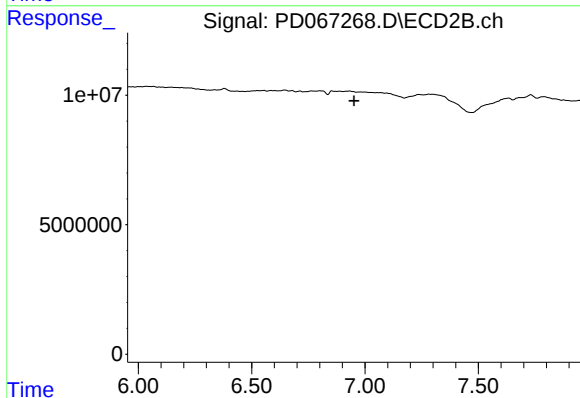


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.952 min
Response: 0
Conc: N.D.

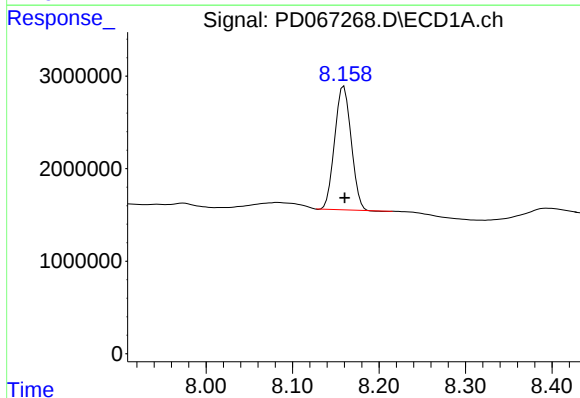

#28 Decachlorobiphenyl

R.T.: 8.160 min
Delta R.T.: 0.000 min
Response: 17564015
Conc: 15.50 ng/ml

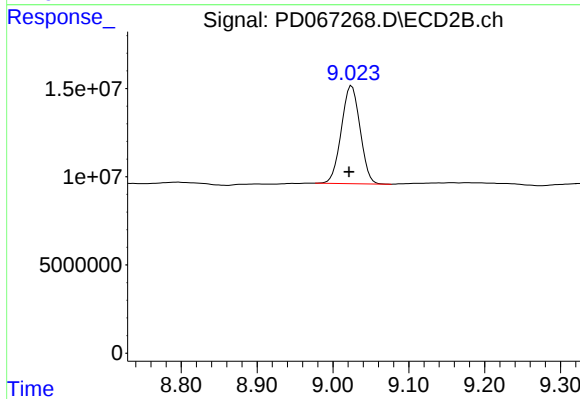

#28 Decachlorobiphenyl

R.T.: 9.025 min
Delta R.T.: 0.004 min
Response: 95174189
Conc: 18.93 ng/ml