

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121321\
 Data File : PD067272.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Dec 2021 11:25
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 14 02:23:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD113021.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 17:33:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	3.965	35195300	158.5E6	17.033	21.831 #
28)	SA Decachlor...	8.169	9.029	18277797	84232321	16.132	16.755
Target Compounds							
2)	A alpha-BHC	0.000	4.368	0	5376594	N.D.	0.517 #
4)	MA Heptachlor	4.417f	5.128f	1311974	1658348	0.403	0.184 #
6)	B beta-BHC	4.417	0.000	1311974	0	0.961	N.D. #
14)	MA Endrin	0.000	6.673	0	304812	N.D.	0.054 #
15)	B Endosulfa...	0.000	6.887	0	1478646	N.D.	0.246 #
21)	B Endrin ke...	0.000	7.724f	0	14114709	N.D.	1.952 #
22)	Mirex	0.000	8.161	0	2584576	N.D.	0.528 #
27)	Chlordane-5	6.276f	0.000	1199832	0	13.204	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121321\
Data File : PD067272.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Dec 2021 11:25
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 14 02:23:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD113021.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 17:33:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

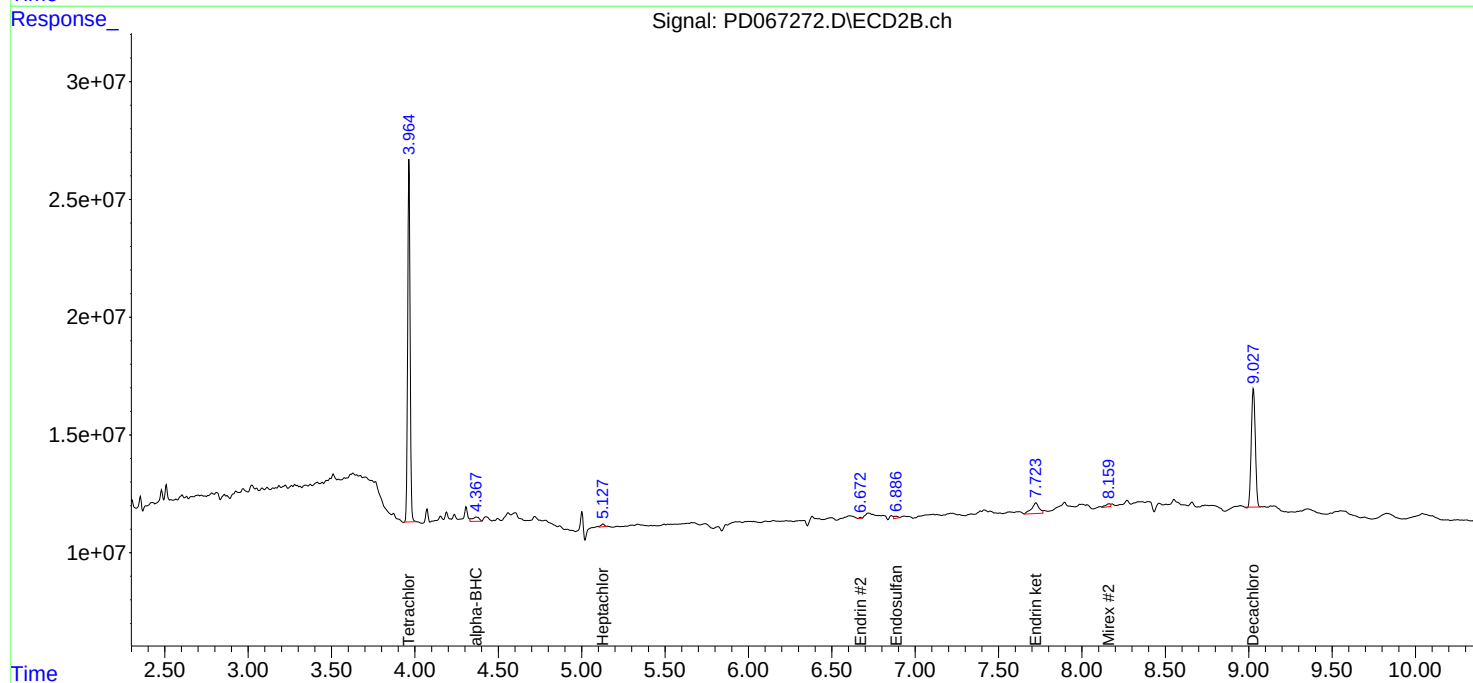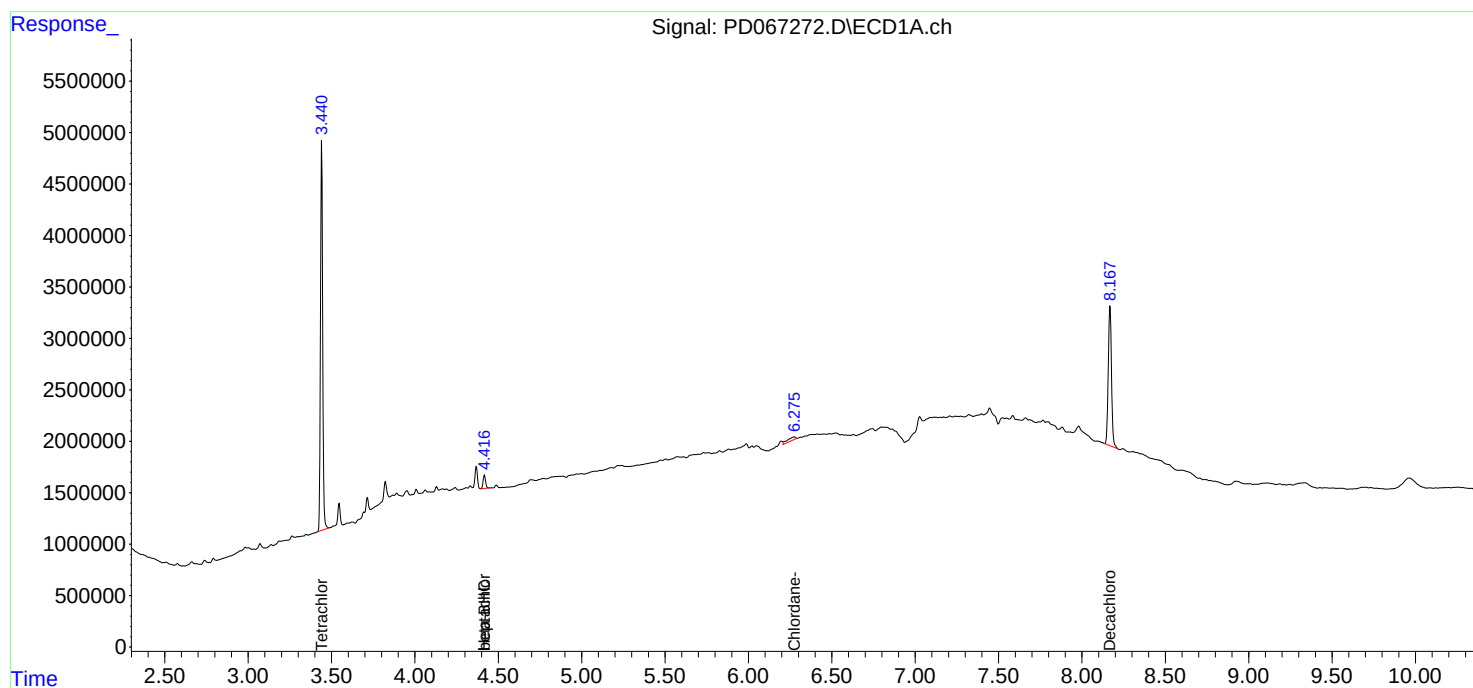


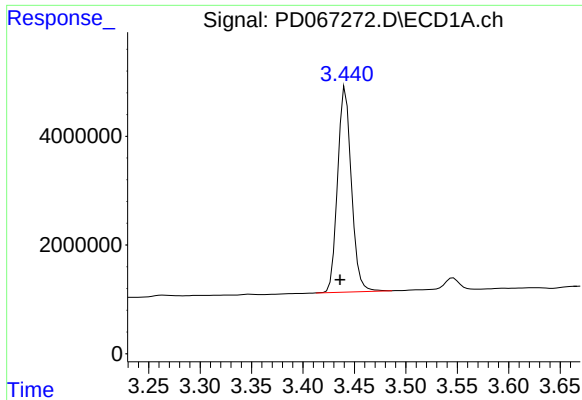

#1 Tetrachloro-m-xylene


R.T.: 3.441 min
Delta R.T.: 0.005 min
Response: 35195300
Conc: 17.03 ng/ml

Instrument :
ECD_D
ClientSampleId :

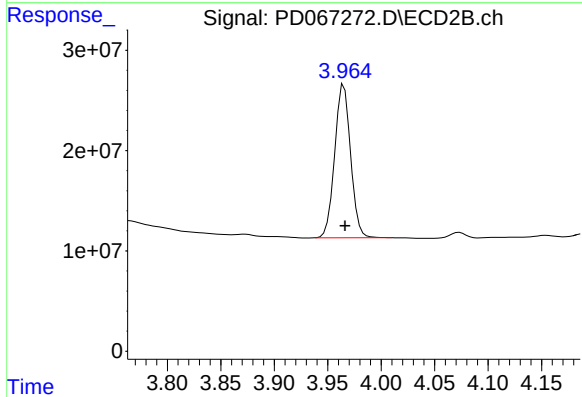


#1 Tetrachloro-m-xylene

R.T.: 3.965 min
Delta R.T.: -0.001 min
Response: 158450743
Conc: 21.83 ng/ml

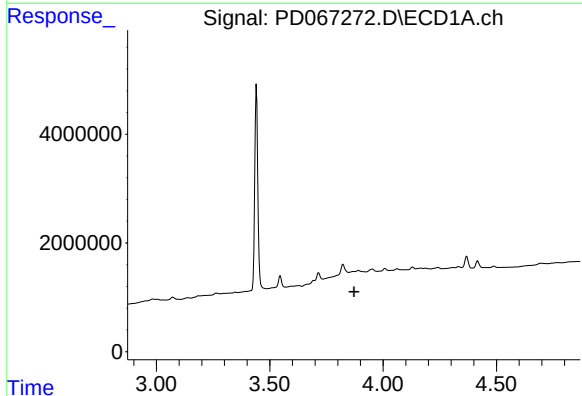


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.873 min
Response: 0
Conc: N.D.

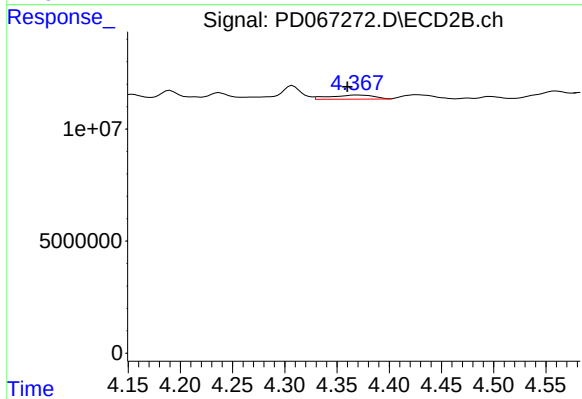

#2 alpha-BHC


R.T.: 4.368 min
Delta R.T.: 0.008 min
Response: 5376594
Conc: 0.52 ng/ml

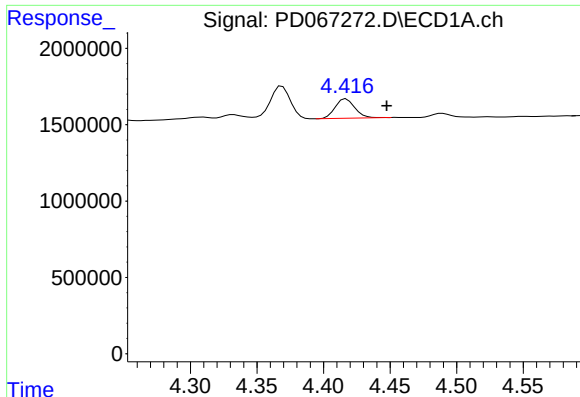

#4 Heptachlor


R.T.: 4.417 min
Delta R.T.: -0.030 min
Response: 1311974
Conc: 0.40 ng/ml

Instrument :
ECD_D
ClientSampleId :

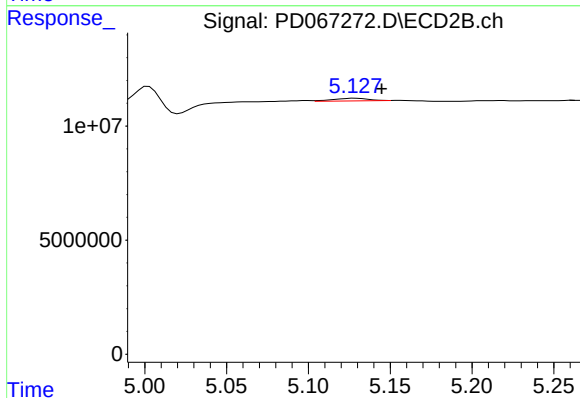


#4 Heptachlor

R.T.: 5.128 min
Delta R.T.: -0.016 min
Response: 1658348
Conc: 0.18 ng/ml

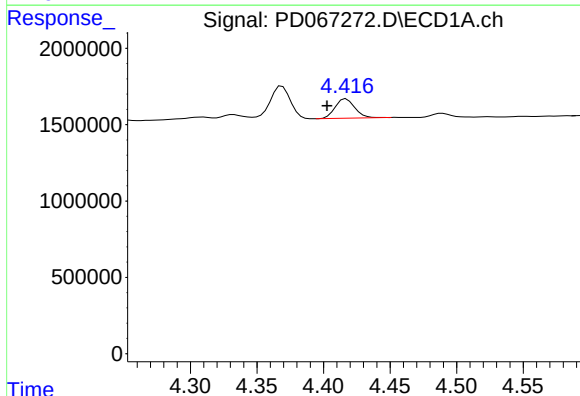


#6 beta-BHC

R.T.: 4.417 min
Delta R.T.: 0.014 min
Response: 1311974
Conc: 0.96 ng/ml

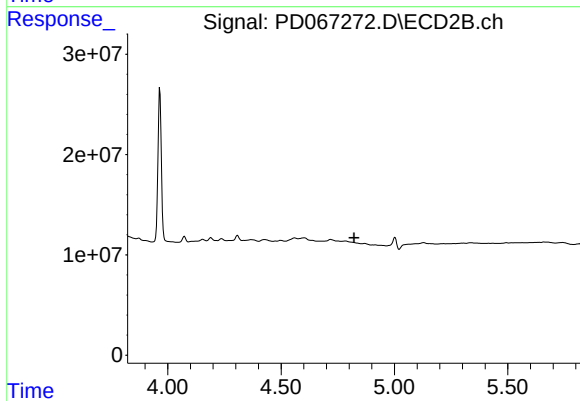

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.822 min
Response: 0
Conc: N.D.

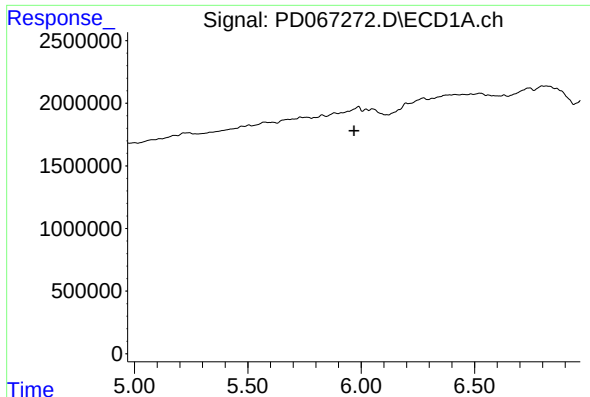

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 5.968 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

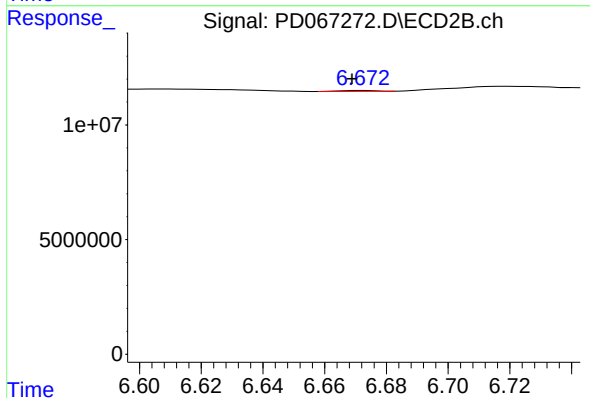


#14 Endrin

R.T.: 6.673 min
Delta R.T.: 0.004 min
Response: 304812
Conc: 0.05 ng/ml

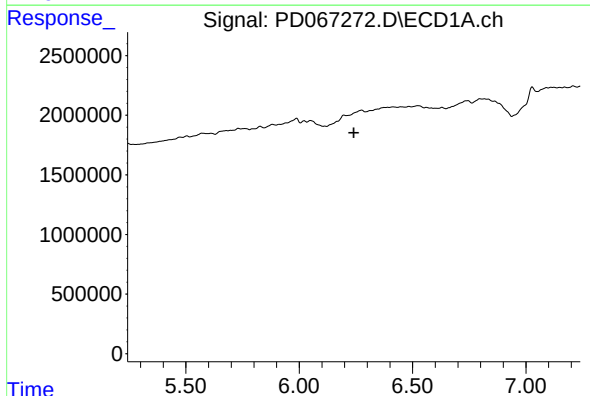


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.241 min
Response: 0
Conc: N.D.

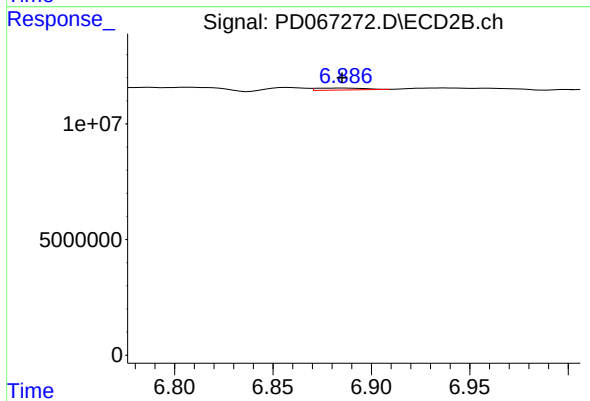

#15 Endosulfan II


R.T.: 6.887 min
Delta R.T.: 0.001 min
Response: 1478646
Conc: 0.25 ng/ml

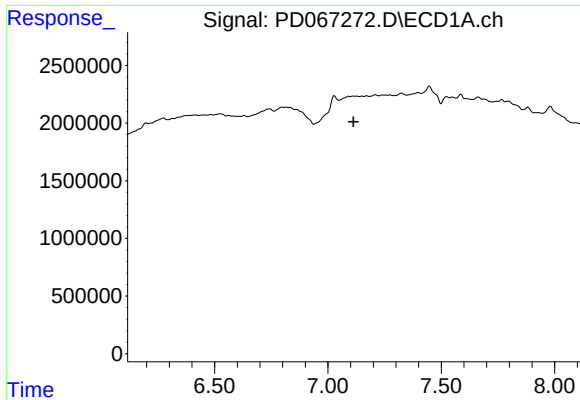

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.113 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

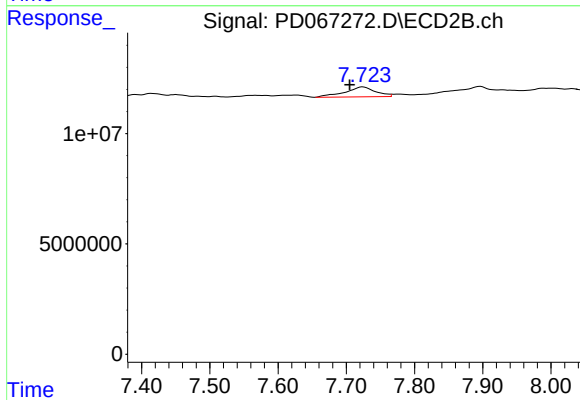


#21 Endrin ketone

R.T.: 7.724 min
Delta R.T.: 0.019 min
Response: 14114709
Conc: 1.95 ng/ml

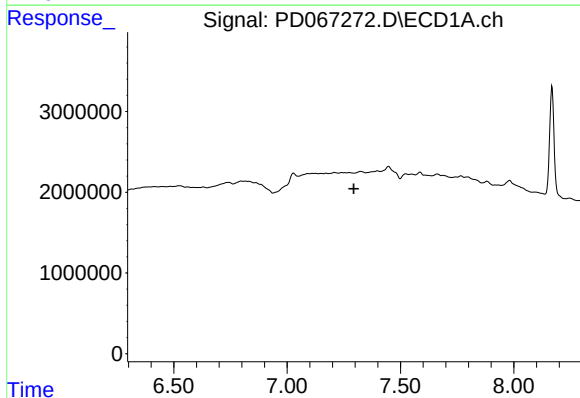


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 7.294 min
Response: 0
Conc: N.D.

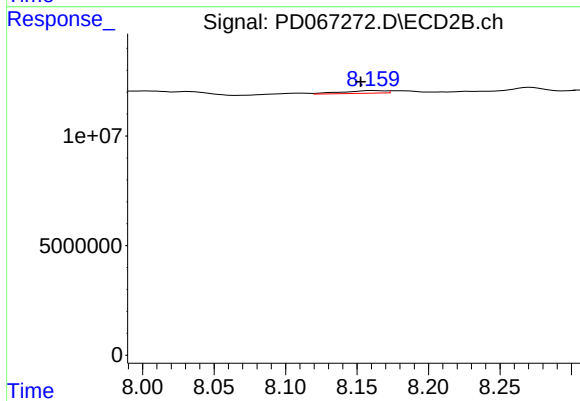

#22 Mirex


R.T.: 8.161 min
Delta R.T.: 0.008 min
Response: 2584576
Conc: 0.53 ng/ml

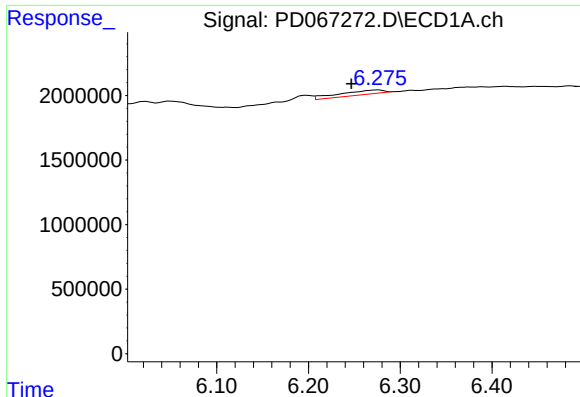

#27 Chlordane-5


R.T.: 6.276 min
Delta R.T.: 0.030 min
Response: 1199832
Conc: 13.20 ng/ml

Instrument :
ECD_D
ClientSampleId :

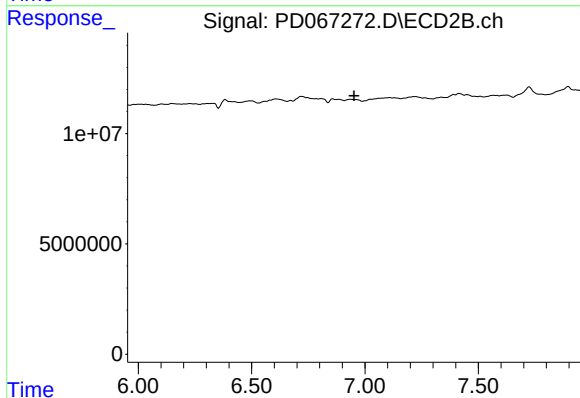


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.952 min
Response: 0
Conc: N.D.

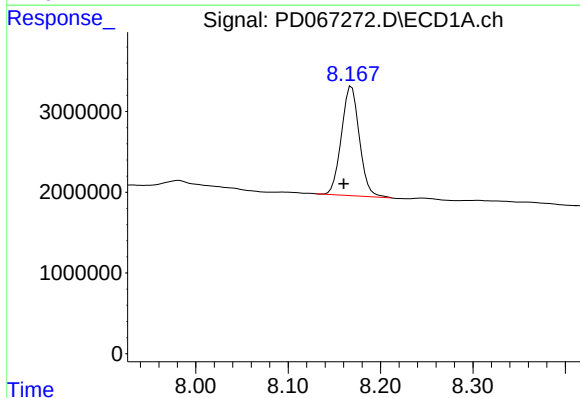

#28 Decachlorobiphenyl

R.T.: 8.169 min
Delta R.T.: 0.008 min
Response: 18277797
Conc: 16.13 ng/ml

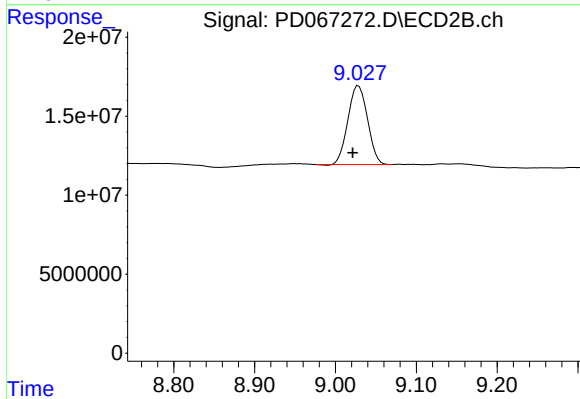

#28 Decachlorobiphenyl

R.T.: 9.029 min
Delta R.T.: 0.007 min
Response: 84232321
Conc: 16.76 ng/ml