

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121321\
 Data File : PD067301.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Dec 2021 21:53
 Operator : AR\AJ
 Sample : M5051-03 10X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 P-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 14 02:33:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD113021.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 17:33:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.435	3.965	2024087	10336055	0.980	1.424 #
28) SA Decachlor...	8.158	9.025	1931469	7353721	1.705m	1.463
Target Compounds						
12) B 4,4'-DDE	5.575	6.302	1004997	5566373	0.374m	0.804 #
16) A 4,4'-DDD	6.090	6.798	935754	4557190	0.445m	0.779 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121321\
Data File : PD067301.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Dec 2021 21:53
Operator : AR\AJ
Sample : M5051-03 10X
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
P-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 14 02:33:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD113021.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 17:33:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

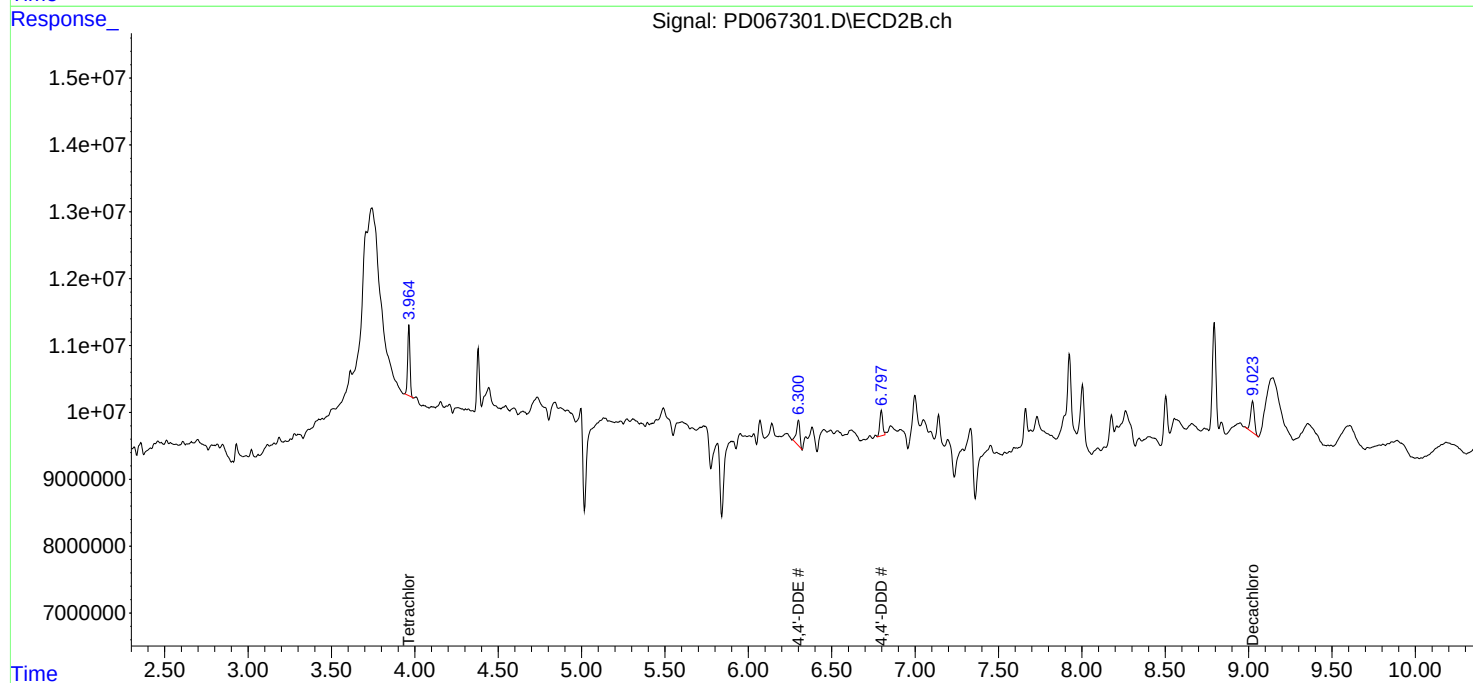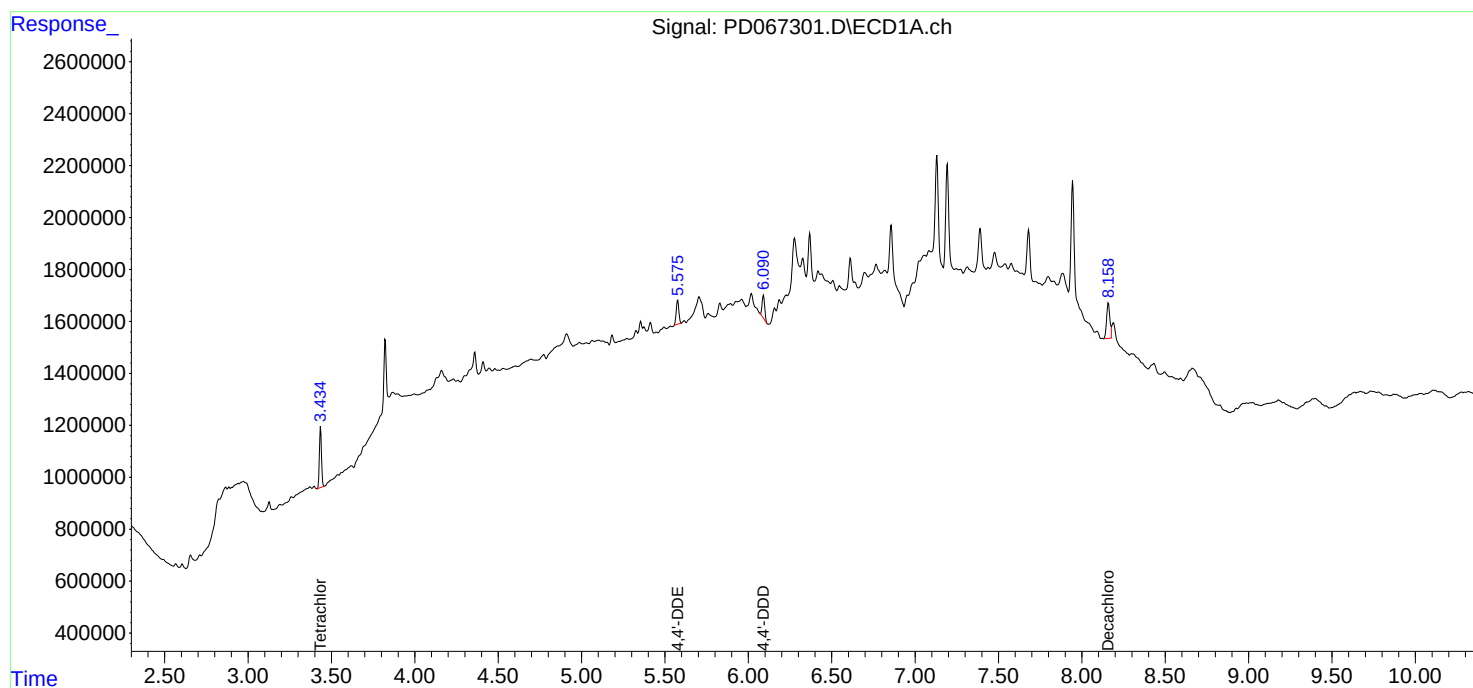


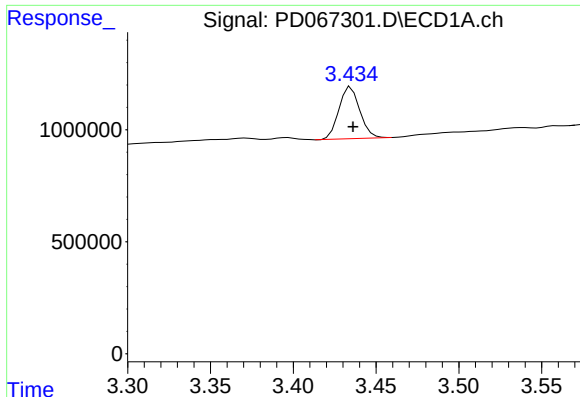

#1 Tetrachloro-m-xylene


R.T.: 3.435 min
Delta R.T.: 0.000 min
Response: 2024087
Conc: 0.98 ng/ml

Instrument :
ECD_D
ClientSampleId :
P-3

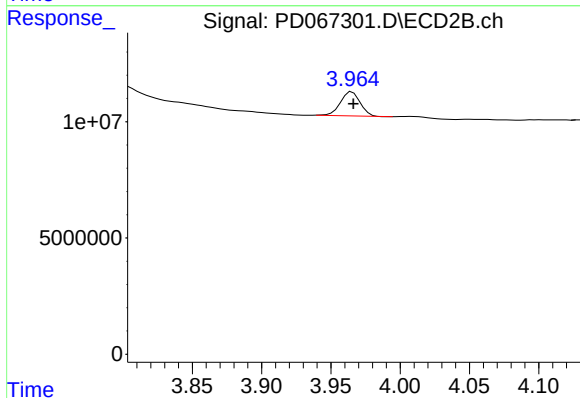


#1 Tetrachloro-m-xylene

R.T.: 3.965 min
Delta R.T.: -0.001 min
Response: 10336055
Conc: 1.42 ng/ml

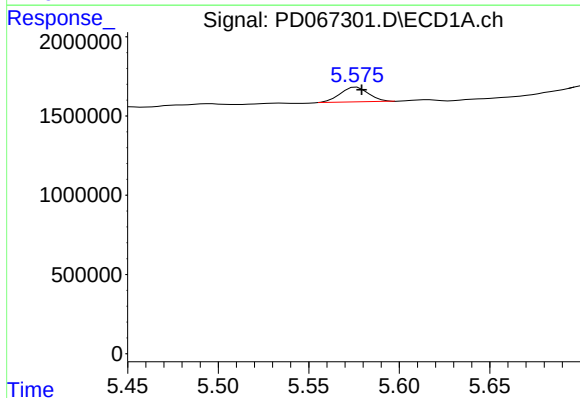


#12 4,4'-DDE

R.T.: 5.575 min
Delta R.T.: -0.004 min
Response: 1004997
Conc: 0.37 ng/ml m

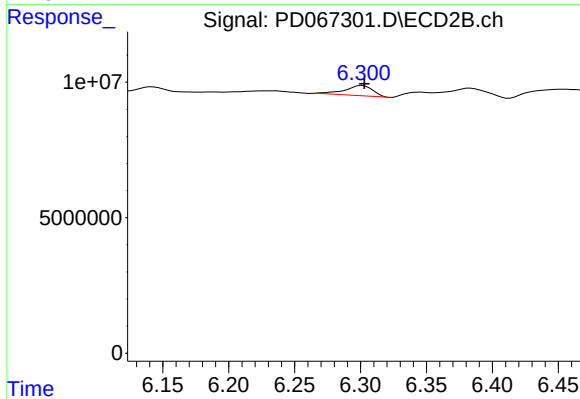

#12 4,4'-DDE


R.T.: 6.302 min
Delta R.T.: -0.001 min
Response: 5566373
Conc: 0.80 ng/ml

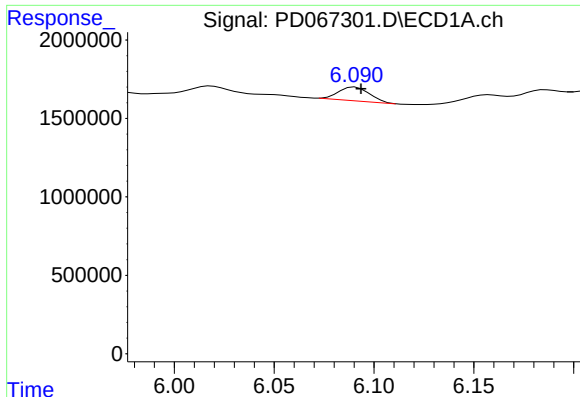

#16 4,4'-DDD


R.T.: 6.090 min
Delta R.T.: -0.004 min
Response: 935754
Conc: 0.45 ng/ml

Instrument :
ECD_D
ClientSampleId :
P-3

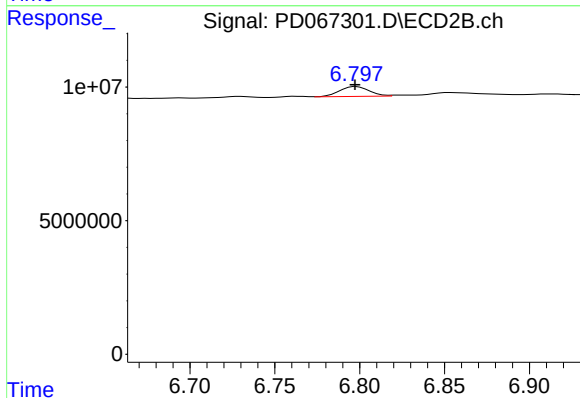


#16 4,4'-DDD

R.T.: 6.798 min
Delta R.T.: 0.000 min
Response: 4557190
Conc: 0.78 ng/ml

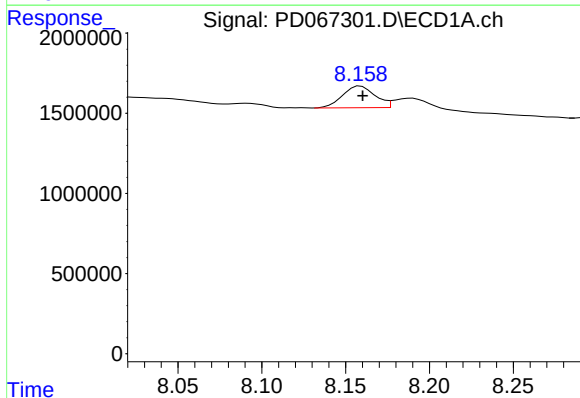

#28 Decachlorobiphenyl

R.T.: 8.158 min
Delta R.T.: -0.003 min
Response: 1931469
Conc: 1.70 ng/ml m

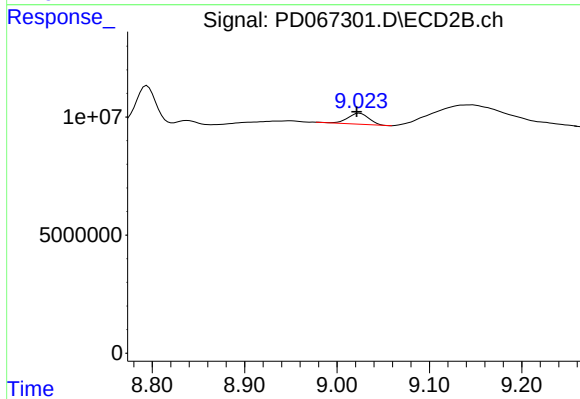

#28 Decachlorobiphenyl

R.T.: 9.025 min
Delta R.T.: 0.003 min
Response: 7353721
Conc: 1.46 ng/ml