

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121421\
 Data File : PD067307.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Dec 2021 15:20
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 04:40:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121421.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 15 04:06:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.435	3.965	41185644	207.1E6	22.512	23.468
28)	SA Decachlor...	8.154	9.020	20778434	97366720	22.539	21.904
Target Compounds							
9)	A Endosulfan I	5.466	6.191	23967804	77342705	10.473	11.236
10)	B gamma-Chl...	5.353	6.068	26721565	81744429	10.486	11.234
12)	B 4,4'-DDE	5.575	6.300	46774782	144.5E6	20.374	21.527
13)	MA Dieldrin	5.707	6.450	51123949	152.6E6	20.893	21.613
19)	B Endosulfa...	6.617	7.231	34397863	108.0E6	19.456	19.774
20)	A Methoxychlor	6.875	7.555	88210536	260.0E6	91.159	89.251
21)	B Endrin ke...	7.109	7.704	39116332	127.7E6	20.813	20.662



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121421\
Data File : PD067307.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Dec 2021 15:20
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 04:40:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121421.M
Quant Title : GC Extractables
QLast Update : Wed Dec 15 04:06:22 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

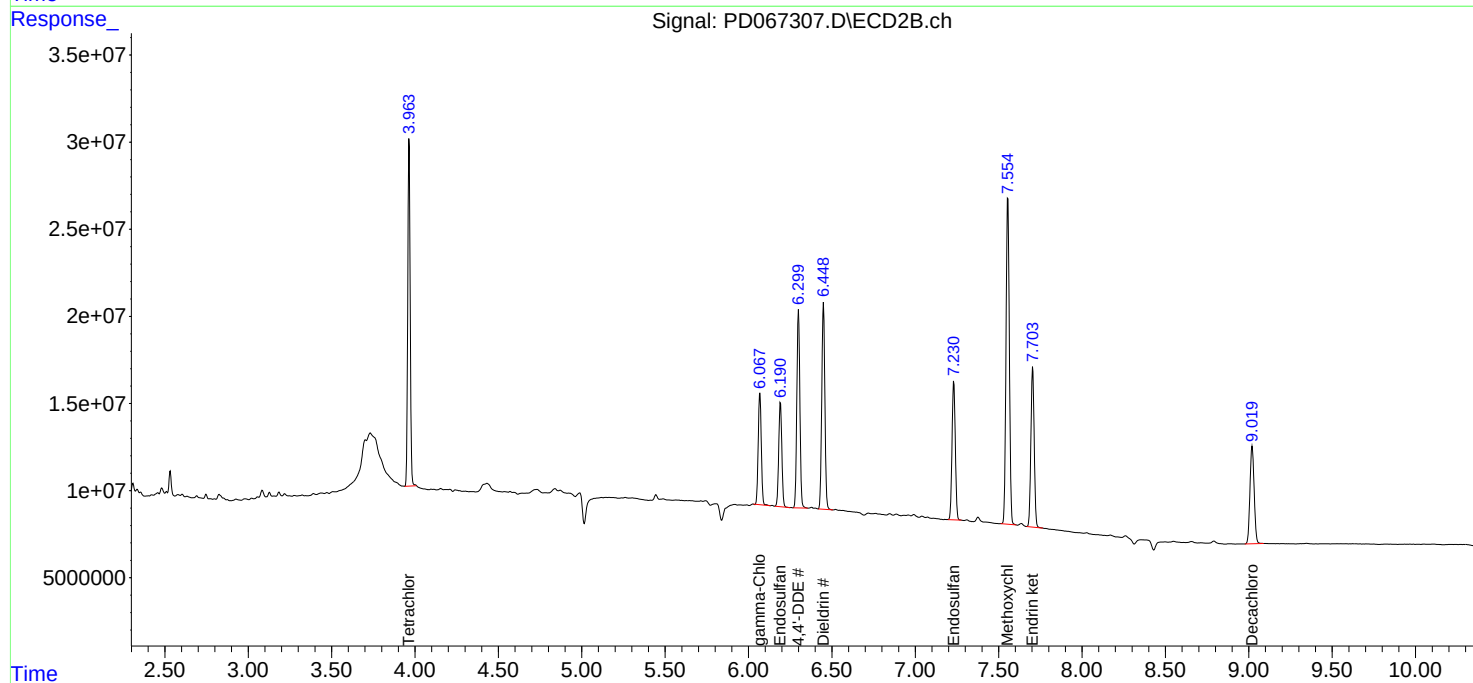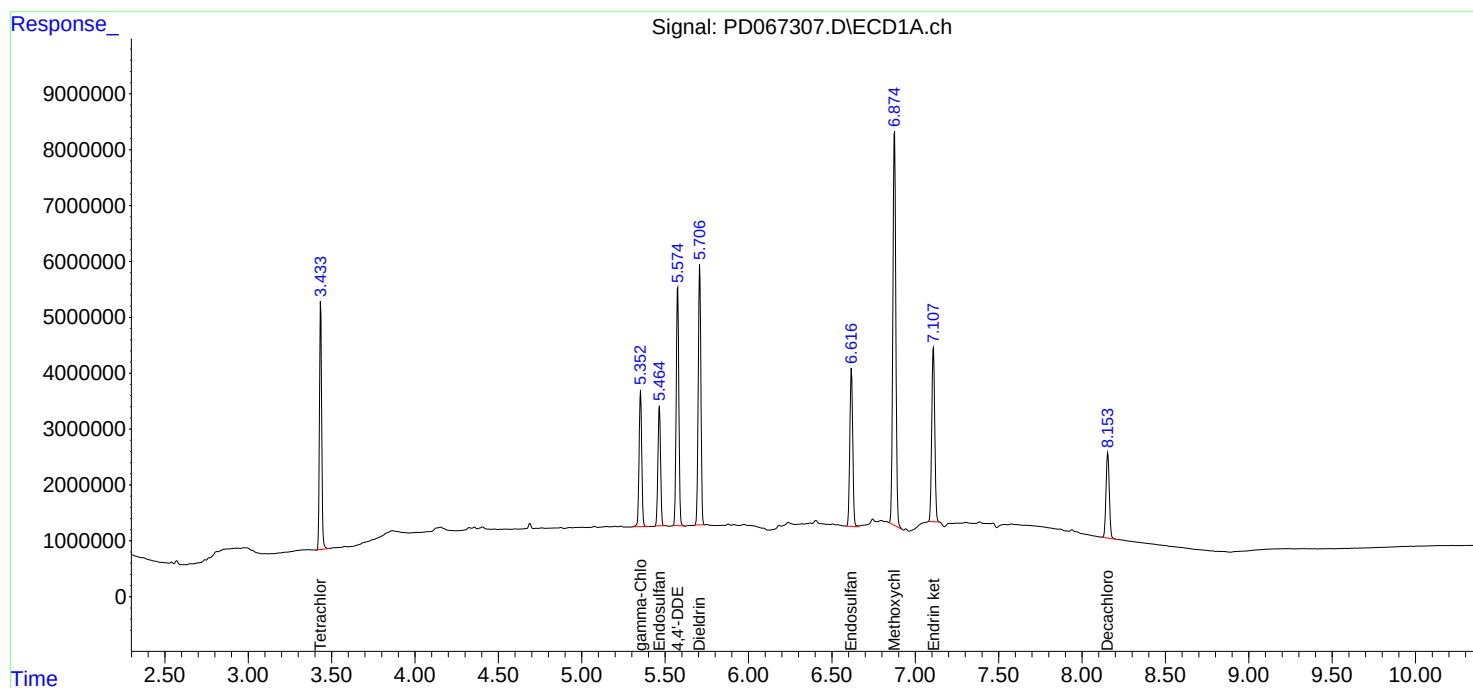


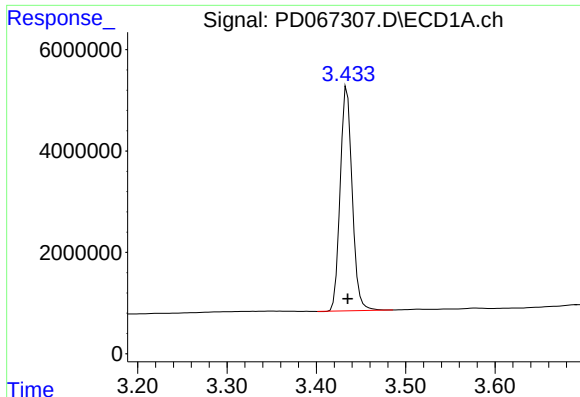

#1 Tetrachloro-m-xylene


R.T.: 3.435 min
Delta R.T.: 0.000 min
Response: 41185644
Conc: 22.51 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

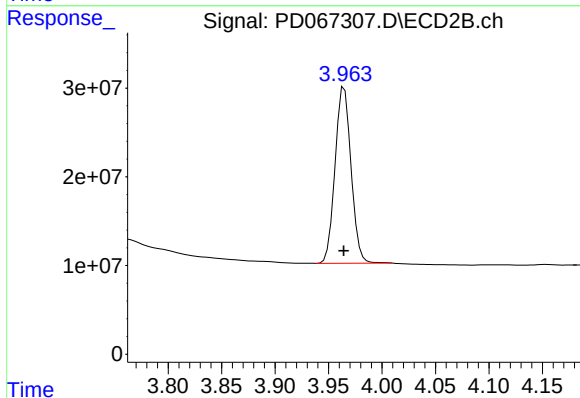


#1 Tetrachloro-m-xylene

R.T.: 3.965 min
Delta R.T.: 0.000 min
Response: 207066747
Conc: 23.47 ng/ml

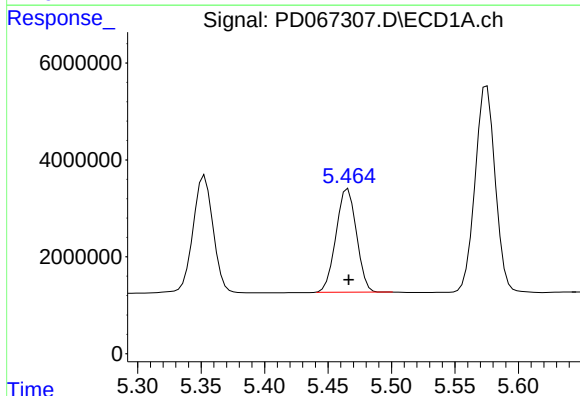


#9 Endosulfan I

R.T.: 5.466 min
Delta R.T.: 0.000 min
Response: 23967804
Conc: 10.47 ng/ml

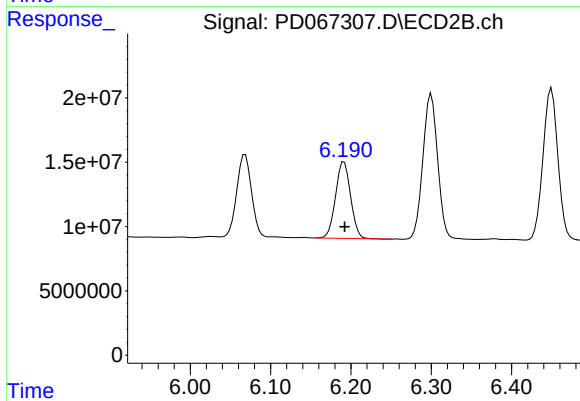

#9 Endosulfan I


R.T.: 6.191 min
Delta R.T.: 0.000 min
Response: 77342705
Conc: 11.24 ng/ml

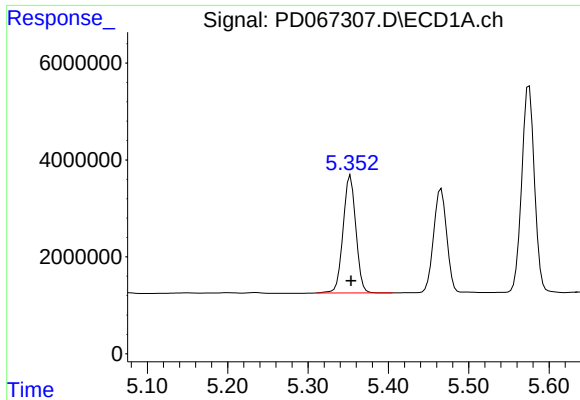

#10 gamma-Chlordane


R.T.: 5.353 min
Delta R.T.: 0.000 min
Response: 26721565
Conc: 10.49 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

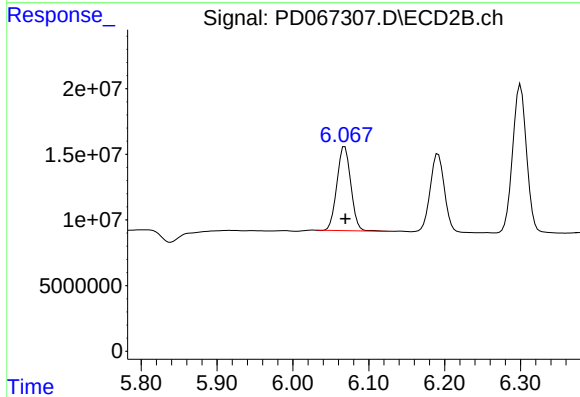


#10 gamma-Chlordane

R.T.: 6.068 min
Delta R.T.: 0.000 min
Response: 81744429
Conc: 11.23 ng/ml

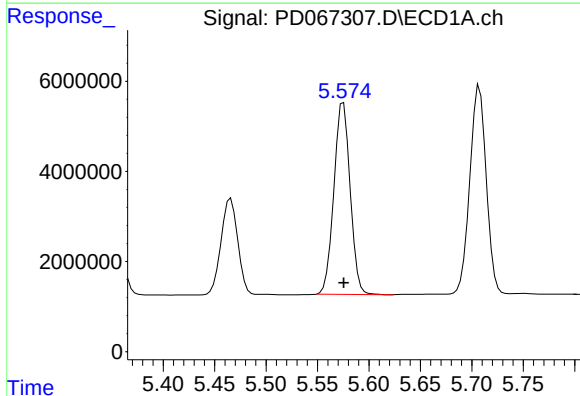


#12 4,4'-DDE

R.T.: 5.575 min
Delta R.T.: 0.000 min
Response: 46774782
Conc: 20.37 ng/ml

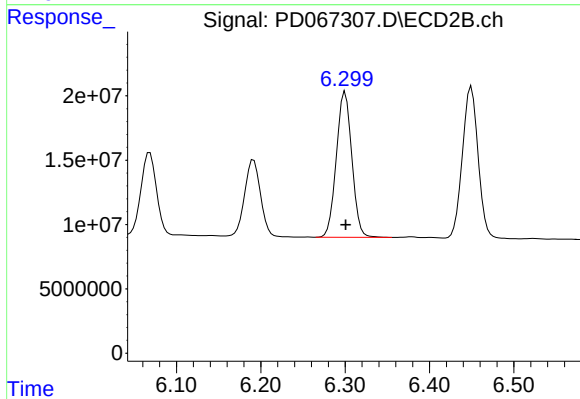

#12 4,4'-DDE


R.T.: 6.300 min
Delta R.T.: 0.000 min
Response: 144534485
Conc: 21.53 ng/ml

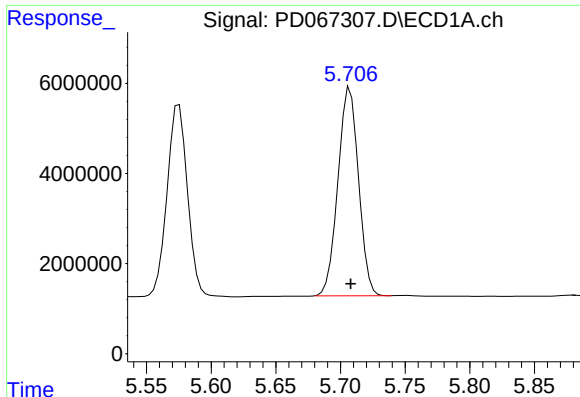

#13 Dieldrin


R.T.: 5.707 min
Delta R.T.: 0.000 min
Response: 51123949
Conc: 20.89 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

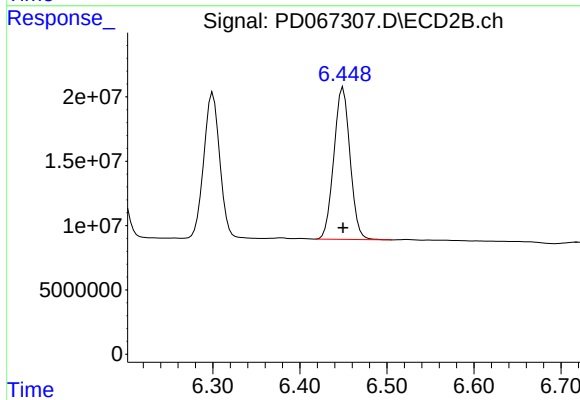


#13 Dieldrin

R.T.: 6.450 min
Delta R.T.: 0.000 min
Response: 152641836
Conc: 21.61 ng/ml

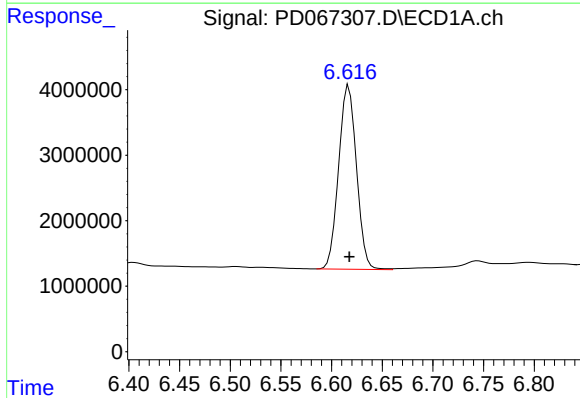


#19 Endosulfan Sulfate

R.T.: 6.617 min
Delta R.T.: 0.000 min
Response: 34397863
Conc: 19.46 ng/ml

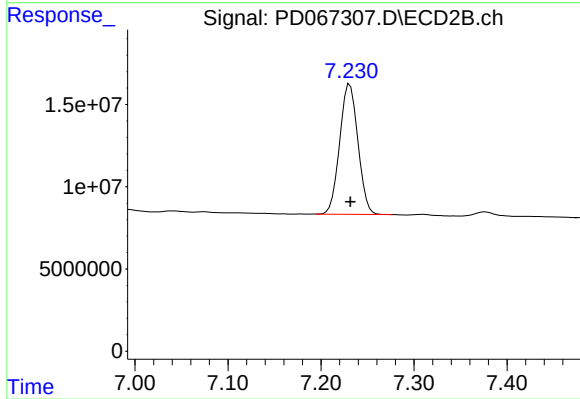

#19 Endosulfan Sulfate


R.T.: 7.231 min
Delta R.T.: 0.000 min
Response: 107958120
Conc: 19.77 ng/ml

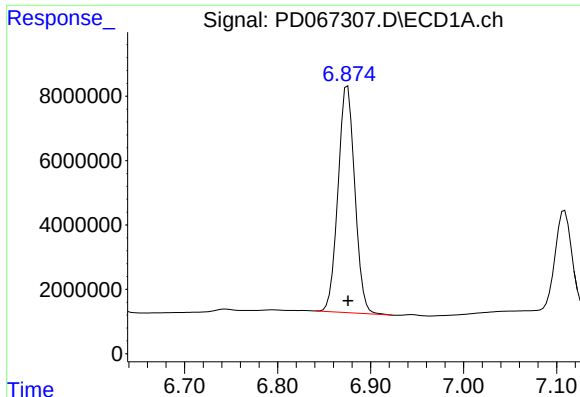

#20 Methoxychlor


R.T.: 6.875 min
Delta R.T.: 0.000 min
Response: 88210536
Conc: 91.16 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

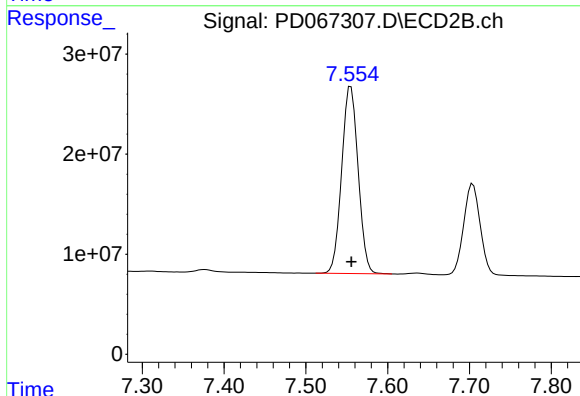


#20 Methoxychlor

R.T.: 7.555 min
Delta R.T.: 0.000 min
Response: 260025487
Conc: 89.25 ng/ml

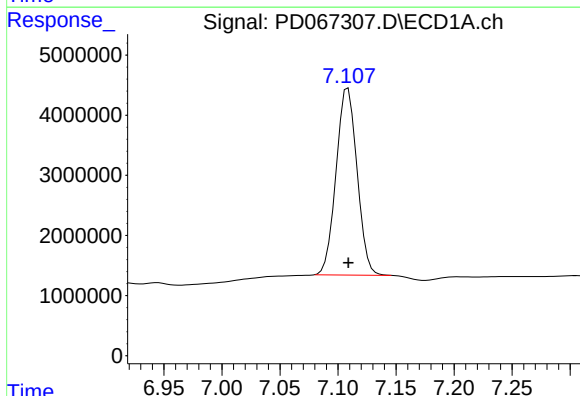


#21 Endrin ketone

R.T.: 7.109 min
Delta R.T.: 0.000 min
Response: 39116332
Conc: 20.81 ng/ml

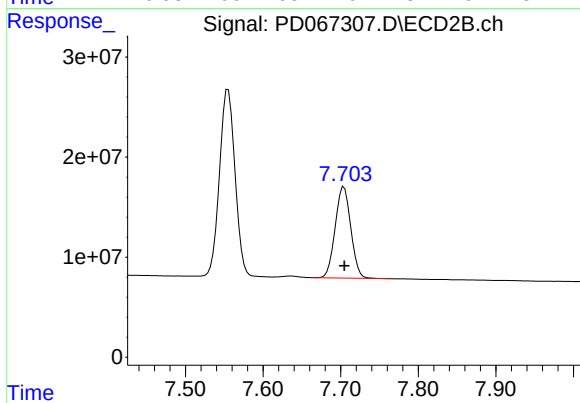

#21 Endrin ketone


R.T.: 7.704 min
Delta R.T.: 0.000 min
Response: 127668850
Conc: 20.66 ng/ml

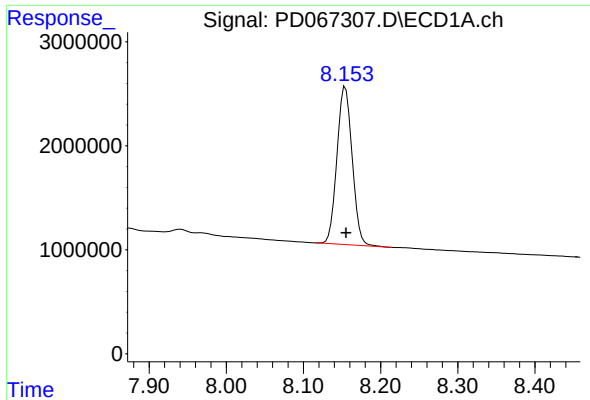

#28 Decachlorobiphenyl

R.T.: 8.154 min
Delta R.T.: 0.000 min
Response: 20778434
Conc: 22.54 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

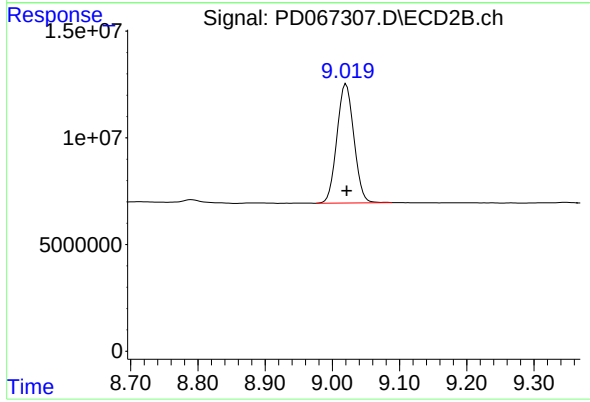

#28 Decachlorobiphenyl

R.T.: 9.020 min
Delta R.T.: 0.000 min
Response: 97366720
Conc: 21.90 ng/ml