

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121421\
 Data File : PD067313.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Dec 2021 18:12
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 04:04:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121421.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 15 04:04:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.434	3.964	108.5E6	429.1E6	50.000	50.000
28)	SA Decachlor...	8.156	9.019	44313928	216.1E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.296	4.953	35564035	144.0E6	500.000	500.000
24)	Chlordane-2	4.792	5.421	41936605	135.4E6	500.000	500.000
25)	Chlordane-3	5.355	6.068	121.0E6	454.2E6	500.000	500.000
26)	Chlordane-4	5.412	6.140	96412848	530.1E6	500.000	500.000
27)	Chlordane-5	6.246	6.949	40090639	102.5E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121421\
Data File : PD067313.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Dec 2021 18:12
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 04:04:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121421.M
Quant Title : GC Extractables
QLast Update : Wed Dec 15 04:04:22 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

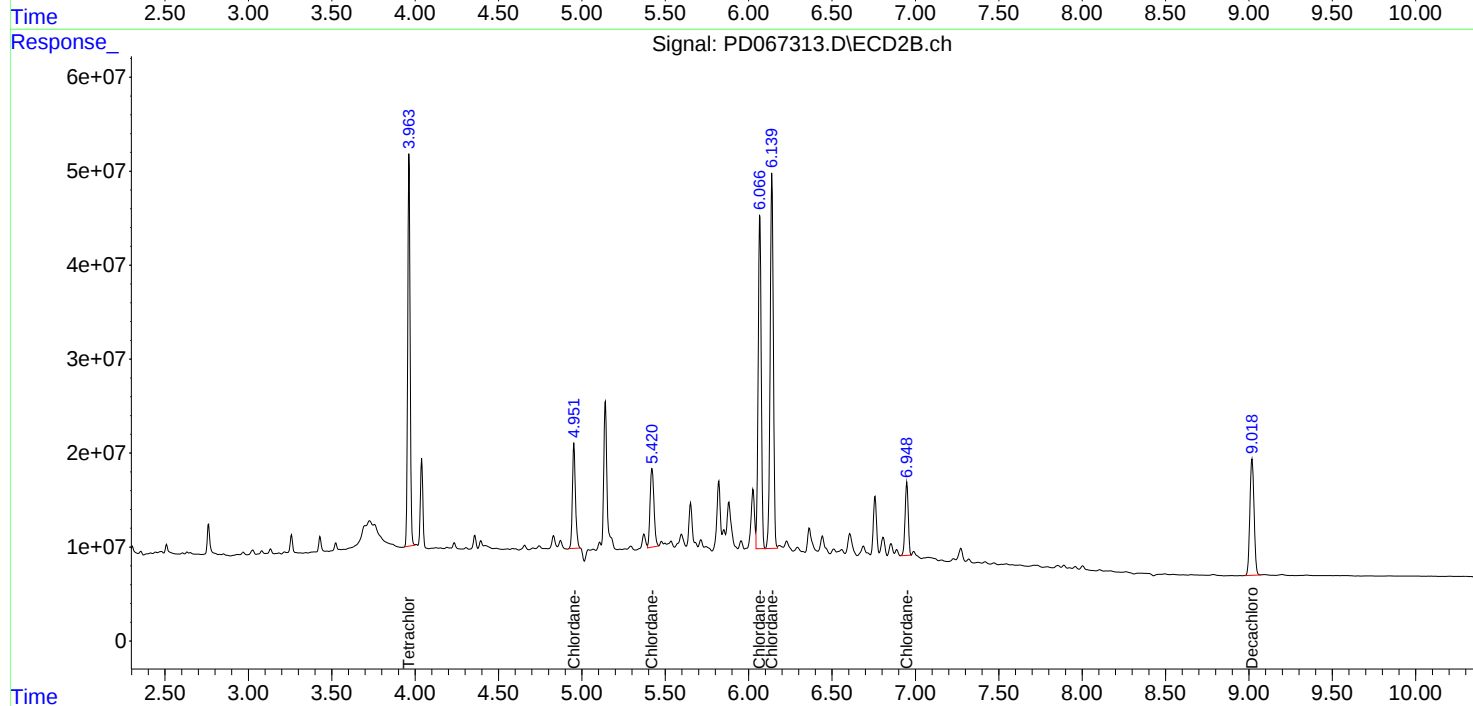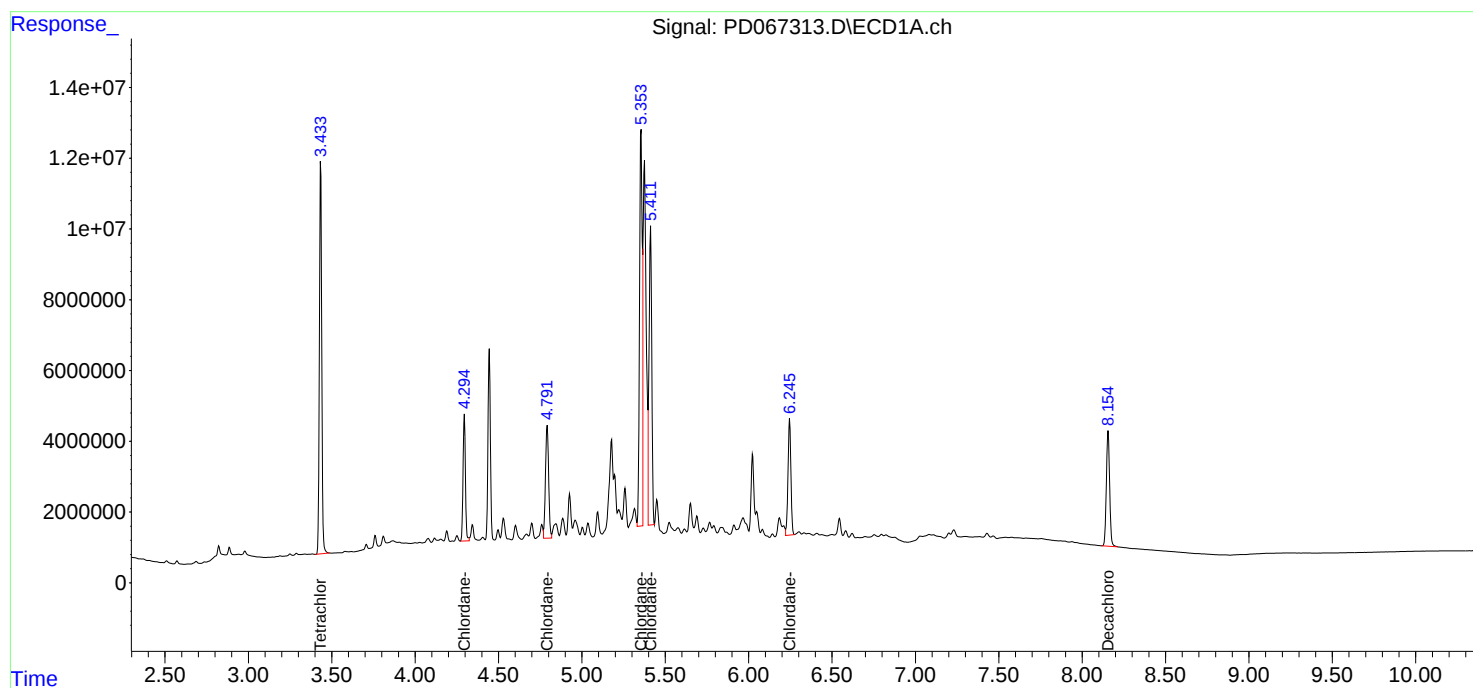


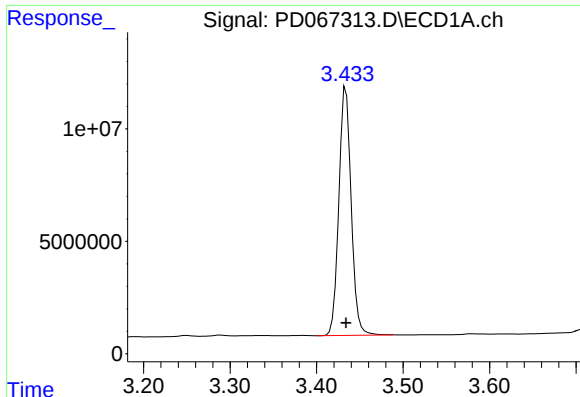

#1 Tetrachloro-m-xylene


R.T.: 3.434 min
Delta R.T.: 0.000 min
Response: 108530034
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

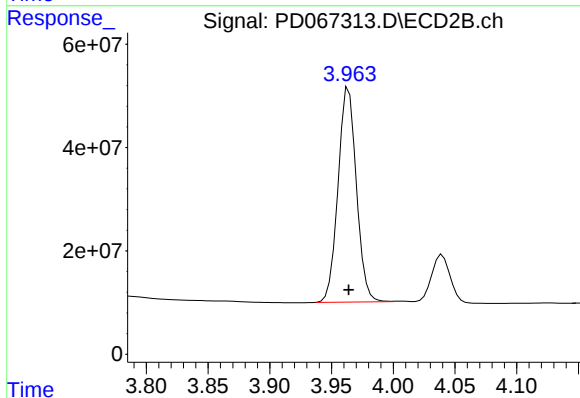


#1 Tetrachloro-m-xylene

R.T.: 3.964 min
Delta R.T.: 0.000 min
Response: 429099435
Conc: 50.00 ng/ml

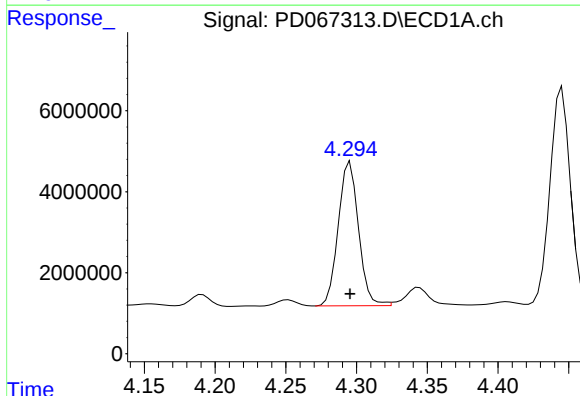


#23 Chlordane-1

R.T.: 4.296 min
Delta R.T.: 0.000 min
Response: 35564035
Conc: 500.00 ng/ml

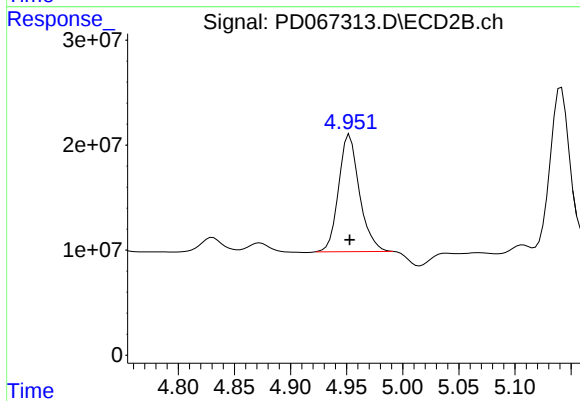

#23 Chlordane-1


R.T.: 4.953 min
Delta R.T.: 0.000 min
Response: 143969611
Conc: 500.00 ng/ml

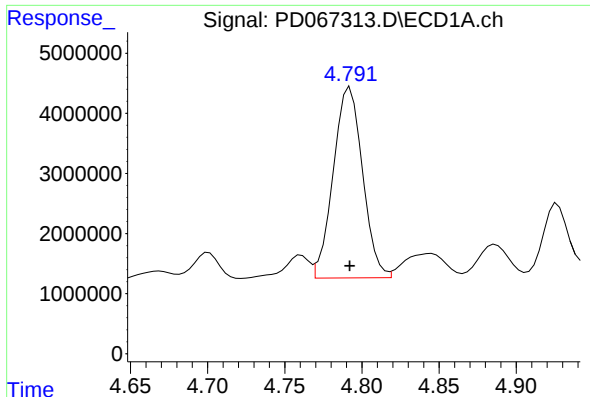

#24 Chlordane-2


R.T.: 4.792 min
Delta R.T.: 0.000 min
Response: 41936605
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

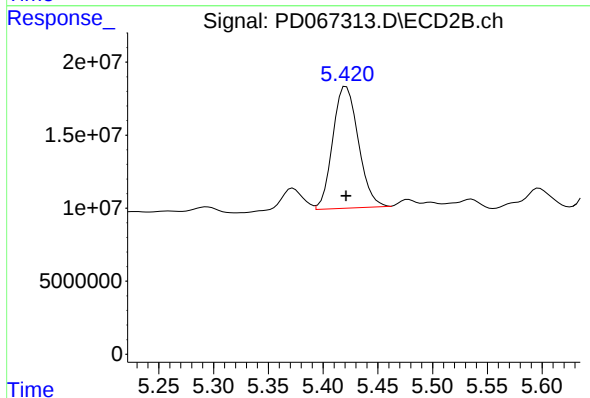


#24 Chlordane-2

R.T.: 5.421 min
Delta R.T.: 0.000 min
Response: 135357084
Conc: 500.00 ng/ml

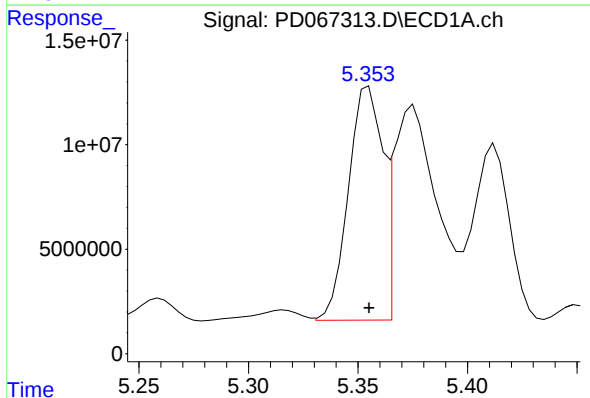


#25 Chlordane-3

R.T.: 5.355 min
Delta R.T.: 0.000 min
Response: 120993436
Conc: 500.00 ng/ml

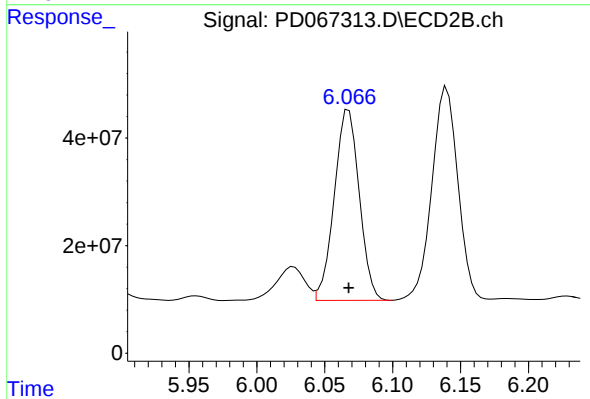

#25 Chlordane-3


R.T.: 6.068 min
Delta R.T.: 0.000 min
Response: 454187492
Conc: 500.00 ng/ml

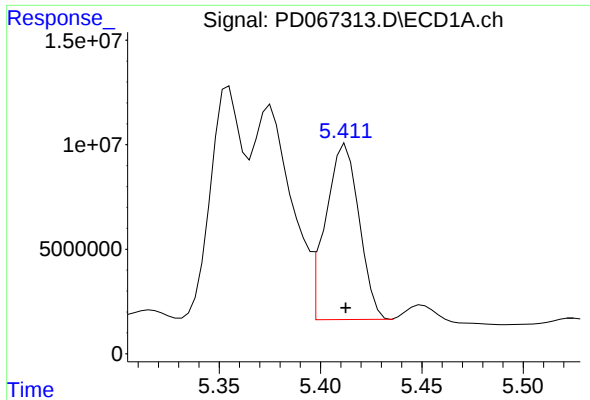

#26 Chlordane-4


R.T.: 5.412 min
Delta R.T.: 0.000 min
Response: 96412848
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

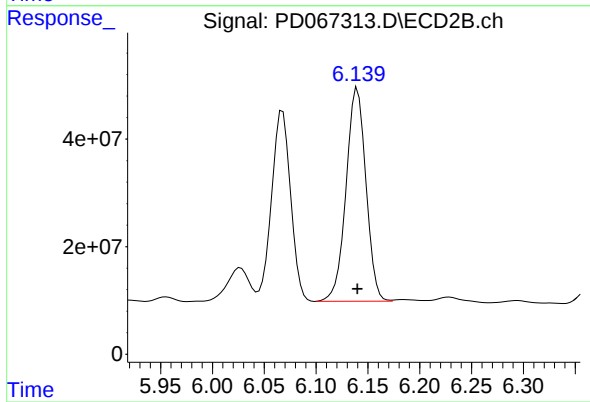


#26 Chlordane-4

R.T.: 6.140 min
Delta R.T.: 0.000 min
Response: 530132901
Conc: 500.00 ng/ml

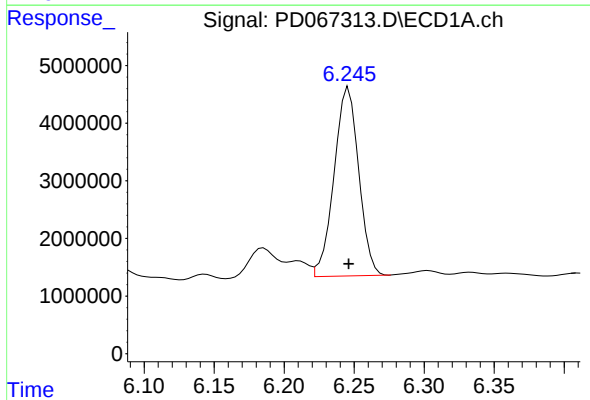


#27 Chlordane-5

R.T.: 6.246 min
Delta R.T.: 0.000 min
Response: 40090639
Conc: 500.00 ng/ml

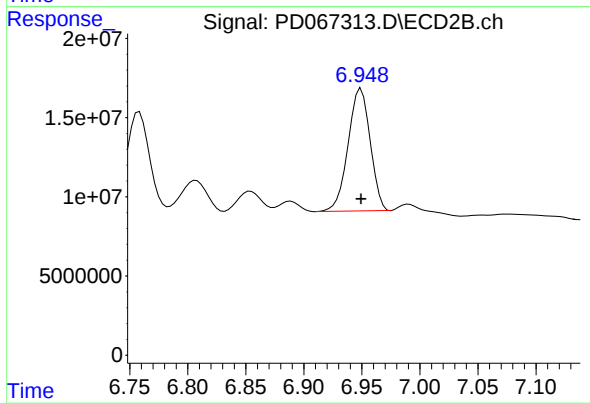

#27 Chlordane-5


R.T.: 6.949 min
Delta R.T.: 0.000 min
Response: 102483691
Conc: 500.00 ng/ml

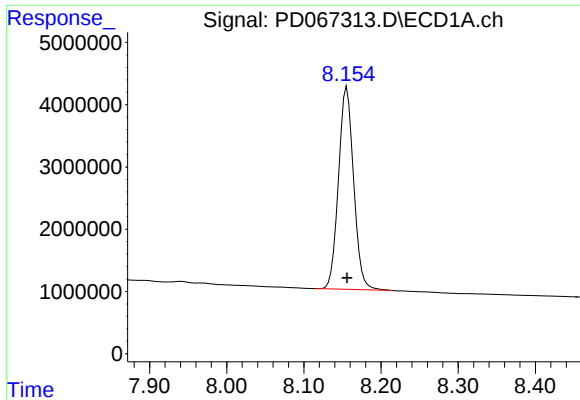

#28 Decachlorobiphenyl

R.T.: 8.156 min
Delta R.T.: 0.000 min
Response: 44313928
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

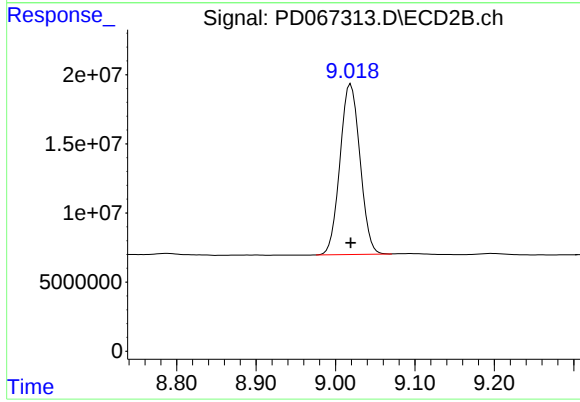

#28 Decachlorobiphenyl

R.T.: 9.019 min
Delta R.T.: 0.000 min
Response: 216079090
Conc: 50.00 ng/ml