

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121422\
 Data File : PD073315.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Dec 2022 16:40
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 05:01:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 15 04:59:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.695	3.456	11245748	362.2E6	5.356	5.901
27)	SA Decachlor...	7.822	8.907	27794947	167.6E6	10.762	10.496
Target Compounds							
2)	A alpha-BHC	3.197	3.919	15534899	494.3E6	4.705	6.013 #
3)	MA gamma-BHC...	3.527	4.253	13769480	413.2E6	4.670	6.218 #
4)	MA Heptachlor	3.859	4.819	16003238	287.5E6	4.943	5.999
9)	A Endosulfan I	5.011	5.974	13572553	181.0E6	4.998	5.464
13)	MA Dieldrin	5.277	6.252	28586252	372.3E6	9.505	10.703
14)	MA Endrin	5.554	6.483	25525902	310.6E6	9.401	10.793
16)	A 4,4'-DDD	5.700	6.617	22404161	275.7E6	9.311	10.583
17)	MA 4,4'-DDT	5.949	6.925	21471582	250.6E6	8.864	10.115
20)	A Methoxychlor	6.532	7.405	68273110	577.9E6	49.434	54.093

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121422\
Data File : PD073315.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Dec 2022 16:40
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 05:01:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Dec 15 04:59:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

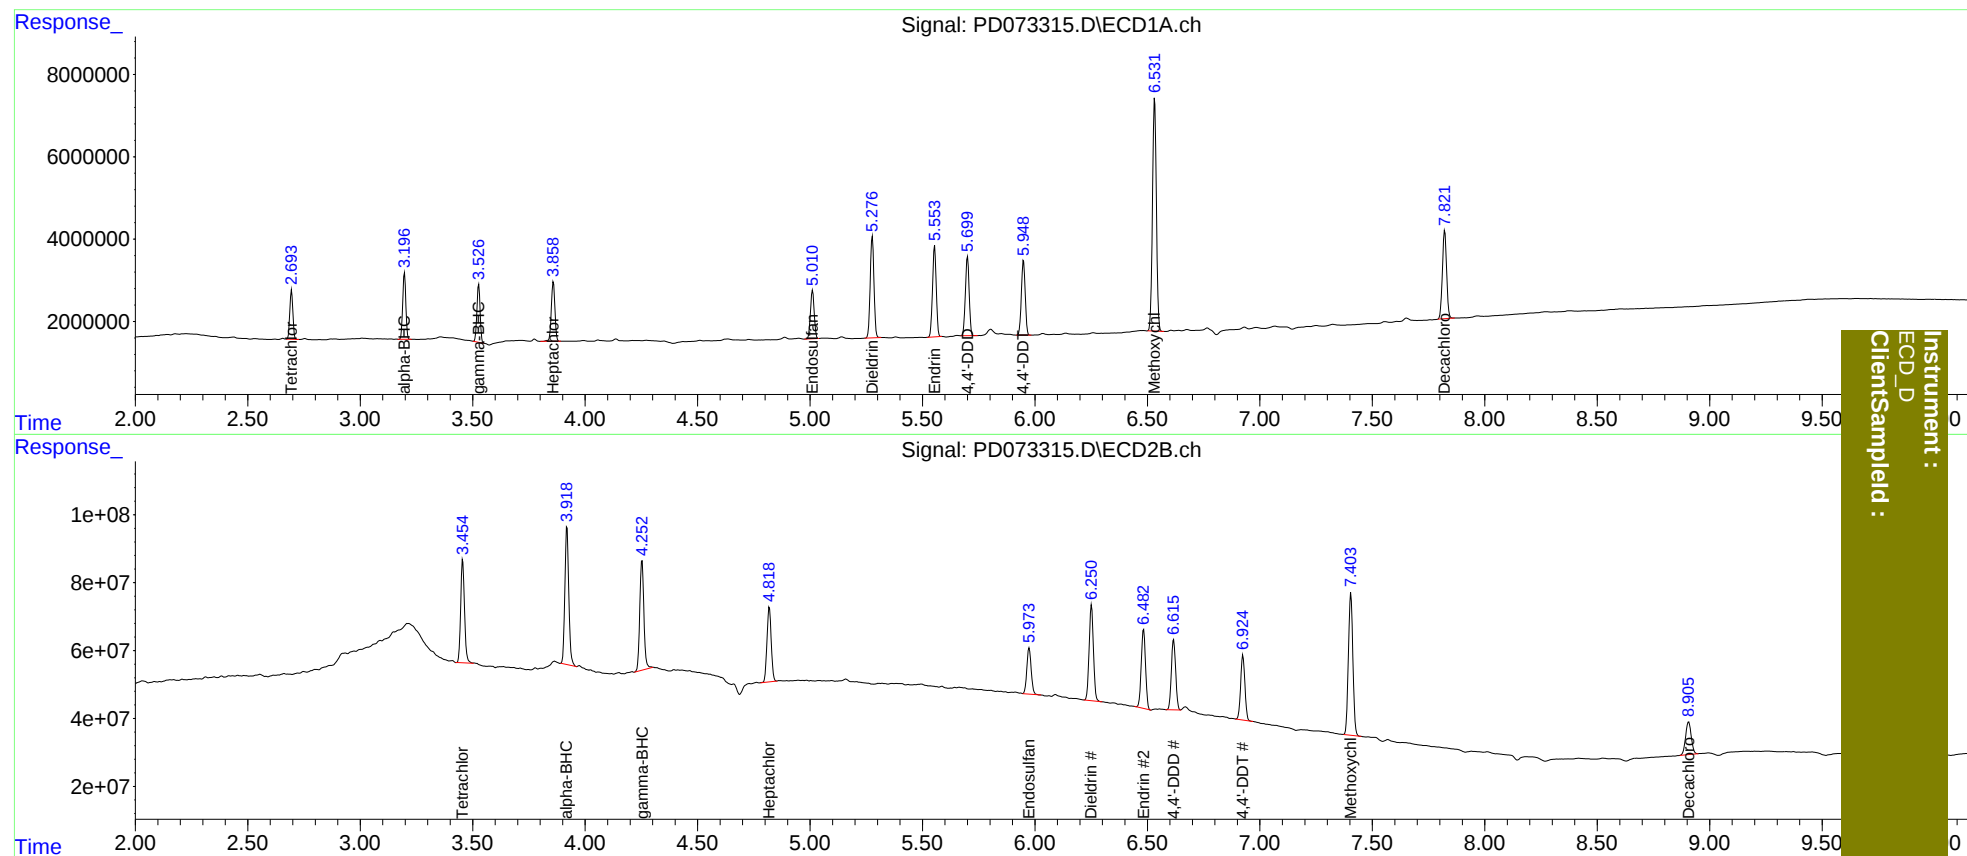


Instrument :
ECD_D
ClientSampled :
0

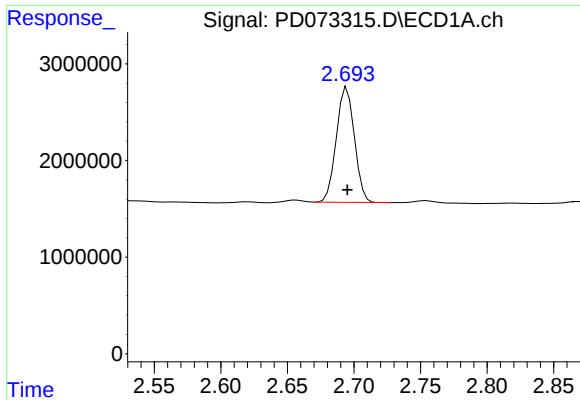

#1 Tetrachloro-m-xylene


R.T.: 2.695 min
Delta R.T.: 0.000 min
Response: 11245748
Conc: 5.36 ng/ml

Instrument :
ECD_D
ClientSampleId :

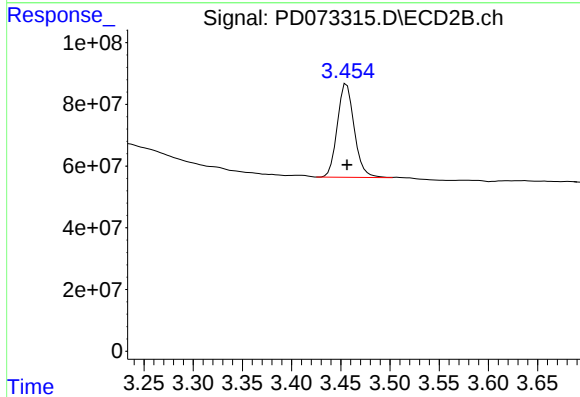


#1 Tetrachloro-m-xylene

R.T.: 3.456 min
Delta R.T.: 0.000 min
Response: 362190933
Conc: 5.90 ng/ml

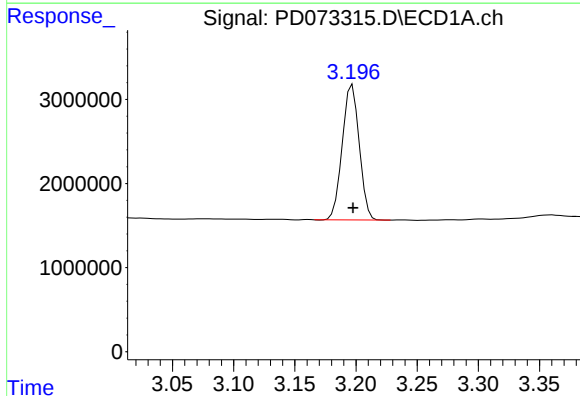


#2 alpha-BHC

R.T.: 3.197 min
Delta R.T.: 0.000 min
Response: 15534899
Conc: 4.71 ng/ml

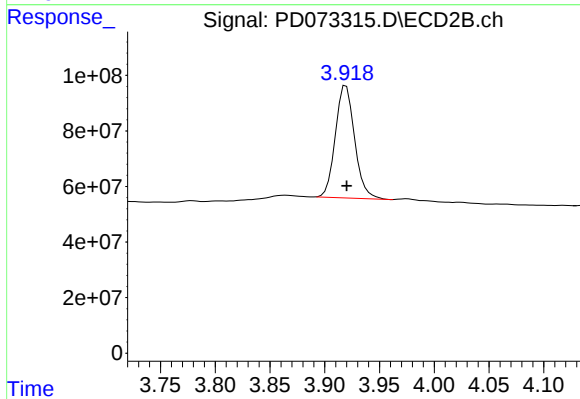

#2 alpha-BHC


R.T.: 3.919 min
Delta R.T.: 0.000 min
Response: 494275730
Conc: 6.01 ng/ml

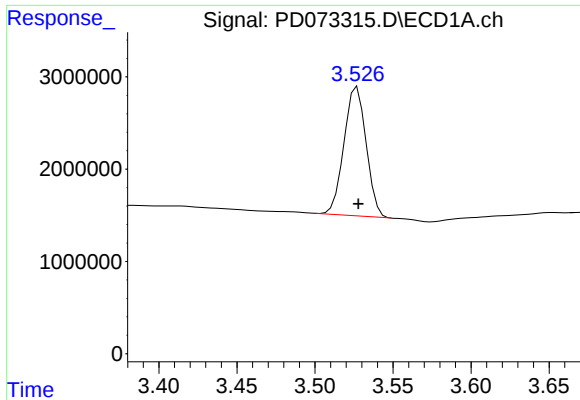

#3 gamma-BHC (Lindane)


R.T.: 3.527 min
Delta R.T.: 0.000 min
Response: 13769480
Conc: 4.67 ng/ml

Instrument :
ECD_D
ClientSampleId :

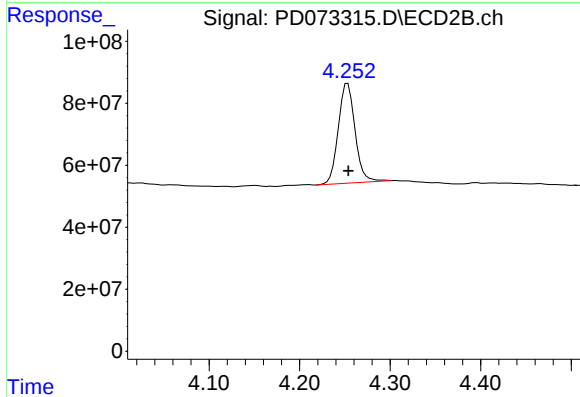


#3 gamma-BHC (Lindane)

R.T.: 4.253 min
Delta R.T.: 0.000 min
Response: 413157331
Conc: 6.22 ng/ml

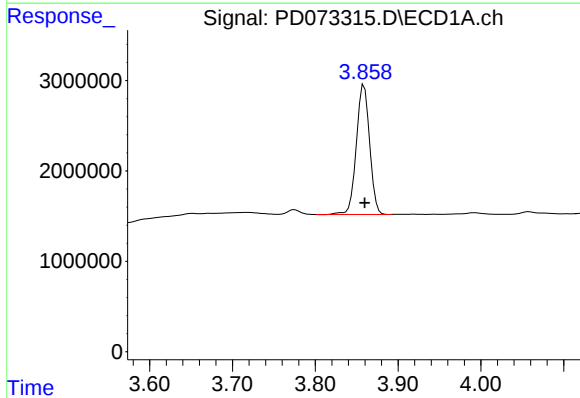


#4 Heptachlor

R.T.: 3.859 min
Delta R.T.: 0.000 min
Response: 16003238
Conc: 4.94 ng/ml

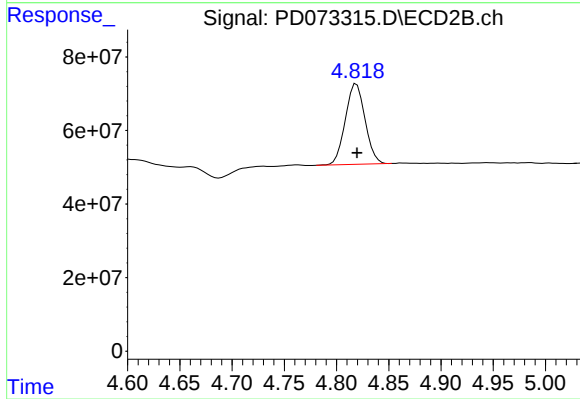

#4 Heptachlor


R.T.: 4.819 min
Delta R.T.: 0.000 min
Response: 287499825
Conc: 6.00 ng/ml

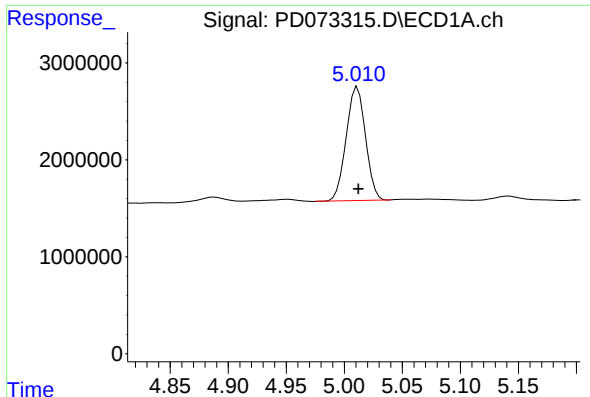

#9 Endosulfan I


R.T.: 5.011 min
Delta R.T.: 0.000 min
Response: 13572553
Conc: 5.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

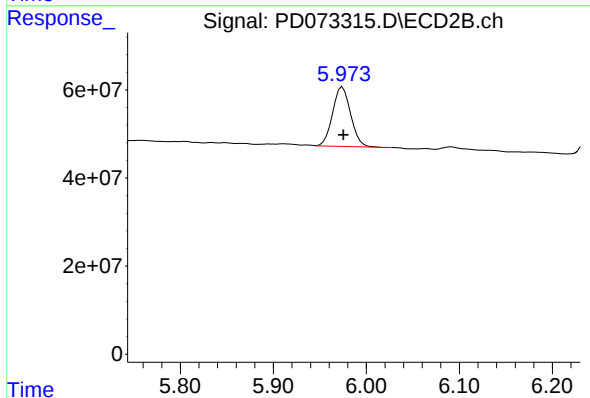


#9 Endosulfan I

R.T.: 5.974 min
Delta R.T.: 0.000 min
Response: 180978678
Conc: 5.46 ng/ml

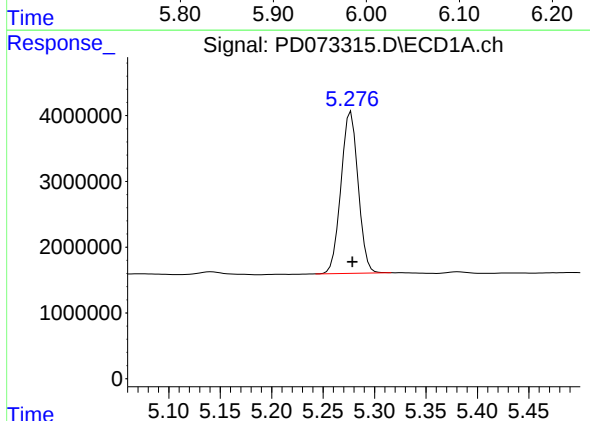


#13 Dieldrin

R.T.: 5.277 min
Delta R.T.: -0.001 min
Response: 28586252
Conc: 9.51 ng/ml

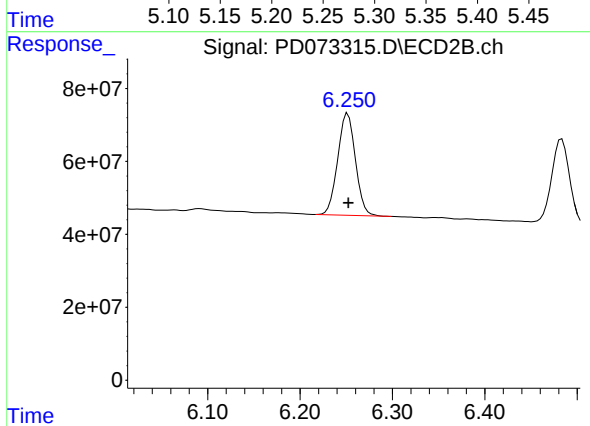

#13 Dieldrin


R.T.: 6.252 min
Delta R.T.: 0.000 min
Response: 372280192
Conc: 10.70 ng/ml

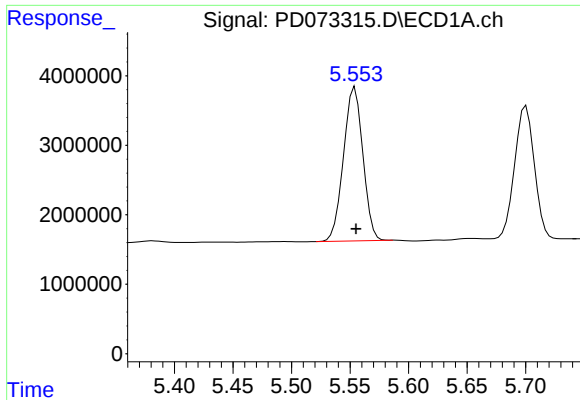

#14 Endrin


R.T.: 5.554 min
Delta R.T.: -0.001 min
Response: 25525902
Conc: 9.40 ng/ml

Instrument :
ECD_D
ClientSampleId :

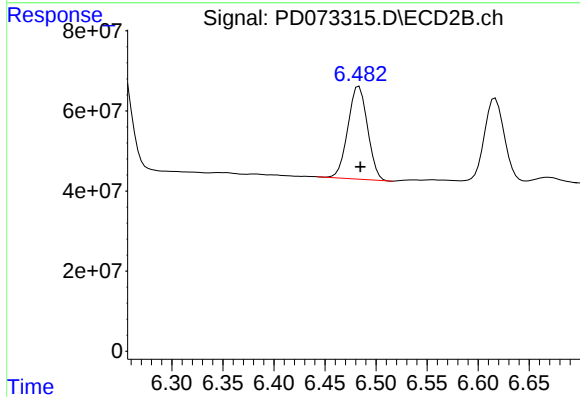


#14 Endrin

R.T.: 6.483 min
Delta R.T.: -0.001 min
Response: 310648378
Conc: 10.79 ng/ml

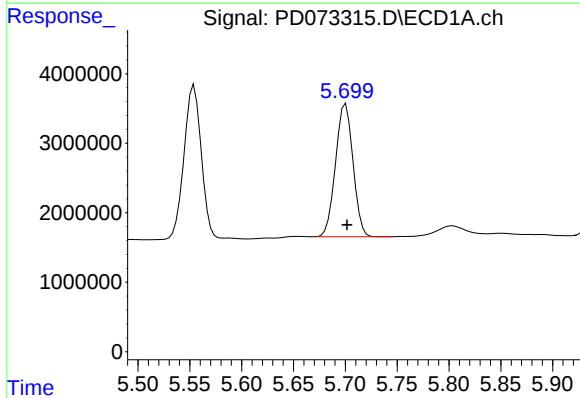


#16 4,4'-DDD

R.T.: 5.700 min
Delta R.T.: -0.001 min
Response: 22404161
Conc: 9.31 ng/ml

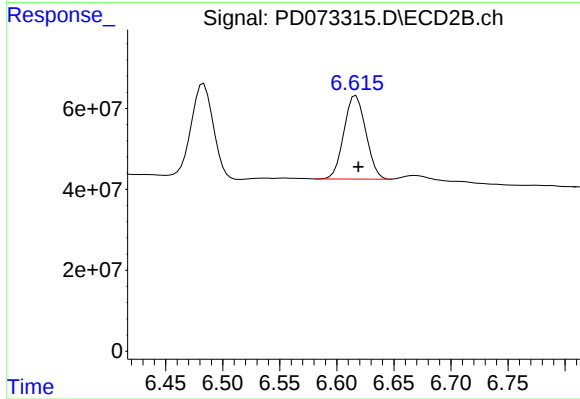

#16 4,4'-DDD


R.T.: 6.617 min
Delta R.T.: -0.002 min
Response: 275740404
Conc: 10.58 ng/ml

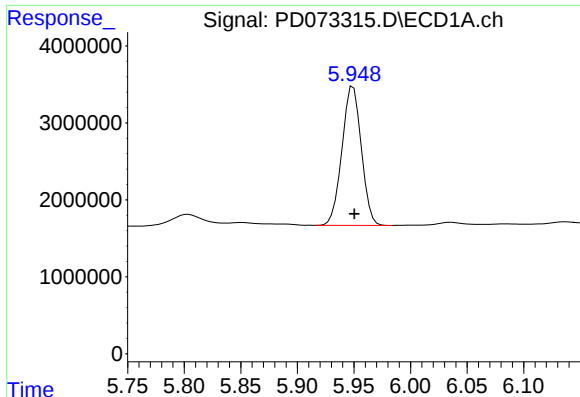

#17 4,4'-DDT


R.T.: 5.949 min
Delta R.T.: -0.001 min
Response: 21471582
Conc: 8.86 ng/ml

Instrument :
ECD_D
ClientSampleId :

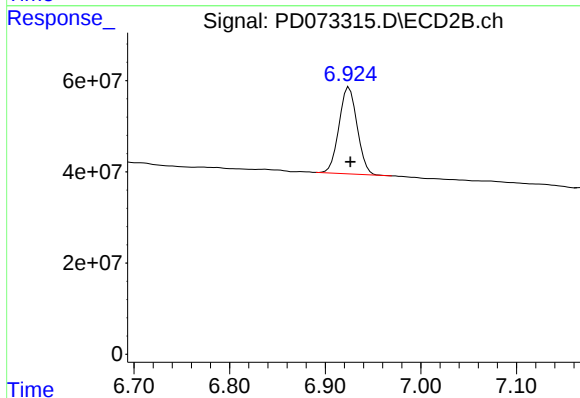


#17 4,4'-DDT

R.T.: 6.925 min
Delta R.T.: -0.001 min
Response: 250570394
Conc: 10.11 ng/ml

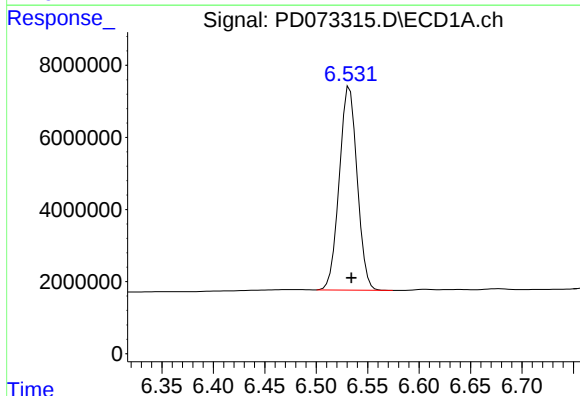


#20 Methoxychlor

R.T.: 6.532 min
Delta R.T.: -0.002 min
Response: 68273110
Conc: 49.43 ng/ml

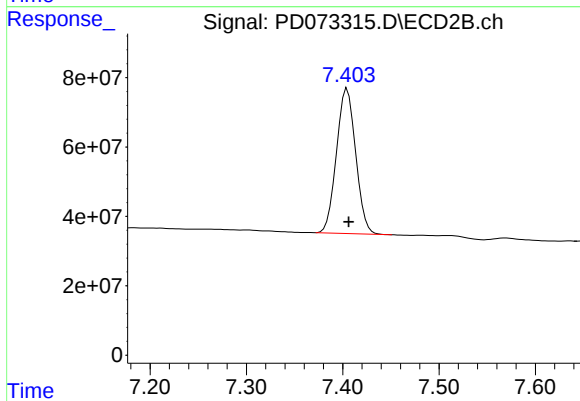

#20 Methoxychlor


R.T.: 7.405 min
Delta R.T.: -0.001 min
Response: 577944810
Conc: 54.09 ng/ml

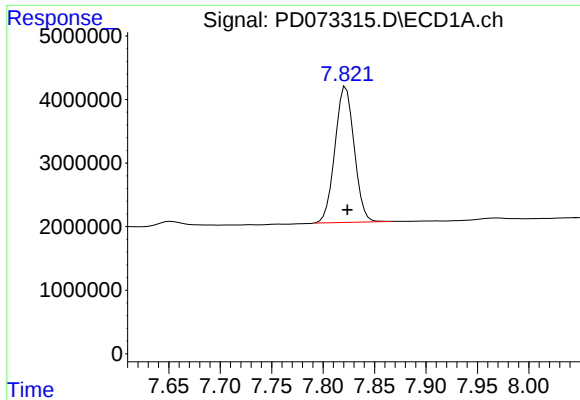

#27 Decachlorobiphenyl

R.T.: 7.822 min
Delta R.T.: -0.002 min
Response: 27794947
Conc: 10.76 ng/ml

Instrument :
ECD_D
ClientSampleId :

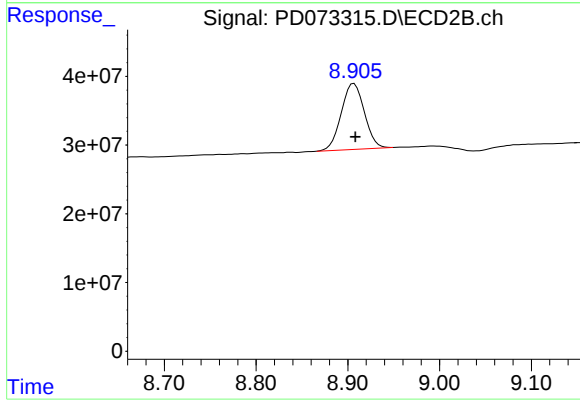

#27 Decachlorobiphenyl

R.T.: 8.907 min
Delta R.T.: -0.001 min
Response: 167555847
Conc: 10.50 ng/ml