

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121422\
 Data File : PD073317.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Dec 2022 17:06
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 05:01:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 15 04:59:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.695	3.456	22409184	690.5E6	10.674	11.251
27)	SA Decachlor...	7.822	8.907	54802746	339.3E6	21.220	21.254
Target Compounds							
2)	A alpha-BHC	3.198	3.919	32964412	938.4E6	9.984	11.416
3)	MA gamma-BHC...	3.528	4.253	29209426	770.2E6	9.907	11.591
4)	MA Heptachlor	3.860	4.819	33132904	545.7E6	10.233	11.386
9)	A Endosulfan I	5.012	5.974	28063784	360.2E6	10.335	10.874
13)	MA Dieldrin	5.278	6.251	60179434	746.2E6	20.011	21.455
14)	MA Endrin	5.555	6.483	53948201	613.0E6	19.868	21.297
16)	A 4,4'-DDD	5.701	6.617	47902780	552.1E6	19.909	21.188
17)	MA 4,4'-DDT	5.950	6.925	46861569	518.1E6	19.347	20.916
20)	A Methoxychlor	6.533	7.405	141.3E6	1141.2E6	102.324	106.809


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121422\
Data File : PD073317.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Dec 2022 17:06
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 05:01:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Dec 15 04:59:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

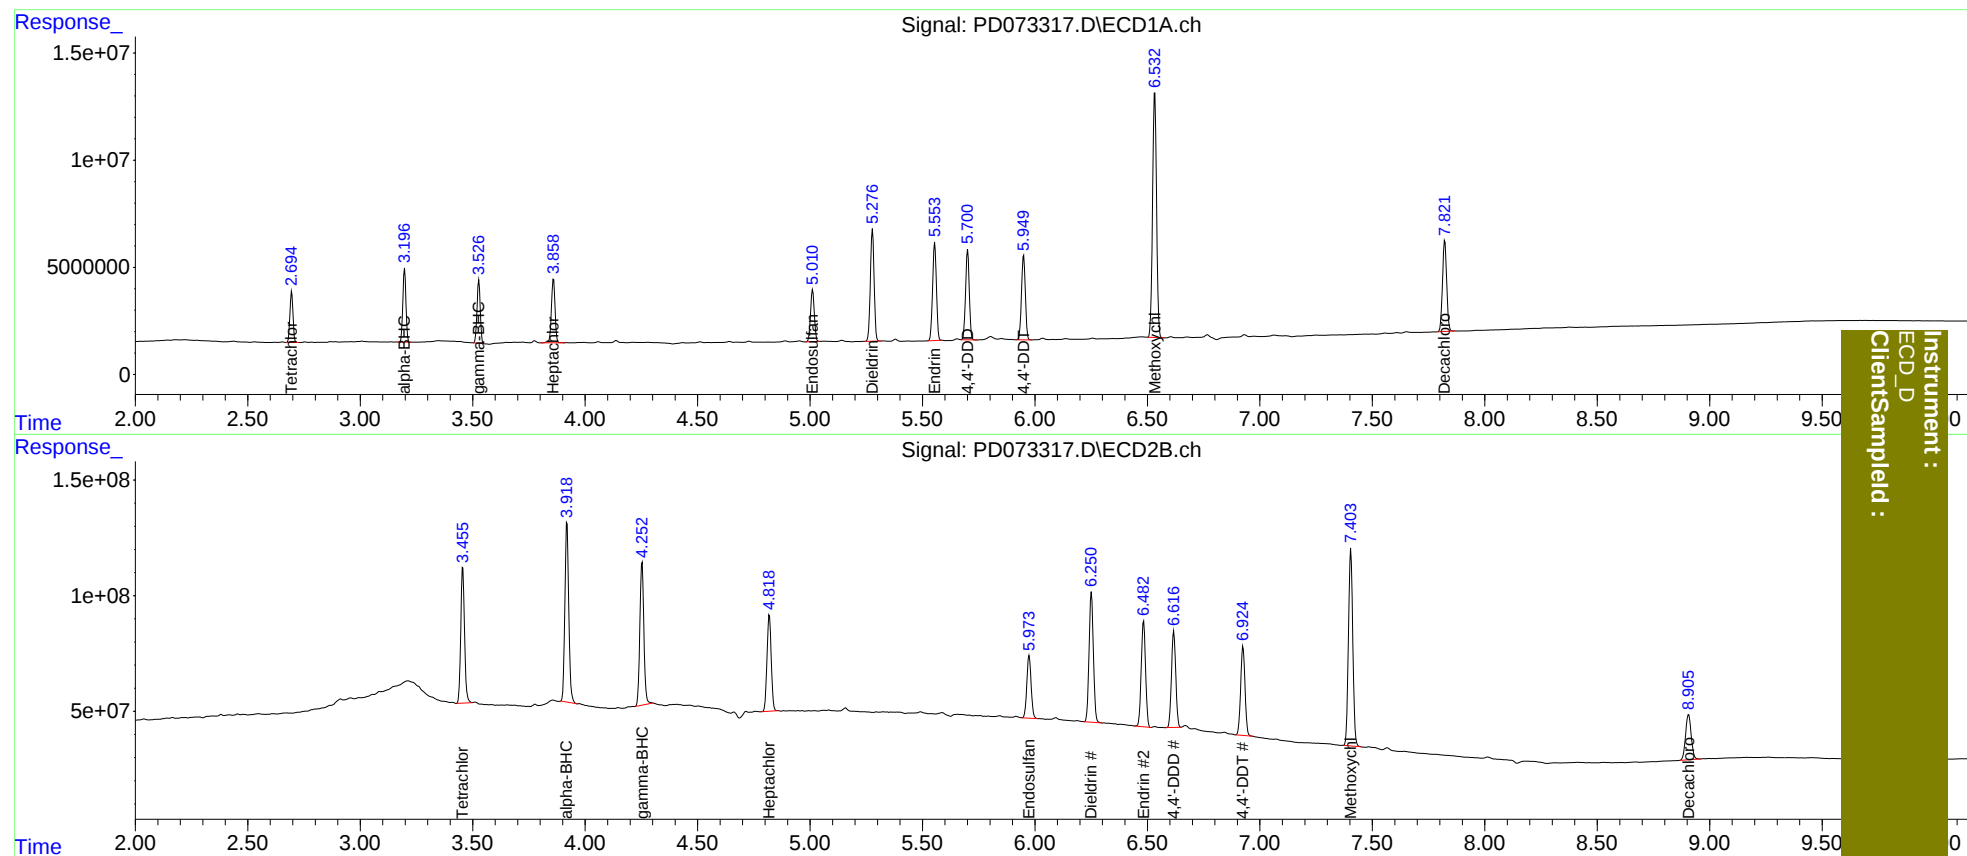


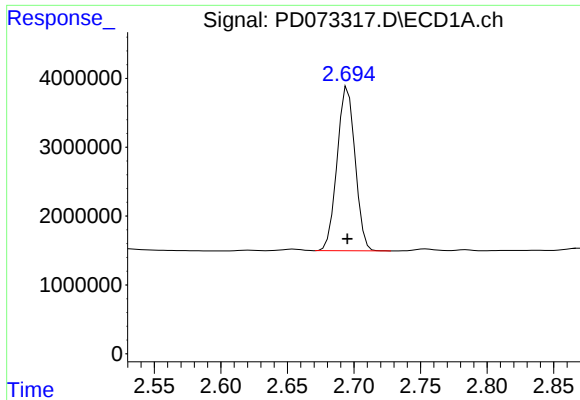

#1 Tetrachloro-m-xylene


R.T.: 2.695 min
Delta R.T.: 0.000 min
Response: 22409184
Conc: 10.67 ng/ml

Instrument :
ECD_D
ClientSampleId :

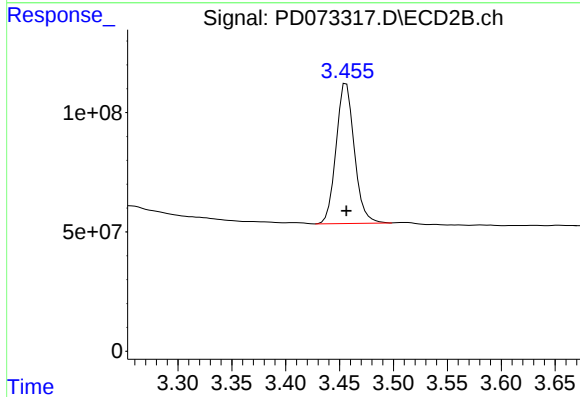


#1 Tetrachloro-m-xylene

R.T.: 3.456 min
Delta R.T.: 0.000 min
Response: 690517692
Conc: 11.25 ng/ml

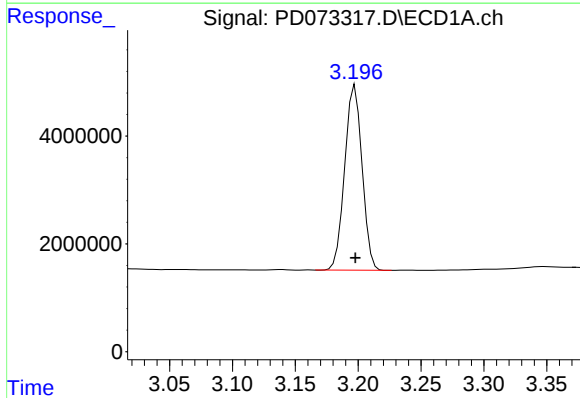


#2 alpha-BHC

R.T.: 3.198 min
Delta R.T.: 0.000 min
Response: 32964412
Conc: 9.98 ng/ml

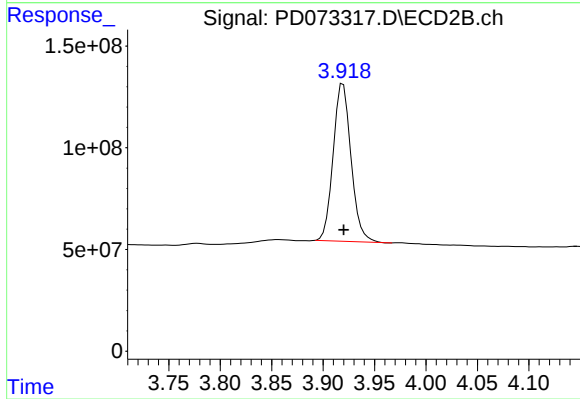

#2 alpha-BHC


R.T.: 3.919 min
Delta R.T.: 0.000 min
Response: 938412522
Conc: 11.42 ng/ml

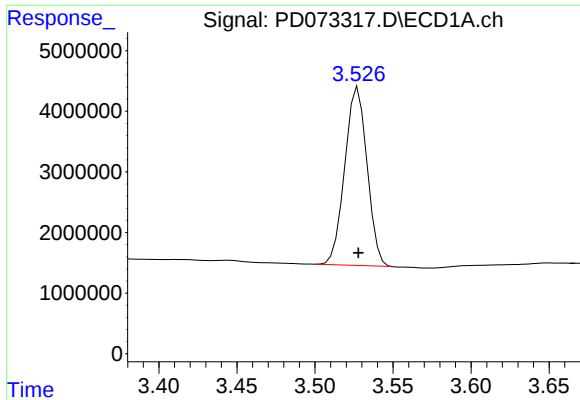

#3 gamma-BHC (Lindane)


R.T.: 3.528 min
Delta R.T.: 0.000 min
Response: 29209426
Conc: 9.91 ng/ml

Instrument :
ECD_D
ClientSampleId :

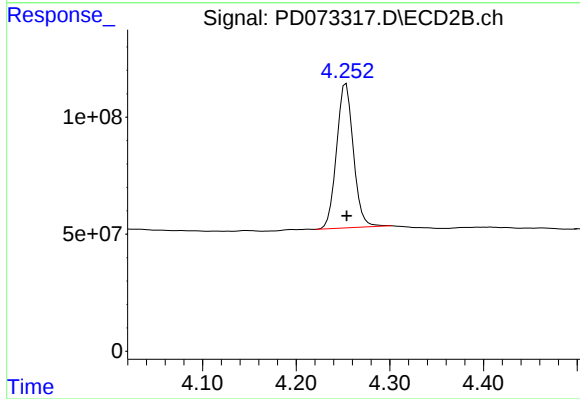


#3 gamma-BHC (Lindane)

R.T.: 4.253 min
Delta R.T.: 0.000 min
Response: 770180367
Conc: 11.59 ng/ml

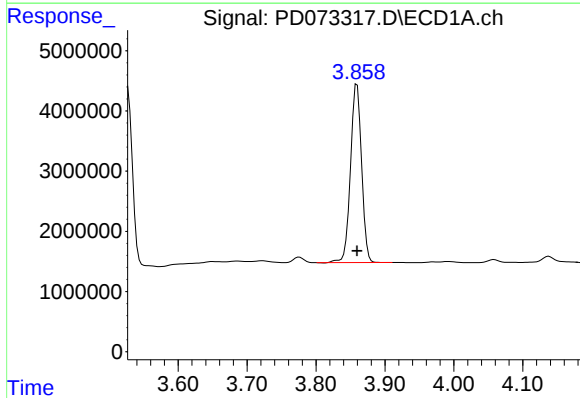


#4 Heptachlor

R.T.: 3.860 min
Delta R.T.: 0.000 min
Response: 33132904
Conc: 10.23 ng/ml

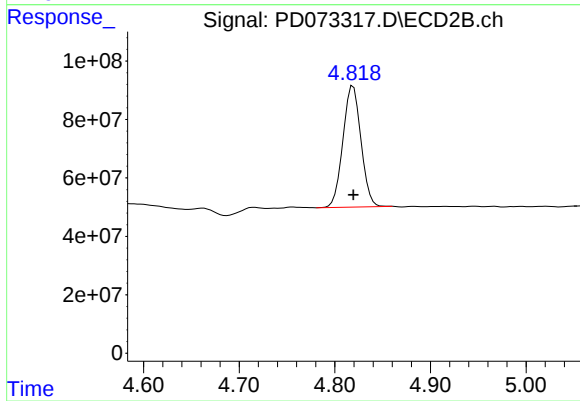

#4 Heptachlor


R.T.: 4.819 min
Delta R.T.: 0.000 min
Response: 545668157
Conc: 11.39 ng/ml

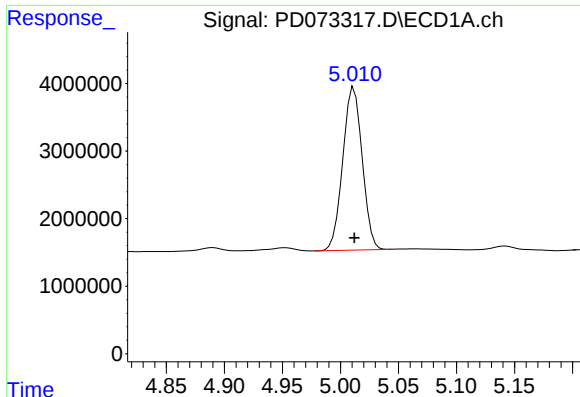

#9 Endosulfan I


R.T.: 5.012 min
Delta R.T.: 0.000 min
Response: 28063784
Conc: 10.34 ng/ml

Instrument :
ECD_D
ClientSampleId :

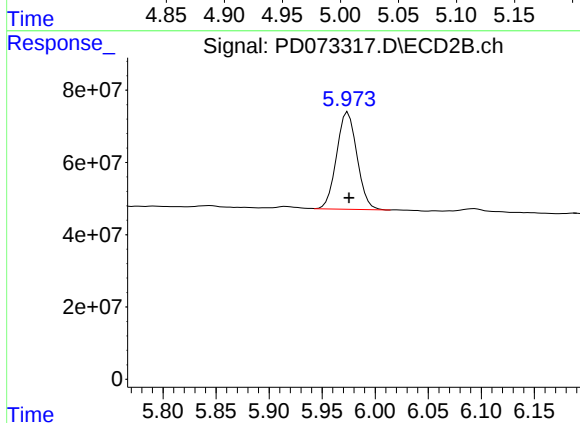


#9 Endosulfan I

R.T.: 5.974 min
Delta R.T.: 0.000 min
Response: 360179862
Conc: 10.87 ng/ml

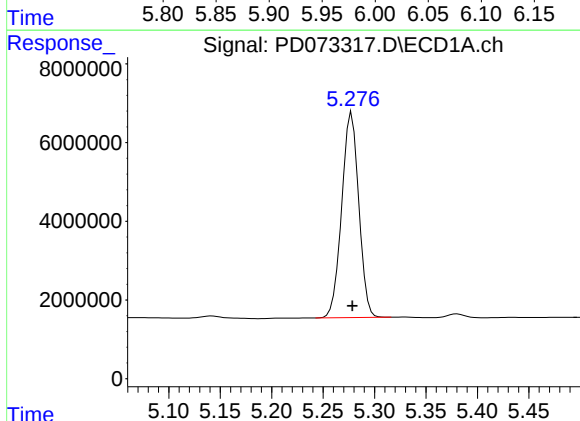


#13 Dieldrin

R.T.: 5.278 min
Delta R.T.: 0.000 min
Response: 60179434
Conc: 20.01 ng/ml

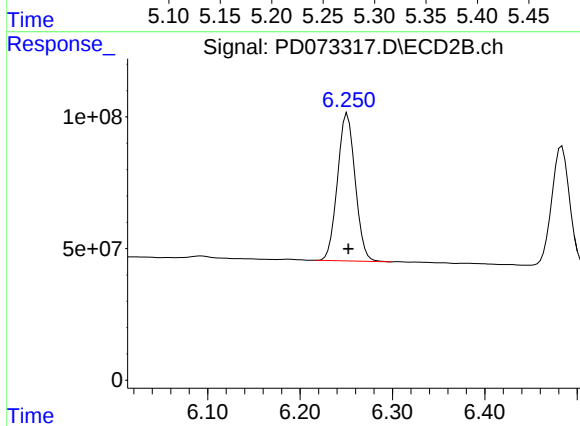

#13 Dieldrin


R.T.: 6.251 min
Delta R.T.: -0.001 min
Response: 746227830
Conc: 21.45 ng/ml

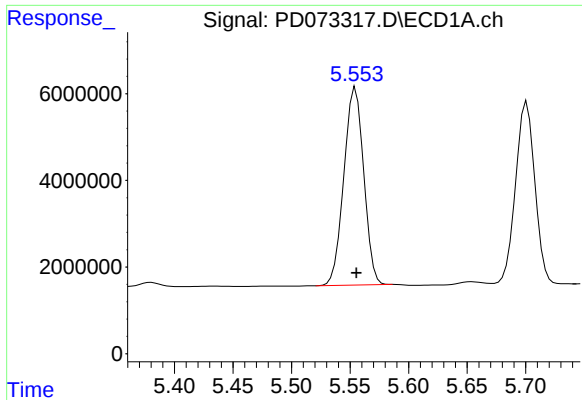

#14 Endrin


R.T.: 5.555 min
Delta R.T.: 0.000 min
Response: 53948201
Conc: 19.87 ng/ml

Instrument :
ECD_D
ClientSampleId :

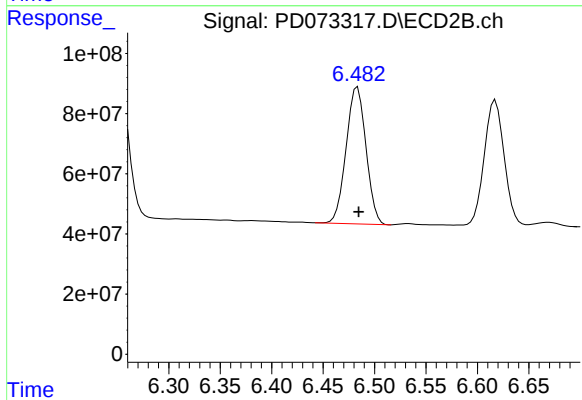


#14 Endrin

R.T.: 6.483 min
Delta R.T.: -0.001 min
Response: 613004642
Conc: 21.30 ng/ml

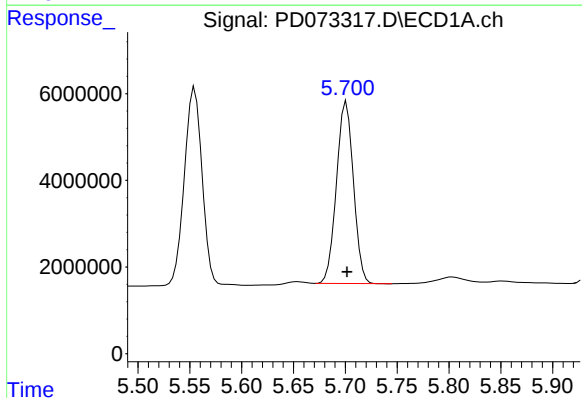


#16 4,4'-DDD

R.T.: 5.701 min
Delta R.T.: 0.000 min
Response: 47902780
Conc: 19.91 ng/ml

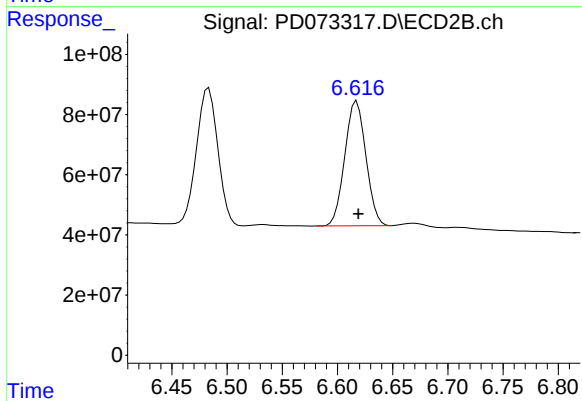

#16 4,4'-DDD


R.T.: 6.617 min
Delta R.T.: -0.001 min
Response: 552076350
Conc: 21.19 ng/ml

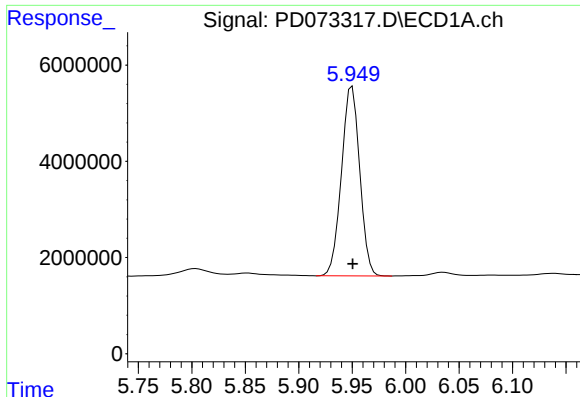

#17 4,4'-DDT


R.T.: 5.950 min
Delta R.T.: 0.000 min
Response: 46861569
Conc: 19.35 ng/ml

Instrument :
ECD_D
ClientSampleId :

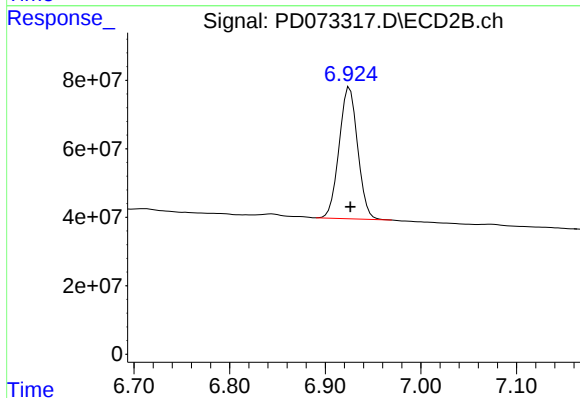


#17 4,4'-DDT

R.T.: 6.925 min
Delta R.T.: 0.000 min
Response: 518136777
Conc: 20.92 ng/ml

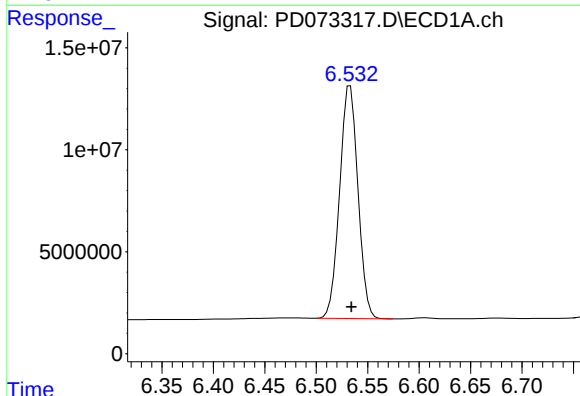


#20 Methoxychlor

R.T.: 6.533 min
Delta R.T.: -0.001 min
Response: 141318913
Conc: 102.32 ng/ml

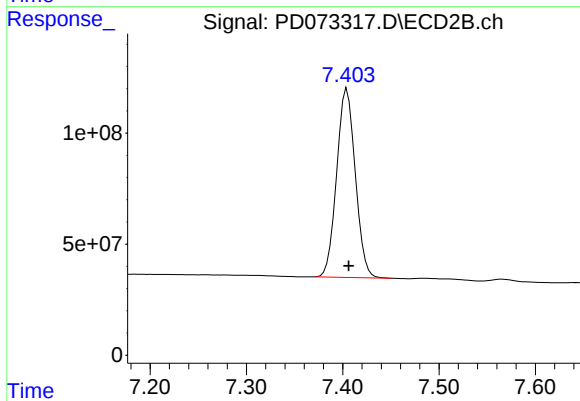

#20 Methoxychlor

R.T.: 7.405 min
Delta R.T.: -0.001 min
Response: 1141174610
Conc: 106.81 ng/ml

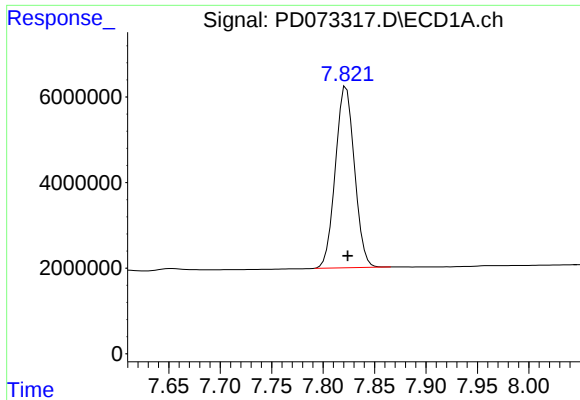

#27 Decachlorobiphenyl


R.T.: 7.822 min

Delta R.T.: -0.001 min

Response: 54802746

Conc: 21.22 ng/ml

Instrument :
ECD_D
ClientSampleId :

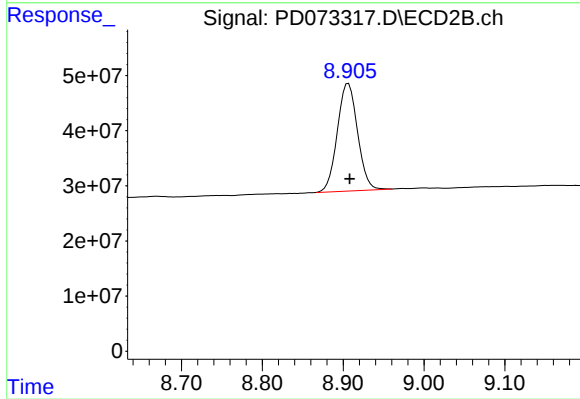

#27 Decachlorobiphenyl

R.T.: 8.907 min

Delta R.T.: -0.002 min

Response: 339281963

Conc: 21.25 ng/ml