

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121422\
 Data File : PD073319.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Dec 2022 17:33
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 05:01:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 15 04:59:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.695	3.456	41989663	1227.5E6	20.000	20.000
27)	SA Decachlor...	7.824	8.908	103.3E6	638.5E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.198	3.920	66033973	1644.0E6	20.000	20.000
3)	MA gamma-BHC...	3.528	4.254	58966531	1328.9E6	20.000	20.000
4)	MA Heptachlor	3.860	4.820	64755072	958.5E6	20.000	20.000
9)	A Endosulfan I	5.012	5.975	54306864	662.4E6	20.000	20.000
13)	MA Dieldrin	5.278	6.252	120.3E6	1391.3E6	40.000	40.000
14)	MA Endrin	5.555	6.485	108.6E6	1151.3E6	40.000	40.000
16)	A 4,4'-DDD	5.702	6.619	96244831	1042.2E6	40.000	40.000
17)	MA 4,4'-DDT	5.951	6.926	96888548	990.9E6	40.000	40.000
20)	A Methoxychlor	6.534	7.406	276.2E6	2136.9E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121422\
Data File : PD073319.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Dec 2022 17:33
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 05:01:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Dec 15 04:59:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

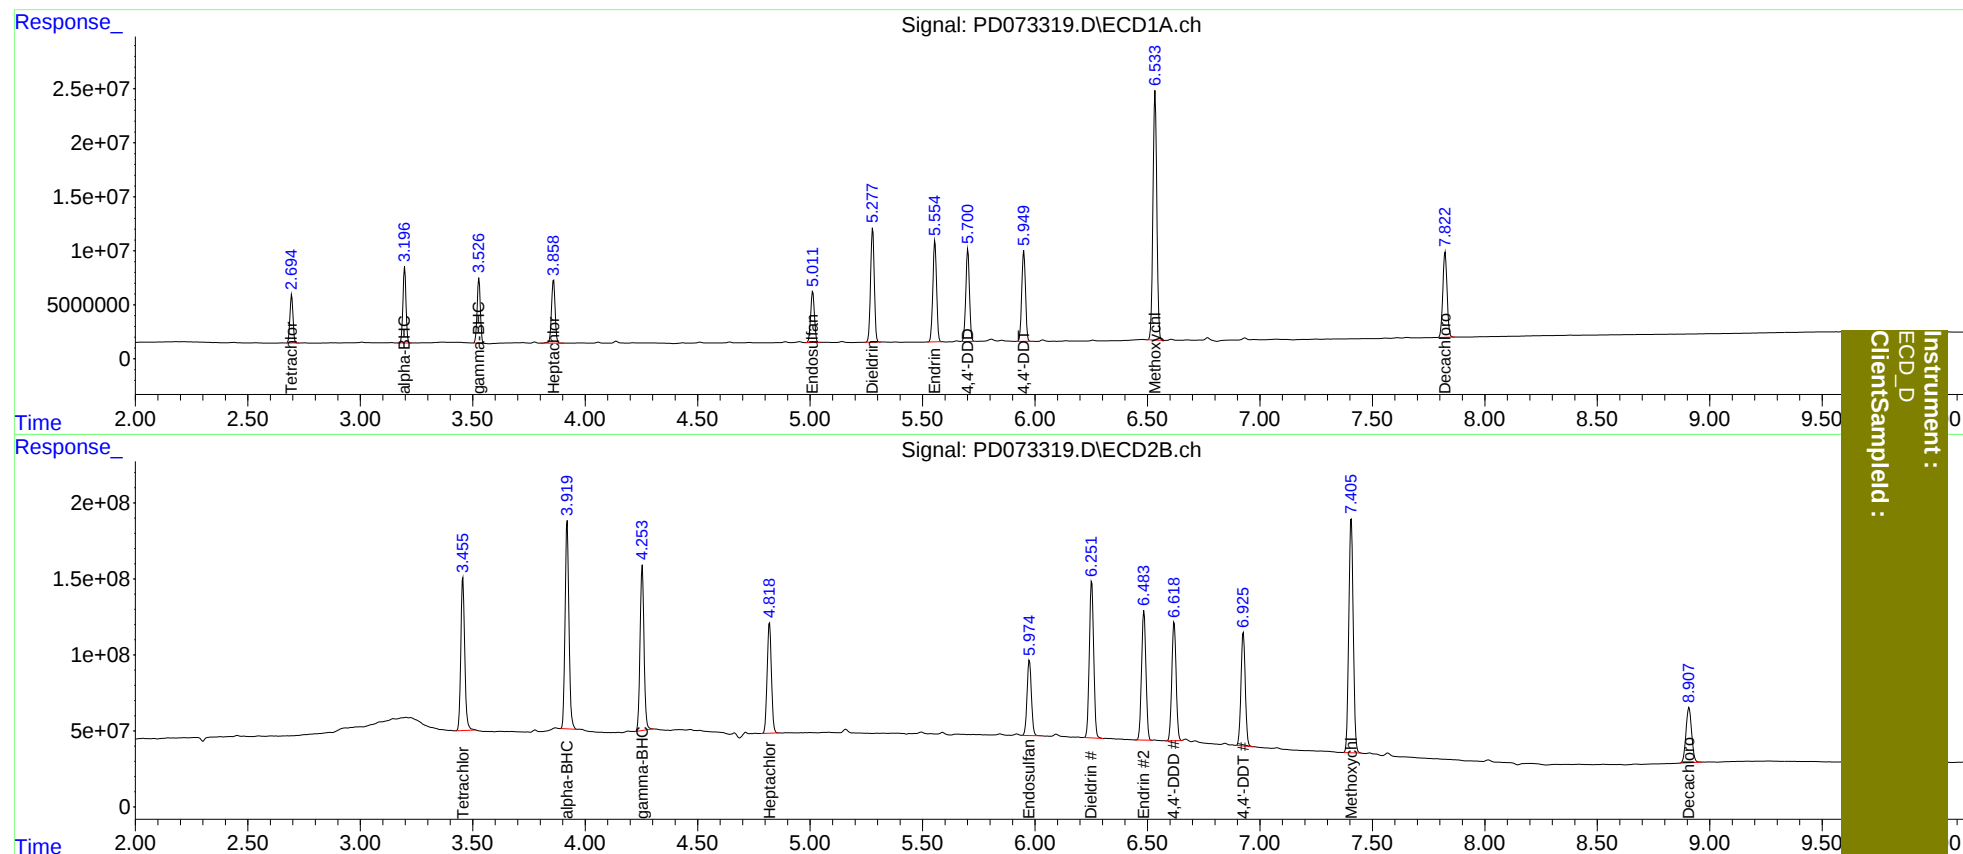


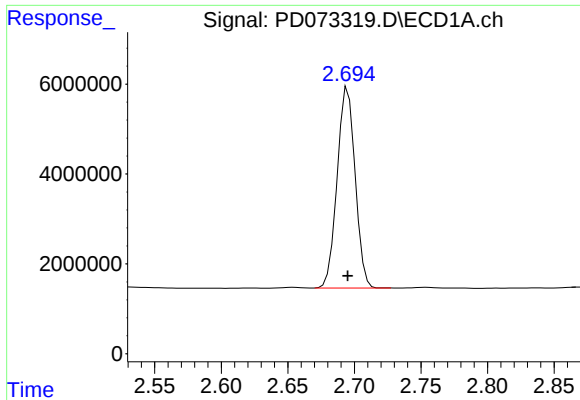

#1 Tetrachloro-m-xylene


R.T.: 2.695 min
Delta R.T.: 0.000 min
Response: 41989663
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

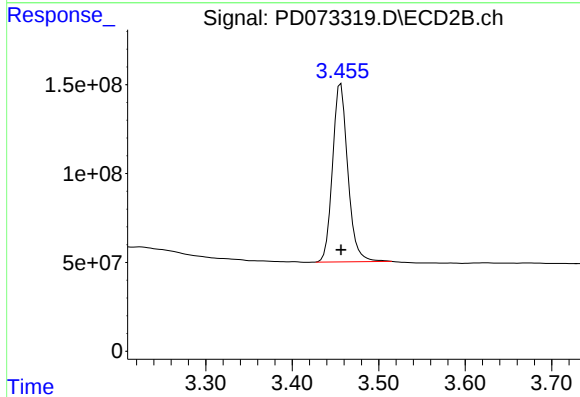


#1 Tetrachloro-m-xylene

R.T.: 3.456 min
Delta R.T.: 0.000 min
Response: 1227511048
Conc: 20.00 ng/ml

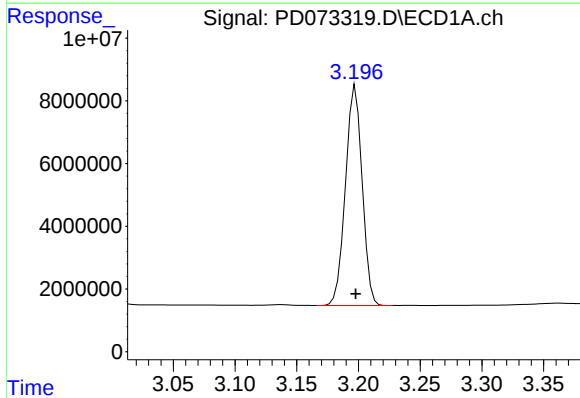


#2 alpha-BHC

R.T.: 3.198 min
Delta R.T.: 0.000 min
Response: 66033973
Conc: 20.00 ng/ml

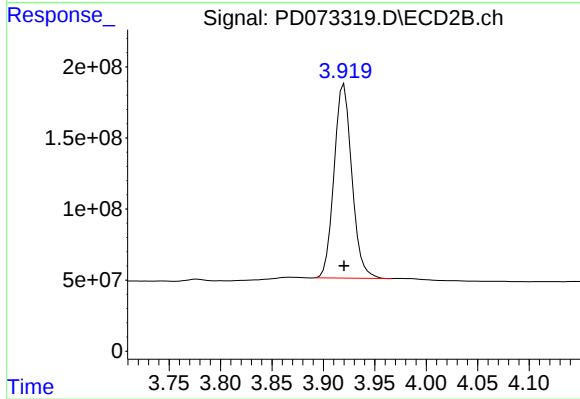

#2 alpha-BHC


R.T.: 3.920 min
Delta R.T.: 0.000 min
Response: 1643967956
Conc: 20.00 ng/ml

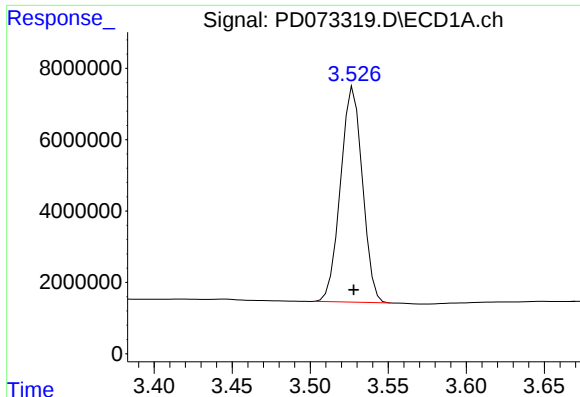

#3 gamma-BHC (Lindane)


R.T.: 3.528 min
Delta R.T.: 0.000 min
Response: 58966531
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

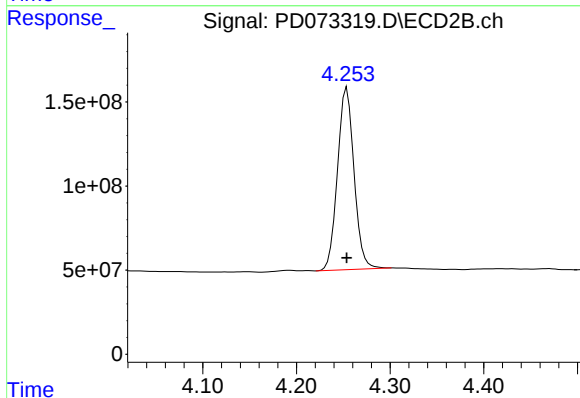


#3 gamma-BHC (Lindane)

R.T.: 4.254 min
Delta R.T.: 0.000 min
Response: 1328917244
Conc: 20.00 ng/ml

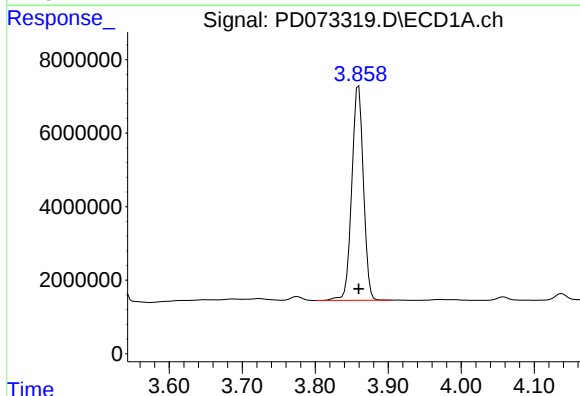


#4 Heptachlor

R.T.: 3.860 min
Delta R.T.: 0.000 min
Response: 64755072
Conc: 20.00 ng/ml

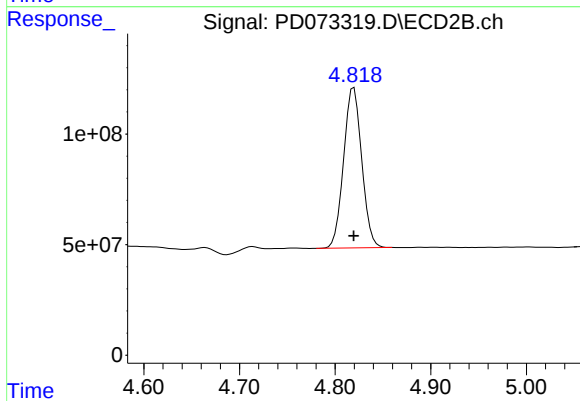

#4 Heptachlor


R.T.: 4.820 min
Delta R.T.: 0.000 min
Response: 958511797
Conc: 20.00 ng/ml

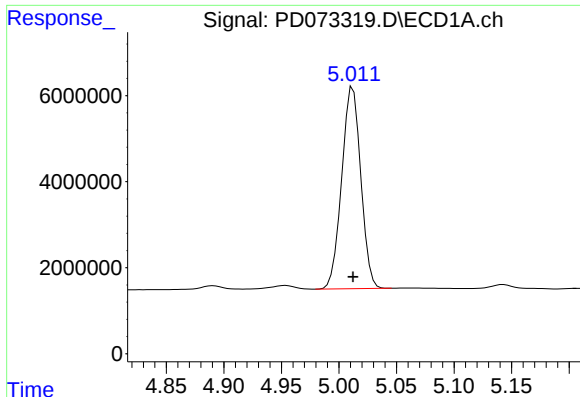

#9 Endosulfan I


R.T.: 5.012 min
Delta R.T.: 0.000 min
Response: 54306864
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

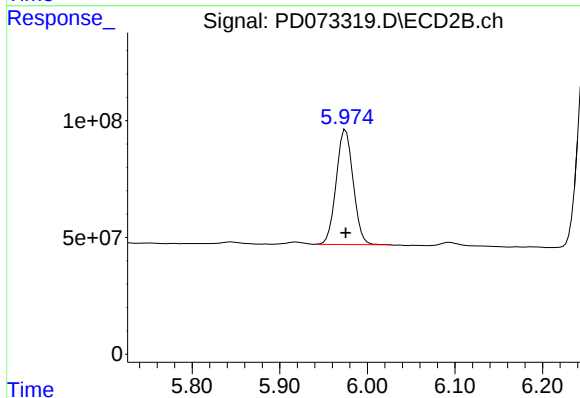


#9 Endosulfan I

R.T.: 5.975 min
Delta R.T.: 0.000 min
Response: 662448429
Conc: 20.00 ng/ml

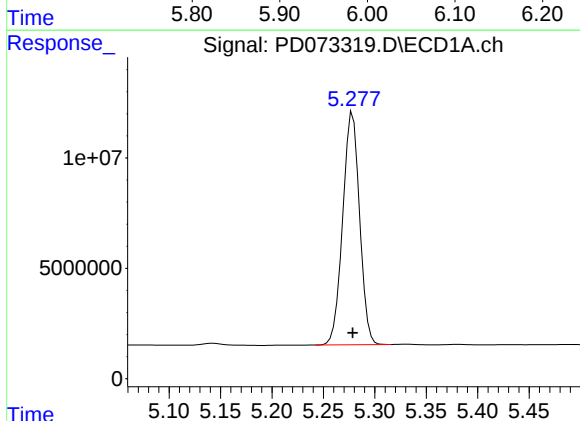


#13 Dieldrin

R.T.: 5.278 min
Delta R.T.: 0.000 min
Response: 120295387
Conc: 40.00 ng/ml

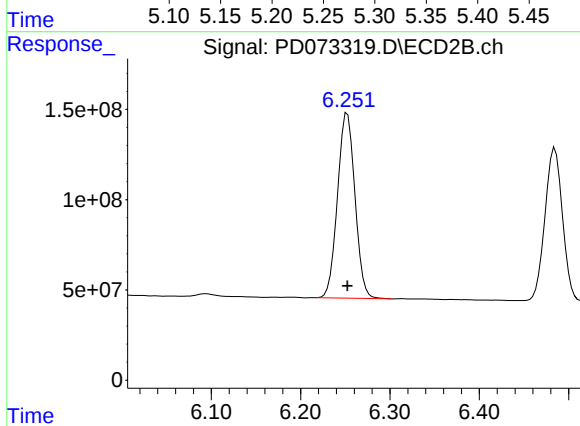

#13 Dieldrin


R.T.: 6.252 min
Delta R.T.: 0.000 min
Response: 1391272560
Conc: 40.00 ng/ml

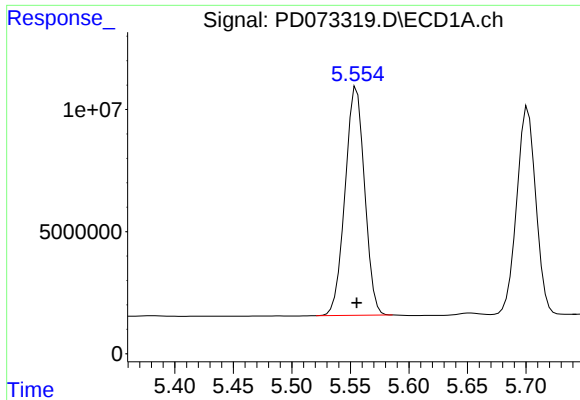

#14 Endrin


R.T.: 5.555 min
Delta R.T.: 0.000 min
Response: 108611443
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

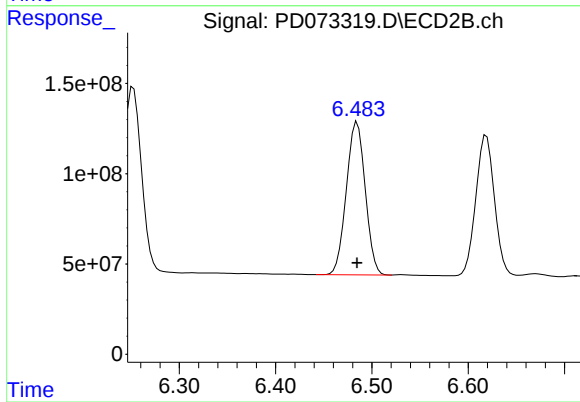


#14 Endrin

R.T.: 6.485 min
Delta R.T.: 0.000 min
Response: 1151336599
Conc: 40.00 ng/ml

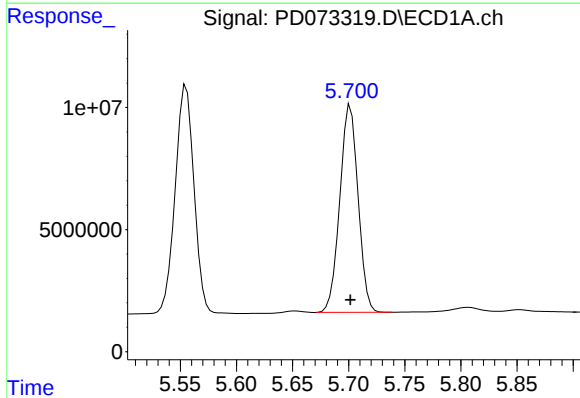


#16 4,4'-DDD

R.T.: 5.702 min
Delta R.T.: 0.000 min
Response: 96244831
Conc: 40.00 ng/ml

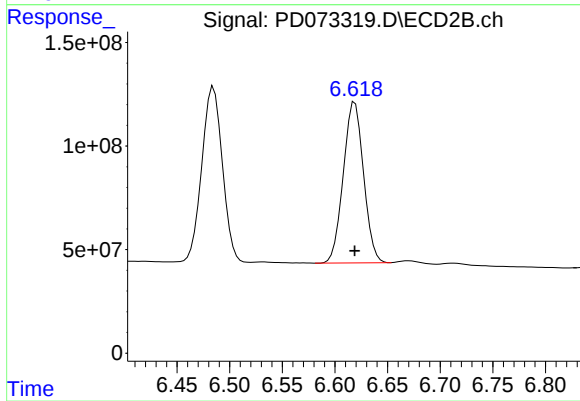

#16 4,4'-DDD


R.T.: 6.619 min
Delta R.T.: 0.000 min
Response: 1042232896
Conc: 40.00 ng/ml

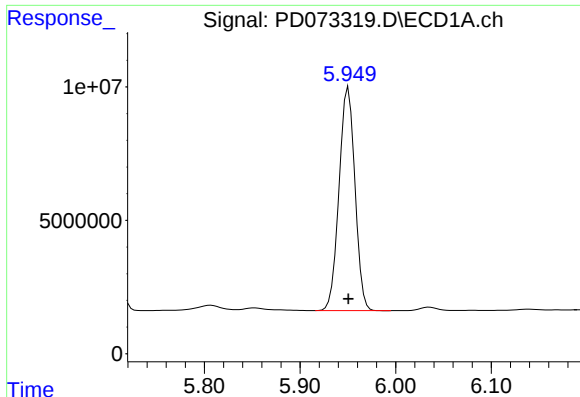

#17 4,4'-DDT


R.T.: 5.951 min
Delta R.T.: 0.000 min
Response: 96888548
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

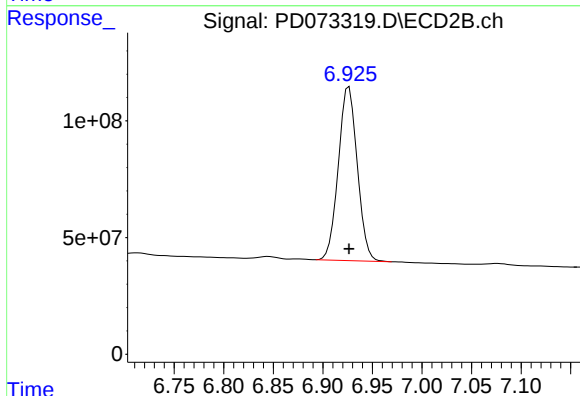


#17 4,4'-DDT

R.T.: 6.926 min
Delta R.T.: 0.000 min
Response: 990894357
Conc: 40.00 ng/ml

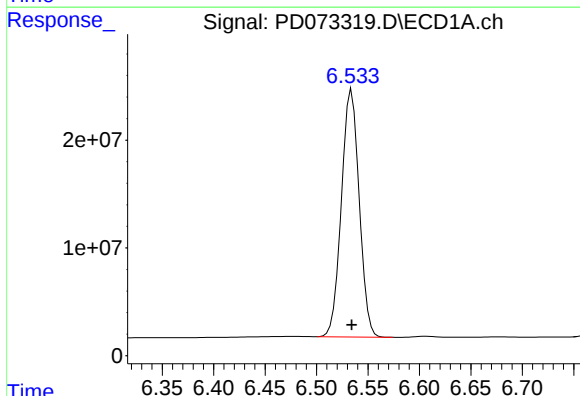


#20 Methoxychlor

R.T.: 6.534 min
Delta R.T.: 0.000 min
Response: 276219656
Conc: 200.00 ng/ml

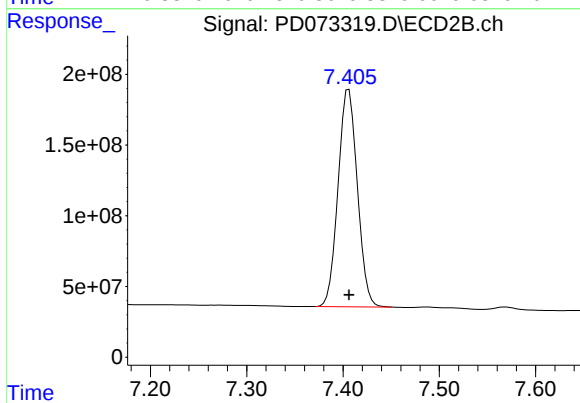

#20 Methoxychlor


R.T.: 7.406 min
Delta R.T.: 0.000 min
Response: 2136850612
Conc: 200.00 ng/ml

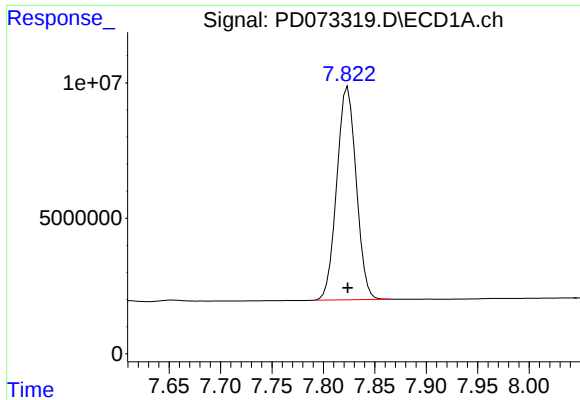

#27 Decachlorobiphenyl

R.T.: 7.824 min
Delta R.T.: 0.000 min
Response: 103306246
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

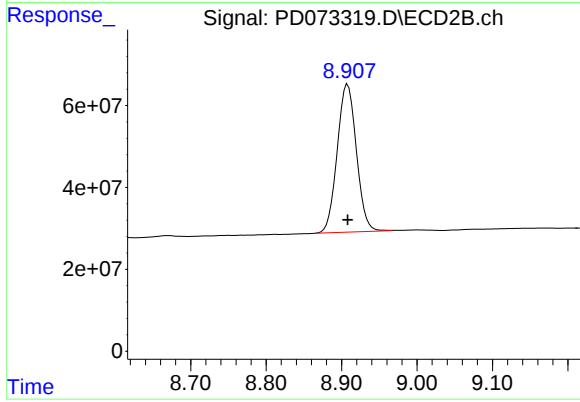

#27 Decachlorobiphenyl

R.T.: 8.908 min
Delta R.T.: 0.000 min
Response: 638527627
Conc: 40.00 ng/ml