

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121422\
 Data File : PD073321.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Dec 2022 17:59
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 05:01:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 15 04:59:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.695	3.456	82374616	2485.0E6	39.236	40.488
27)	SA Decachlor...	7.822	8.906	193.5E6	1194.5E6	74.940	74.828
Target Compounds							
2)	A alpha-BHC	3.198	3.920	138.0E6	3298.3E6	41.810	40.126
3)	MA gamma-BHC...	3.528	4.254	121.6E6	2594.7E6	41.239	39.049
4)	MA Heptachlor	3.859	4.819	130.9E6	1827.3E6	40.419	38.128
9)	A Endosulfan I	5.012	5.974	108.1E6	1248.7E6	39.808	37.699
13)	MA Dieldrin	5.278	6.251	244.5E6	2658.2E6	81.300	76.425
14)	MA Endrin	5.554	6.483	218.3E6	2202.6E6	80.379	76.524
16)	A 4,4'-DDD	5.701	6.618	194.0E6	1979.9E6	80.619	75.986
17)	MA 4,4'-DDT	5.950	6.925	197.2E6	1905.2E6	81.418	76.907
20)	A Methoxychlor	6.533	7.405	528.4E6	3964.3E6	382.579	371.043


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121422\
Data File : PD073321.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Dec 2022 17:59
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 05:01:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Dec 15 04:59:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

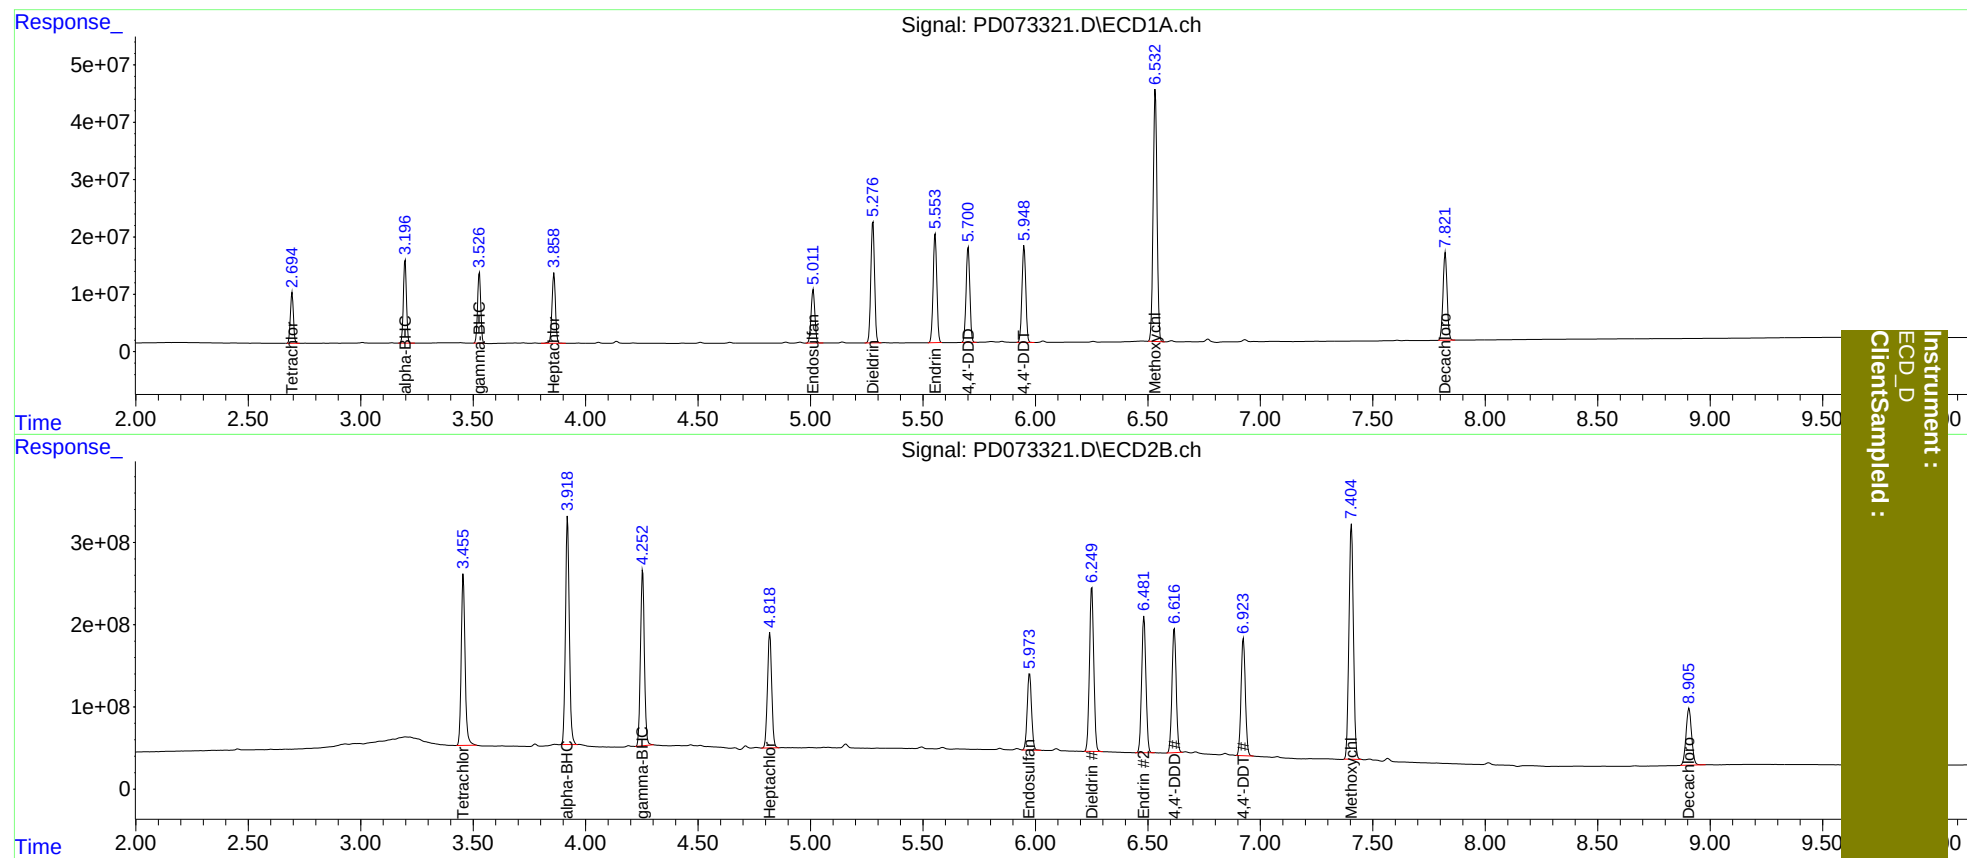


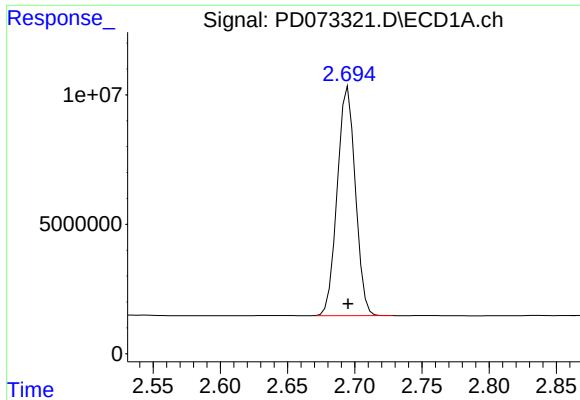

#1 Tetrachloro-m-xylene


R.T.: 2.695 min
Delta R.T.: 0.000 min
Response: 82374616
Conc: 39.24 ng/ml

Instrument :
ECD_D
ClientSampleId :

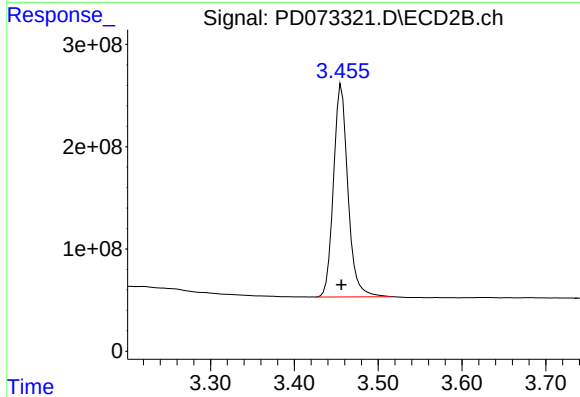


#1 Tetrachloro-m-xylene

R.T.: 3.456 min
Delta R.T.: 0.000 min
Response: 2485000120
Conc: 40.49 ng/ml

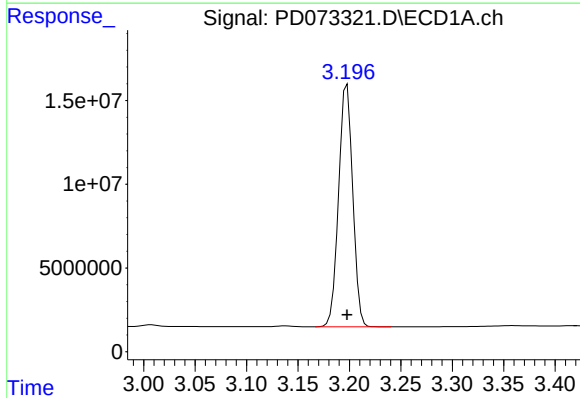


#2 alpha-BHC

R.T.: 3.198 min
Delta R.T.: 0.000 min
Response: 138042574
Conc: 41.81 ng/ml

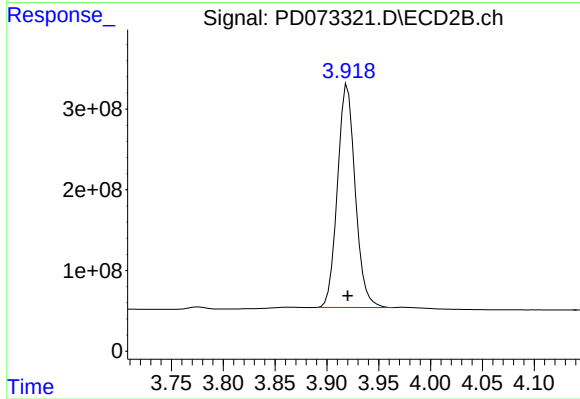

#2 alpha-BHC


R.T.: 3.920 min
Delta R.T.: 0.000 min
Response: 3298302271
Conc: 40.13 ng/ml

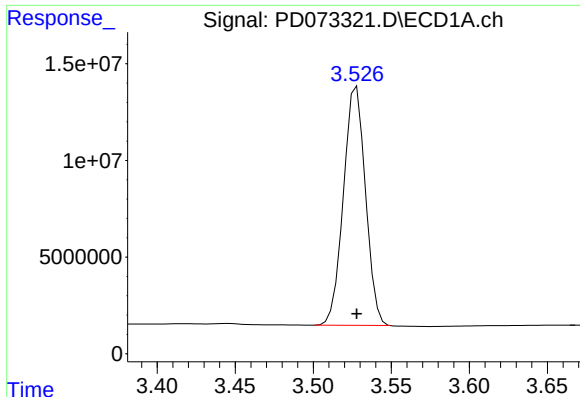

#3 gamma-BHC (Lindane)


R.T.: 3.528 min
Delta R.T.: 0.000 min
Response: 121587407
Conc: 41.24 ng/ml

Instrument :
ECD_D
ClientSampleId :

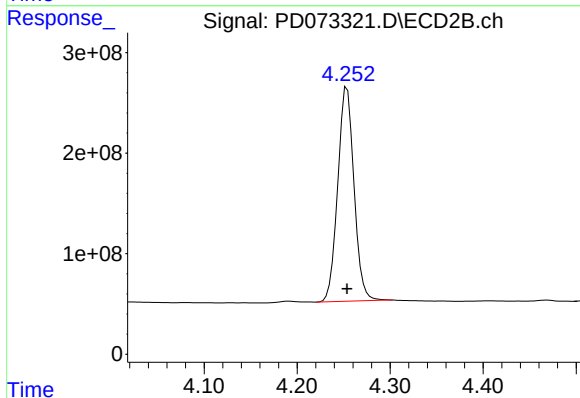


#3 gamma-BHC (Lindane)

R.T.: 4.254 min
Delta R.T.: 0.000 min
Response: 2594660241
Conc: 39.05 ng/ml

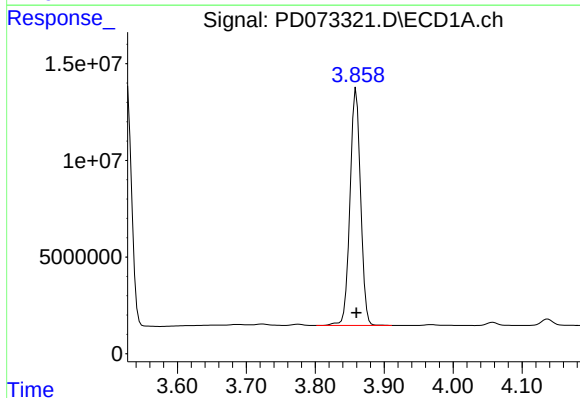


#4 Heptachlor

R.T.: 3.859 min
Delta R.T.: 0.000 min
Response: 130865570
Conc: 40.42 ng/ml

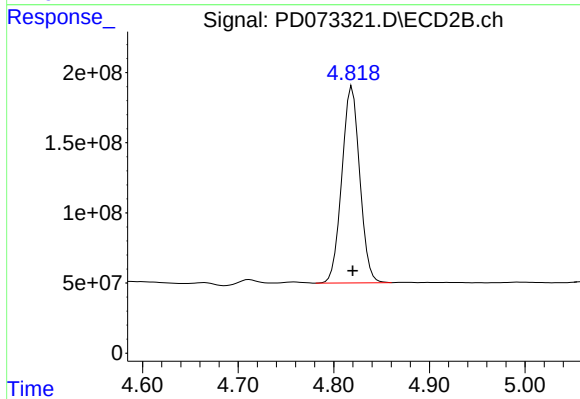

#4 Heptachlor


R.T.: 4.819 min
Delta R.T.: 0.000 min
Response: 1827299352
Conc: 38.13 ng/ml

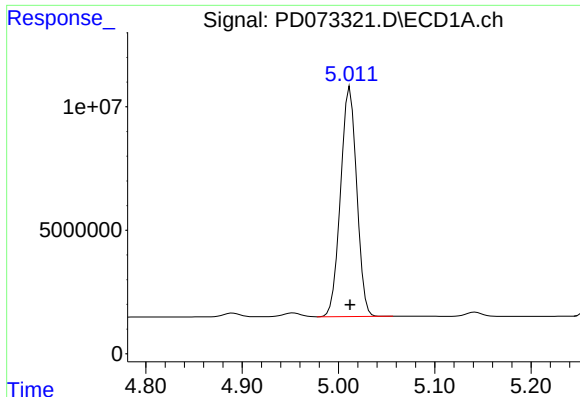

#9 Endosulfan I


R.T.: 5.012 min
Delta R.T.: 0.000 min
Response: 108092369
Conc: 39.81 ng/ml

Instrument :
ECD_D
ClientSampleId :

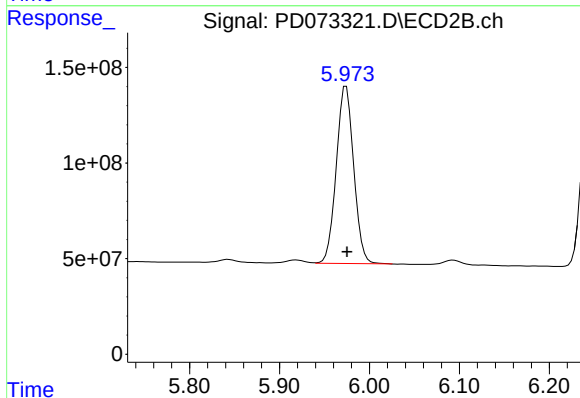


#9 Endosulfan I

R.T.: 5.974 min
Delta R.T.: -0.001 min
Response: 1248667184
Conc: 37.70 ng/ml

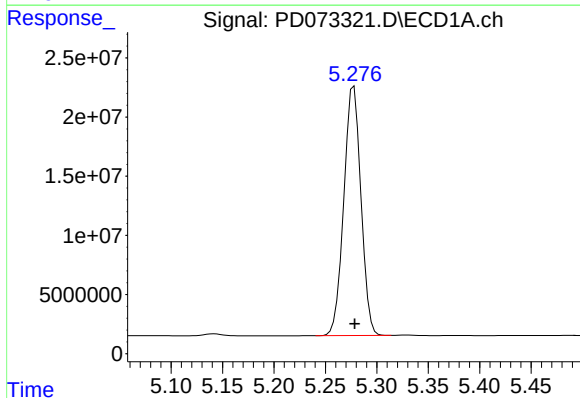


#13 Dieldrin

R.T.: 5.278 min
Delta R.T.: 0.000 min
Response: 244499561
Conc: 81.30 ng/ml

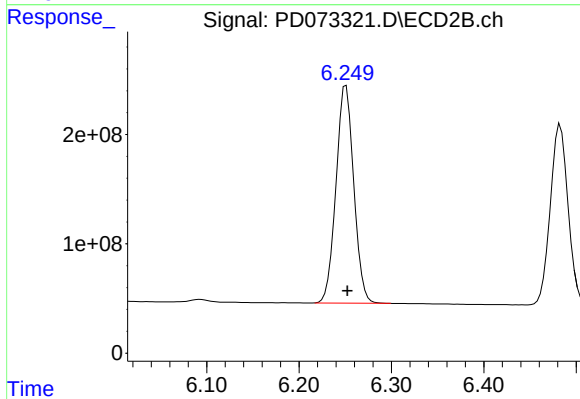

#13 Dieldrin


R.T.: 6.251 min
Delta R.T.: -0.002 min
Response: 2658186707
Conc: 76.42 ng/ml

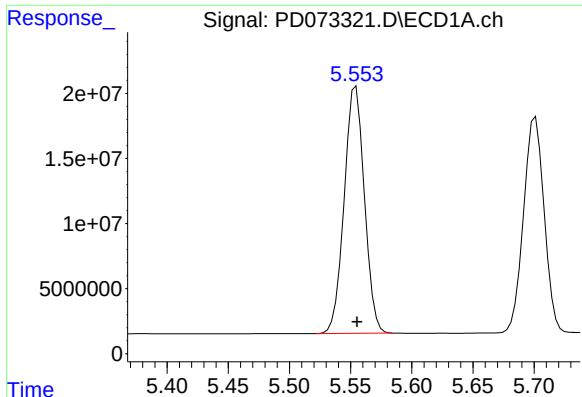

#14 Endrin


R.T.: 5.554 min
Delta R.T.: 0.000 min
Response: 218252186
Conc: 80.38 ng/ml

Instrument :
ECD_D
ClientSampleId :

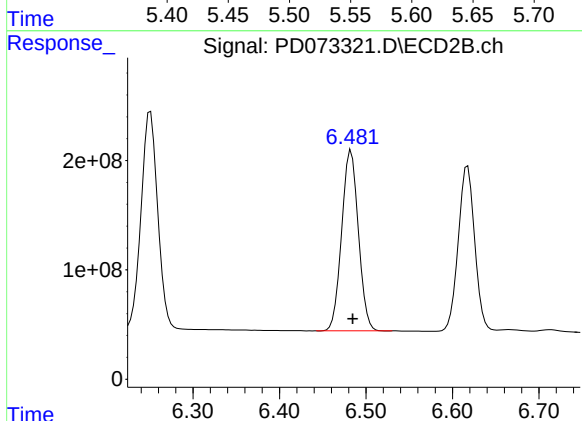


#14 Endrin

R.T.: 6.483 min
Delta R.T.: -0.002 min
Response: 2202615287
Conc: 76.52 ng/ml

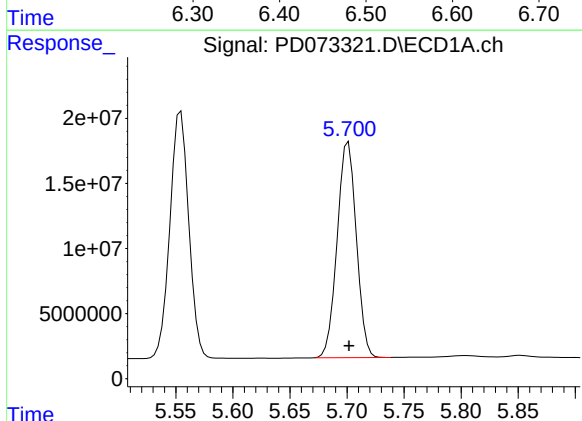


#16 4,4'-DDD

R.T.: 5.701 min
Delta R.T.: 0.000 min
Response: 193979498
Conc: 80.62 ng/ml

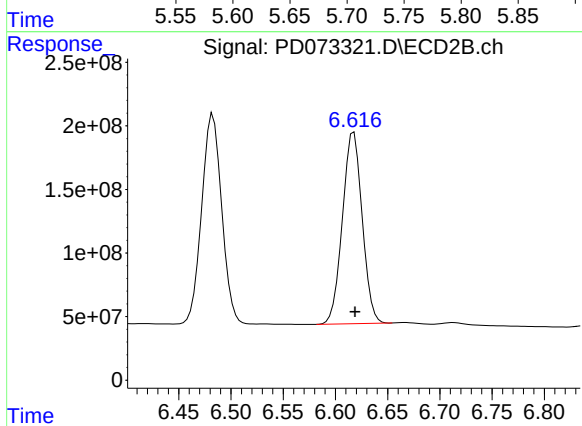

#16 4,4'-DDD


R.T.: 6.618 min
Delta R.T.: -0.001 min
Response: 1979872221
Conc: 75.99 ng/ml

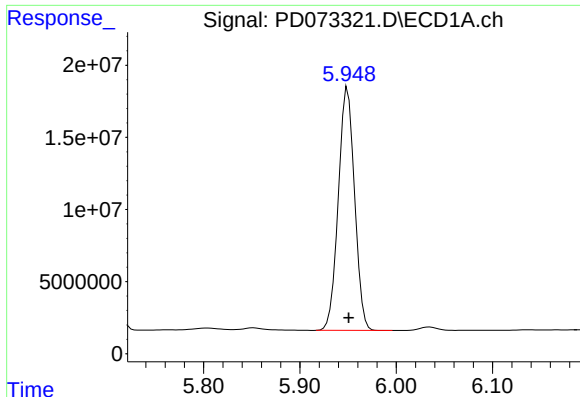

#17 4,4'-DDT


R.T.: 5.950 min
Delta R.T.: 0.000 min
Response: 197210624
Conc: 81.42 ng/ml

Instrument :
ECD_D
ClientSampleId :

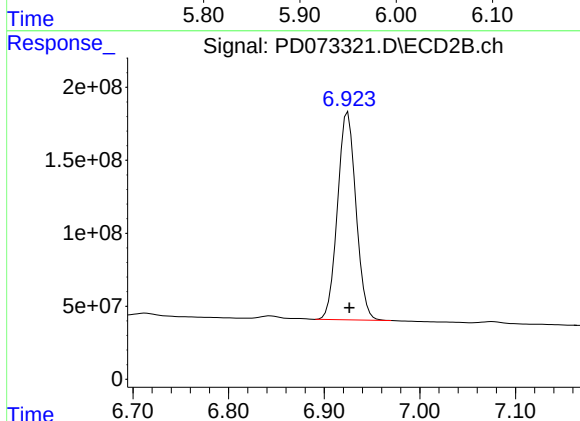


#17 4,4'-DDT

R.T.: 6.925 min
Delta R.T.: -0.002 min
Response: 1905169715
Conc: 76.91 ng/ml

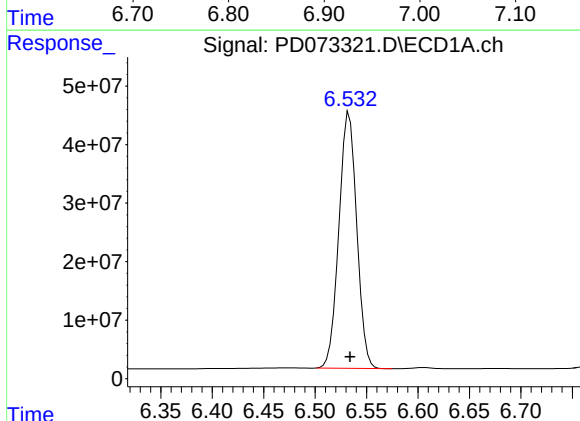


#20 Methoxychlor

R.T.: 6.533 min
Delta R.T.: 0.000 min
Response: 528379244
Conc: 382.58 ng/ml

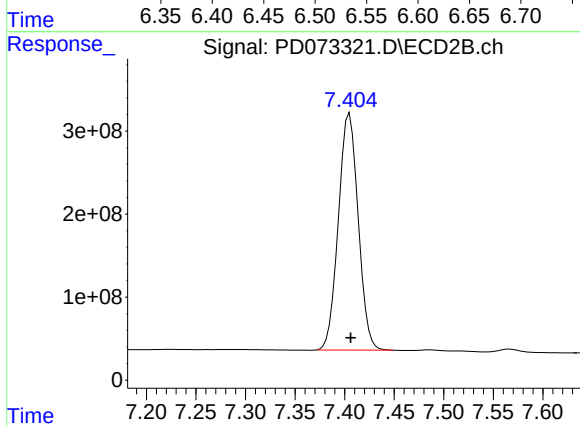

#20 Methoxychlor


R.T.: 7.405 min
Delta R.T.: -0.001 min
Response: 3964322502
Conc: 371.04 ng/ml

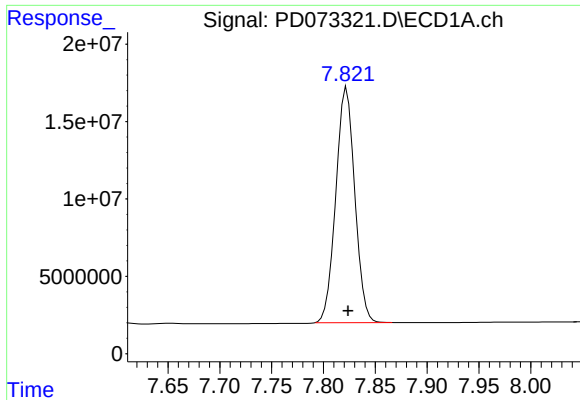

#27 Decachlorobiphenyl

R.T.: 7.822 min
Delta R.T.: -0.001 min
Response: 193544180
Conc: 74.94 ng/ml

Instrument :
ECD_D
ClientSampleId :

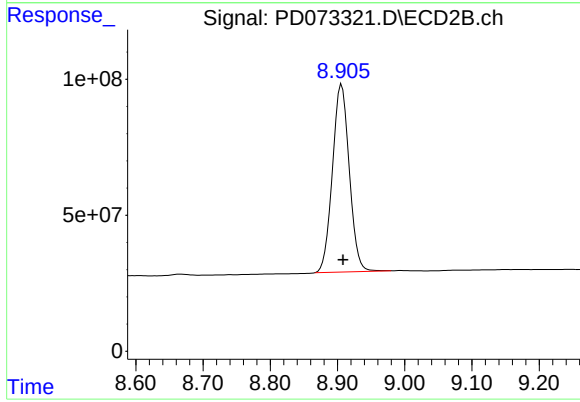

#27 Decachlorobiphenyl

R.T.: 8.906 min
Delta R.T.: -0.002 min
Response: 1194494593
Conc: 74.83 ng/ml