

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121422\
 Data File : PD073323.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Dec 2022 18:26
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 05:01:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 15 04:59:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.695	3.456	165.2E6	4667.5E6	78.699	76.048
27)	SA Decachlor...	7.823	8.907	388.3E6	2307.9E6	150.331	144.575
Target Compounds							
2)	A alpha-BHC	3.197	3.920	289.3E6	6391.5E6	87.627	77.757
3)	MA gamma-BHC...	3.527	4.254	255.9E6	4921.9E6	86.782	74.073
4)	MA Heptachlor	3.859	4.820	272.5E6	3389.7E6	84.177	70.728
9)	A Endosulfan I	5.011	5.974	219.3E6	2362.8E6	80.752	71.336
13)	MA Dieldrin	5.278	6.251	505.4E6	5178.7E6	168.062	148.891
14)	MA Endrin	5.555	6.483	455.8E6	4264.3E6	167.863	148.151
16)	A 4,4'-DDD	5.701	6.618	402.4E6	3854.4E6	167.241	147.927
17)	MA 4,4'-DDT	5.950	6.925	422.2E6	3767.8E6	174.297	152.095
20)	A Methoxychlor	6.533	7.405	1062.4E6	7464.5E6	769.243	698.642


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121422\
Data File : PD073323.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Dec 2022 18:26
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 05:01:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Dec 15 04:59:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

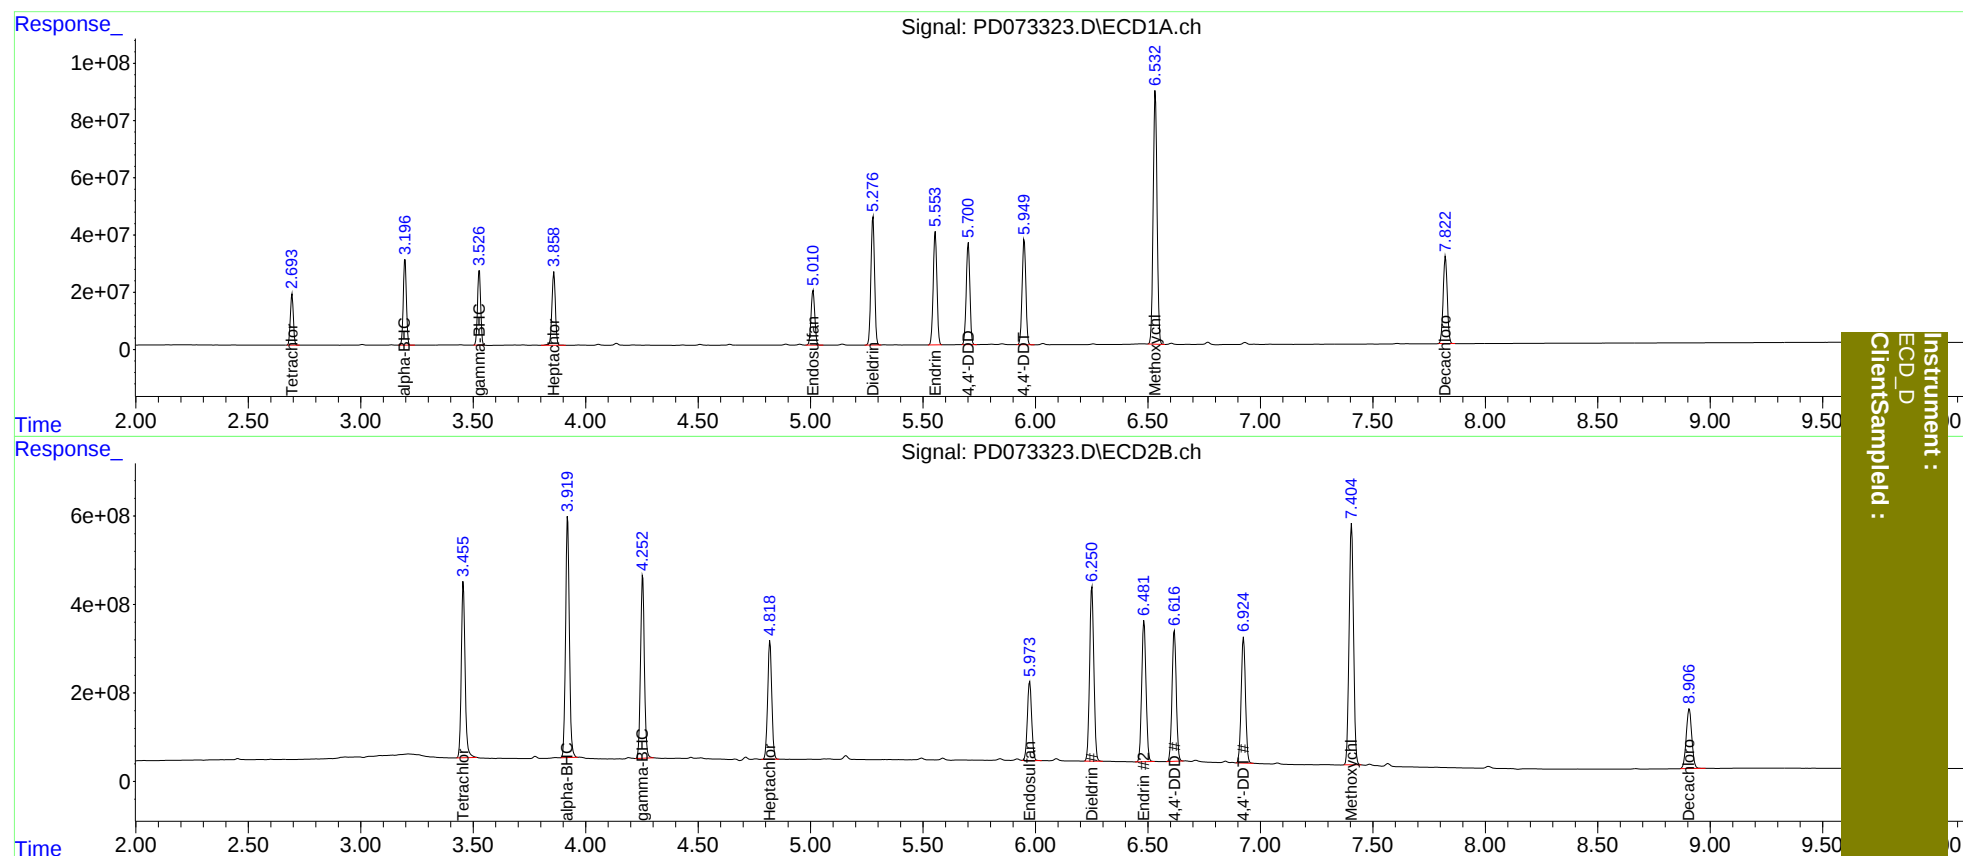


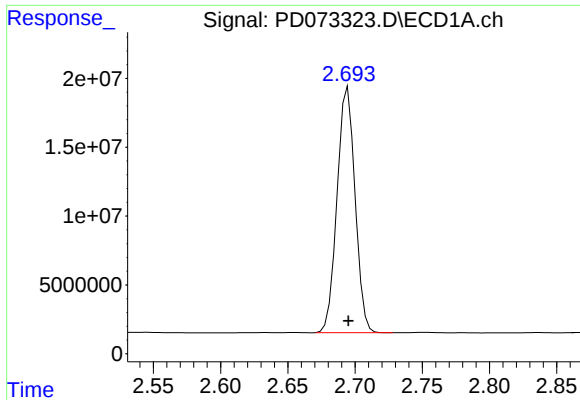

#1 Tetrachloro-m-xylene


R.T.: 2.695 min
Delta R.T.: 0.000 min
Response: 165227969
Conc: 78.70 ng/ml

Instrument :
ECD_D
ClientSampleId :

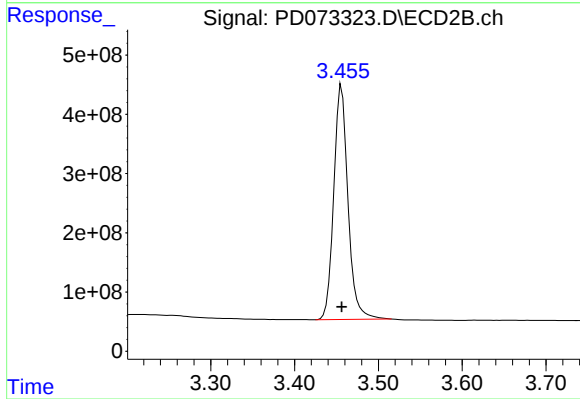


#1 Tetrachloro-m-xylene

R.T.: 3.456 min
Delta R.T.: 0.000 min
Response: 4667473738
Conc: 76.05 ng/ml

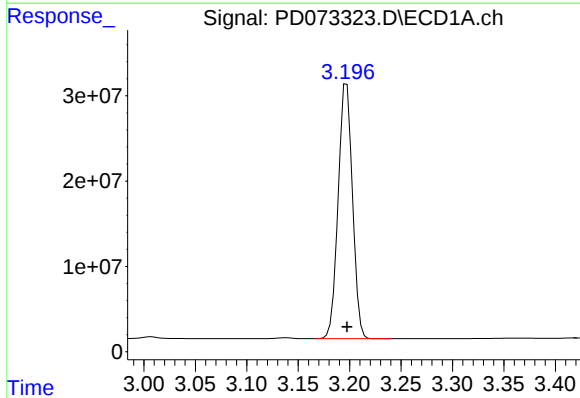


#2 alpha-BHC

R.T.: 3.197 min
Delta R.T.: 0.000 min
Response: 289317170
Conc: 87.63 ng/ml

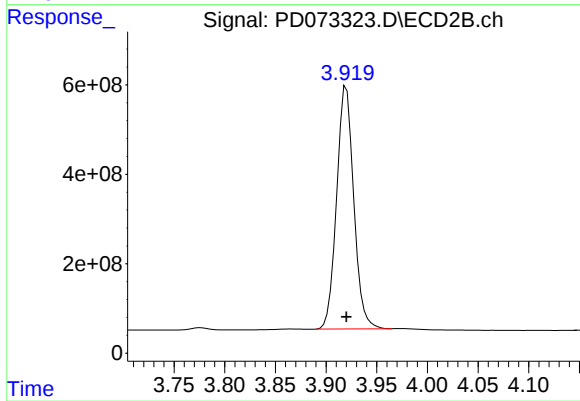

#2 alpha-BHC


R.T.: 3.920 min
Delta R.T.: 0.000 min
Response: 6391529197
Conc: 77.76 ng/ml

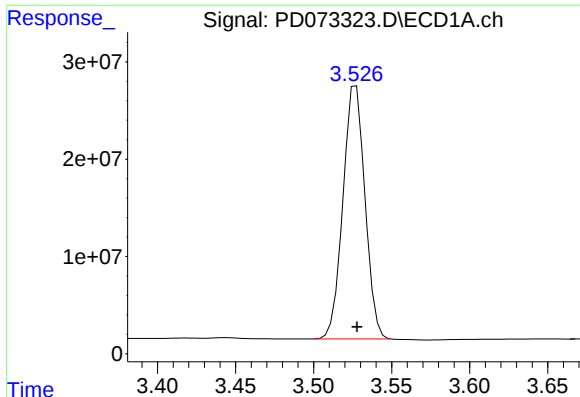

#3 gamma-BHC (Lindane)


R.T.: 3.527 min
Delta R.T.: 0.000 min
Response: 255862311
Conc: 86.78 ng/ml

Instrument :
ECD_D
ClientSampleId :

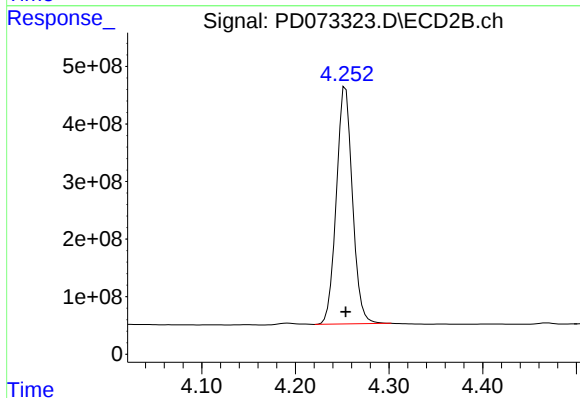


#3 gamma-BHC (Lindane)

R.T.: 4.254 min
Delta R.T.: 0.000 min
Response: 4921853536
Conc: 74.07 ng/ml

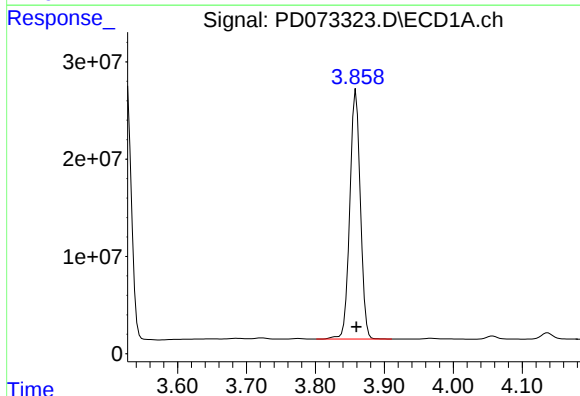


#4 Heptachlor

R.T.: 3.859 min
Delta R.T.: 0.000 min
Response: 272543980
Conc: 84.18 ng/ml

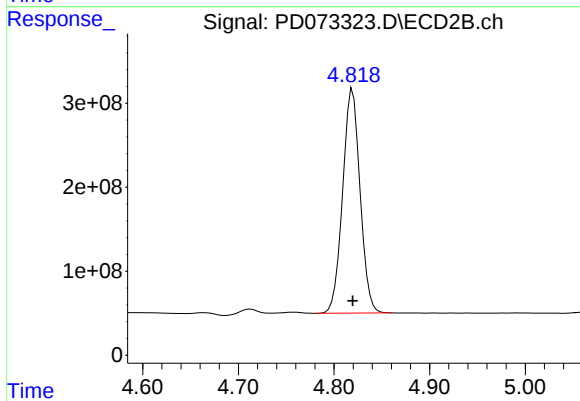

#4 Heptachlor


R.T.: 4.820 min
Delta R.T.: 0.000 min
Response: 3389672776
Conc: 70.73 ng/ml

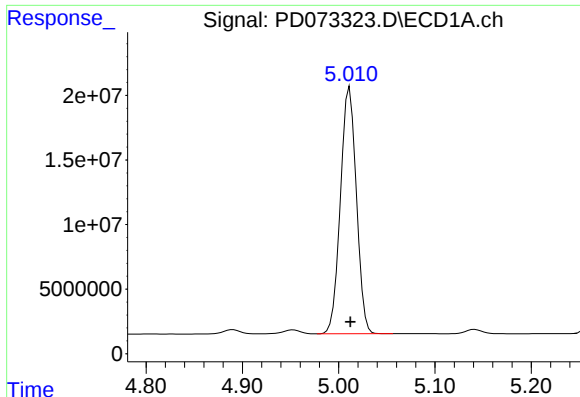

#9 Endosulfan I


R.T.: 5.011 min
Delta R.T.: 0.000 min
Response: 219268892
Conc: 80.75 ng/ml

Instrument :
ECD_D
ClientSampleId :

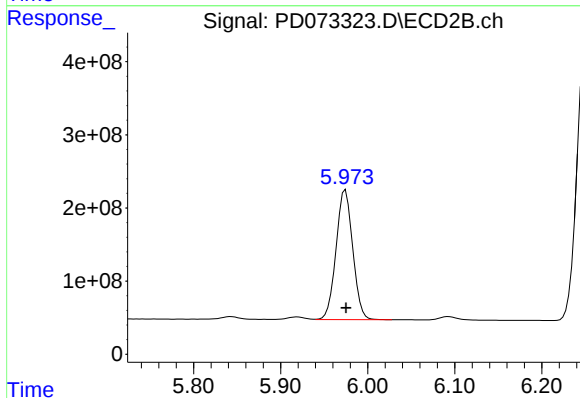


#9 Endosulfan I

R.T.: 5.974 min
Delta R.T.: 0.000 min
Response: 2362804923
Conc: 71.34 ng/ml

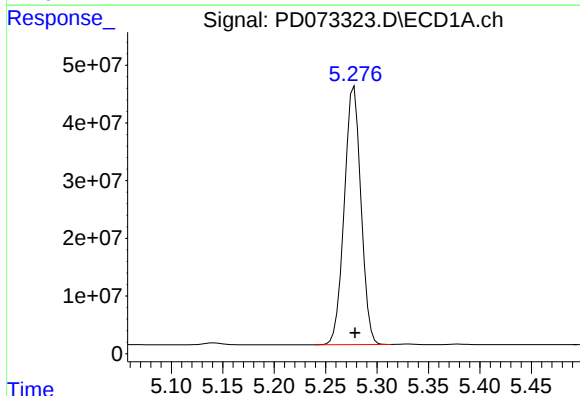


#13 Dieldrin

R.T.: 5.278 min
Delta R.T.: 0.000 min
Response: 505425656
Conc: 168.06 ng/ml

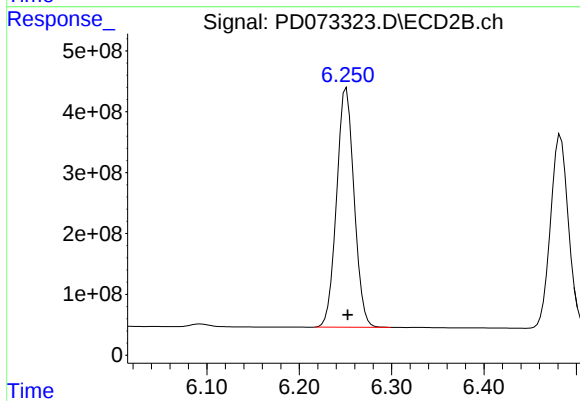

#13 Dieldrin


R.T.: 6.251 min
Delta R.T.: -0.001 min
Response: 5178709577
Conc: 148.89 ng/ml

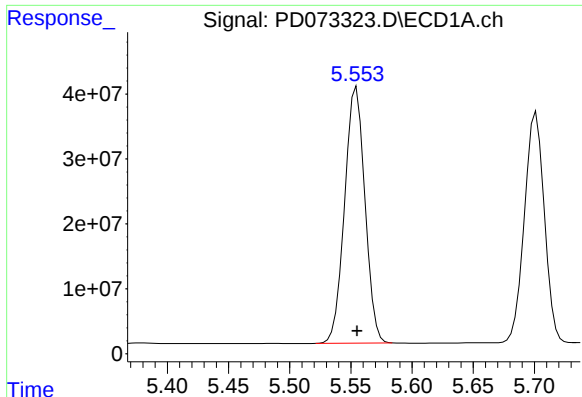

#14 Endrin


R.T.: 5.555 min
Delta R.T.: 0.000 min
Response: 455796547
Conc: 167.86 ng/ml

Instrument :
ECD_D
ClientSampleId :

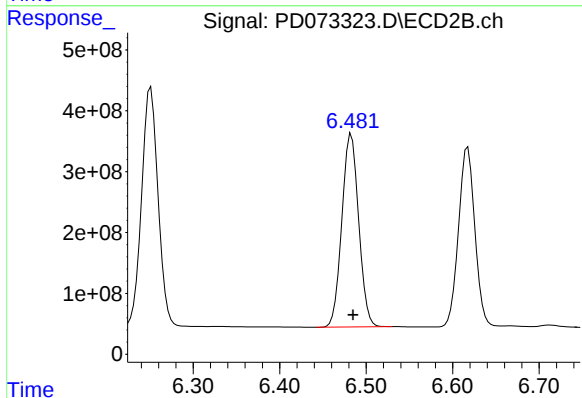


#14 Endrin

R.T.: 6.483 min
Delta R.T.: -0.002 min
Response: 4264289819
Conc: 148.15 ng/ml

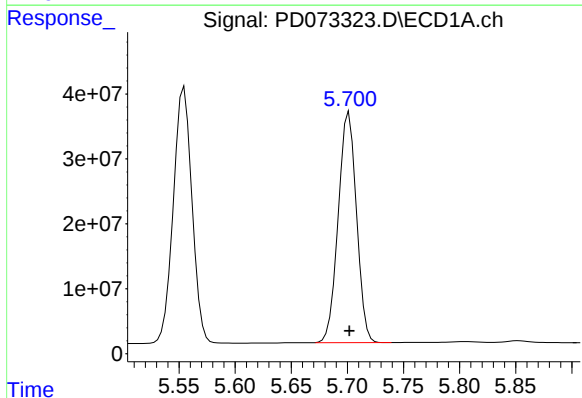


#16 4,4'-DDD

R.T.: 5.701 min
Delta R.T.: 0.000 min
Response: 402401010
Conc: 167.24 ng/ml

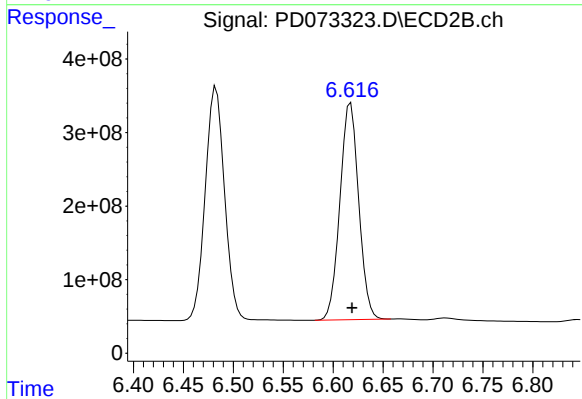

#16 4,4'-DDD


R.T.: 6.618 min
Delta R.T.: -0.001 min
Response: 3854372142
Conc: 147.93 ng/ml

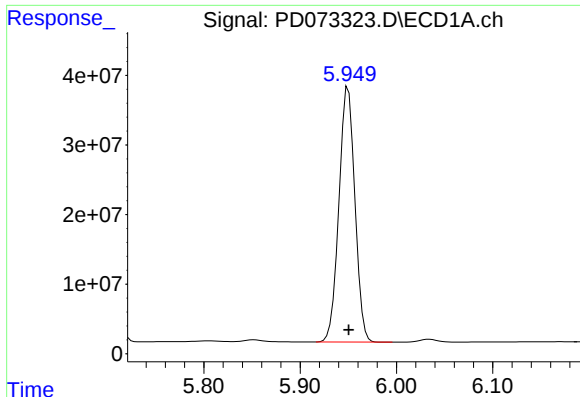

#17 4,4'-DDT


R.T.: 5.950 min
Delta R.T.: 0.000 min
Response: 422183825
Conc: 174.30 ng/ml

Instrument :
ECD_D
ClientSampleId :

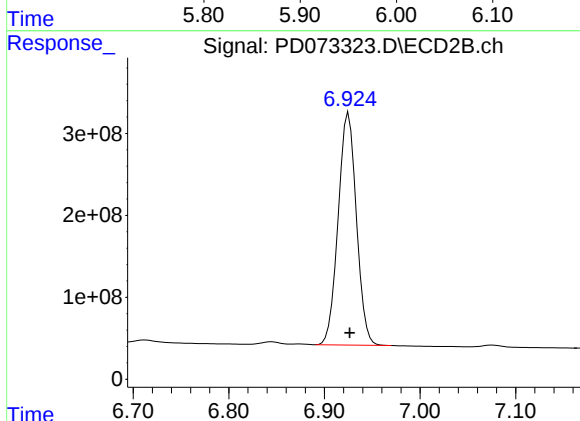


#17 4,4'-DDT

R.T.: 6.925 min
Delta R.T.: -0.001 min
Response: 3767760452
Conc: 152.10 ng/ml

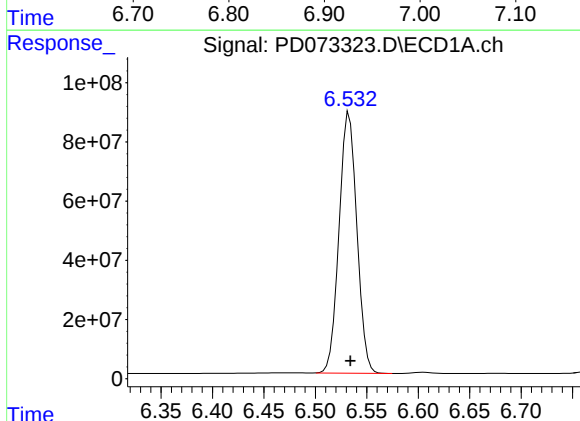


#20 Methoxychlor

R.T.: 6.533 min
Delta R.T.: -0.001 min
Response: 1062400156
Conc: 769.24 ng/ml

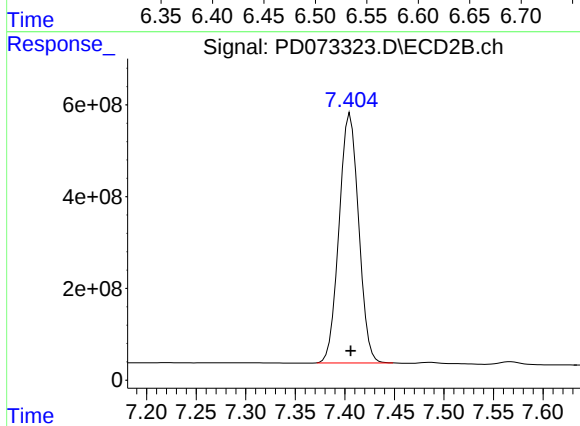

#20 Methoxychlor


R.T.: 7.405 min
Delta R.T.: 0.000 min
Response: 7464471358
Conc: 698.64 ng/ml

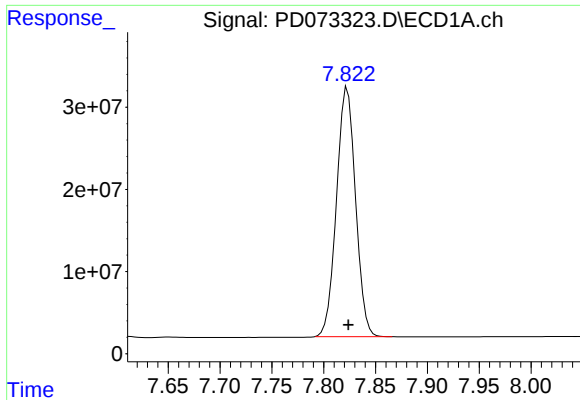

#27 Decachlorobiphenyl

R.T.: 7.823 min
Delta R.T.: 0.000 min
Response: 388252625
Conc: 150.33 ng/ml

Instrument :
ECD_D
ClientSampleId :

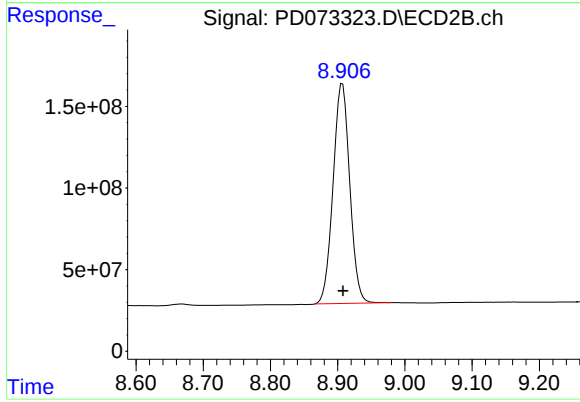

#27 Decachlorobiphenyl

R.T.: 8.907 min
Delta R.T.: -0.001 min
Response: 2307876414
Conc: 144.57 ng/ml