

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121422\
 Data File : PD073319.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Dec 2022 17:33
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA3006

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 05:01:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 15 04:59:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.695	3.456	41989663	1227.5E6	20.000	20.000
27)	SA Decachlor...	7.824	8.908	103.3E6	638.5E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.198	3.920	66033973	1644.0E6	20.000	20.000
3)	MA gamma-BHC...	3.528	4.254	58966531	1328.9E6	20.000	20.000
4)	MA Heptachlor	3.860	4.820	64755072	958.5E6	20.000	20.000
9)	A Endosulfan I	5.012	5.975	54306864	662.4E6	20.000	20.000
13)	MA Dieldrin	5.278	6.252	120.3E6	1391.3E6	40.000	40.000
14)	MA Endrin	5.555	6.485	108.6E6	1151.3E6	40.000	40.000
16)	A 4,4'-DDD	5.702	6.619	96244831	1042.2E6	40.000	40.000
17)	MA 4,4'-DDT	5.951	6.926	96888548	990.9E6	40.000	40.000
20)	A Methoxychlor	6.534	7.406	276.2E6	2136.9E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121422\
Data File : PD073319.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Dec 2022 17:33
Operator : AR\AJ
Sample : INDA3001
Misc :
ALS Vial : 13 Sample Multiplier: 1


Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 05:01:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121422CLP.M
Quant Title : GC Extractables
Qlast Update : Thu Dec 15 04:59:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm
Signal #2 Phase: ZB-MR1

Signal: PD073319.D\ECD1A.ch

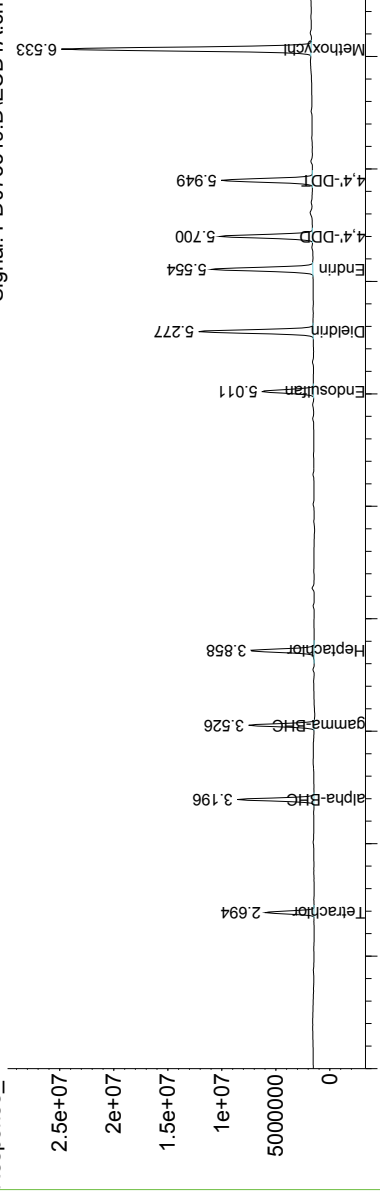

Signal: PD073319.D\ECD2B.ch

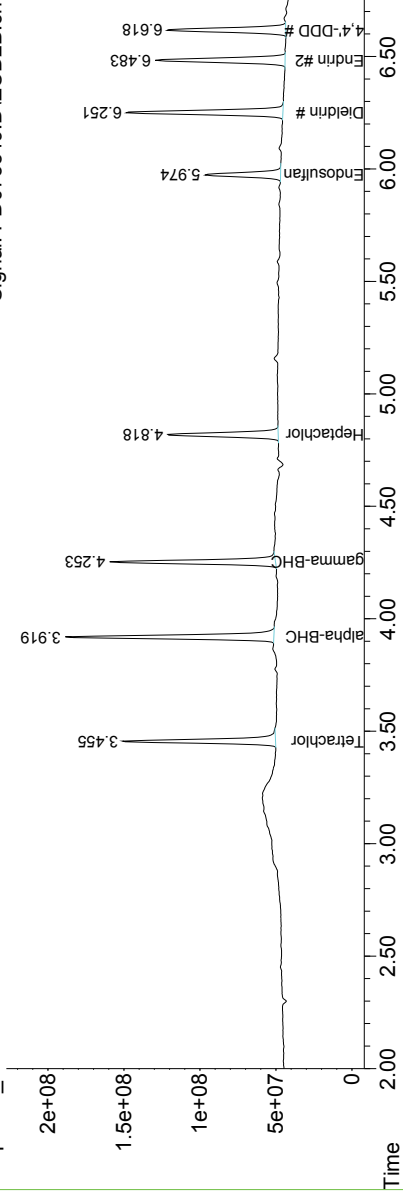

Instrument :
ECD_D
ClientSampleId :
INDA3006