

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121422\
 Data File : PD073317.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Dec 2022 17:06
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA2004

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 05:05:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 15 05:05:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.695	3.456	22409184	690.5E6	10.202	10.211
27)	SA Decachlor...	7.822	8.907	54802746	339.3E6	20.292	20.487
Target Compounds							
2)	A alpha-BHC	3.198	3.919	32964412	938.4E6	10.190	10.241
3)	MA gamma-BHC...	3.528	4.253	29209426	770.2E6	10.162	10.219
4)	MA Heptachlor	3.860	4.819	33132904	545.7E6	10.193	10.232
9)	A Endosulfan I	5.012	5.974	28063784	360.2E6	10.222	10.258
13)	MA Dieldrin	5.278	6.251	60179434	746.2E6	20.342	20.478
14)	MA Endrin	5.555	6.483	53948201	613.0E6	20.319	20.321
16)	A 4,4'-DDD	5.701	6.617	47902780	552.1E6	20.408	20.388
17)	MA 4,4'-DDT	5.950	6.925	46861569	518.1E6	20.338	20.524
20)	A Methoxychlor	6.533	7.405	141.3E6	1141.2E6	101.919	101.724


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121422\
Data File : PD073317.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Dec 2022 17:06
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1


Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 05:05:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121422CLP.M
Quant Title : GC Extractables
Qlast Update : Thu Dec 15 05:05:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm
Signal #2 Phase: ZB-MR1

Signal: PD073317.D\ECD1A.ch

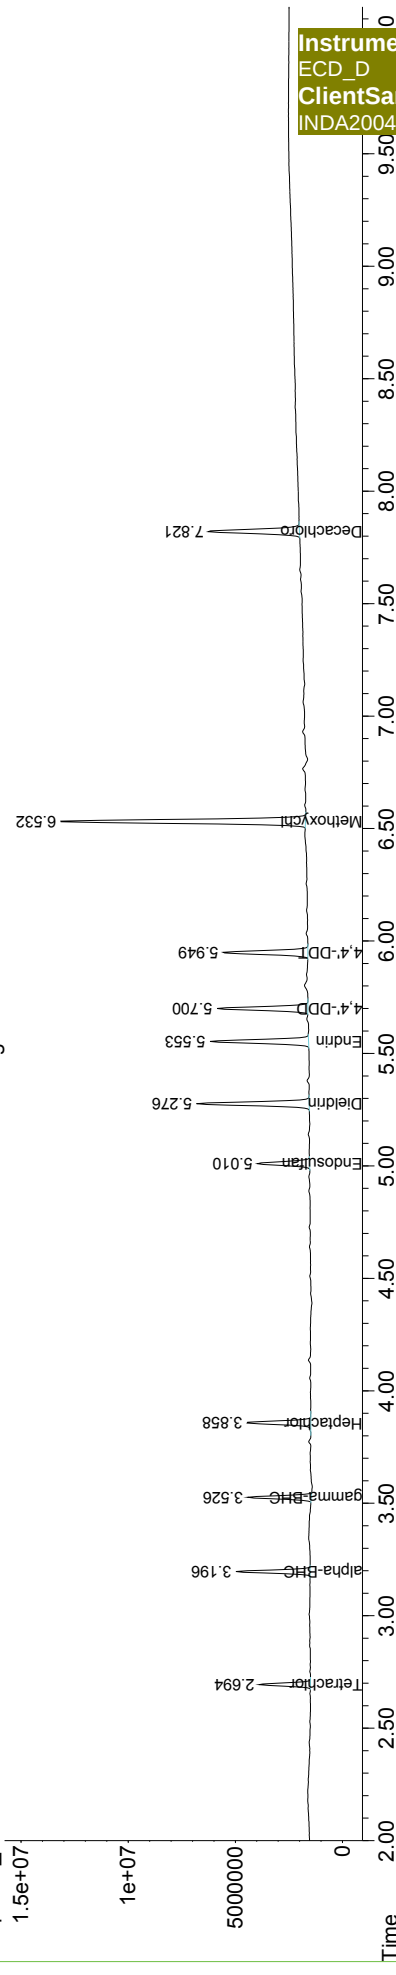

Signal: PD073317.D\ECD2B.ch

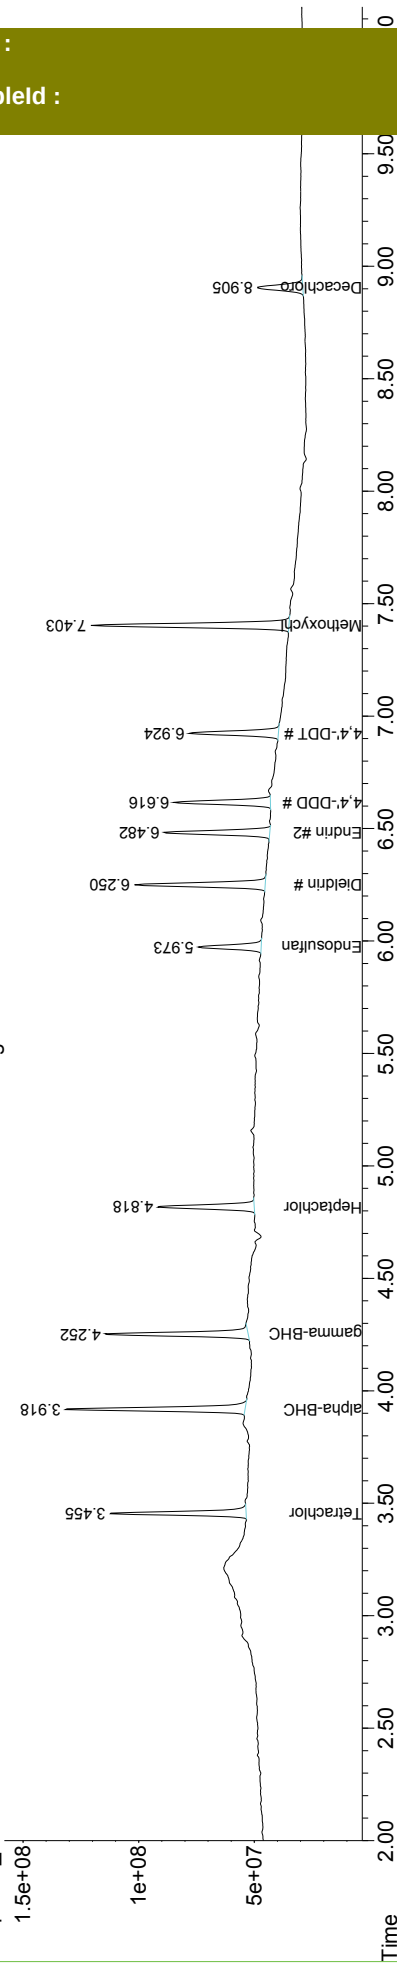

Instrument :
ECD_D
ClientSampleId :
INDA2004