

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121422\
 Data File : PD073321.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Dec 2022 17:59
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA4008

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 05:07:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 15 05:06:56 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.695	3.456	82374616	2485.0E6	38.097	37.511
27)	SA Decachlor...	7.822	8.906	193.5E6	1194.5E6	73.580	73.946
Target Compounds							
2)	A alpha-BHC	3.198	3.920	138.0E6	3298.3E6	41.970	36.919
3)	MA gamma-BHC...	3.528	4.254	121.6E6	2594.7E6	41.701	35.670
4)	MA Heptachlor	3.859	4.819	130.9E6	1827.3E6	40.194	35.538
9)	A Endosulfan I	5.012	5.974	108.1E6	1248.7E6	39.527	36.577
13)	MA Dieldrin	5.278	6.251	244.5E6	2658.2E6	81.970	74.590
14)	MA Endrin	5.554	6.483	218.3E6	2202.6E6	81.640	74.645
16)	A 4,4'-DDD	5.701	6.618	194.0E6	1979.9E6	81.965	74.725
17)	MA 4,4'-DDT	5.950	6.925	197.2E6	1905.2E6	84.120	76.551
20)	A Methoxychlor	6.533	7.405	528.4E6	3964.3E6	385.629	363.986


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121422\
Data File : PD073321.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Dec 2022 17:59
Operator : AR\AJ
Sample : INDA4001
Misc :
ALS Vial : 15 Sample Multiplier: 1


Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 05:07:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121422CLP.M
Quant Title : GC Extractables
Qlast Update : Thu Dec 15 05:06:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm
Signal #2 Phase: ZB-MR1

Signal: PD073321.D\ECD1A.ch

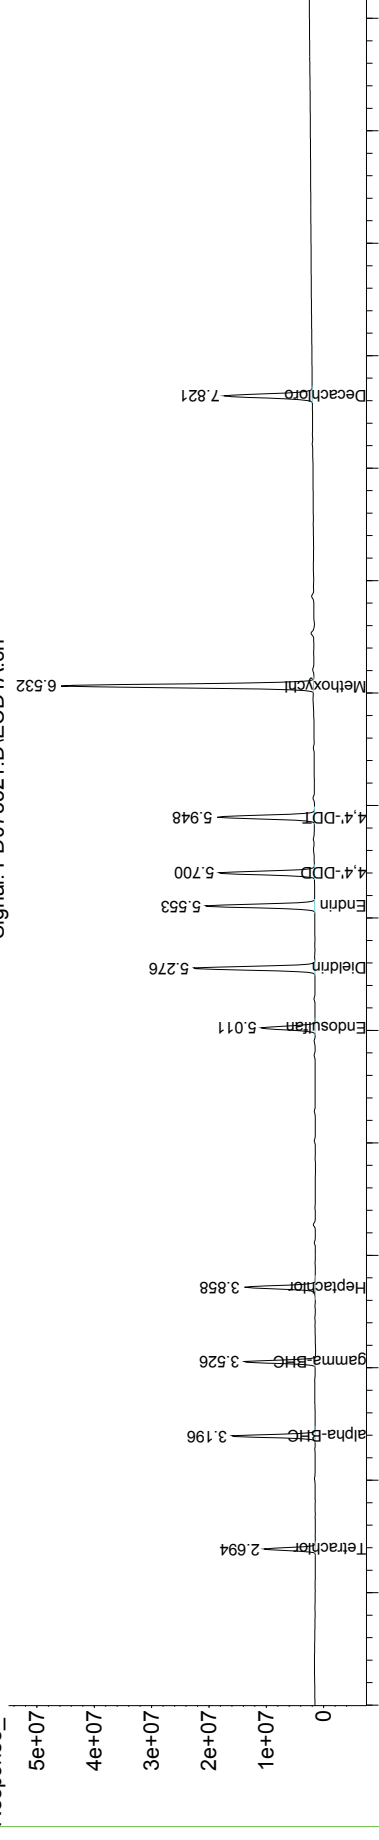

Signal: PD073321.D\ECD2B.ch

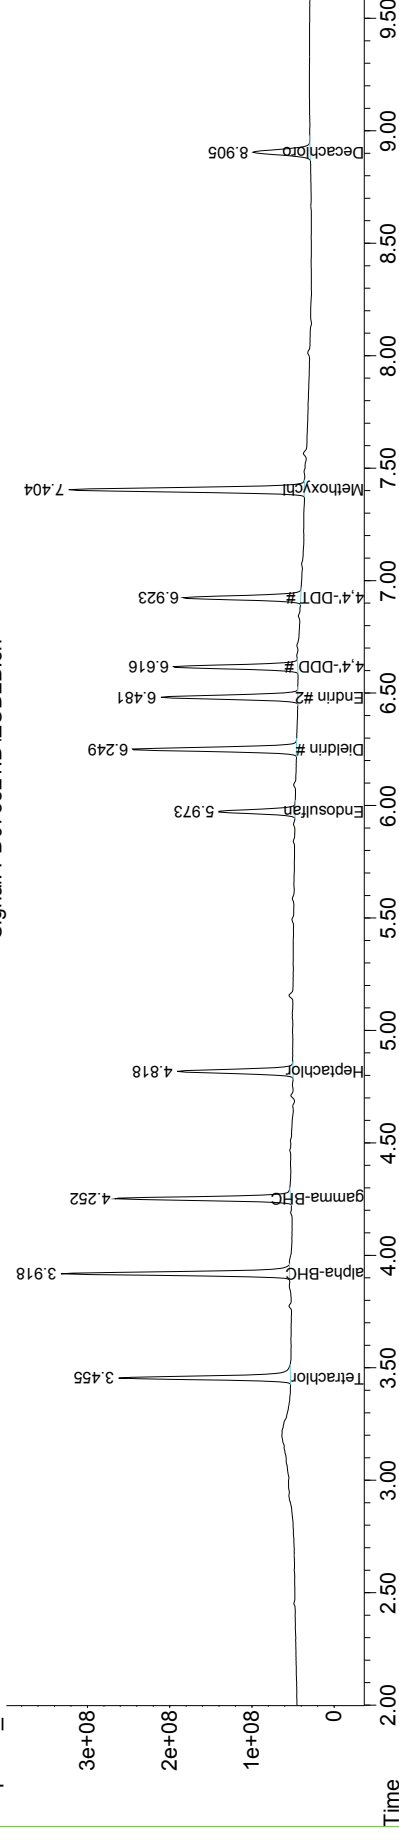

Instrument :
ECD_D
ClientSampleId :
INDA4008