

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121422\
 Data File : PD073323.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Dec 2022 18:26
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA5010

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 05:08:45 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 15 05:08:38 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.695	3.456	165.2E6	4667.5E6	77.107	72.177
27)	SA Decachlor...	7.823	8.907	388.3E6	2307.9E6	149.926	145.997
Target Compounds							
2)	A alpha-BHC	3.197	3.920	289.3E6	6391.5E6	86.247	73.088
3)	MA gamma-BHC...	3.527	4.254	255.9E6	4921.9E6	86.084	69.816
4)	MA Heptachlor	3.859	4.820	272.5E6	3389.7E6	82.940	68.328
9)	A Endosulfan I	5.011	5.974	219.3E6	2362.8E6	80.146	71.131
13)	MA Dieldrin	5.278	6.251	505.4E6	5178.7E6	167.469	148.035
14)	MA Endrin	5.555	6.483	455.8E6	4264.3E6	168.288	147.367
16)	A 4,4'-DDD	5.701	6.618	402.4E6	3854.4E6	167.927	148.163
17)	MA 4,4'-DDT	5.950	6.925	422.2E6	3767.8E6	175.672	153.037
20)	A Methoxychlor	6.533	7.405	1062.4E6	7464.5E6	780.179	705.576

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121422\
Data File : PD073323.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Dec 2022 18:26
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 05:08:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121422CLP.M
Quant Title : GC Extractables
Qlast Update : Thu Dec 15 05:08:38 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm
Signal #2 Phase: ZB-MR1


Response_

Signal: PD073323.D\ECD1A.ch

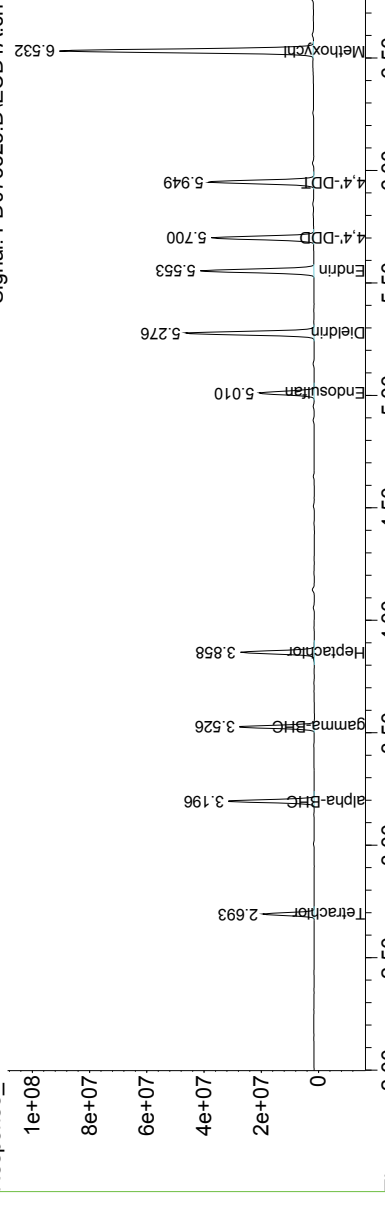

Response_

Signal: PD073323.D\ECD2B.ch

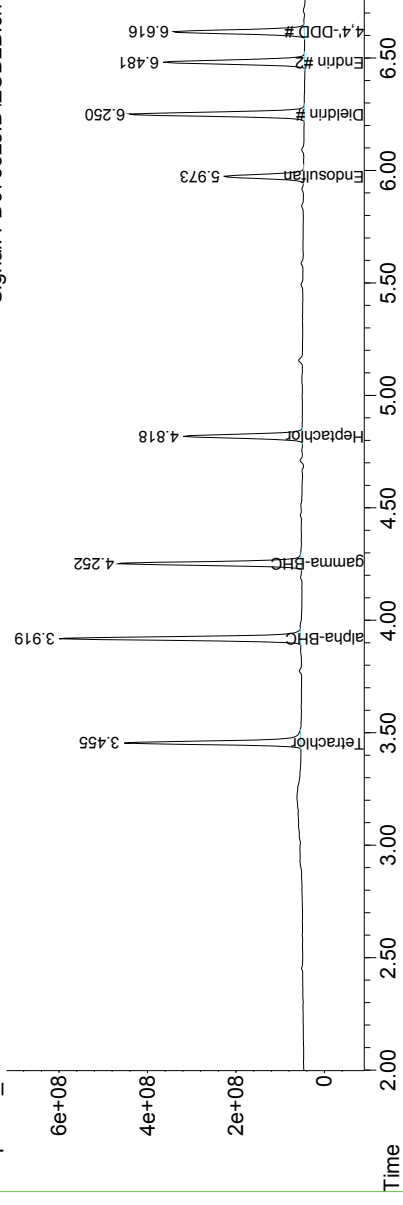

Instrument :
ECD_D
ClientSampleId :
INDA5010