

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121521\
 Data File : PD067331.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Dec 2021 14:20
 Operator : AR\AJ
 Sample : M4971-08MSD
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BG3D6MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/16/2021
 Supervised By : Ankita Jodhani 12/16/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 16 04:24:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112921CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 05:28:01 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.435	3.965	35916065	224.1E6	16.449	27.976 #
27)	SA Decachlor...	8.155	9.020	21449742	112.3E6	18.893	22.139
Target Compounds							
2)	A alpha-BHC	3.871	4.358	140.0E6	548.5E6	42.812	51.124
3)	MA gamma-BHC...	4.152	4.643	141.4E6	507.5E6	44.426	50.587
4)	MA Heptachlor	4.445	5.142	148.0E6	441.7E6	46.167	47.352
5)	MB Aldrin	4.690	5.445	144.1E6	392.4E6	46.568	45.508
6)	B beta-BHC	4.401	4.821	62024868	231.3E6	46.591	50.134
7)	B delta-BHC	4.602	5.035	25836406	107.1E6	9.032	12.104 #
8)	B Heptachlo...	5.130	5.834	140.9E6	353.4E6	51.015	50.426
9)	A Endosulfan I	5.466	6.191	123.6E6	349.1E6	46.473	48.161
10)	B trans-Chl...	5.354	6.068	141.1E6	372.7E6	50.071	49.099
11)	B cis-Chlor...	5.412	6.140	134.7E6	362.0E6	48.534	48.937
12)	B 4,4'-DDE	5.576	6.299	272.3E6	714.1E6	108.785	106.565m
13)	MA Dieldrin	5.708	6.450	290.0E6	739.7E6	100.722	99.415
14)	MA Endrin	5.965	6.669	249.3E6	628.8E6	109.013	108.388
15)	B Endosulfa...	6.237	6.883	217.9E6	595.1E6	97.066	98.024
16)	A 4,4'-DDD	6.090	6.795	200.2E6	549.3E6	94.687	93.929
17)	MA 4,4'-DDT	6.328	7.092	204.8E6	537.5E6	96.340	93.276
18)	B Endrin al...	6.406	7.008	169.4E6	481.3E6	102.753	102.117
19)	B Endosulfa...	6.618	7.231	138.4E6	418.7E6	71.742	72.913
20)	A Methoxychlor	6.876	7.555	468.6E6	1324.0E6	471.553	475.685
21)	B Endrin ke...	7.110	7.703	200.7E6	633.2E6	96.668	95.898m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121521\
Data File : PD067331.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Dec 2021 14:20
Operator : AR\AJ
Sample : M4971-08MSD
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 04:24:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112921CLP.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 05:28:01 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

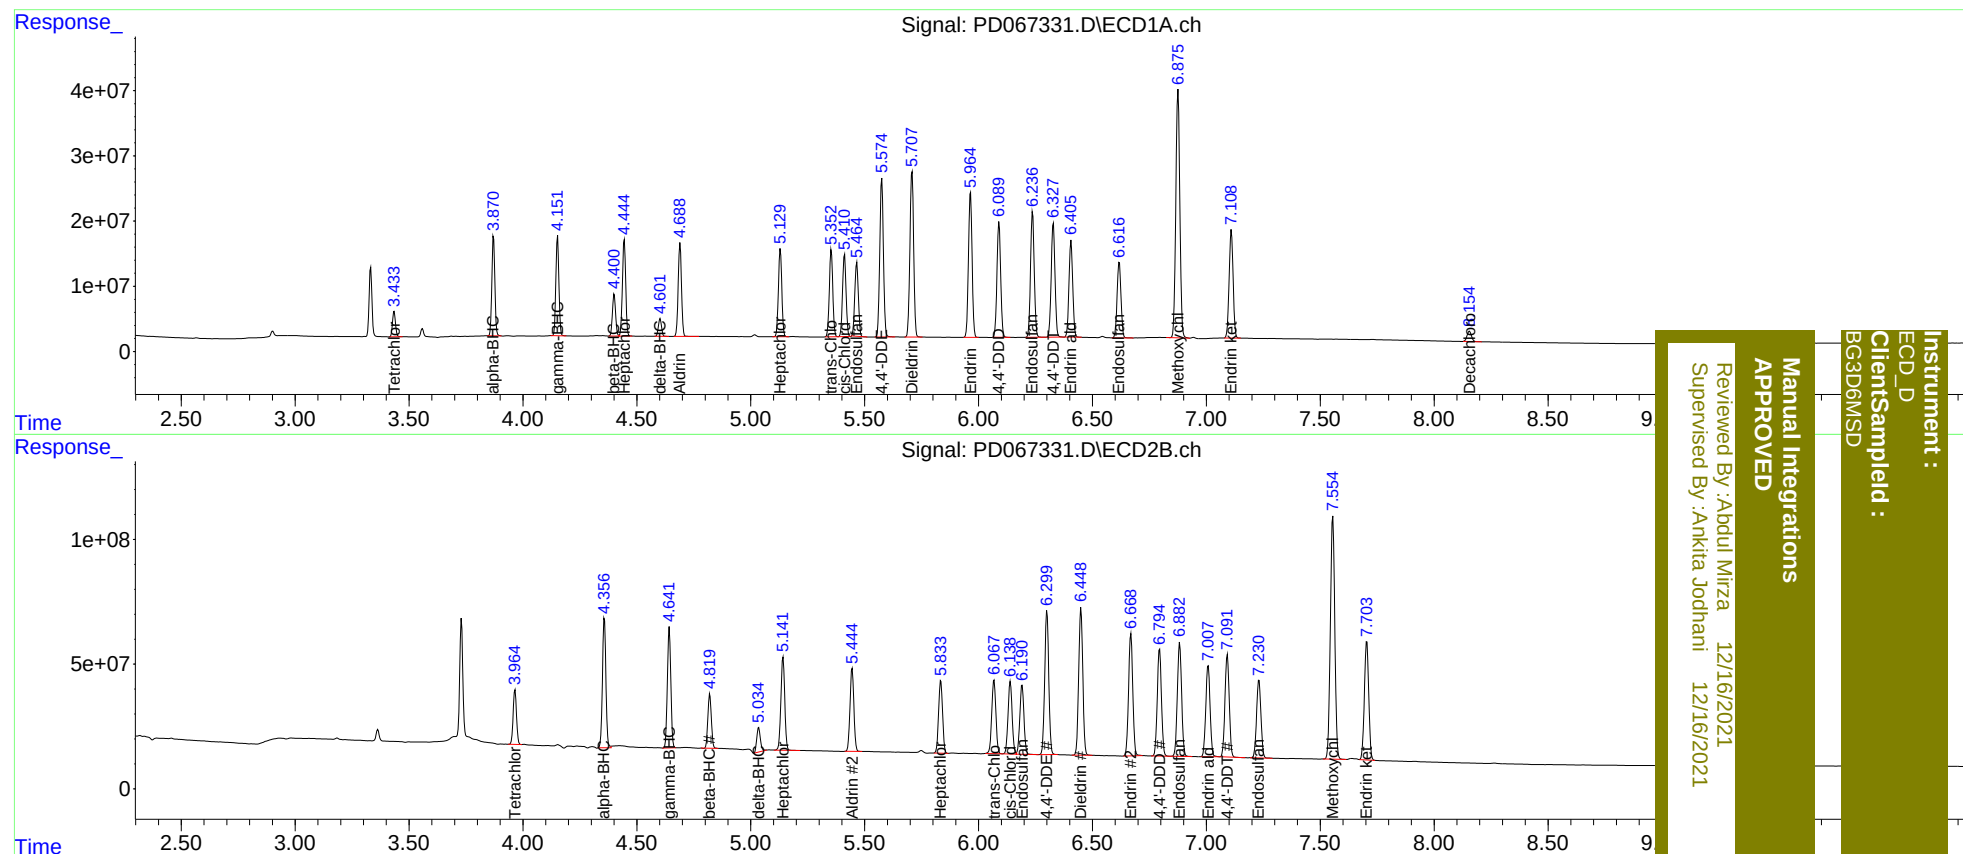

Reviewed By: Abdul Mirza 12/16/2021
Supervised By: Ankita Jodhani 12/16/2021

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
BG3D6MSD