

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121521\
 Data File : PD067358.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Dec 2021 22:18
 Operator : AR\AJ
 Sample : M5037-11MSD
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C00W9MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/16/2021
 Supervised By : Ankita Jodhani 12/16/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 16 04:28:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112921CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 05:28:01 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.435	3.965	40325632	254.0E6	18.468	31.706 #
27)	SA Decachlor...	8.155	9.021	31466575	166.2E6	27.716	32.778
Target Compounds							
2)	A alpha-BHC	3.871	4.358	140.3E6	546.2E6	42.905	50.910
3)	MA gamma-BHC...	4.152	4.643	142.1E6	522.3E6	44.664	52.070
4)	MA Heptachlor	4.445	5.143	157.4E6	483.4E6	49.105	51.823
5)	MB Aldrin	4.690	5.445	155.6E6	436.6E6	50.302	50.629
6)	B beta-BHC	4.401	4.821	62869573	244.7E6	47.226	53.032
7)	B delta-BHC	4.603	5.036	26276633	109.3E6	9.186	12.347 #
8)	B Heptachlo...	5.131	5.835	141.0E6	370.2E6	51.044	52.816
9)	A Endosulfan I	5.467	6.191	123.9E6	361.7E6	46.613	49.897
10)	B trans-Chl...	5.354	6.069	141.6E6	385.2E6	50.273	50.755
11)	B cis-Chlor...	5.412	6.140	134.8E6	374.6E6	48.561	50.642
12)	B 4,4'-DDE	5.576	6.300	270.1E6	728.2E6	107.914	108.675
13)	MA Dieldrin	5.708	6.450	288.2E6	753.2E6	100.091	101.223
14)	MA Endrin	5.965	6.669	242.2E6	628.3E6	105.910	108.304
15)	B Endosulfa...	6.238	6.884	219.2E6	611.3E6	97.627	100.698
16)	A 4,4'-DDD	6.090	6.796	197.5E6	558.9E6	93.403	95.574
17)	MA 4,4'-DDT	6.328	7.092	202.3E6	548.1E6	95.176	95.119
18)	B Endrin al...	6.406	7.009	169.9E6	495.1E6	103.053	105.052
19)	B Endosulfa...	6.618	7.232	139.7E6	432.0E6	72.391	75.223
20)	A Methoxychlor	6.876	7.555	456.2E6	1313.3E6	459.067	471.848
21)	B Endrin ke...	7.110	7.704	203.6E6	653.0E6	98.062	98.886m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121521\
Data File : PD067358.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Dec 2021 22:18
Operator : AR\AJ
Sample : M5037-11MSD
Misc :
ALS Vial : 38 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 04:28:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112921CLP.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 05:28:01 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

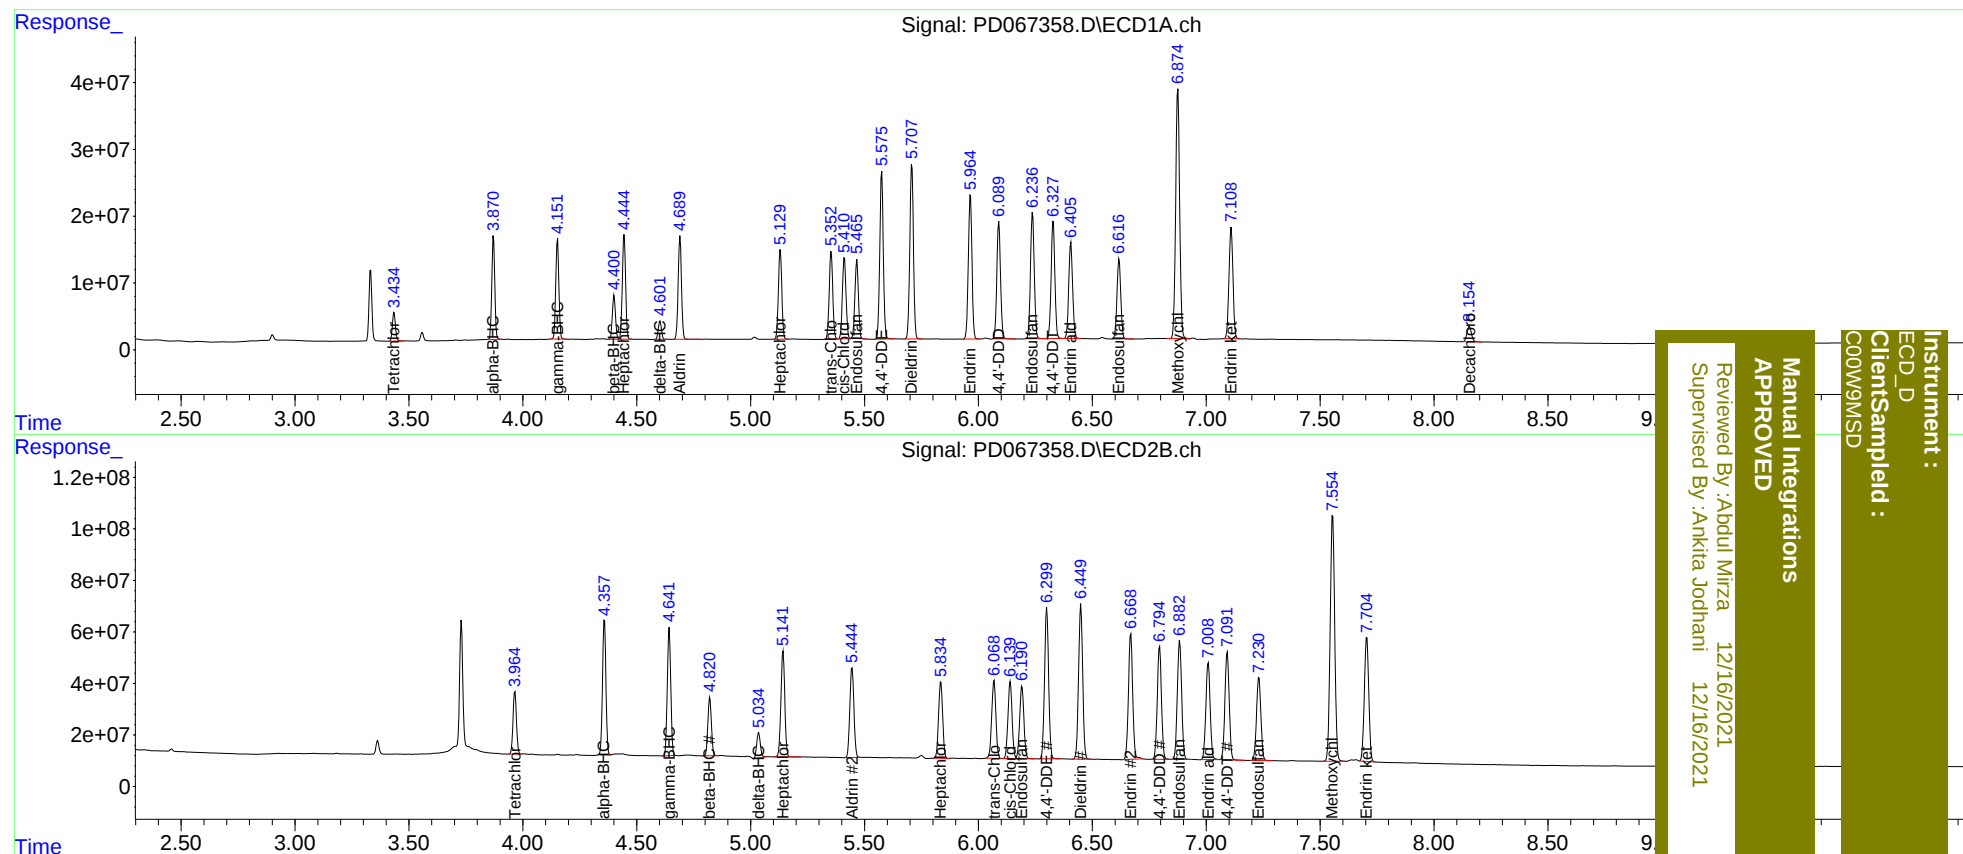

Reviewed By: Abdul Mirza 12/16/2021
Supervised By: Ankita Jodhani 12/16/2021

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
C00W9MSD