

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121523\
 Data File : PD080088.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Dec 2023 09:44
 Operator : AR\AJ
 Sample : 05796-04
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RT-SB-04-13-14

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/15/2023
 Supervised By :Ankita Jodhani 12/15/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 01:02:25 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120623.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 06 14:11:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.566	2.801	22572399	39907725	14.976m	15.875
2) SA Decachlor...	9.110	7.943	13766641	26688599	6.801m	9.468m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121523\
Data File : PD080088.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Dec 2023 09:44
Operator : AR\AJ
Sample : 05796-04
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
RT-SB-04-13-14


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/15/2023
Supervised By : Ankita Jodhani 12/15/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 01:02:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD120623.M
Quant Title : GC Extractables
QLast Update : Wed Dec 06 14:11:45 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

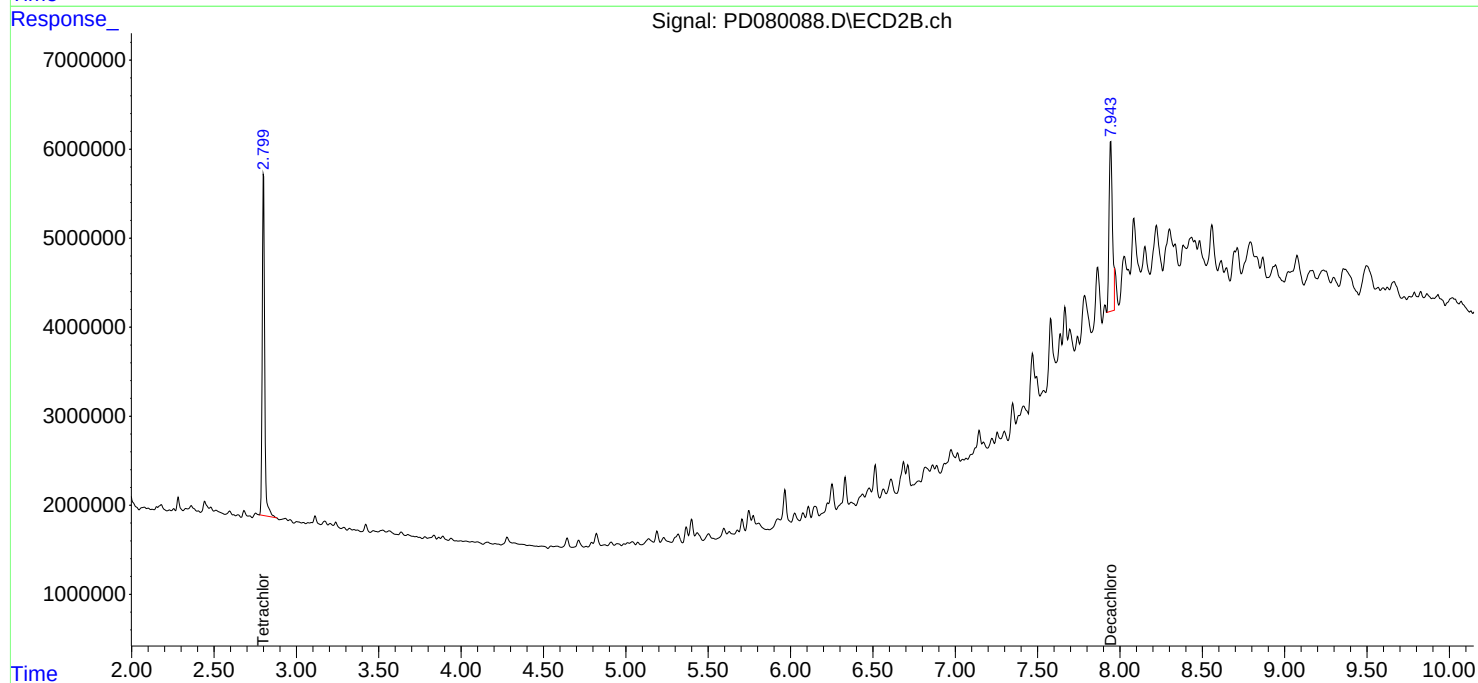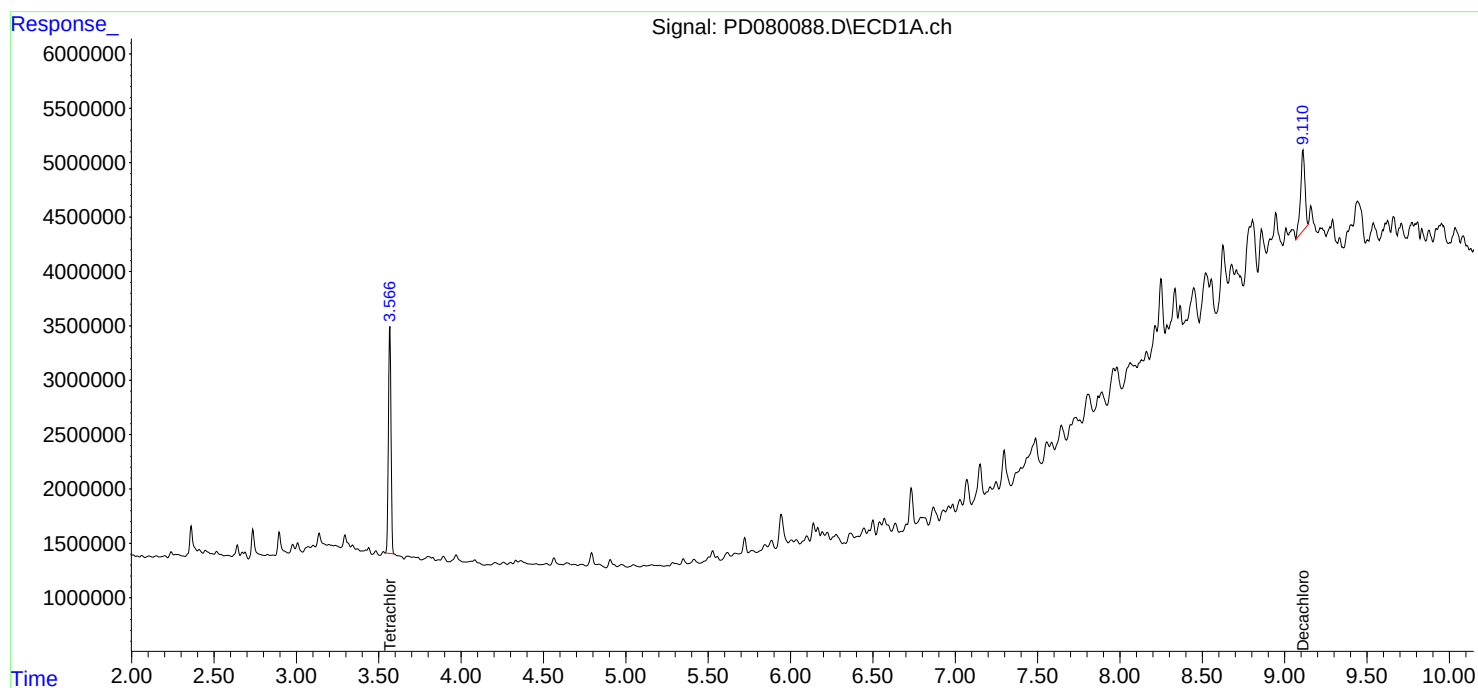

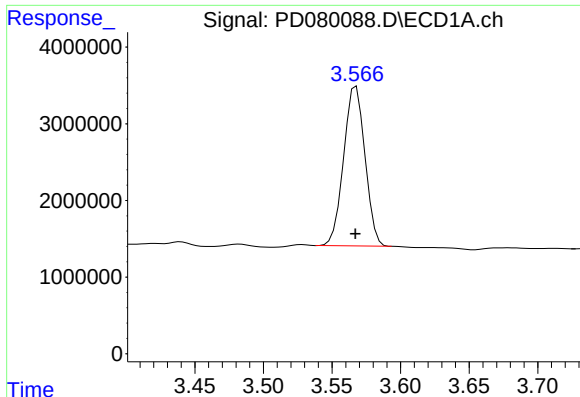


#1 Tetrachloro-m-xylene

R.T.: 3.566 min
Delta R.T.: 0.000 min
Response: 22572399
Conc: 14.98 ng/ml

Instrument :
ECD_D
ClientSampleId :
RT-SB-04-13-14


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/15/2023
Supervised By :Ankita Jodhani 12/15/2023

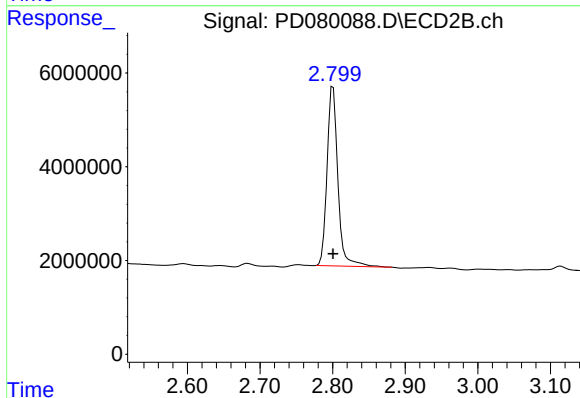


#1 Tetrachloro-m-xylene

R.T.: 2.801 min
Delta R.T.: 0.000 min
Response: 39907725
Conc: 15.88 ng/ml

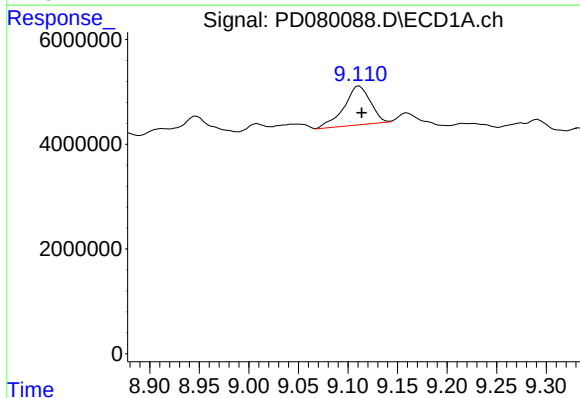

#28 Decachlorobiphenyl

R.T.: 9.110 min
Delta R.T.: -0.004 min
Response: 13766641
Conc: 6.80 ng/ml m

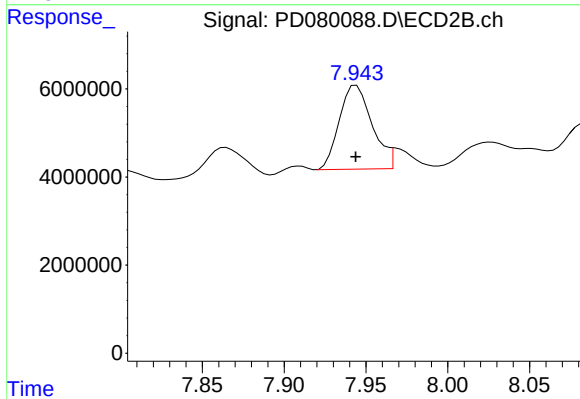

#28 Decachlorobiphenyl

R.T.: 7.943 min
Delta R.T.: -0.001 min
Response: 26688599
Conc: 9.47 ng/ml m