

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121620\
 Data File : PD060744.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Dec 2020 19:32
 Operator : DD\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 03:39:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121620.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 17 03:37:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.500	0.000	6535813	0	5.115	N.D. #
28)	SA Decachlor...	8.287	0.000	8007906	0	5.837	N.D. #
Target Compounds							
23)	Chlordane-1	4.379	0.000	1718197	0	42.583	N.D. #
24)	Chlordane-2	4.884	0.000	2477744	0	52.347	N.D. #
25)	Chlordane-3	5.458	0.000	6426296	0	47.312	N.D. #
26)	Chlordane-4	5.516	0.000	5296505	0	48.197	N.D. #
27)	Chlordane-5	6.358	0.000	2565222	0	51.650	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121620\
Data File : PD060744.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Dec 2020 19:32
Operator : DD\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 03:39:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121620.M
Quant Title : GC Extractables
QLast Update : Thu Dec 17 03:37:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

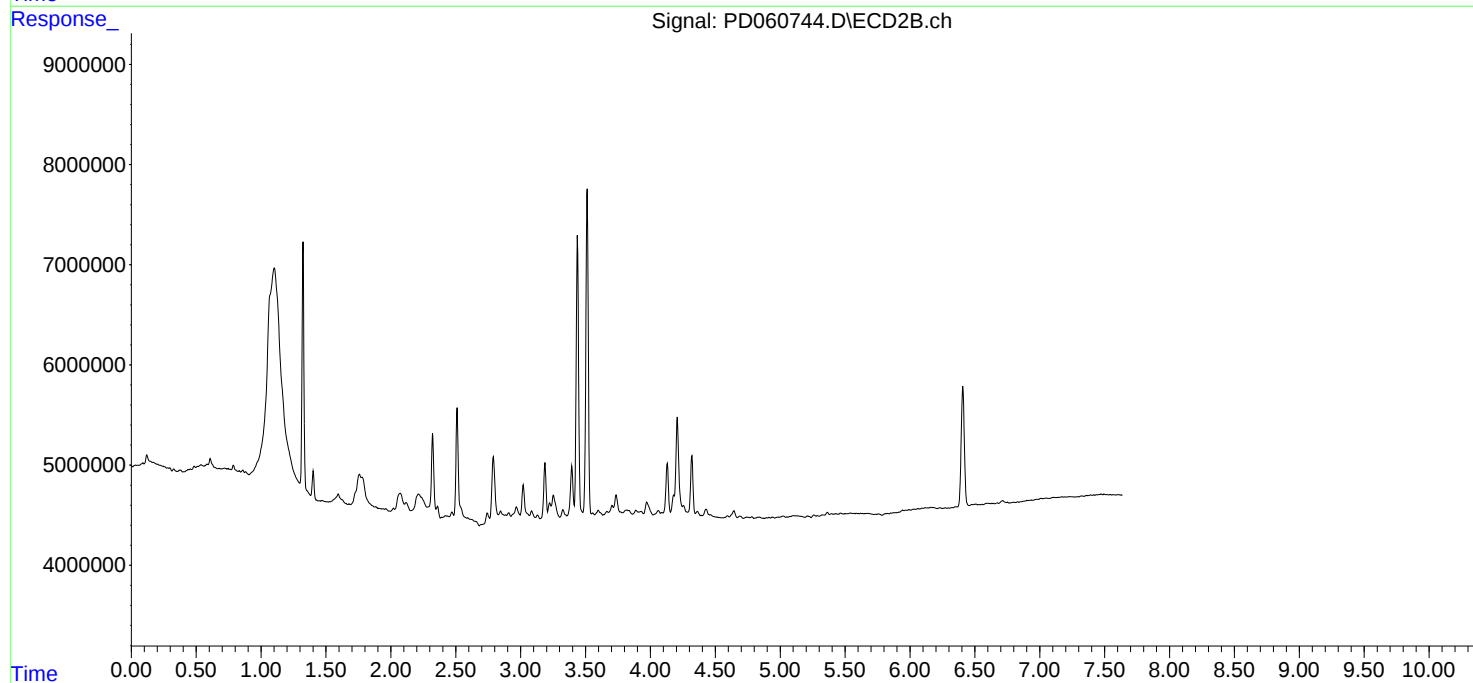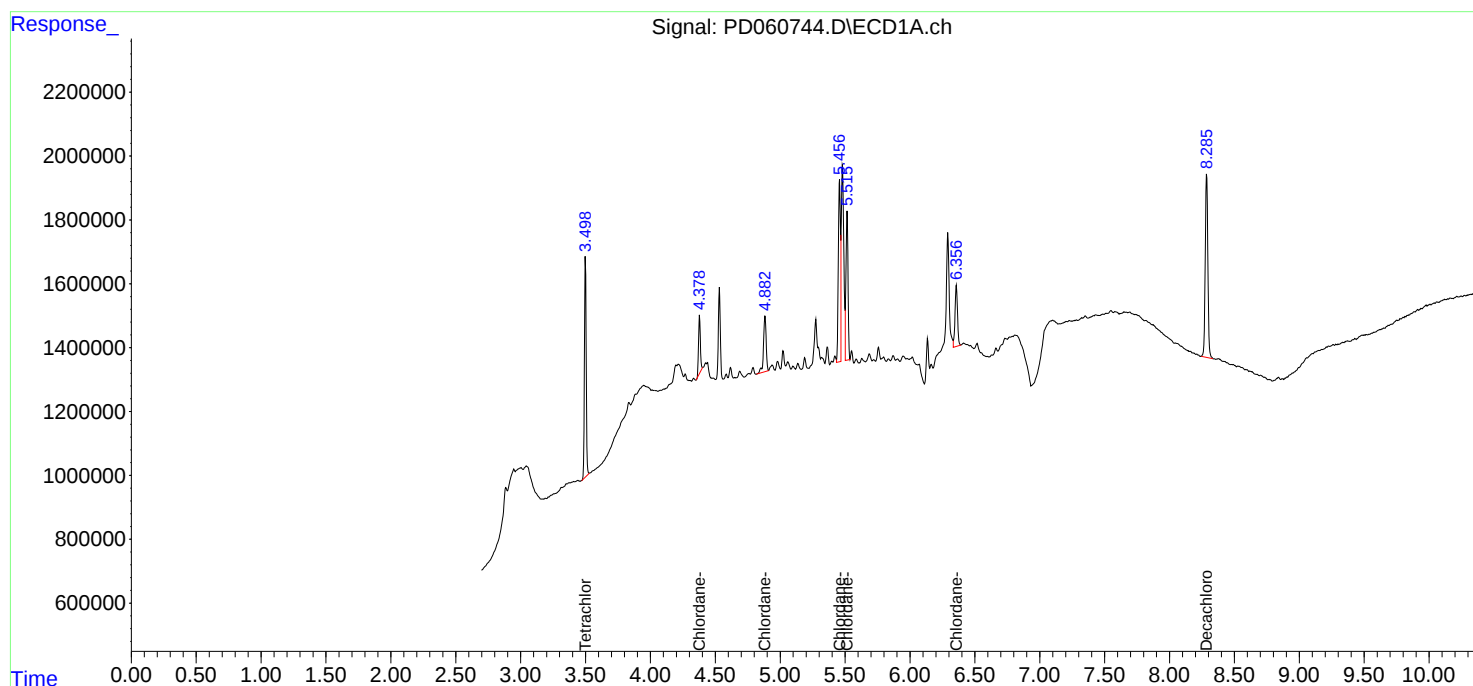


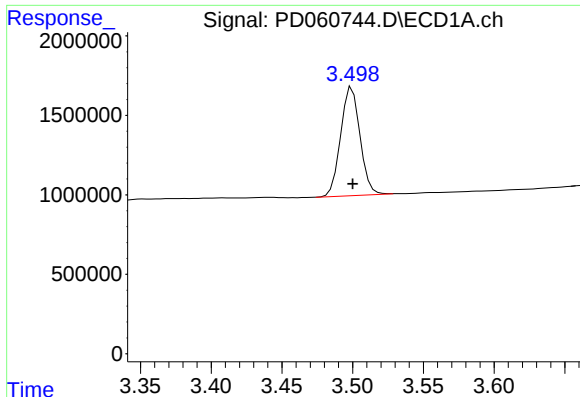

#1 Tetrachloro-m-xylene


R.T.: 3.500 min
Delta R.T.: 0.000 min
Response: 6535813
Conc: 5.12 ng/ml

Instrument :
ECD_D
ClientSampleId :

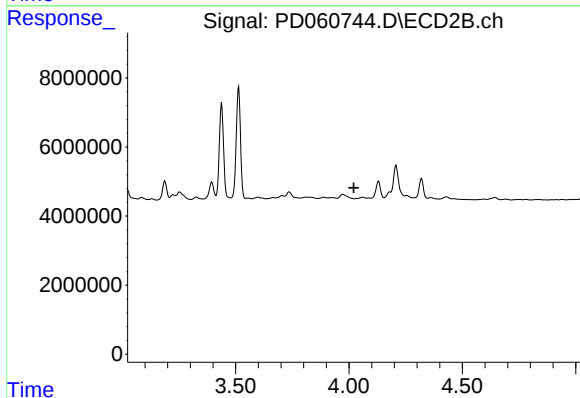


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.021 min
Response: 0
Conc: N.D.

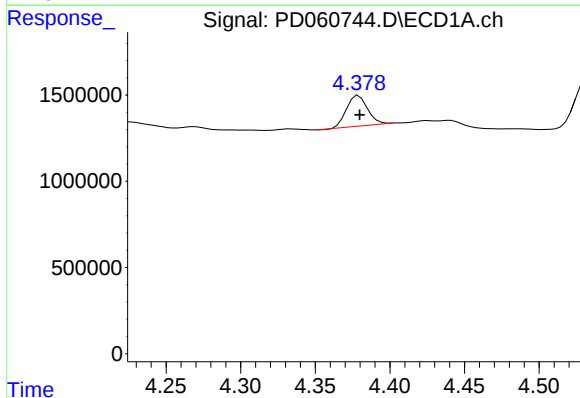


#23 Chlordane-1

R.T.: 4.379 min
Delta R.T.: 0.000 min
Response: 1718197
Conc: 42.58 ng/ml

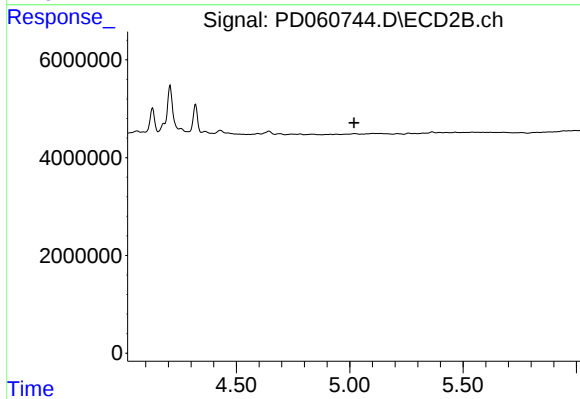

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.020 min
Response: 0
Conc: N.D.

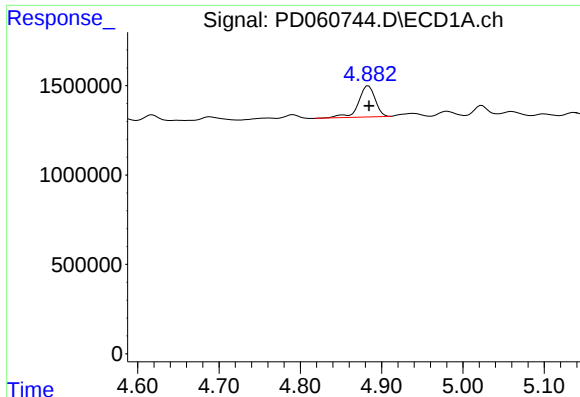

#24 Chlordane-2


R.T.: 4.884 min
Delta R.T.: 0.000 min
Response: 2477744
Conc: 52.35 ng/ml

Instrument :
ECD_D
ClientSampleId :

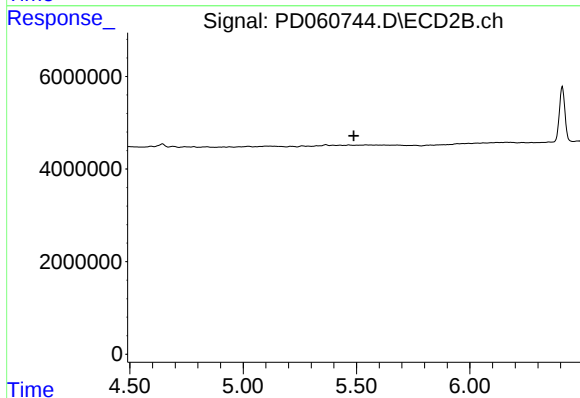


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.488 min
Response: 0
Conc: N.D.

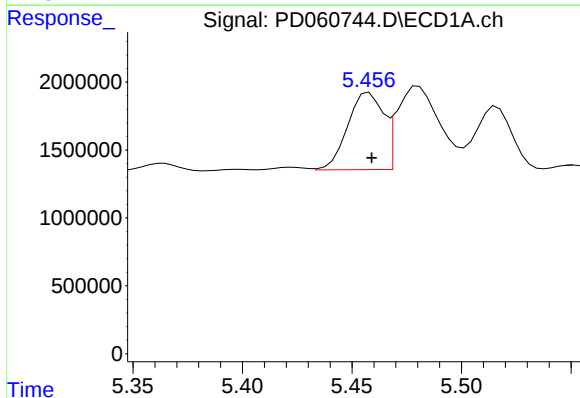


#25 Chlordane-3

R.T.: 5.458 min
Delta R.T.: -0.001 min
Response: 6426296
Conc: 47.31 ng/ml

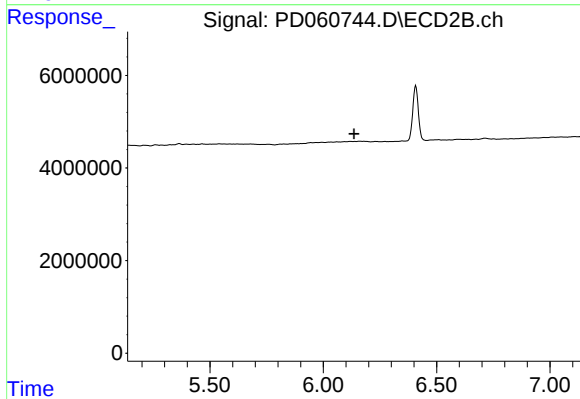

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.136 min
Response: 0
Conc: N.D.

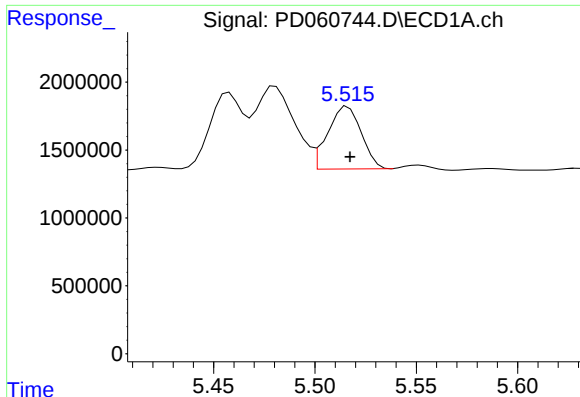

#26 Chlordane-4


R.T.: 5.516 min
Delta R.T.: -0.001 min
Response: 5296505
Conc: 48.20 ng/ml

Instrument :
ECD_D
ClientSampleId :

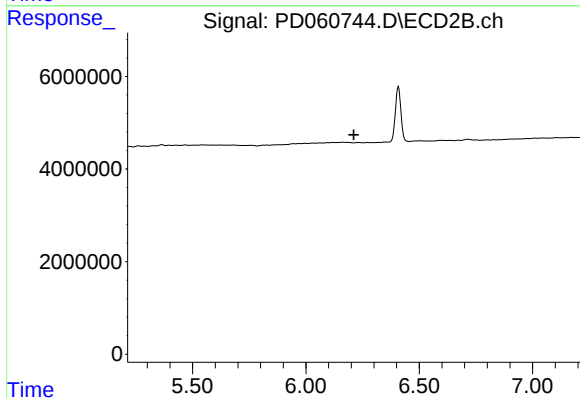


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.211 min
Response: 0
Conc: N.D.

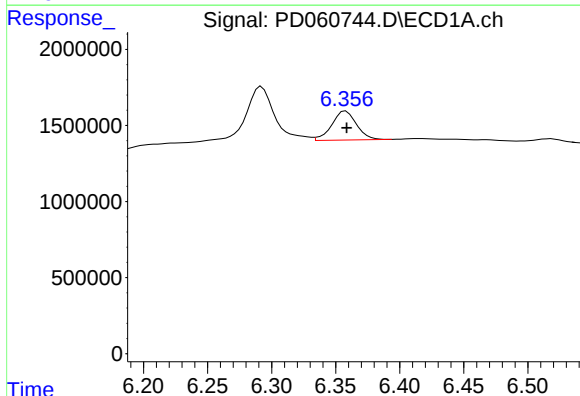


#27 Chlordane-5

R.T.: 6.358 min
Delta R.T.: 0.000 min
Response: 2565222
Conc: 51.65 ng/ml

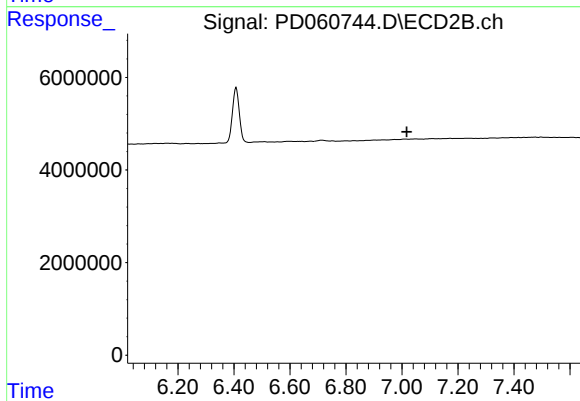

#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.017 min
Response: 0
Conc: N.D.

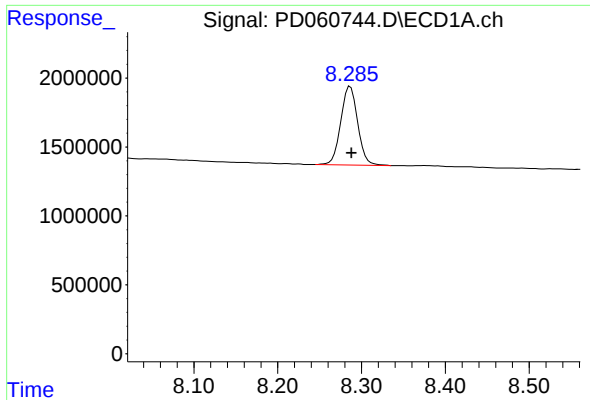

#28 Decachlorobiphenyl


R.T.: 8.287 min

Delta R.T.: -0.001 min

Response: 8007906

Conc: 5.84 ng/ml

Instrument :
ECD_D
ClientSampleId :

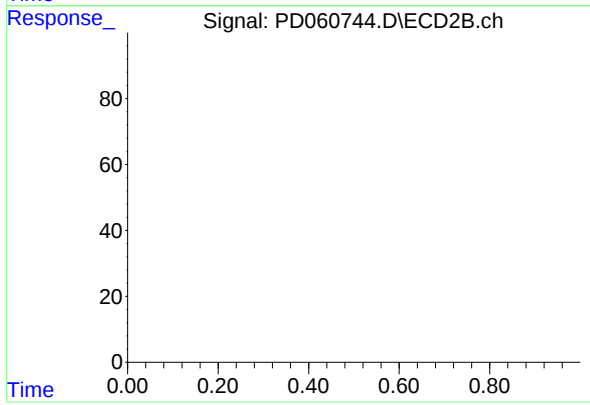

#28 Decachlorobiphenyl

R.T.: 0.000 min

Exp R.T. : 9.104 min

Response: 0

Conc: N.D.