

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121620\
 Data File : PD060740.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Dec 2020 18:36
 Operator : DD\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 03:37:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121620.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 17 03:37:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.501	4.021	124.4E6	446.4E6	97.341	95.187
28)	SA Decachlor...	8.288	9.105	128.4E6	341.1E6	93.600	93.534
Target Compounds							
23)	Chlordane-1	4.380	5.020	38421788	172.8E6	952.229	946.569
24)	Chlordane-2	4.885	5.488	43871425	176.6E6	926.875	918.000
25)	Chlordane-3	5.460	6.137	134.5E6	682.4E6	990.476	961.252
26)	Chlordane-4	5.517	6.212	109.5E6	791.0E6	996.622	954.597
27)	Chlordane-5	6.359	7.018	47851987	147.1E6	963.491	956.765



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121620\
Data File : PD060740.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Dec 2020 18:36
Operator : DD\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 03:37:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121620.M
Quant Title : GC Extractables
QLast Update : Thu Dec 17 03:37:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

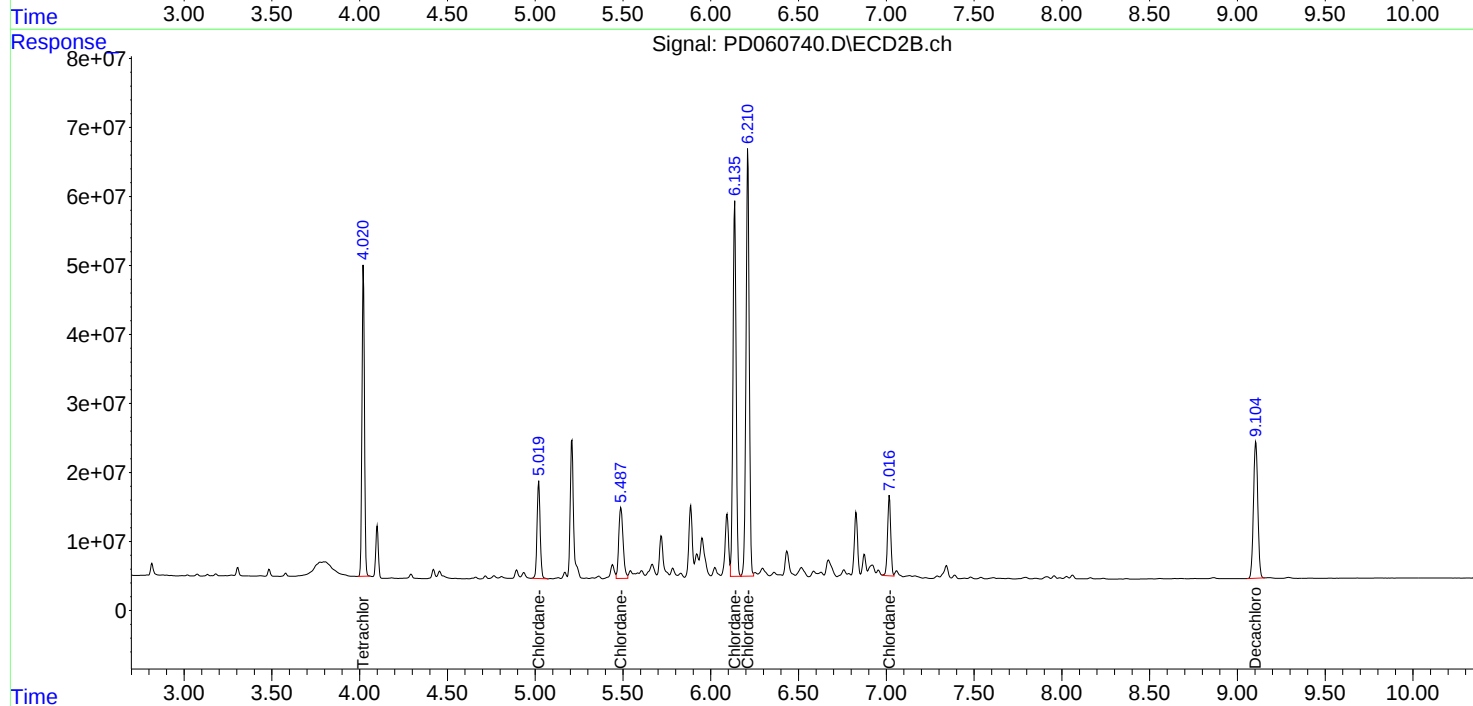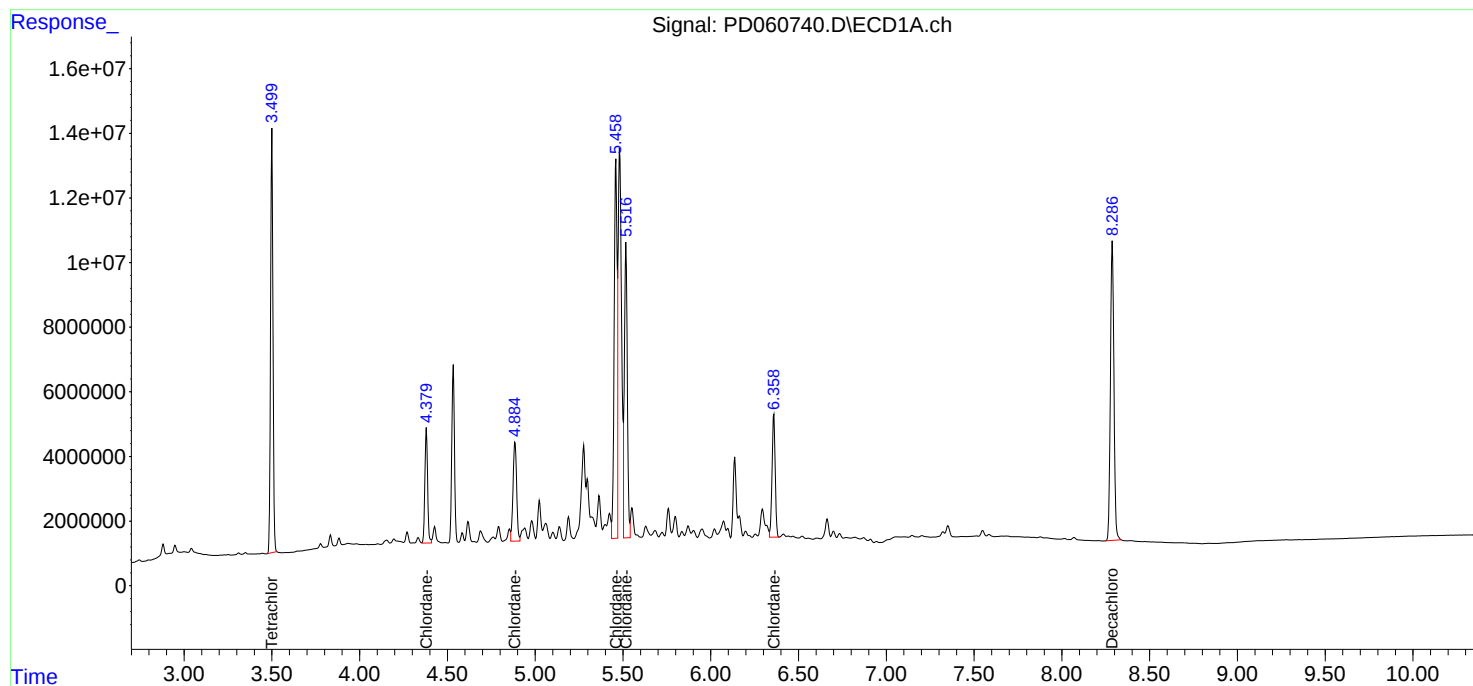


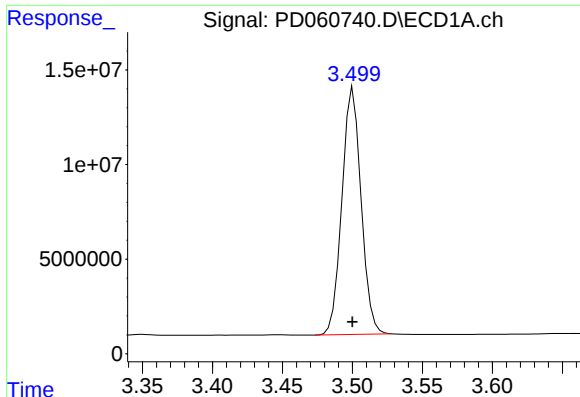

#1 Tetrachloro-m-xylene


R.T.: 3.501 min
Delta R.T.: 0.000 min
Response: 124370720
Conc: 97.34 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

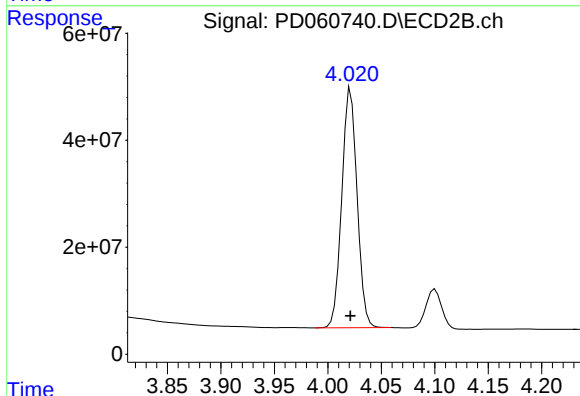


#1 Tetrachloro-m-xylene

R.T.: 4.021 min
Delta R.T.: 0.000 min
Response: 446385590
Conc: 95.19 ng/ml

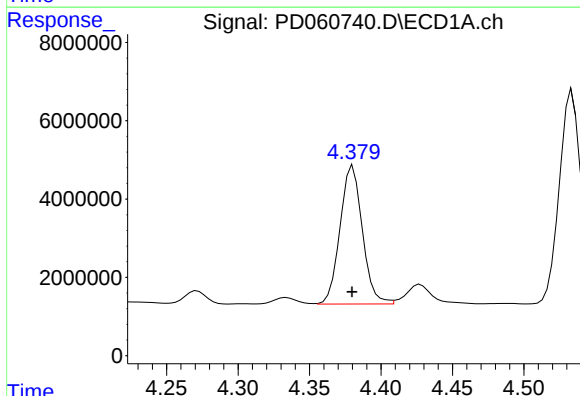


#23 Chlordane-1

R.T.: 4.380 min
Delta R.T.: 0.000 min
Response: 38421788
Conc: 952.23 ng/ml

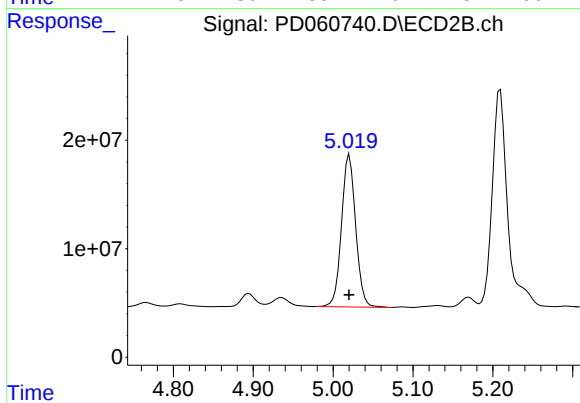

#23 Chlordane-1


R.T.: 5.020 min
Delta R.T.: 0.000 min
Response: 172795411
Conc: 946.57 ng/ml

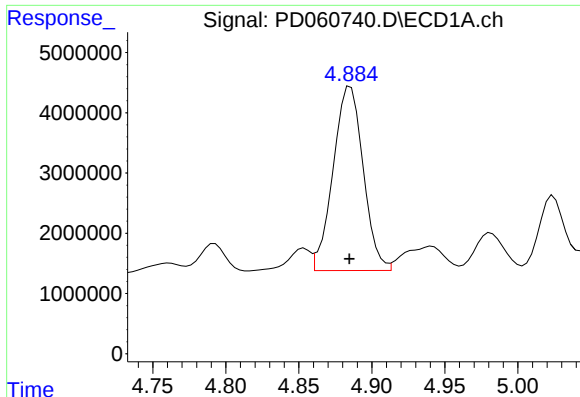

#24 Chlordane-2


R.T.: 4.885 min
Delta R.T.: 0.000 min
Response: 43871425
Conc: 926.87 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

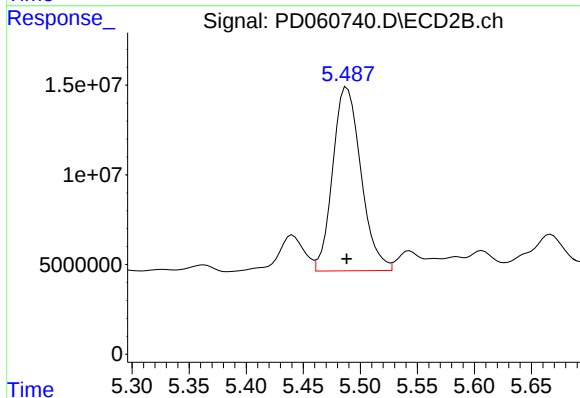


#24 Chlordane-2

R.T.: 5.488 min
Delta R.T.: 0.000 min
Response: 176564853
Conc: 918.00 ng/ml

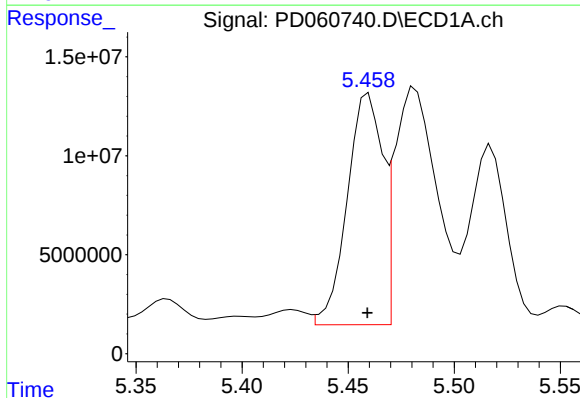


#25 Chlordane-3

R.T.: 5.460 min
Delta R.T.: 0.000 min
Response: 134534743
Conc: 990.48 ng/ml

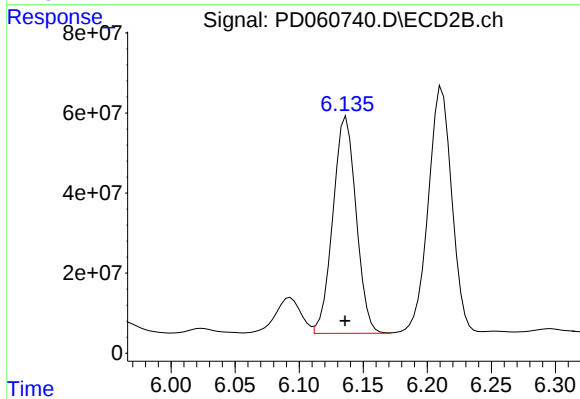

#25 Chlordane-3


R.T.: 6.137 min
Delta R.T.: 0.000 min
Response: 682438311
Conc: 961.25 ng/ml

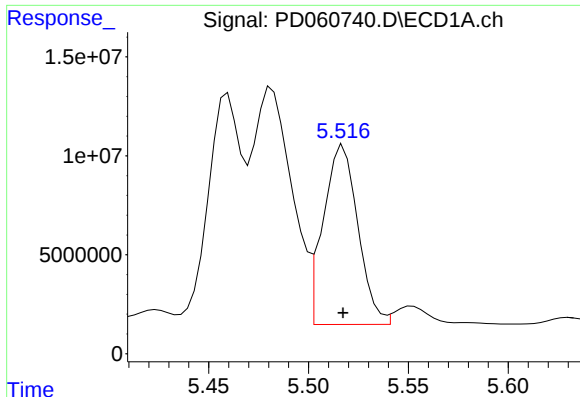

#26 Chlordane-4


R.T.: 5.517 min
Delta R.T.: 0.000 min
Response: 109521466
Conc: 996.62 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

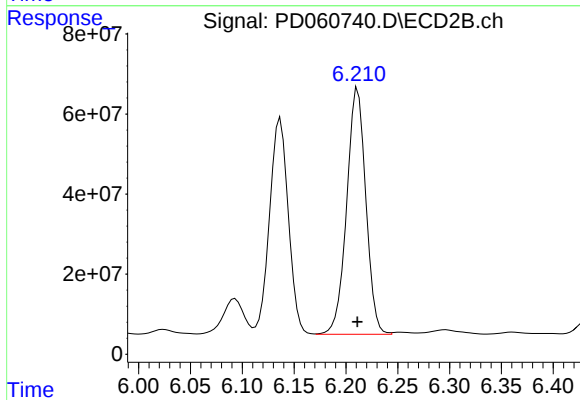


#26 Chlordane-4

R.T.: 6.212 min
Delta R.T.: 0.000 min
Response: 791031520
Conc: 954.60 ng/ml

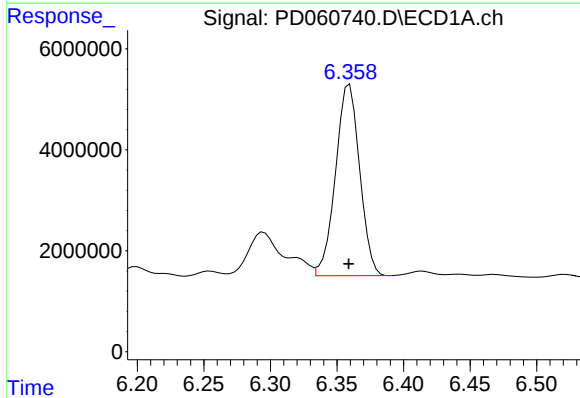


#27 Chlordane-5

R.T.: 6.359 min
Delta R.T.: 0.000 min
Response: 47851987
Conc: 963.49 ng/ml

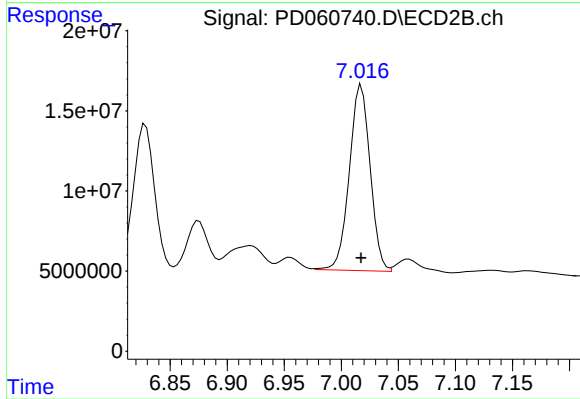

#27 Chlordane-5


R.T.: 7.018 min
Delta R.T.: 0.000 min
Response: 147142758
Conc: 956.77 ng/ml

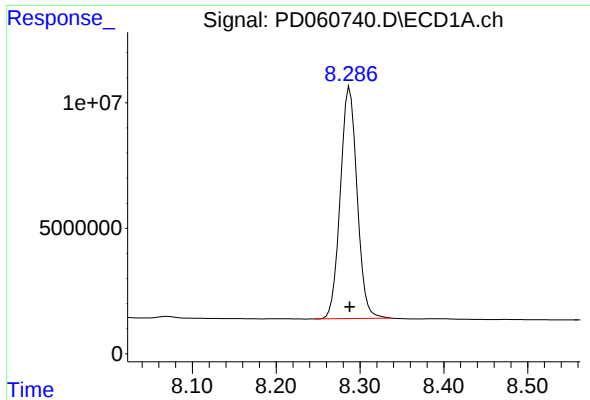

#28 Decachlorobiphenyl

R.T.: 8.288 min
Delta R.T.: 0.000 min
Response: 128412023
Conc: 93.60 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

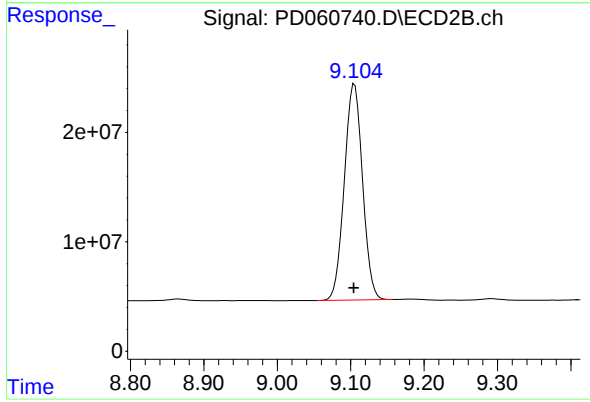

#28 Decachlorobiphenyl

R.T.: 9.105 min
Delta R.T.: 0.000 min
Response: 341090122
Conc: 93.53 ng/ml