

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121620\
 Data File : PD060742.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Dec 2020 19:04
 Operator : DD\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 03:38:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121620.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 17 03:37:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.500	4.021	63883796	234.5E6	50.000	50.000
28)	SA Decachlor...	8.288	9.104	68595825	182.3E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.380	5.020	20174666	91274608	500.000	500.000
24)	Chlordane-2	4.885	5.488	23666323	96168235	500.000	500.000
25)	Chlordane-3	5.459	6.136	67914186	355.0E6	500.000	500.000
26)	Chlordane-4	5.517	6.211	54946331	414.3E6	500.000	500.000
27)	Chlordane-5	6.359	7.017	24832604	76895972	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121620\
Data File : PD060742.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Dec 2020 19:04
Operator : DD\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 03:38:31 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121620.M
Quant Title : GC Extractables
QLast Update : Thu Dec 17 03:37:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

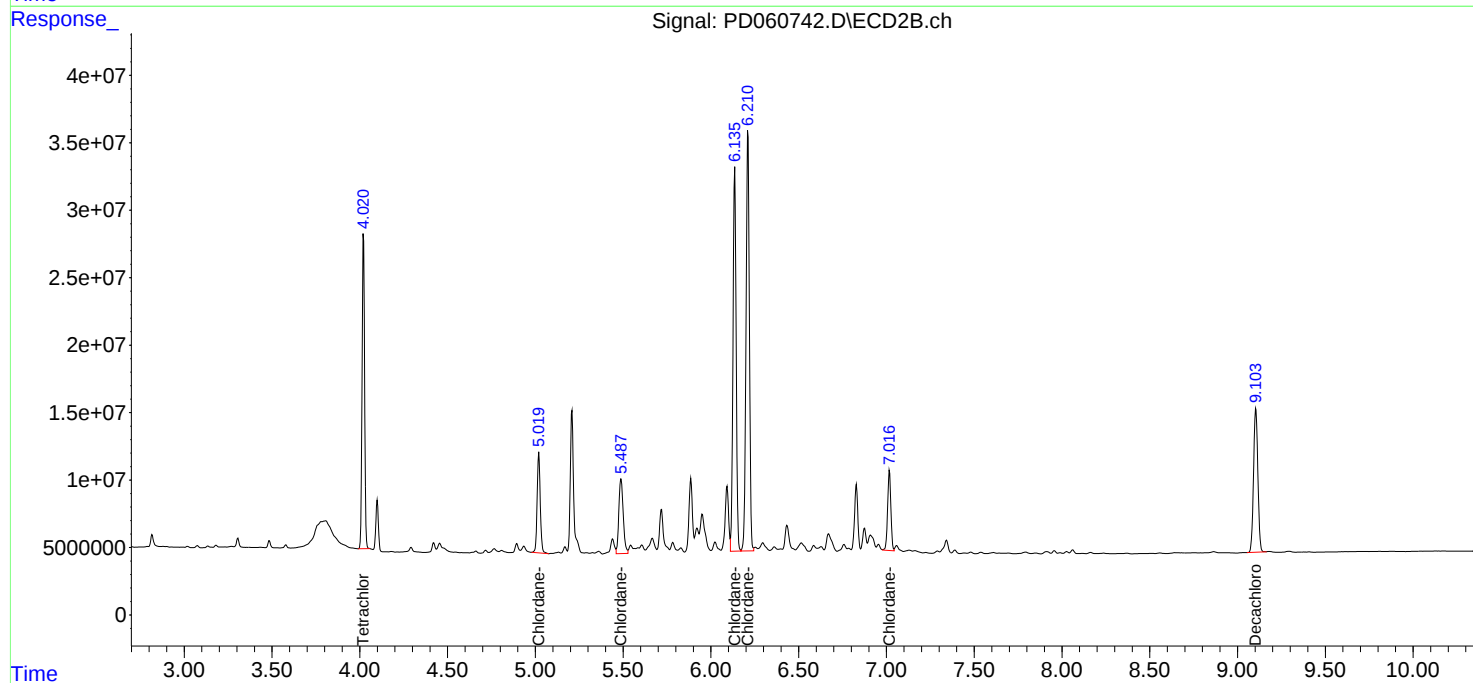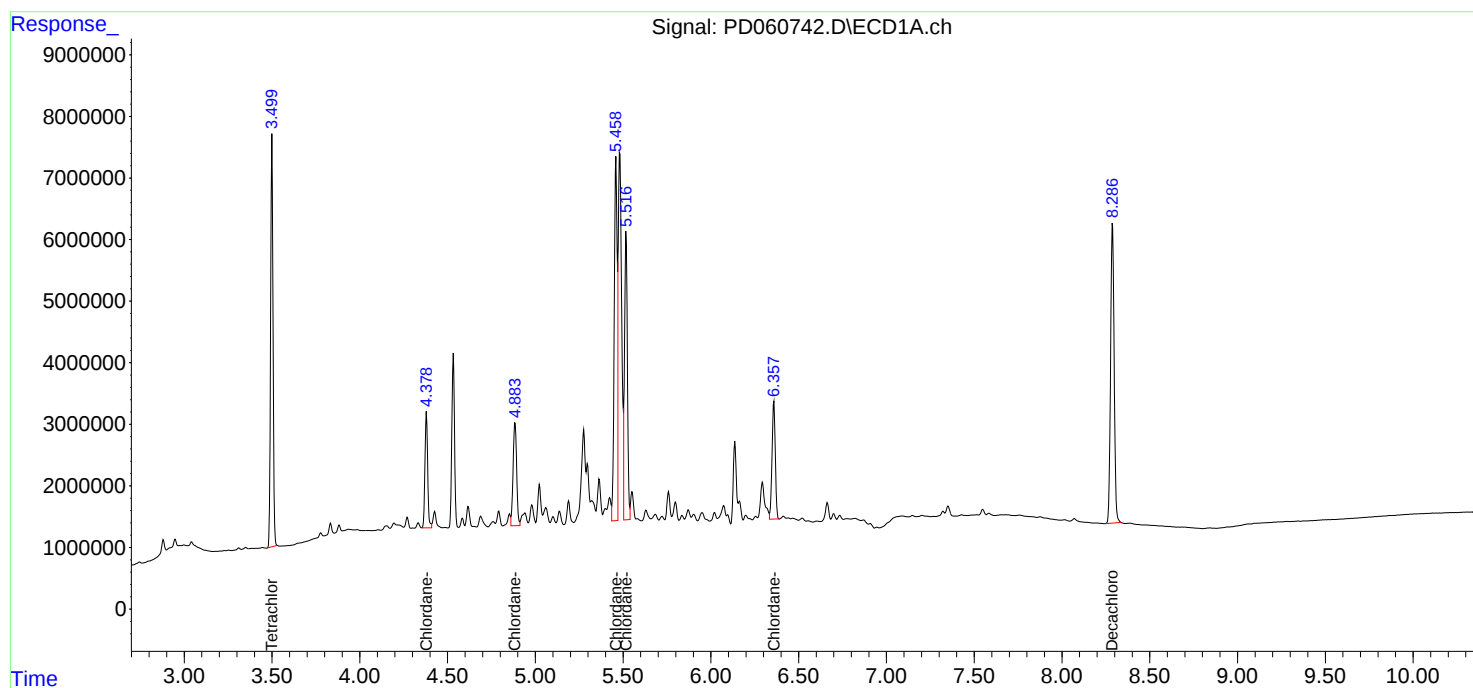


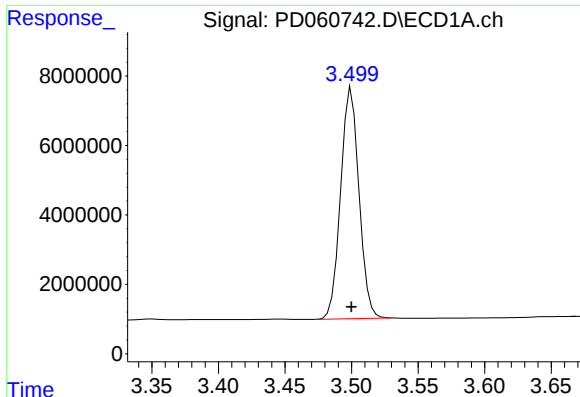

#1 Tetrachloro-m-xylene


R.T.: 3.500 min
Delta R.T.: 0.000 min
Response: 63883796
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

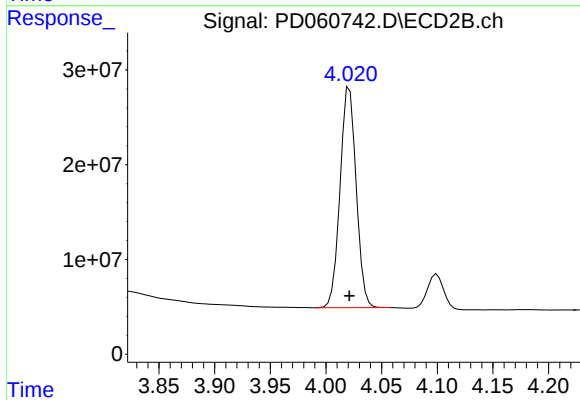


#1 Tetrachloro-m-xylene

R.T.: 4.021 min
Delta R.T.: 0.000 min
Response: 234477065
Conc: 50.00 ng/ml

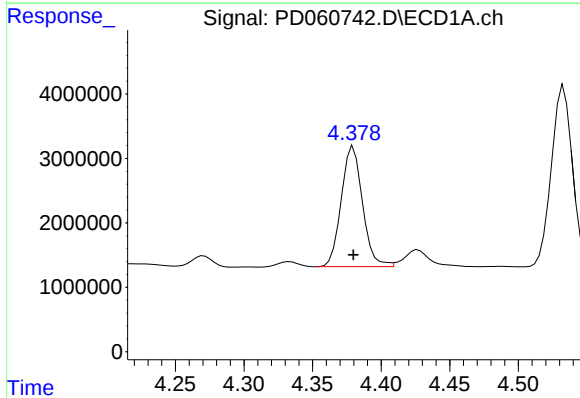


#23 Chlordane-1

R.T.: 4.380 min
Delta R.T.: 0.000 min
Response: 20174666
Conc: 500.00 ng/ml

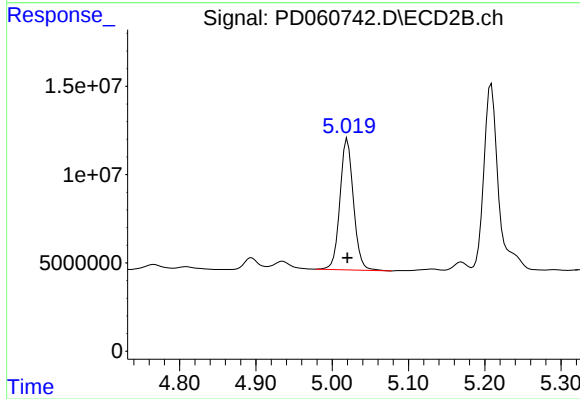

#23 Chlordane-1


R.T.: 5.020 min
Delta R.T.: 0.000 min
Response: 91274608
Conc: 500.00 ng/ml

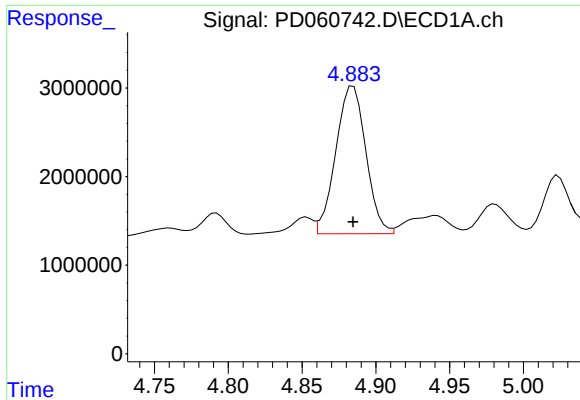

#24 Chlordane-2


R.T.: 4.885 min
Delta R.T.: 0.000 min
Response: 23666323
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

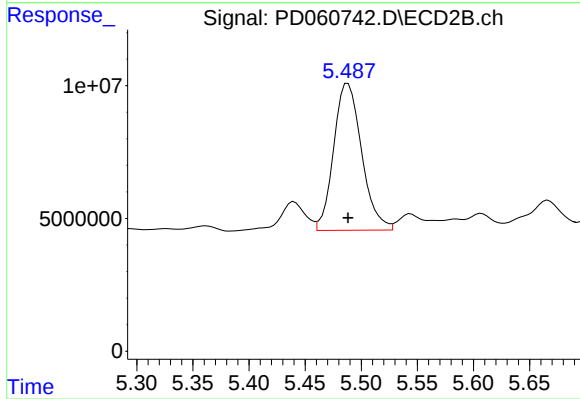


#24 Chlordane-2

R.T.: 5.488 min
Delta R.T.: 0.000 min
Response: 96168235
Conc: 500.00 ng/ml

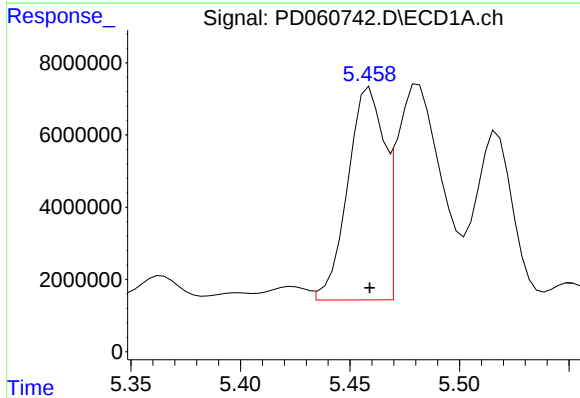


#25 Chlordane-3

R.T.: 5.459 min
Delta R.T.: 0.000 min
Response: 67914186
Conc: 500.00 ng/ml

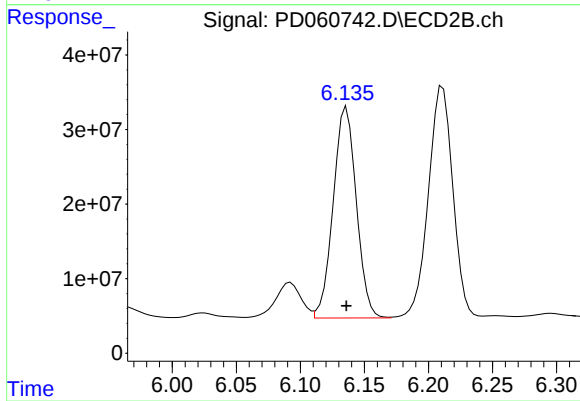

#25 Chlordane-3


R.T.: 6.136 min
Delta R.T.: 0.000 min
Response: 354973748
Conc: 500.00 ng/ml

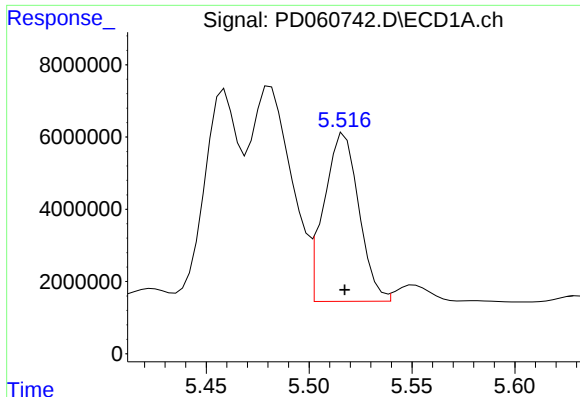

#26 Chlordane-4


R.T.: 5.517 min
Delta R.T.: 0.000 min
Response: 54946331
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

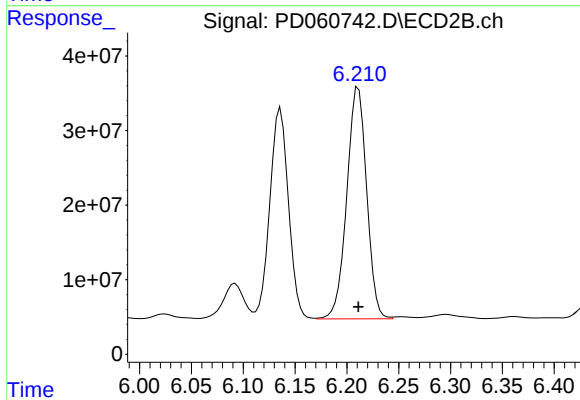


#26 Chlordane-4

R.T.: 6.211 min
Delta R.T.: 0.000 min
Response: 414327561
Conc: 500.00 ng/ml

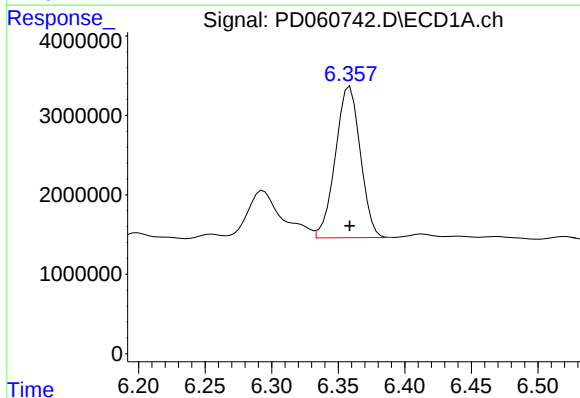


#27 Chlordane-5

R.T.: 6.359 min
Delta R.T.: 0.000 min
Response: 24832604
Conc: 500.00 ng/ml

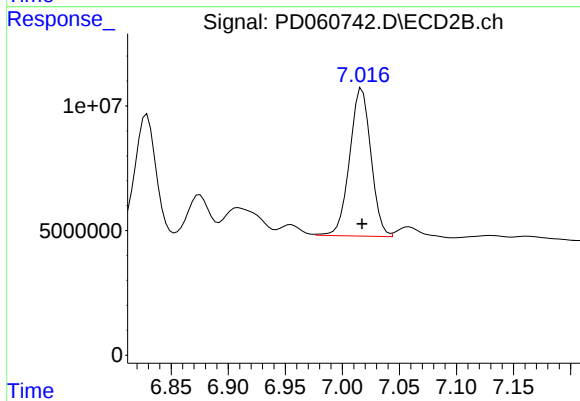

#27 Chlordane-5


R.T.: 7.017 min
Delta R.T.: 0.000 min
Response: 76895972
Conc: 500.00 ng/ml

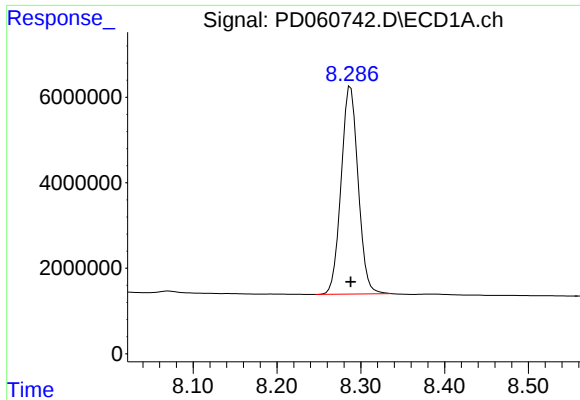

#28 Decachlorobiphenyl

R.T.: 8.288 min
Delta R.T.: 0.000 min
Response: 68595825
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

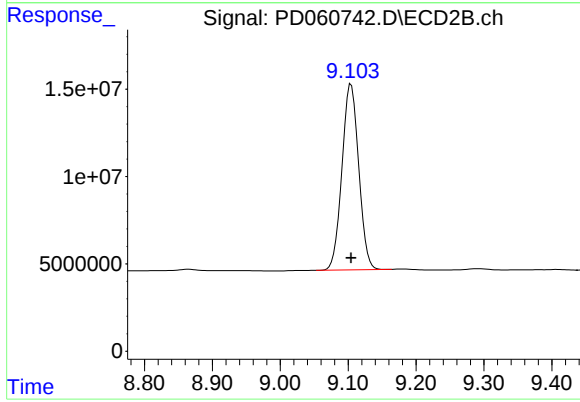

#28 Decachlorobiphenyl

R.T.: 9.104 min
Delta R.T.: 0.000 min
Response: 182334759
Conc: 50.00 ng/ml