

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121620\
 Data File : PD060743.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Dec 2020 19:18
 Operator : DD\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 03:38:45 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121620.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 17 03:37:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.500	4.021	31425682	117.0E6	24.596	24.947
28)	SA Decachlor...	8.288	9.106	35521420	93774878	25.892	25.715
Target Compounds							
23)	Chlordane-1	4.380	5.020	10463865	46782372	259.332	256.273
24)	Chlordane-2	4.885	5.488	11742043	50656208	248.075	263.373
25)	Chlordane-3	5.459	6.136	32980613	176.4E6	242.811	248.447
26)	Chlordane-4	5.517	6.211	27303259	207.3E6	248.454	250.176
27)	Chlordane-5	6.359	7.017	12534375	38194267	252.377	248.350



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121620\
Data File : PD060743.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Dec 2020 19:18
Operator : DD\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 03:38:45 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121620.M
Quant Title : GC Extractables
QLast Update : Thu Dec 17 03:37:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

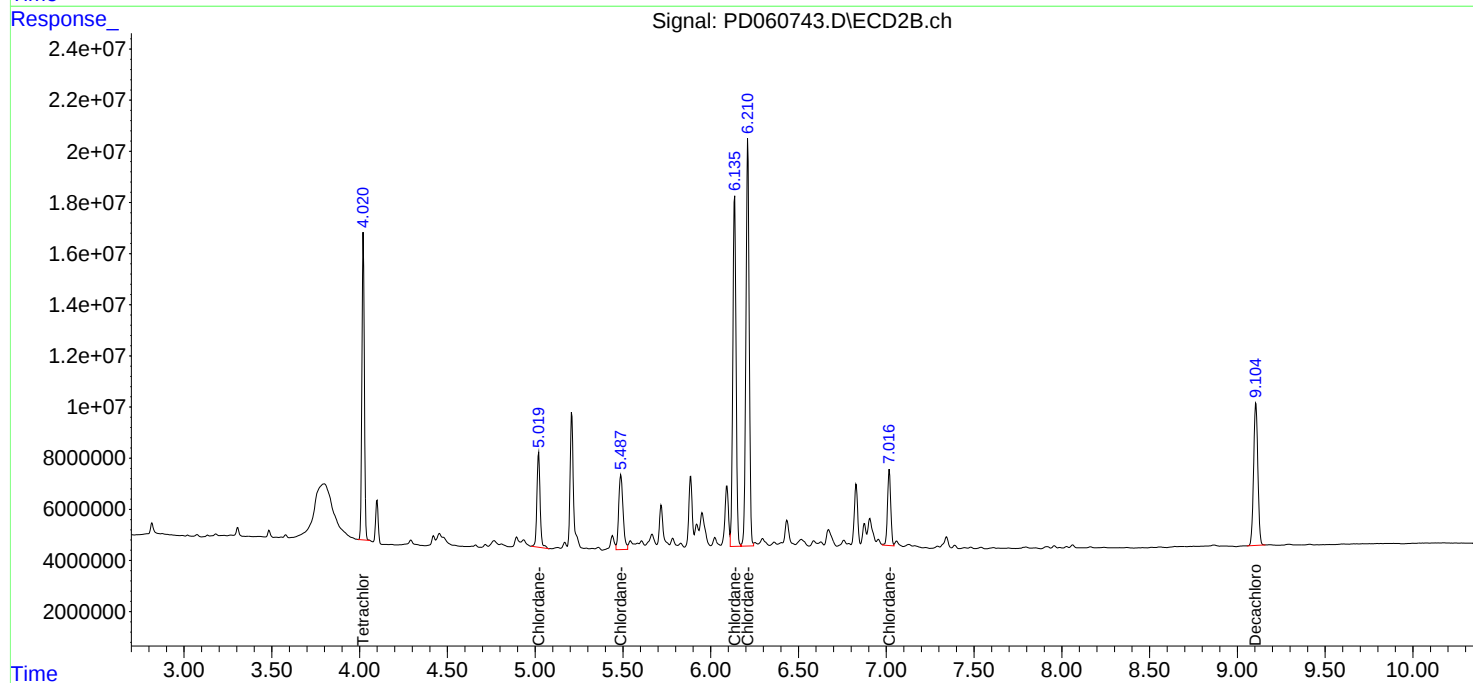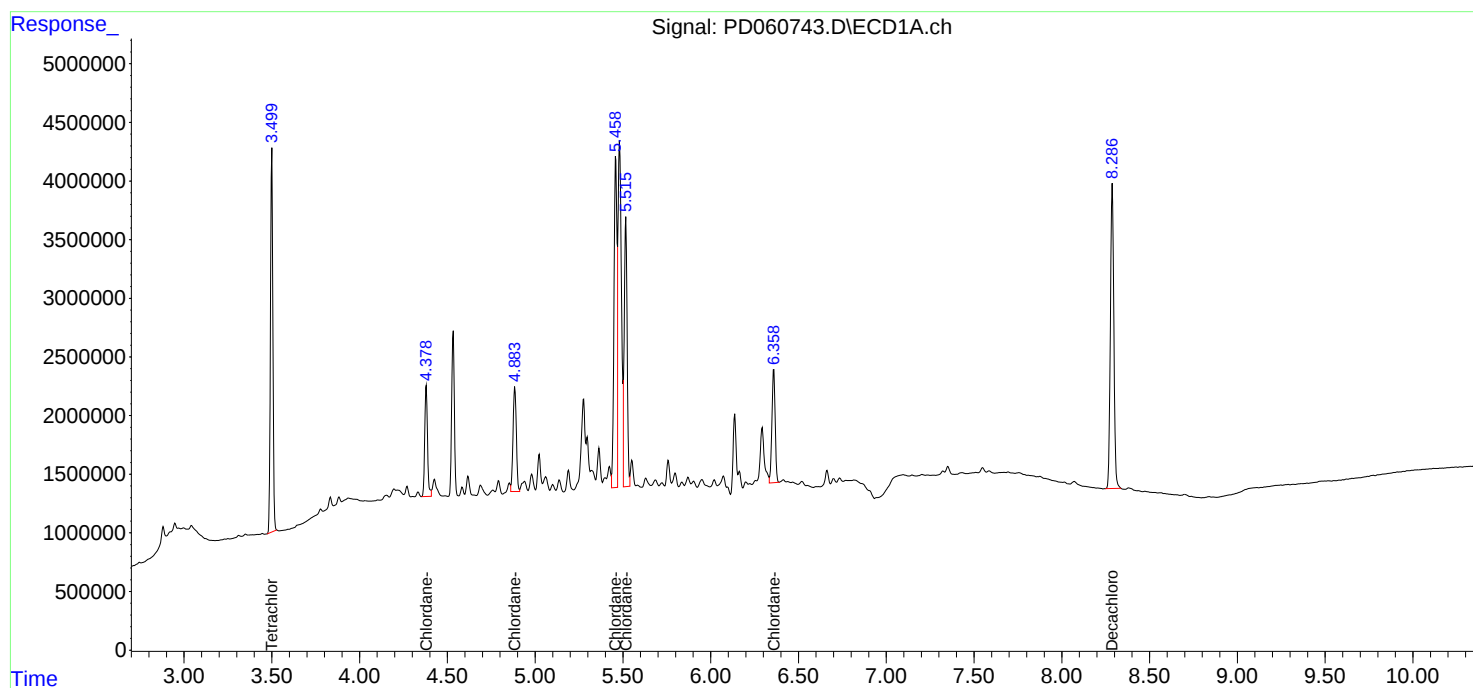


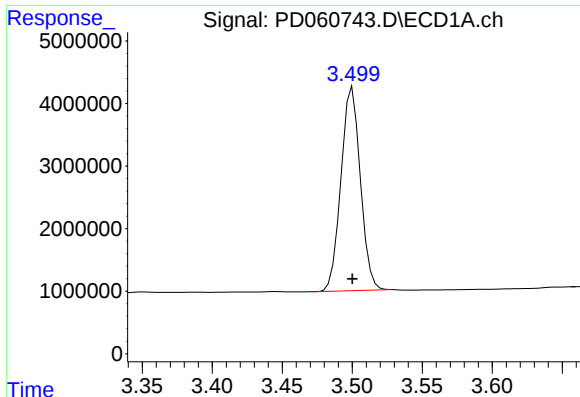

#1 Tetrachloro-m-xylene


R.T.: 3.500 min
Delta R.T.: 0.000 min
Response: 31425682
Conc: 24.60 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

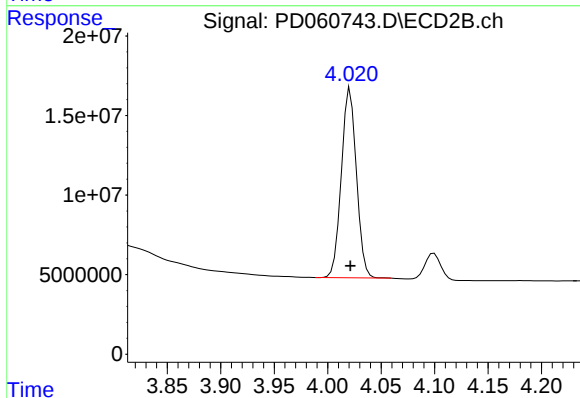


#1 Tetrachloro-m-xylene

R.T.: 4.021 min
Delta R.T.: 0.000 min
Response: 116990921
Conc: 24.95 ng/ml

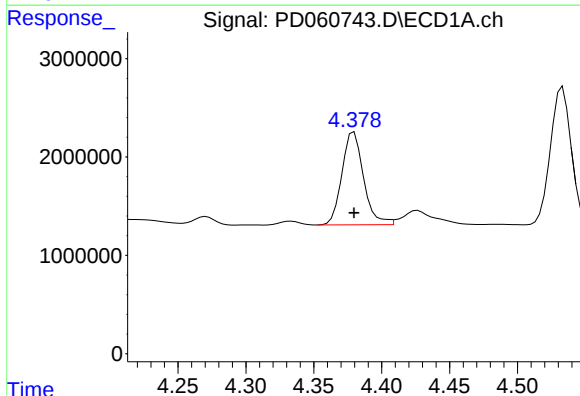


#23 Chlordane-1

R.T.: 4.380 min
Delta R.T.: 0.000 min
Response: 10463865
Conc: 259.33 ng/ml

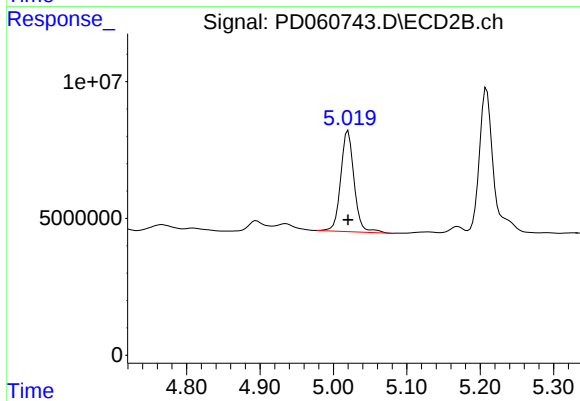

#23 Chlordane-1


R.T.: 5.020 min
Delta R.T.: 0.000 min
Response: 46782372
Conc: 256.27 ng/ml

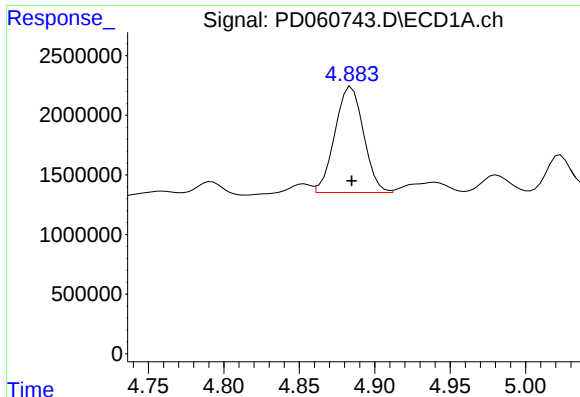

#24 Chlordane-2


R.T.: 4.885 min
Delta R.T.: 0.000 min
Response: 11742043
Conc: 248.07 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

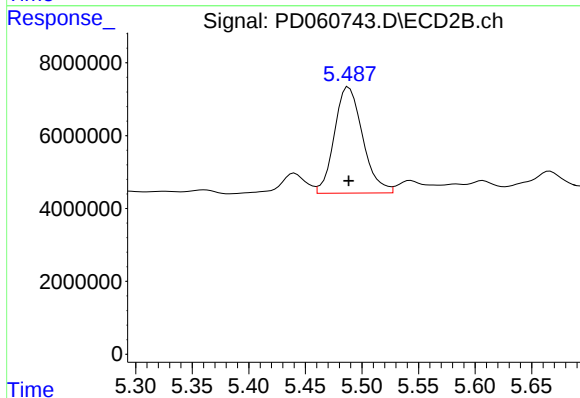


#24 Chlordane-2

R.T.: 5.488 min
Delta R.T.: 0.000 min
Response: 50656208
Conc: 263.37 ng/ml

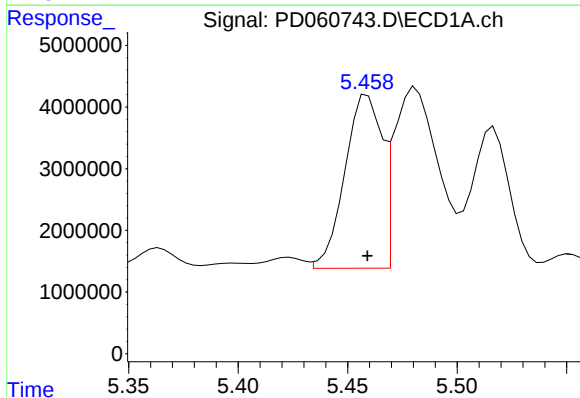


#25 Chlordane-3

R.T.: 5.459 min
Delta R.T.: 0.000 min
Response: 32980613
Conc: 242.81 ng/ml

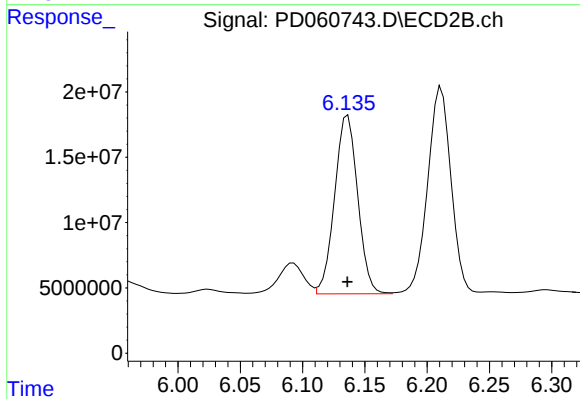

#25 Chlordane-3


R.T.: 6.136 min
Delta R.T.: 0.000 min
Response: 176384453
Conc: 248.45 ng/ml

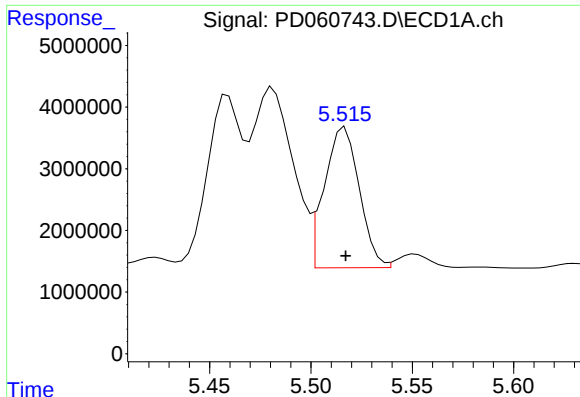

#26 Chlordane-4


R.T.: 5.517 min
Delta R.T.: 0.000 min
Response: 27303259
Conc: 248.45 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

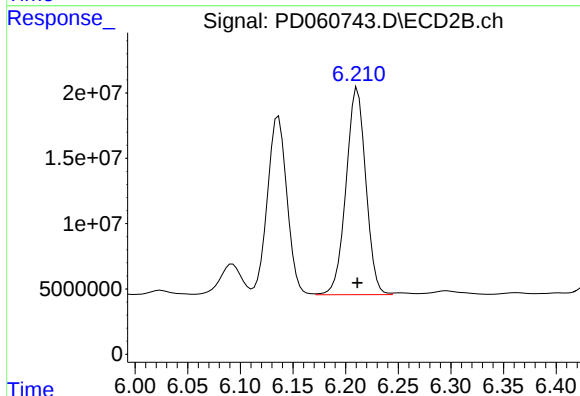


#26 Chlordane-4

R.T.: 6.211 min
Delta R.T.: 0.000 min
Response: 207309805
Conc: 250.18 ng/ml

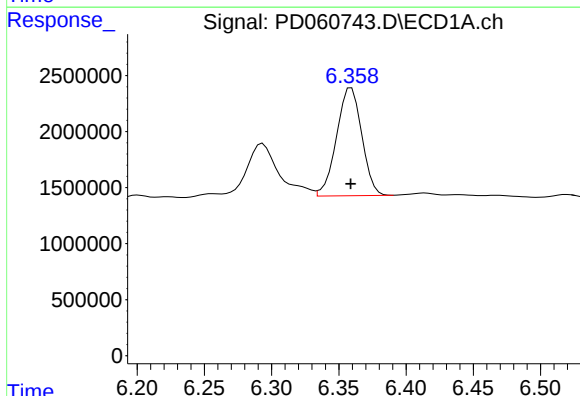


#27 Chlordane-5

R.T.: 6.359 min
Delta R.T.: 0.000 min
Response: 12534375
Conc: 252.38 ng/ml

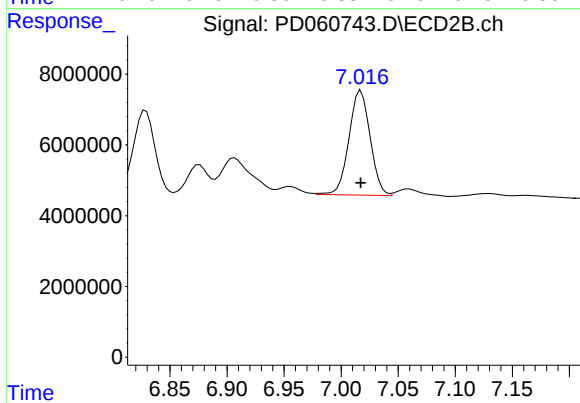

#27 Chlordane-5


R.T.: 7.017 min
Delta R.T.: 0.000 min
Response: 38194267
Conc: 248.35 ng/ml

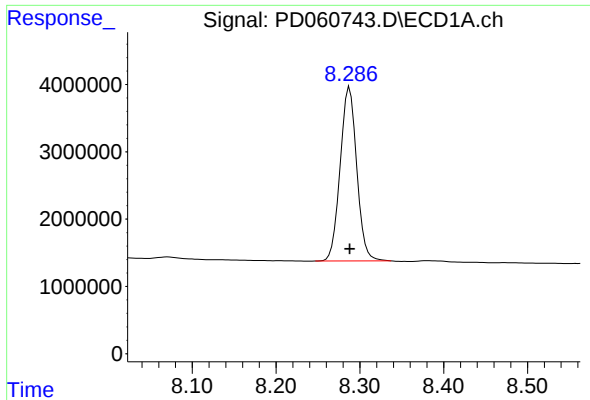

#28 Decachlorobiphenyl

R.T.: 8.288 min
Delta R.T.: 0.000 min
Response: 35521420
Conc: 25.89 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

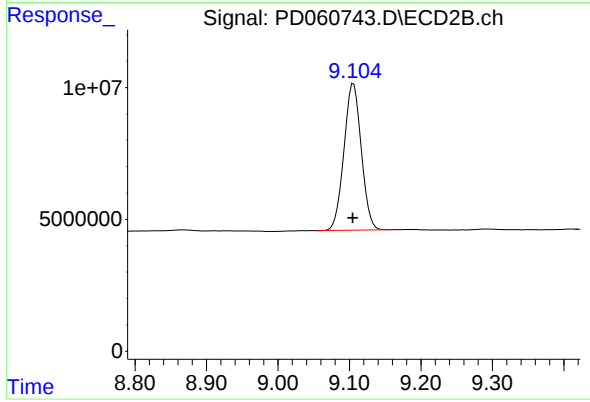

#28 Decachlorobiphenyl

R.T.: 9.106 min
Delta R.T.: 0.001 min
Response: 93774878
Conc: 25.72 ng/ml