

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121621\
 Data File : PD067391.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Dec 2021 18:27
 Operator : AR\AJ
 Sample : M5037-10MS
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C00W9MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/17/2021
 Supervised By : Ankita Jodhani 12/17/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 01:18:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112921CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 30 05:28:01 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.435	3.966	42477005	276.6E6	19.454	34.521 #
27)	SA Decachlor...	8.158	9.026	35040567	195.7E6	30.864	38.590 #
Target Compounds							
2)	A alpha-BHC	3.871	4.359	145.5E6	587.1E6	44.483	54.724
3)	MA gamma-BHC...	4.152	4.644	147.4E6	559.4E6	46.316	55.762
4)	MA Heptachlor	4.446	5.144	163.3E6	518.4E6	50.939	55.577
5)	MB Aldrin	4.691	5.447	161.9E6	466.6E6	52.314	54.109
6)	B beta-BHC	4.402	4.822	65118515	260.7E6	48.915	56.514
7)	B delta-BHC	4.603	5.037	27308625	116.0E6	9.547	13.111 #
8)	B Heptachlo...	5.131	5.837	144.9E6	398.3E6	52.473	56.833
9)	A Endosulfan I	5.467	6.194	128.7E6	384.2E6	48.406	52.996
10)	B trans-Chl...	5.355	6.070	146.8E6	410.5E6	52.112	54.089
11)	B cis-Chlor...	5.413	6.142	138.7E6	398.4E6	49.984	53.857
12)	B 4,4'-DDE	5.577	6.303	279.3E6	778.9E6	111.600	116.242
13)	MA Dieldrin	5.710	6.453	294.6E6	800.4E6	102.306	107.570
14)	MA Endrin	5.966	6.671	240.6E6	641.3E6	105.226	110.536
15)	B Endosulfa...	6.239	6.886	223.4E6	649.7E6	99.516	107.013
16)	A 4,4'-DDD	6.091	6.797	203.4E6	602.8E6	96.218	103.069
17)	MA 4,4'-DDT	6.330	7.095	207.4E6	587.4E6	97.547	101.946
18)	B Endrin al...	6.408	7.011	174.7E6	530.1E6	105.950	112.479
19)	B Endosulfa...	6.620	7.234	142.4E6	459.2E6	73.827	79.962
20)	A Methoxychlor	6.878	7.558	464.2E6	1389.6E6	467.089	499.256
21)	B Endrin ke...	7.112	7.706	209.1E6	711.5E6	100.700	107.748m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121621\
Data File : PD067391.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Dec 2021 18:27
Operator : AR\AJ
Sample : M5037-10MS
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 01:18:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112921CLP.M
Quant Title : GC Extractables
QLast Update : Tue Nov 30 05:28:01 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

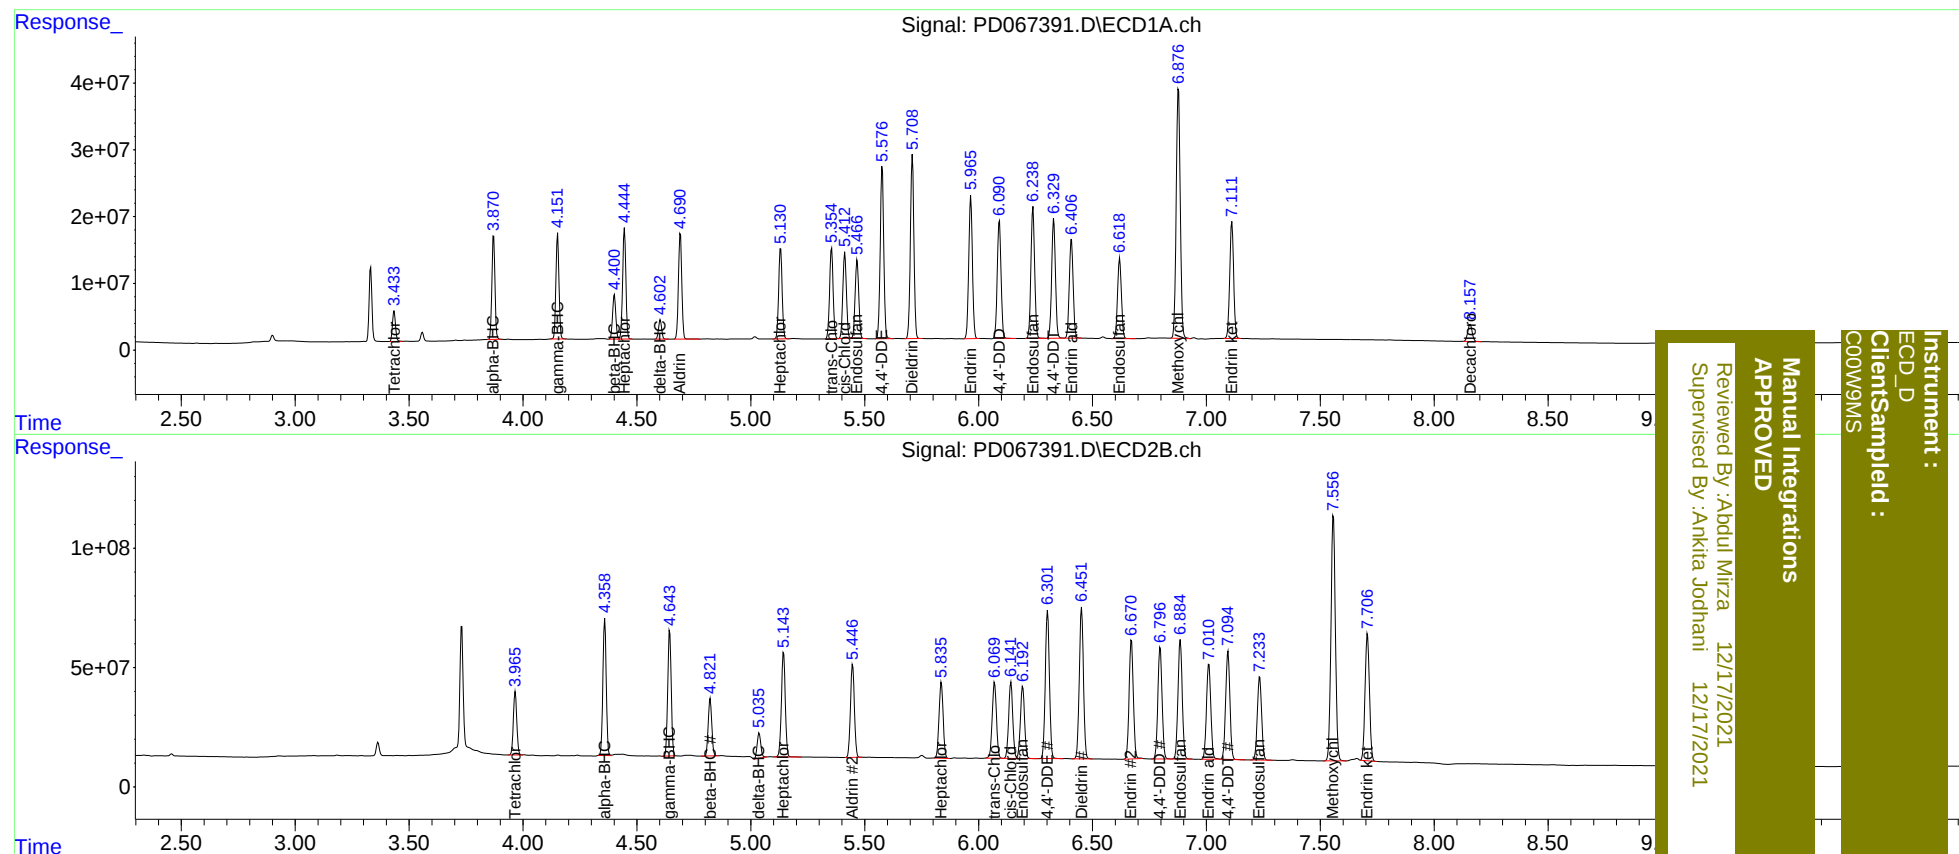

Reviewed By: Abdul Mirza 12/17/2021
Supervised By: Ankita Jodhani 12/17/2021

Manual Integrations
APPROVED

Instrument :
ECD_D
Client/Sample :
COOW9MS