

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121622\
 Data File : PD073336.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Dec 2022 13:13
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 16 14:48:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121622.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 16 14:47:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.696	3.460	256.8E6	10533.7E6	105.067	114.883
28)	SA Decachlor...	7.826	8.911	236.5E6	1711.7E6	97.796	97.413
Target Compounds							
23)	Chlordane-1	3.688	4.608	80121457	2284.8E6	1021.940	954.486
24)	Chlordane-2	4.264	5.139	92223220	1524.0E6	968.129	958.899
25)	Chlordane-3	4.894	5.847	309.5E6	5953.7E6	1050.693	1067.696
26)	Chlordane-4	4.957	5.923	308.0E6	7486.7E6	1035.653	1074.942
27)	Chlordane-5	5.854	6.781	92085200	1150.0E6	1025.473	986.586



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121622\
Data File : PD073336.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Dec 2022 13:13
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 14:48:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121622.M
Quant Title : GC Extractables
QLast Update : Fri Dec 16 14:47:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

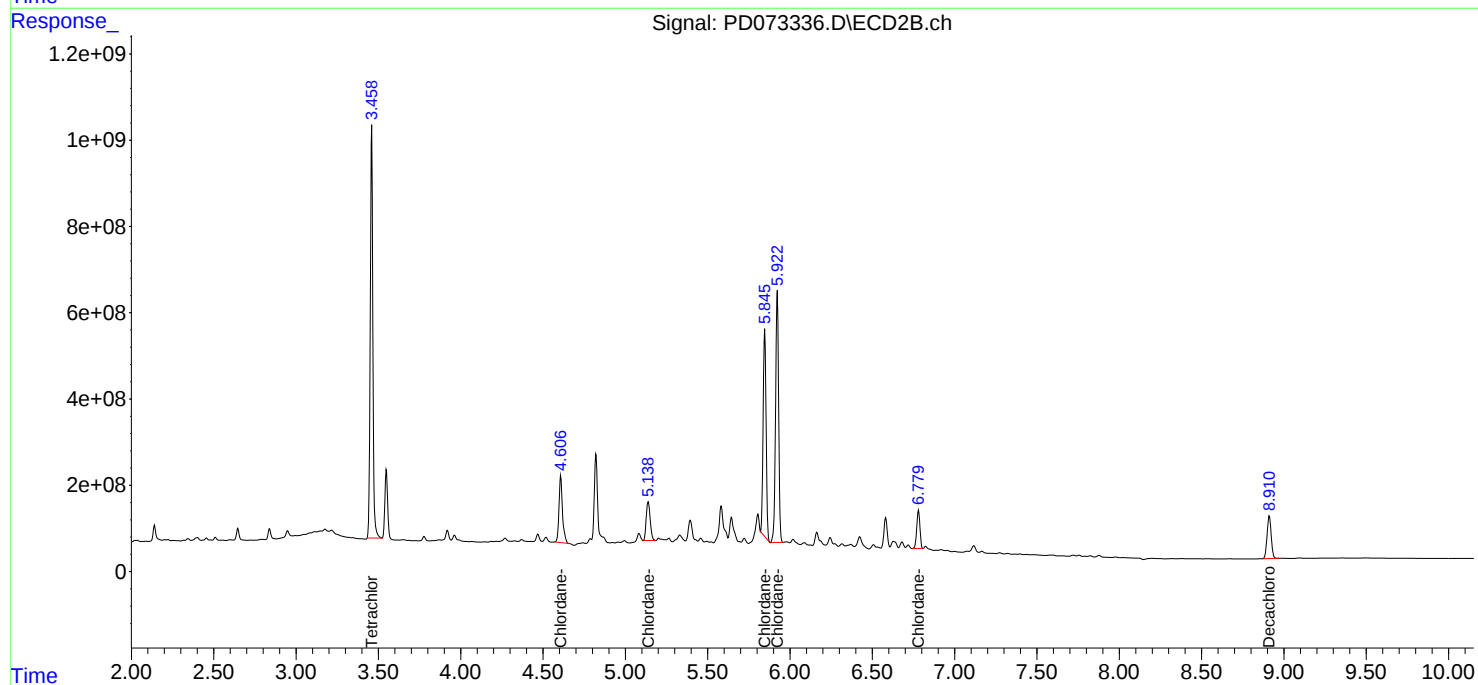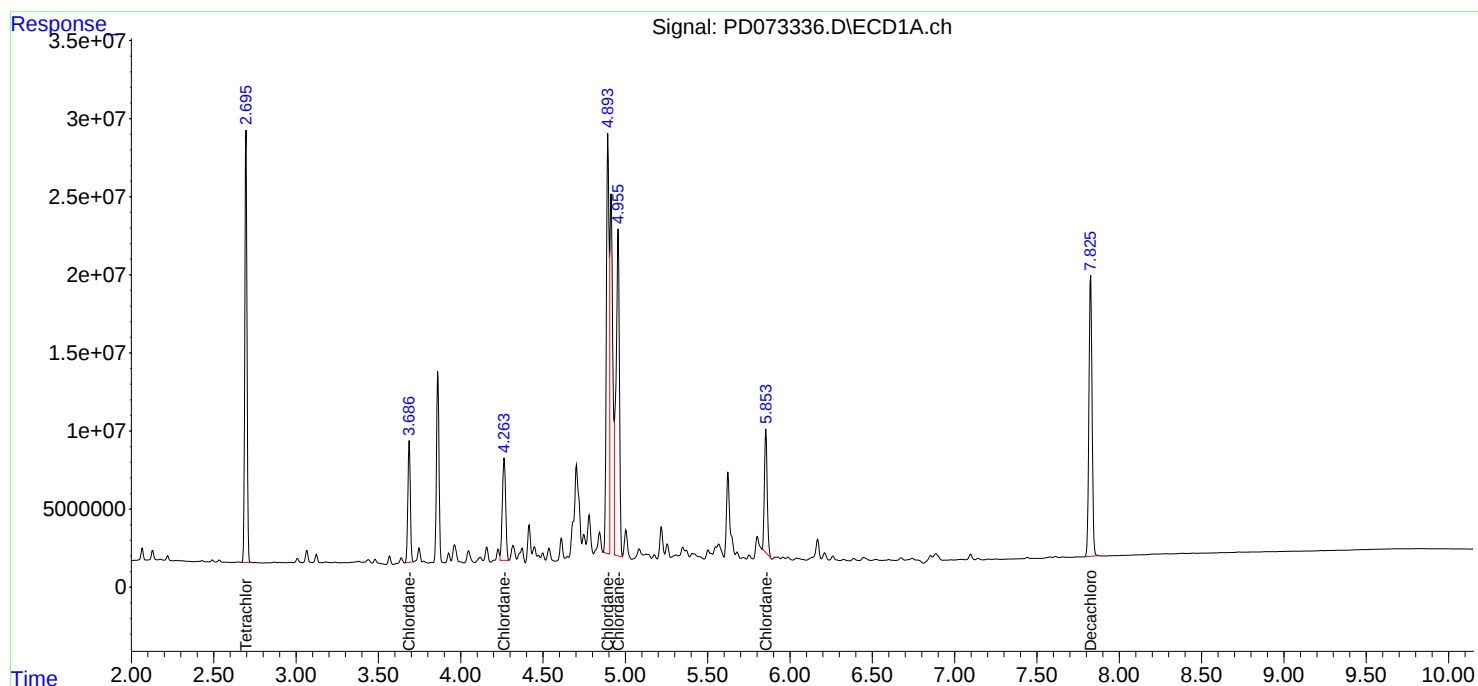


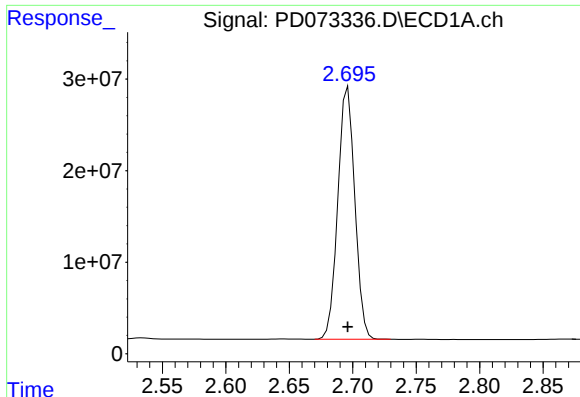

#1 Tetrachloro-m-xylene


R.T.: 2.696 min
Delta R.T.: 0.000 min
Response: 256815705
Conc: 105.07 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

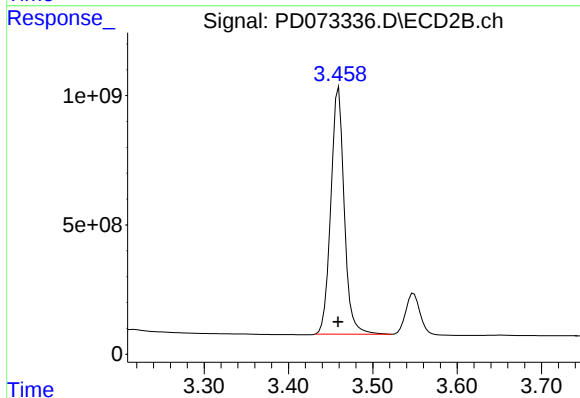


#1 Tetrachloro-m-xylene

R.T.: 3.460 min
Delta R.T.: 0.000 min
Response: 10533709793
Conc: 114.88 ng/ml

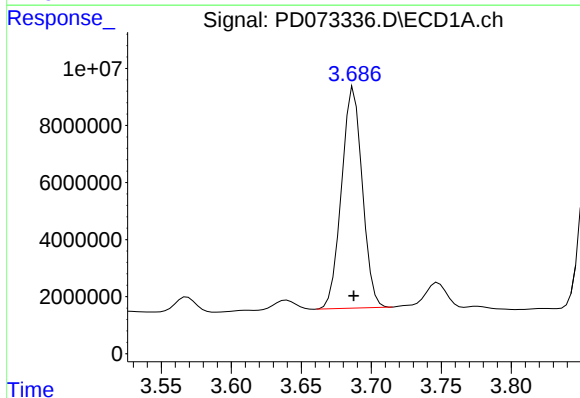


#23 Chlordane-1

R.T.: 3.688 min
Delta R.T.: 0.000 min
Response: 80121457
Conc: 1021.94 ng/ml

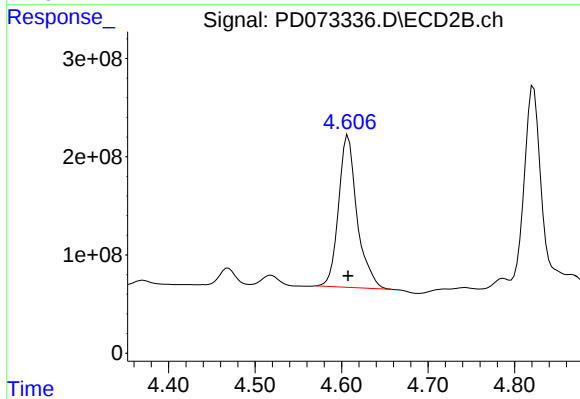

#23 Chlordane-1


R.T.: 4.608 min
Delta R.T.: 0.000 min
Response: 2284777107
Conc: 954.49 ng/ml

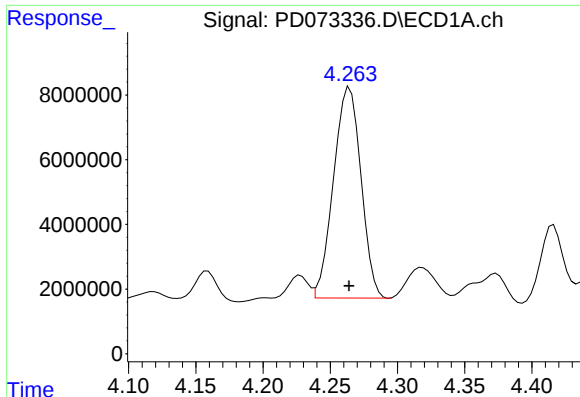

#24 Chlordane-2


R.T.: 4.264 min
Delta R.T.: 0.000 min
Response: 92223220
Conc: 968.13 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

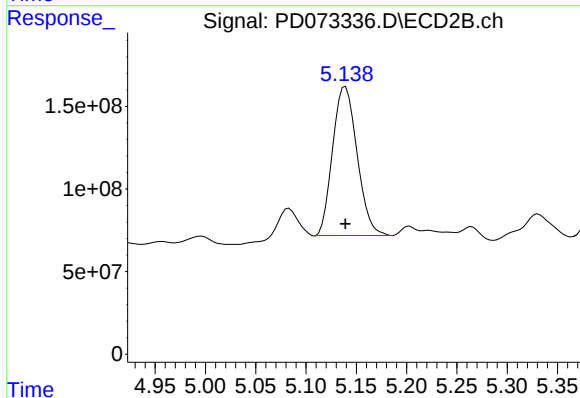


#24 Chlordane-2

R.T.: 5.139 min
Delta R.T.: 0.000 min
Response: 1523968593
Conc: 958.90 ng/ml

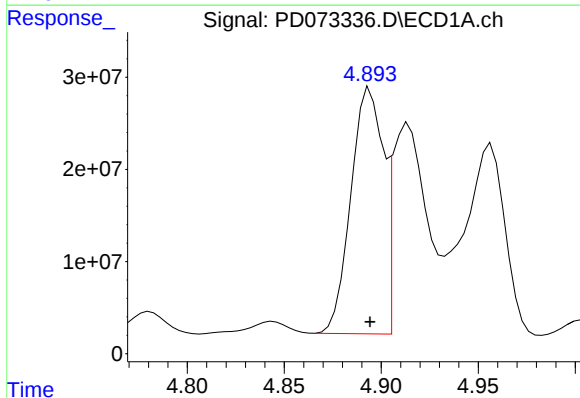


#25 Chlordane-3

R.T.: 4.894 min
Delta R.T.: 0.000 min
Response: 309534232
Conc: 1050.69 ng/ml

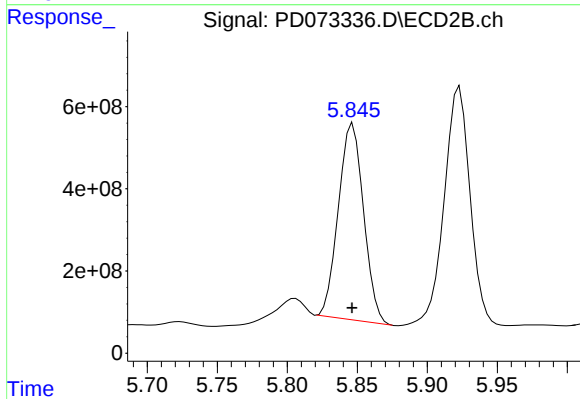

#25 Chlordane-3


R.T.: 5.847 min
Delta R.T.: 0.000 min
Response: 5953679103
Conc: 1067.70 ng/ml

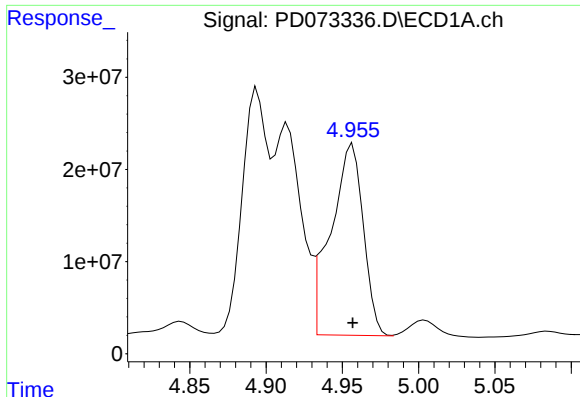

#26 Chlordane-4


R.T.: 4.957 min
Delta R.T.: 0.000 min
Response: 308007496
Conc: 1035.65 ng/m

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

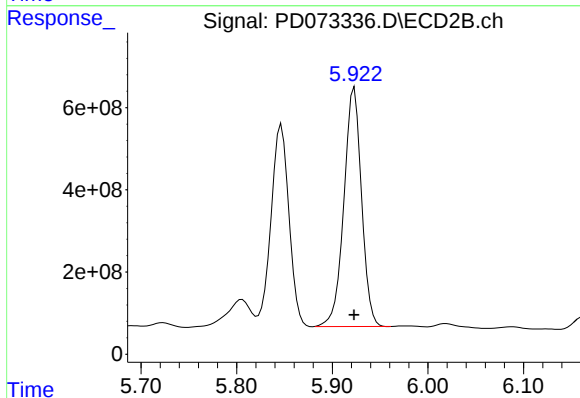


#26 Chlordane-4

R.T.: 5.923 min
Delta R.T.: 0.000 min
Response: 7486675541
Conc: 1074.94 ng/ml

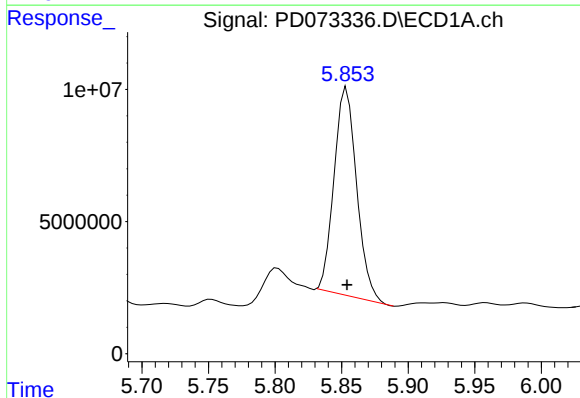


#27 Chlordane-5

R.T.: 5.854 min
Delta R.T.: 0.000 min
Response: 92085200
Conc: 1025.47 ng/ml

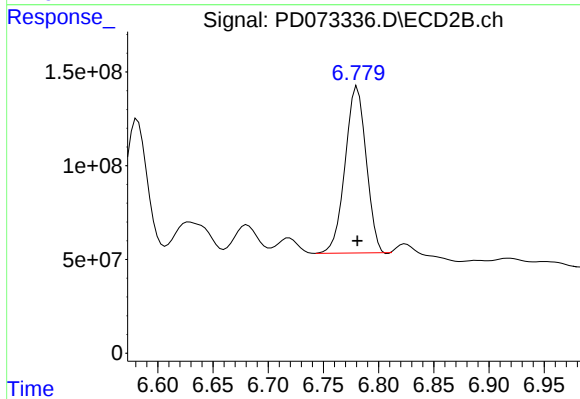

#27 Chlordane-5


R.T.: 6.781 min
Delta R.T.: 0.000 min
Response: 1150042333
Conc: 986.59 ng/ml

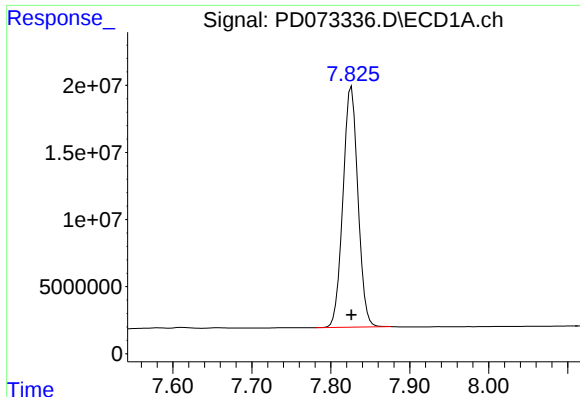

#28 Decachlorobiphenyl

R.T.: 7.826 min
Delta R.T.: 0.000 min
Response: 236515607
Conc: 97.80 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

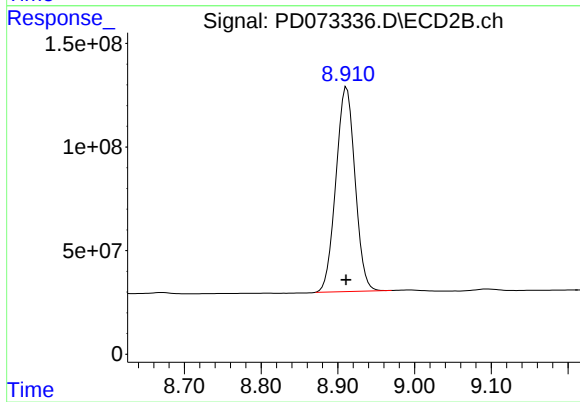

#28 Decachlorobiphenyl

R.T.: 8.911 min
Delta R.T.: 0.000 min
Response: 1711719862
Conc: 97.41 ng/ml