

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121622\
 Data File : PD073337.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Dec 2022 13:27
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 16 14:48:31 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121622.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 16 14:47:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.696	3.459	185.2E6	7004.3E6	75.783	76.390
28)	SA Decachlor...	7.825	8.910	176.3E6	1274.1E6	72.894	72.507
Target Compounds							
23)	Chlordane-1	3.687	4.607	58595847	1693.0E6	747.383	707.257
24)	Chlordane-2	4.264	5.139	68513734	1132.8E6	719.234	712.794
25)	Chlordane-3	4.894	5.847	225.7E6	4161.1E6	766.007	746.228
26)	Chlordane-4	4.957	5.923	222.9E6	5237.2E6	749.341	751.958
27)	Chlordane-5	5.854	6.780	67347268	845.9E6	749.988	725.671



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121622\
Data File : PD073337.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Dec 2022 13:27
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 14:48:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121622.M
Quant Title : GC Extractables
QLast Update : Fri Dec 16 14:47:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

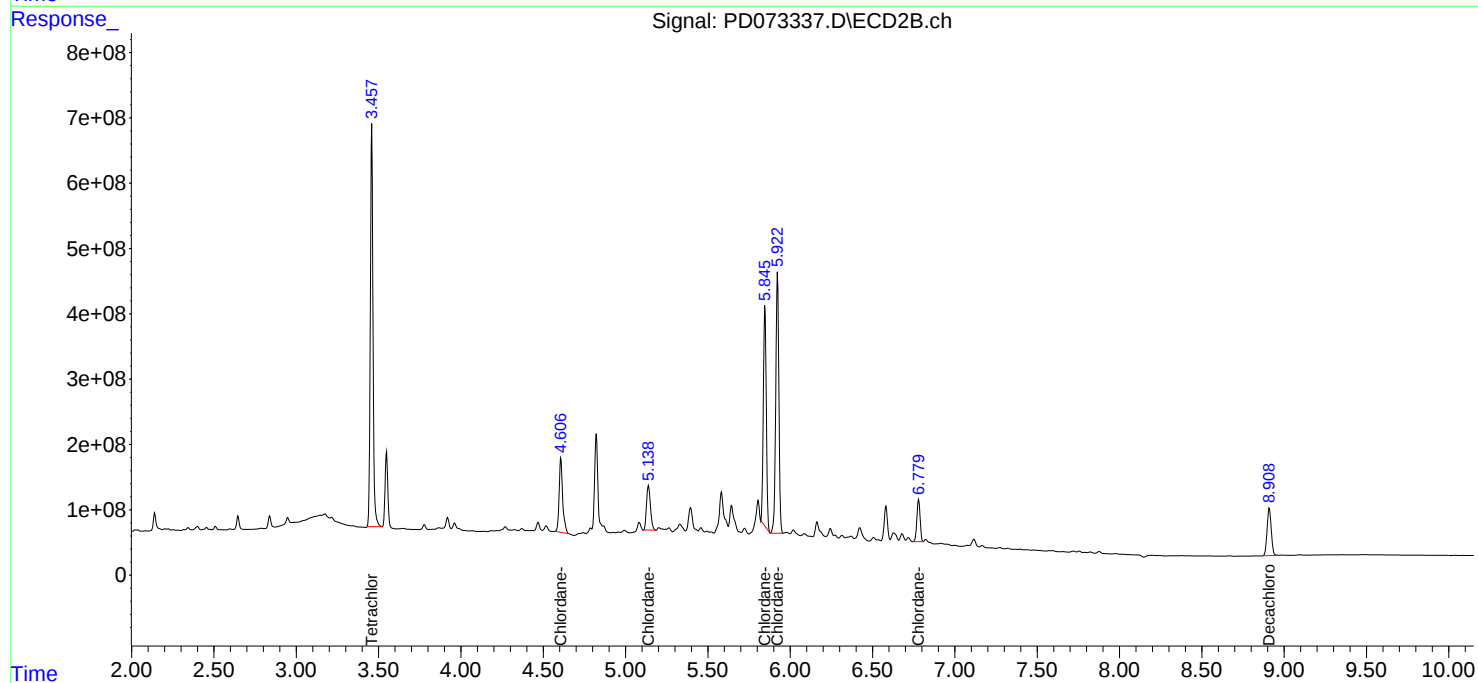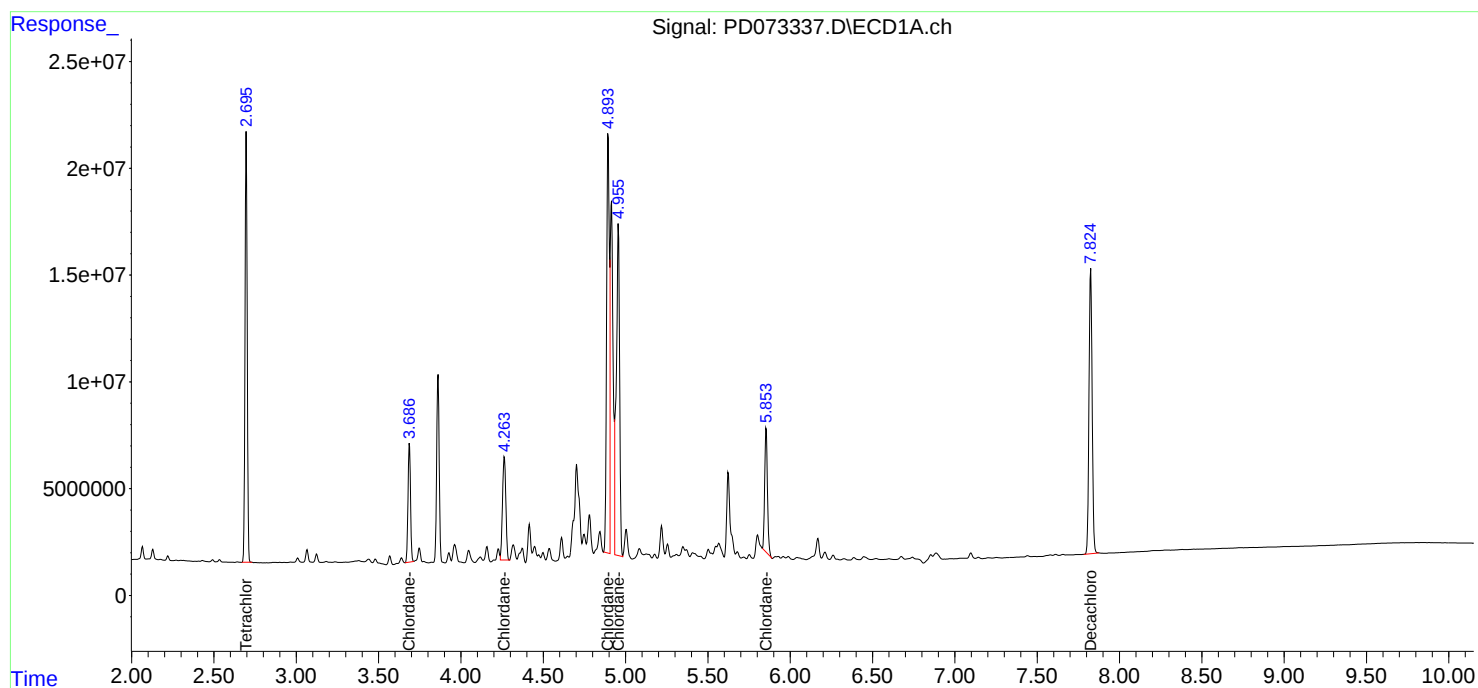


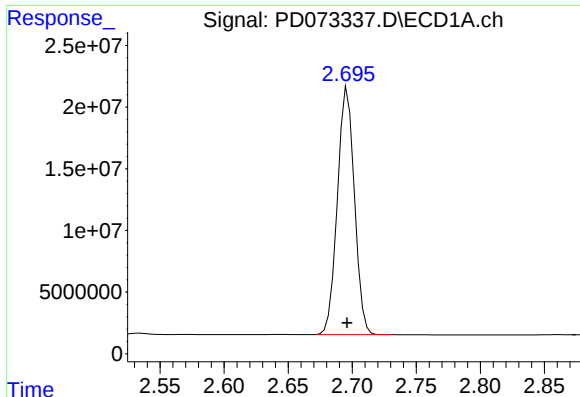

#1 Tetrachloro-m-xylene


R.T.: 2.696 min
Delta R.T.: 0.000 min
Response: 185235956
Conc: 75.78 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

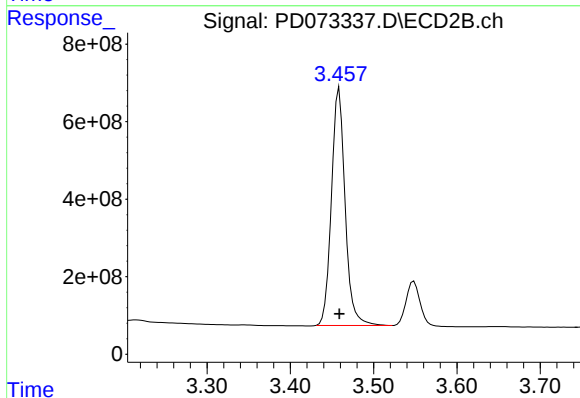


#1 Tetrachloro-m-xylene

R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 7004318710
Conc: 76.39 ng/ml

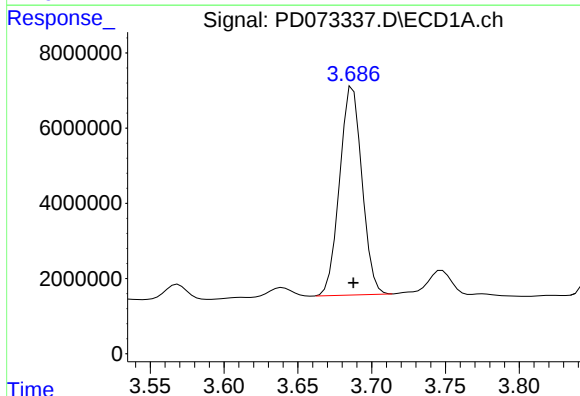


#23 Chlordane-1

R.T.: 3.687 min
Delta R.T.: 0.000 min
Response: 58595847
Conc: 747.38 ng/ml

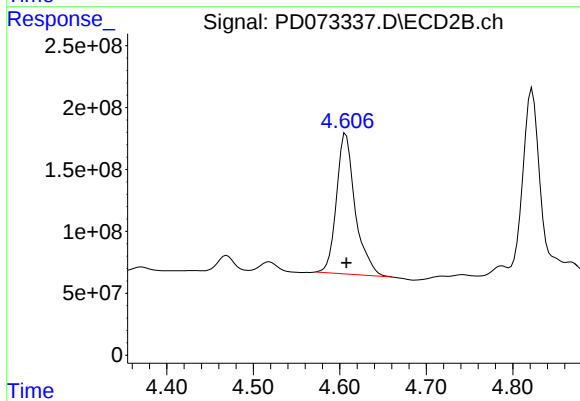

#23 Chlordane-1


R.T.: 4.607 min
Delta R.T.: 0.000 min
Response: 1692977899
Conc: 707.26 ng/ml

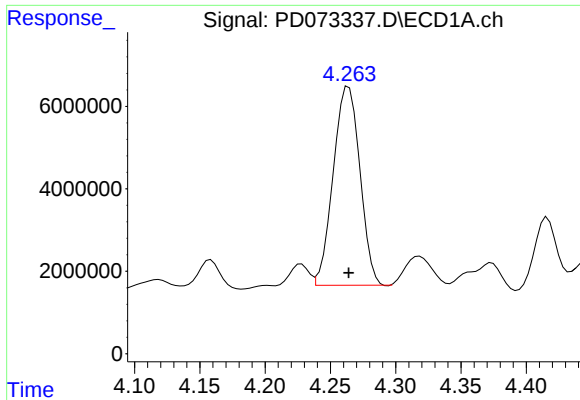

#24 Chlordane-2


R.T.: 4.264 min
Delta R.T.: 0.000 min
Response: 68513734
Conc: 719.23 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

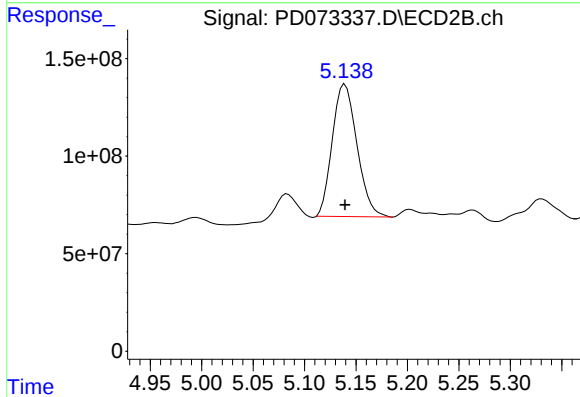


#24 Chlordane-2

R.T.: 5.139 min
Delta R.T.: 0.000 min
Response: 1132836456
Conc: 712.79 ng/ml

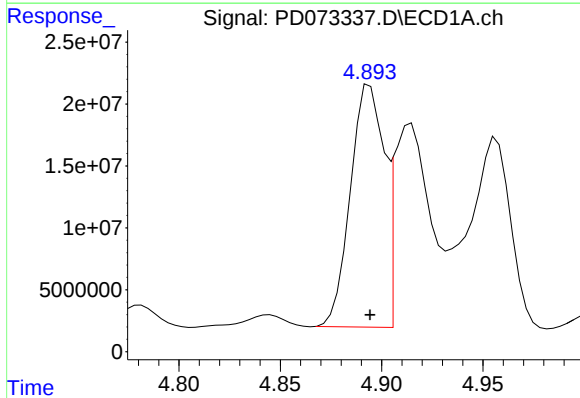


#25 Chlordane-3

R.T.: 4.894 min
Delta R.T.: 0.000 min
Response: 225665684
Conc: 766.01 ng/ml

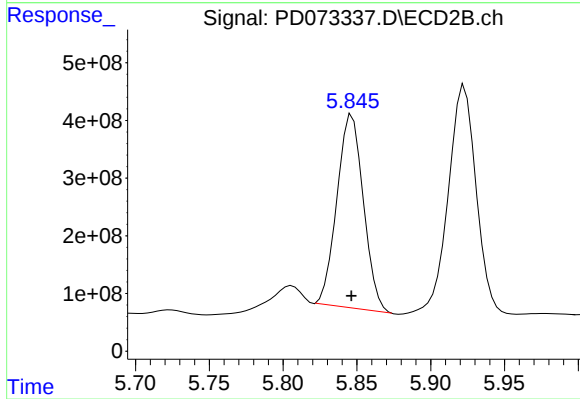

#25 Chlordane-3


R.T.: 5.847 min
Delta R.T.: 0.000 min
Response: 4161111483
Conc: 746.23 ng/ml

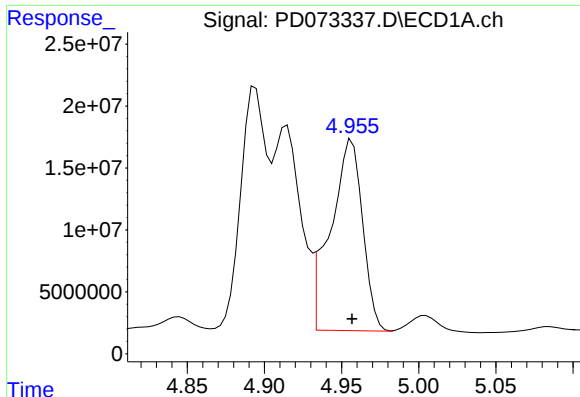

#26 Chlordane-4


R.T.: 4.957 min
Delta R.T.: 0.000 min
Response: 222856961
Conc: 749.34 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

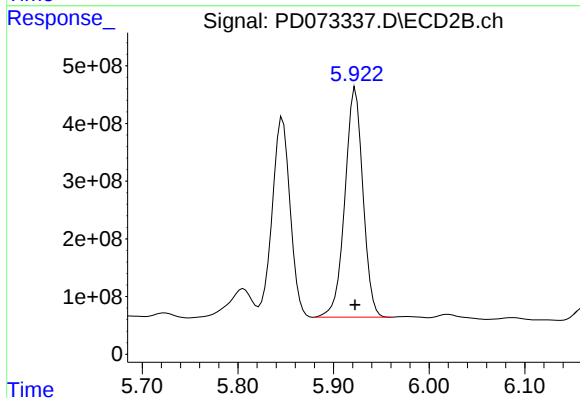


#26 Chlordane-4

R.T.: 5.923 min
Delta R.T.: 0.000 min
Response: 5237179174
Conc: 751.96 ng/ml

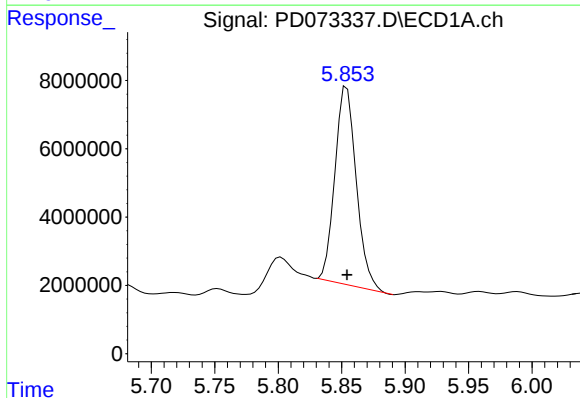


#27 Chlordane-5

R.T.: 5.854 min
Delta R.T.: 0.000 min
Response: 67347268
Conc: 749.99 ng/ml

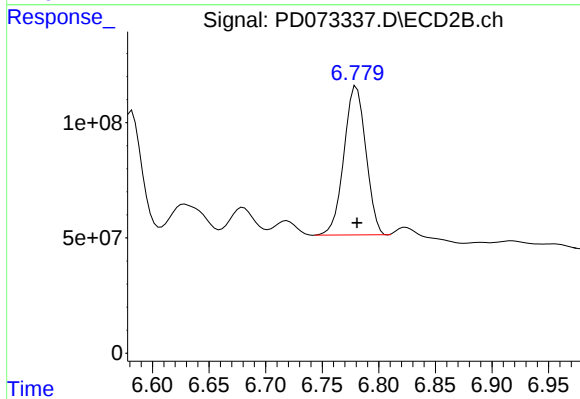

#27 Chlordane-5

R.T.: 6.780 min
Delta R.T.: 0.000 min
Response: 845899472
Conc: 725.67 ng/ml

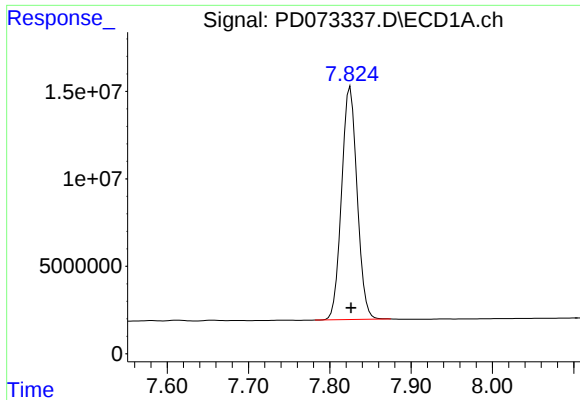

#28 Decachlorobiphenyl


R.T.: 7.825 min

Delta R.T.: 0.000 min

Response: 176289290

Conc: 72.89 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

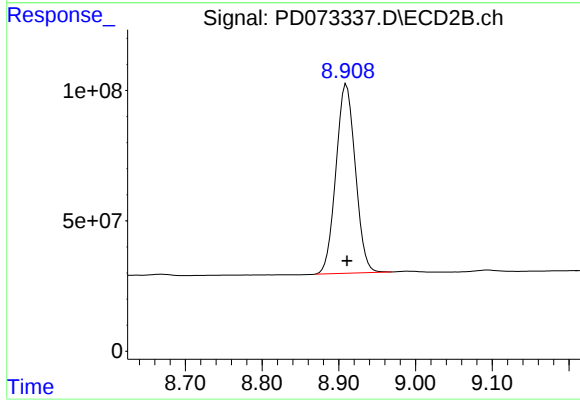

#28 Decachlorobiphenyl

R.T.: 8.910 min

Delta R.T.: 0.000 min

Response: 1274086479

Conc: 72.51 ng/ml