

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121622\
 Data File : PD073339.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Dec 2022 13:53
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 16 14:48:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121622.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 16 14:47:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.697	3.459	60995217	2426.4E6	24.954	26.463
28)	SA Decachlor...	7.826	8.912	63966185	459.8E6	26.449	26.169
Target Compounds							
23)	Chlordane-1	3.688	4.608	20086954	655.1E6	256.207	273.688
24)	Chlordane-2	4.264	5.140	25456028	431.6E6	267.229	271.566
25)	Chlordane-3	4.894	5.847	73174652	1435.8E6	248.387	257.492
26)	Chlordane-4	4.957	5.923	74219737	1785.3E6	249.559	256.337
27)	Chlordane-5	5.854	6.781	22732154	305.0E6	253.148	261.656



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121622\
Data File : PD073339.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Dec 2022 13:53
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 14:48:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121622.M
Quant Title : GC Extractables
QLast Update : Fri Dec 16 14:47:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

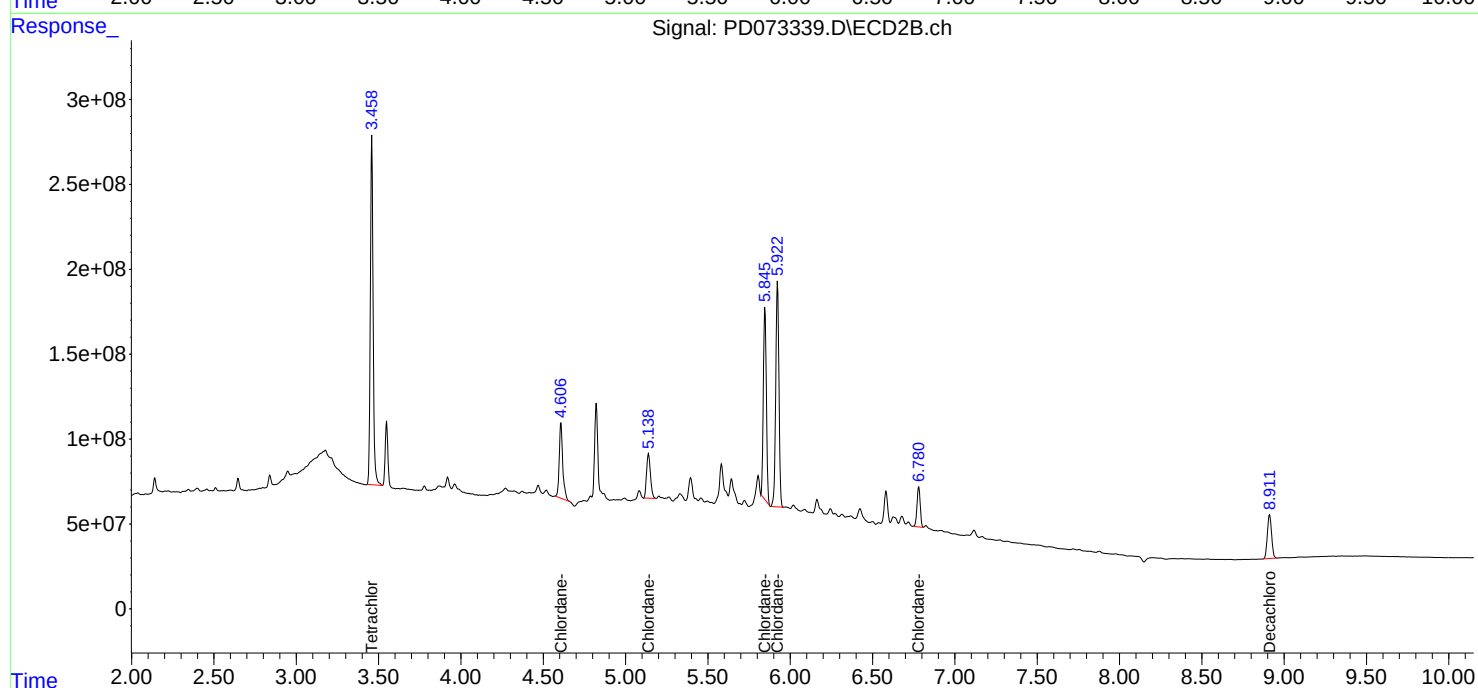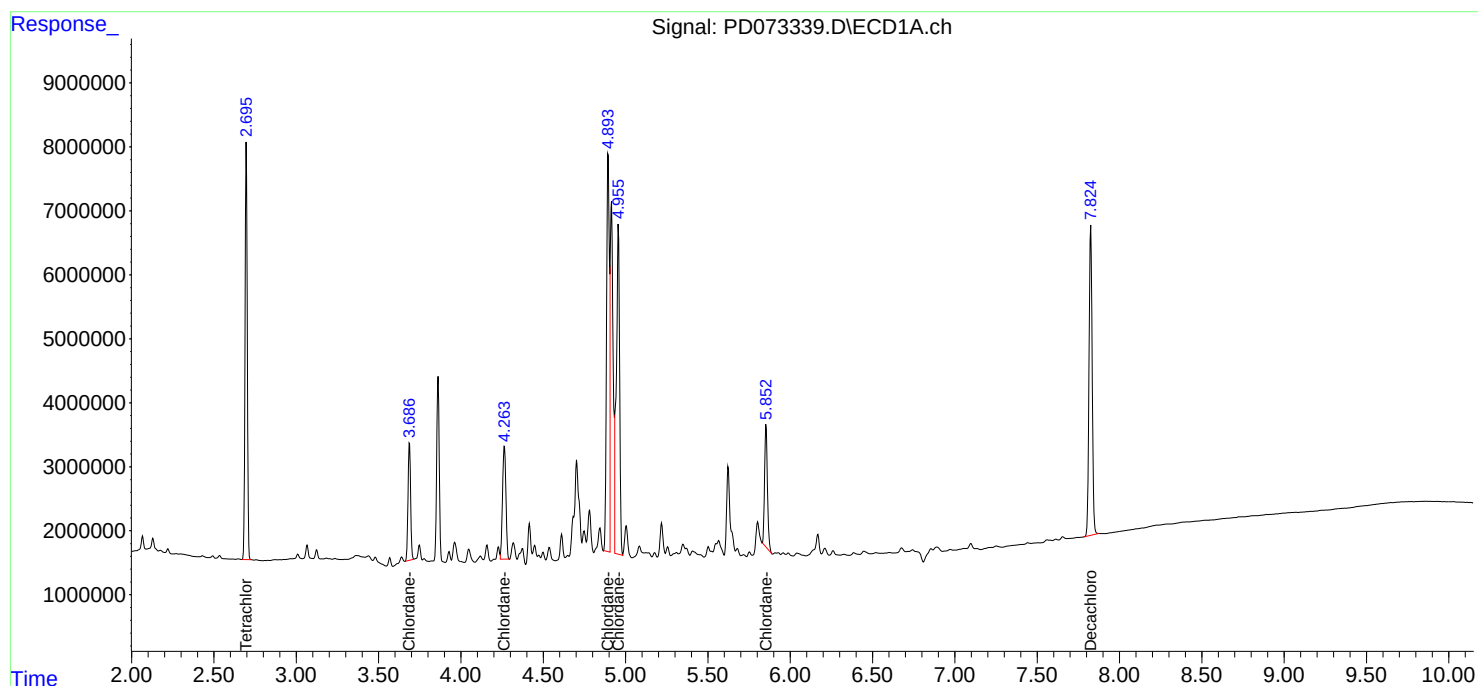


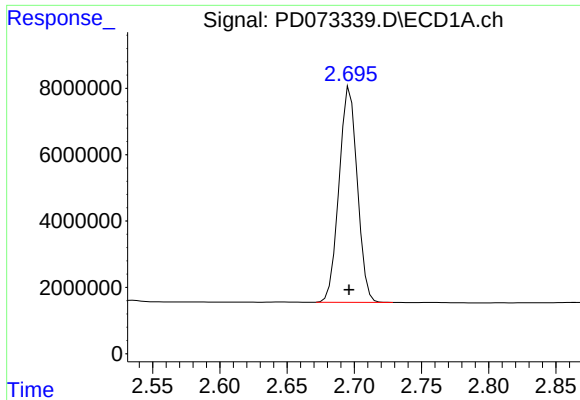

#1 Tetrachloro-m-xylene


R.T.: 2.697 min
Delta R.T.: 0.000 min
Response: 60995217
Conc: 24.95 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

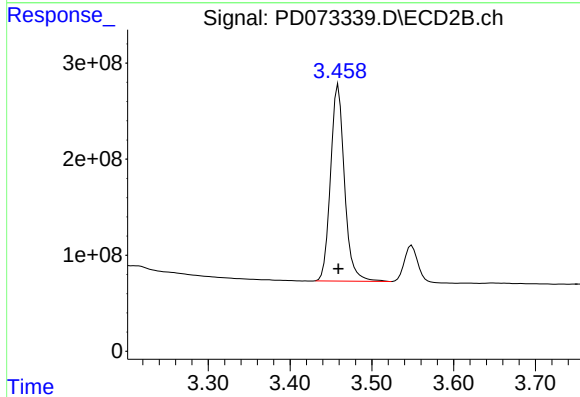


#1 Tetrachloro-m-xylene

R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 2426409358
Conc: 26.46 ng/ml

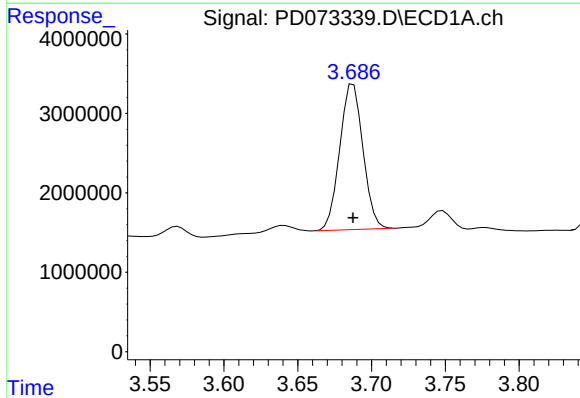


#23 Chlordane-1

R.T.: 3.688 min
Delta R.T.: 0.000 min
Response: 20086954
Conc: 256.21 ng/ml

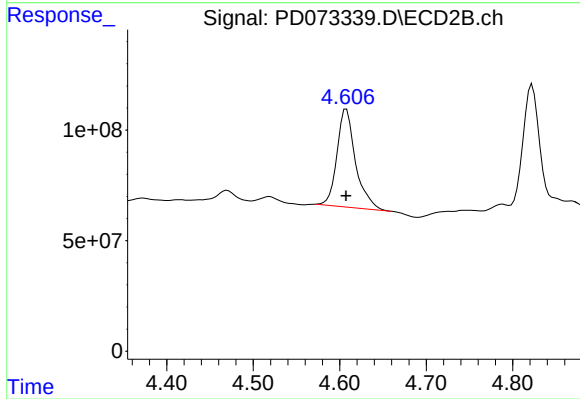

#23 Chlordane-1


R.T.: 4.608 min
Delta R.T.: 0.000 min
Response: 655133866
Conc: 273.69 ng/ml

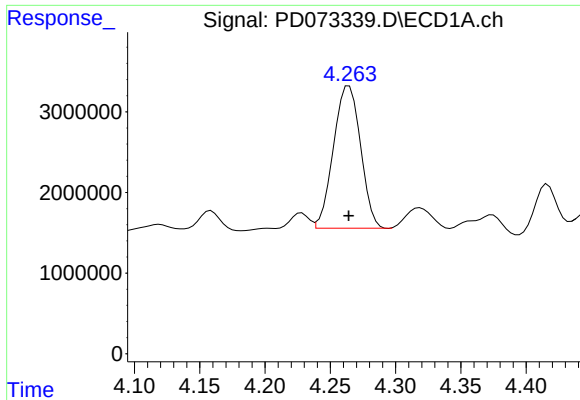

#24 Chlordane-2


R.T.: 4.264 min
Delta R.T.: 0.000 min
Response: 25456028
Conc: 267.23 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

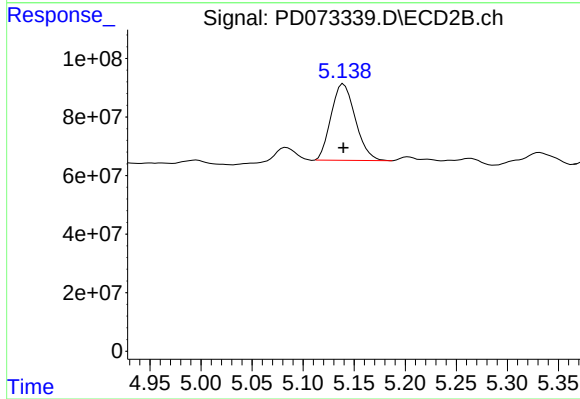


#24 Chlordane-2

R.T.: 5.140 min
Delta R.T.: 0.000 min
Response: 431597438
Conc: 271.57 ng/ml

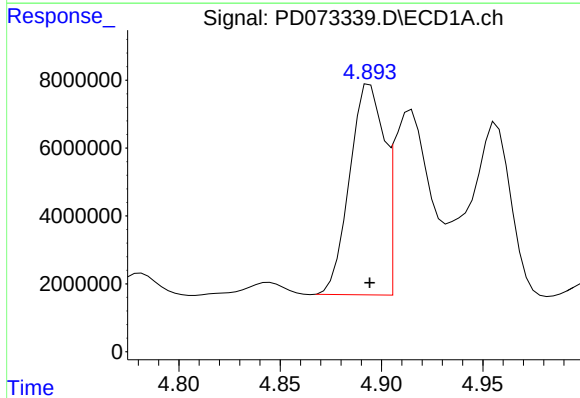


#25 Chlordane-3

R.T.: 4.894 min
Delta R.T.: 0.000 min
Response: 73174652
Conc: 248.39 ng/ml

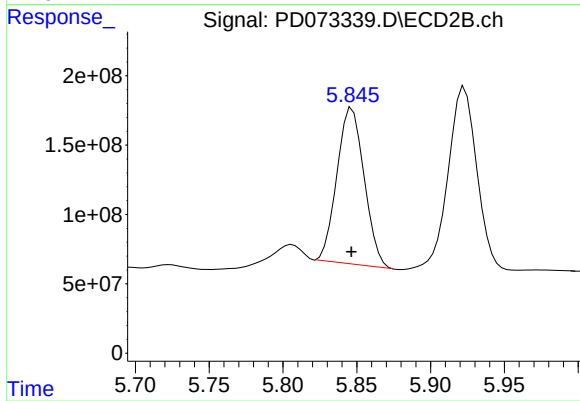

#25 Chlordane-3


R.T.: 5.847 min
Delta R.T.: 0.000 min
Response: 1435827287
Conc: 257.49 ng/ml

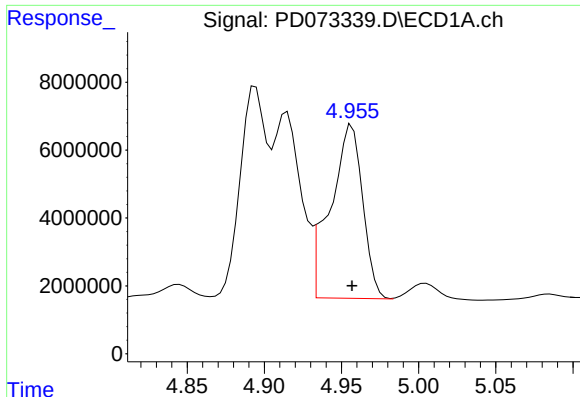

#26 Chlordane-4


R.T.: 4.957 min
Delta R.T.: 0.000 min
Response: 74219737
Conc: 249.56 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

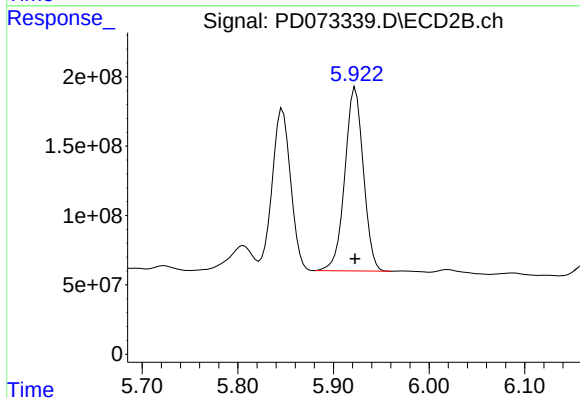


#26 Chlordane-4

R.T.: 5.923 min
Delta R.T.: 0.000 min
Response: 1785314357
Conc: 256.34 ng/ml

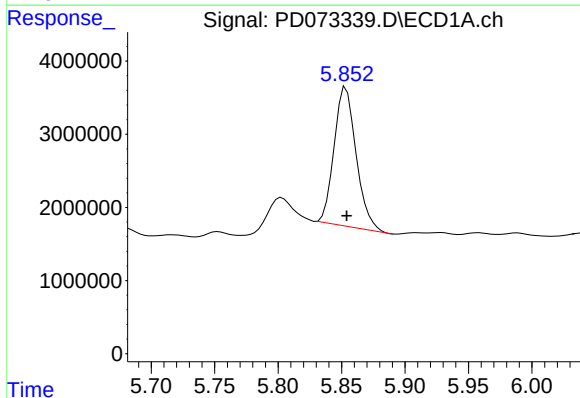


#27 Chlordane-5

R.T.: 5.854 min
Delta R.T.: 0.000 min
Response: 22732154
Conc: 253.15 ng/ml

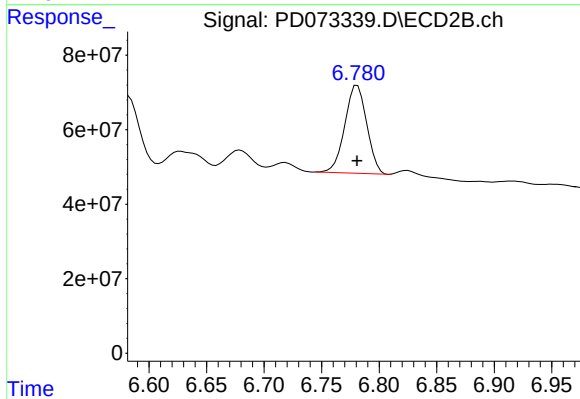

#27 Chlordane-5


R.T.: 6.781 min
Delta R.T.: 0.000 min
Response: 305006678
Conc: 261.66 ng/ml

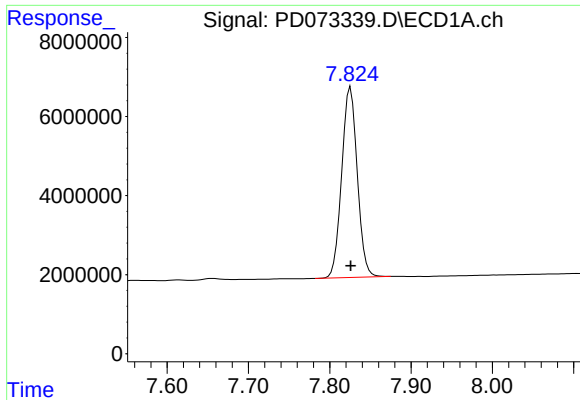

#28 Decachlorobiphenyl

R.T.: 7.826 min
Delta R.T.: 0.000 min
Response: 63966185
Conc: 26.45 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

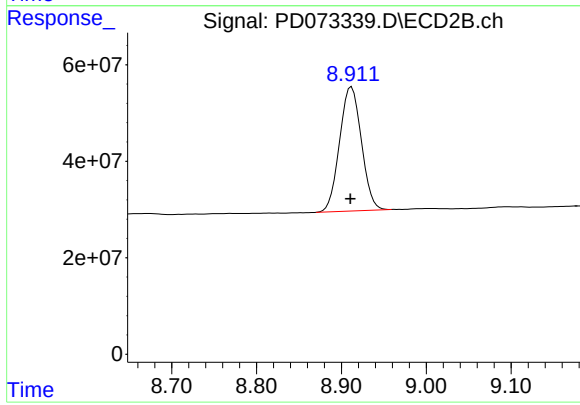

#28 Decachlorobiphenyl

R.T.: 8.912 min
Delta R.T.: 0.001 min
Response: 459833548
Conc: 26.17 ng/ml