

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121622\
 Data File : PD073338.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Dec 2022 13:40
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 16 14:48:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121622.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 16 14:47:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.696	3.459	122.2E6	4584.6E6	50.000	50.000
28)	SA Decachlor...	7.826	8.911	120.9E6	878.6E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	3.688	4.608	39200668	1196.9E6	500.000	500.000
24)	Chlordane-2	4.264	5.139	47629623	794.6E6	500.000	500.000
25)	Chlordane-3	4.894	5.846	147.3E6	2788.1E6	500.000	500.000
26)	Chlordane-4	4.957	5.923	148.7E6	3482.4E6	500.000	500.000
27)	Chlordane-5	5.854	6.781	44898869	582.8E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121622\
Data File : PD073338.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Dec 2022 13:40
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 14:48:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121622.M
Quant Title : GC Extractables
QLast Update : Fri Dec 16 14:47:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

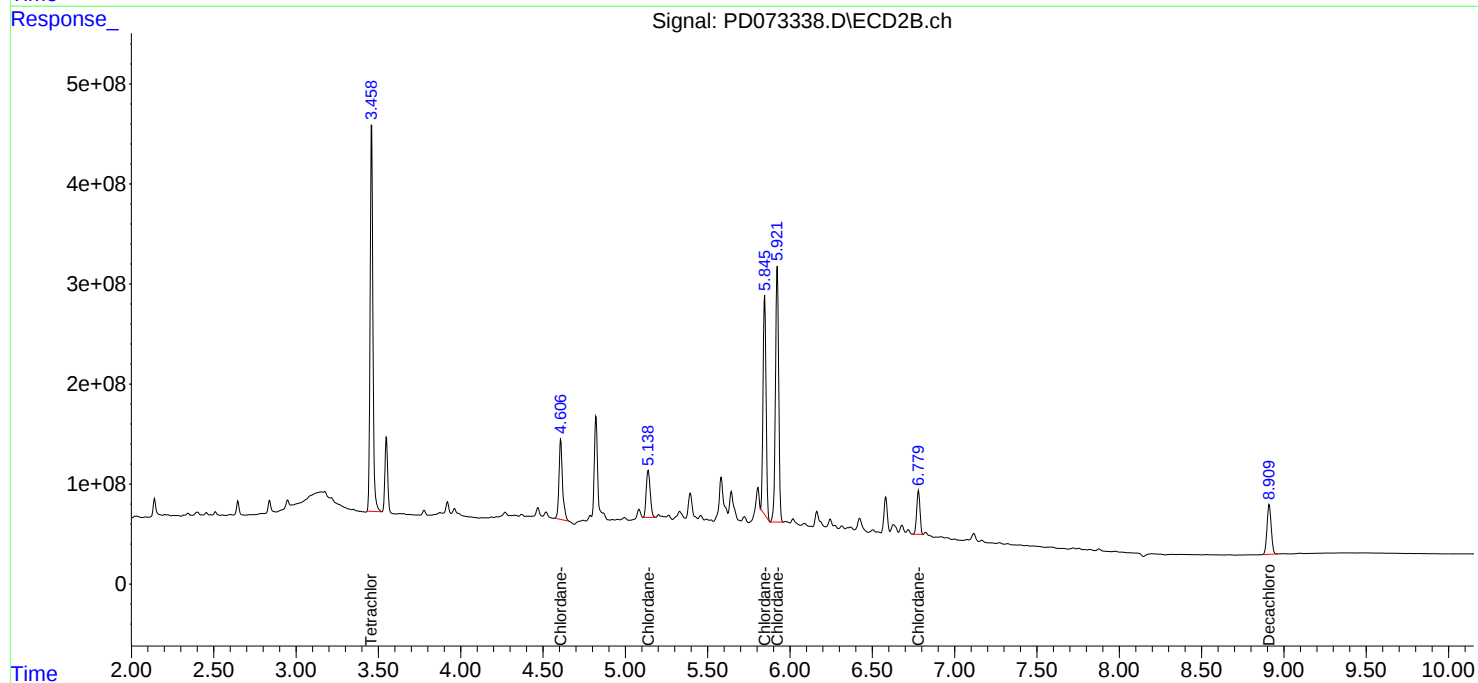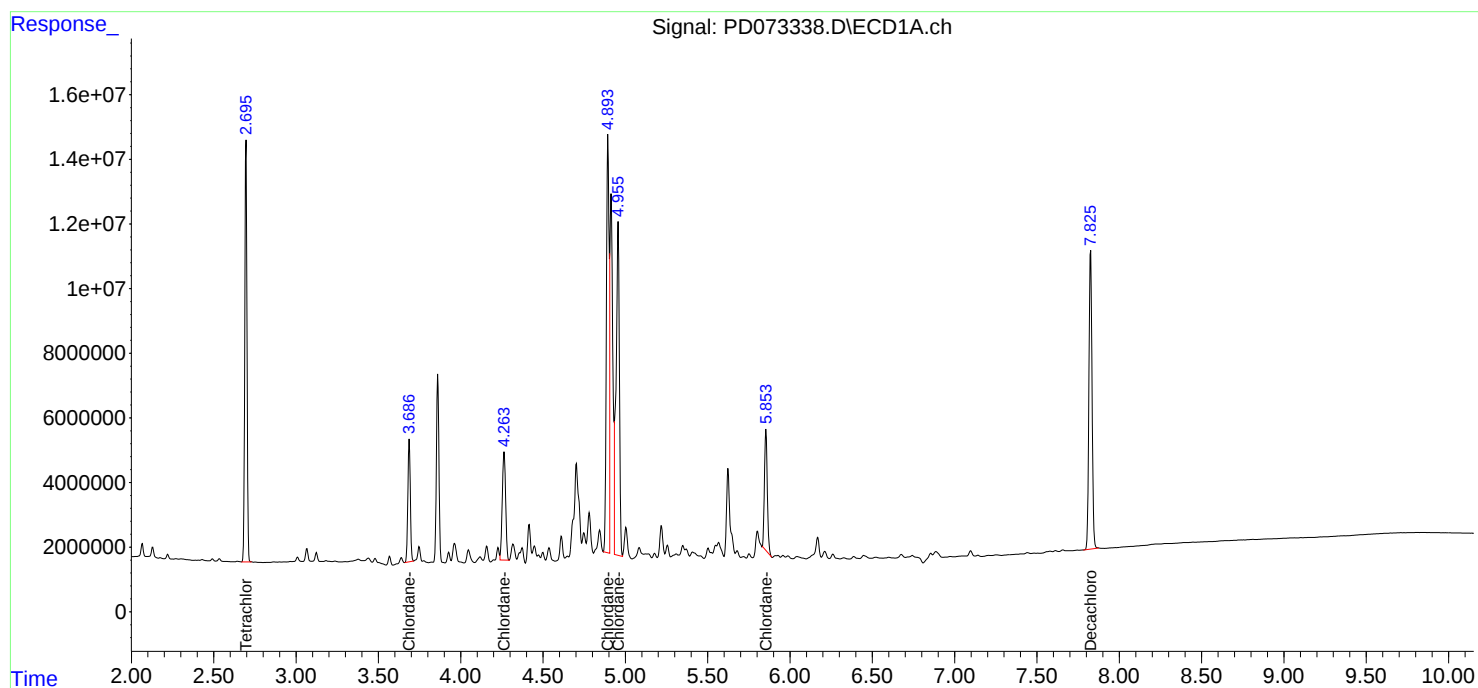


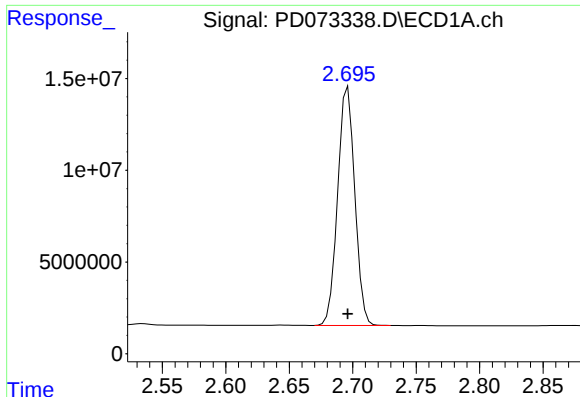

#1 Tetrachloro-m-xylene


R.T.: 2.696 min
Delta R.T.: 0.000 min
Response: 122214669
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

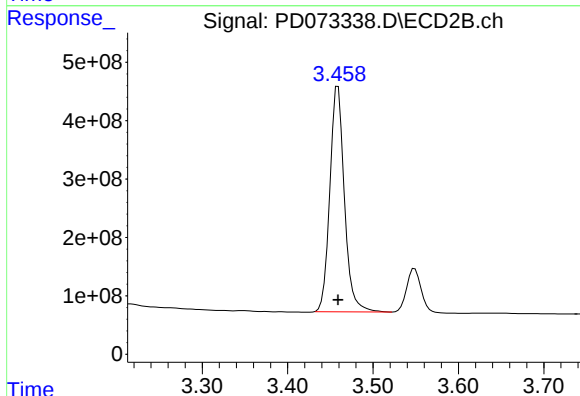


#1 Tetrachloro-m-xylene

R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 4584553209
Conc: 50.00 ng/ml

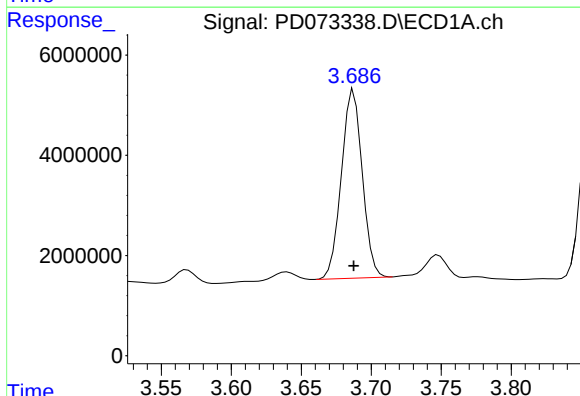


#23 Chlordane-1

R.T.: 3.688 min
Delta R.T.: 0.000 min
Response: 39200668
Conc: 500.00 ng/ml

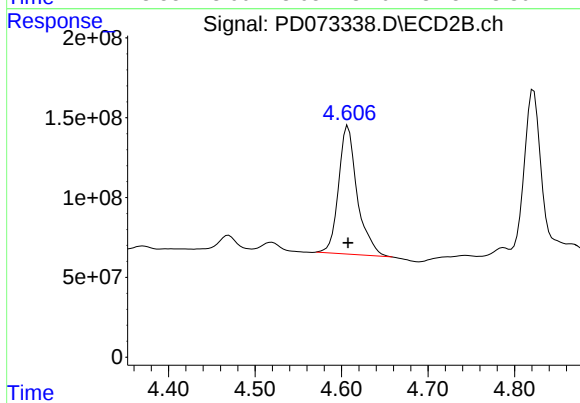

#23 Chlordane-1


R.T.: 4.608 min
Delta R.T.: 0.000 min
Response: 1196862515
Conc: 500.00 ng/ml

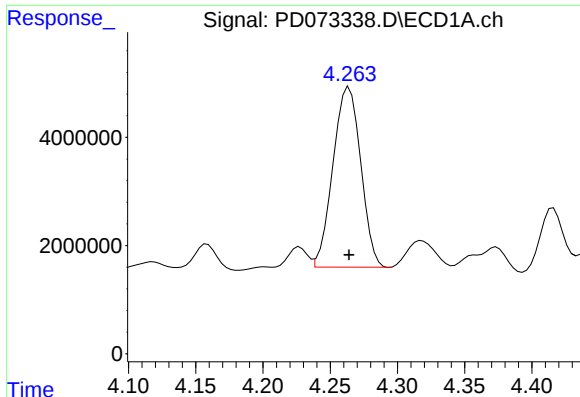

#24 Chlordane-2


R.T.: 4.264 min
Delta R.T.: 0.000 min
Response: 47629623
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

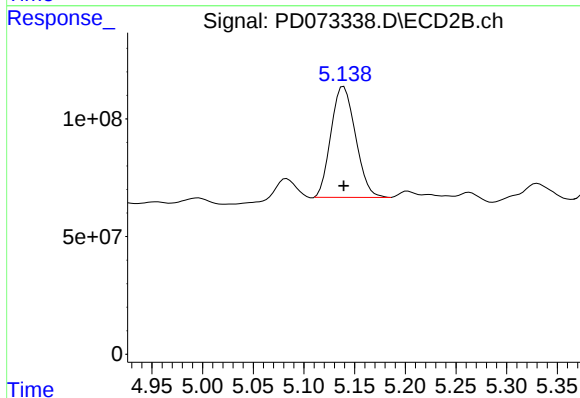


#24 Chlordane-2

R.T.: 5.139 min
Delta R.T.: 0.000 min
Response: 794644837
Conc: 500.00 ng/ml

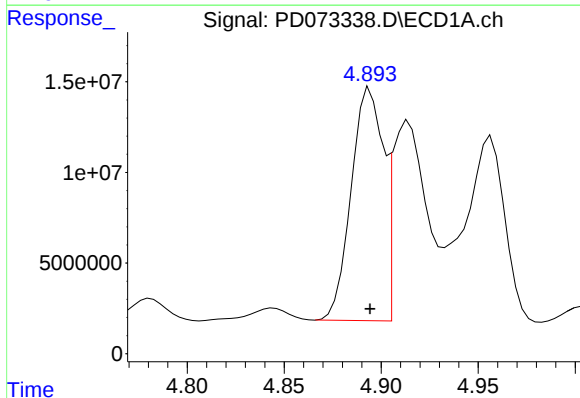


#25 Chlordane-3

R.T.: 4.894 min
Delta R.T.: 0.000 min
Response: 147299968
Conc: 500.00 ng/ml

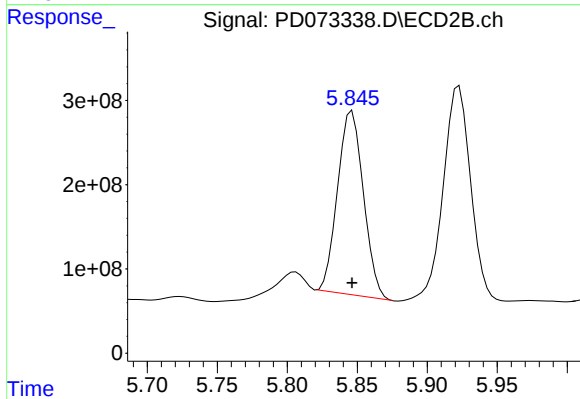

#25 Chlordane-3


R.T.: 5.846 min
Delta R.T.: 0.000 min
Response: 2788097016
Conc: 500.00 ng/ml

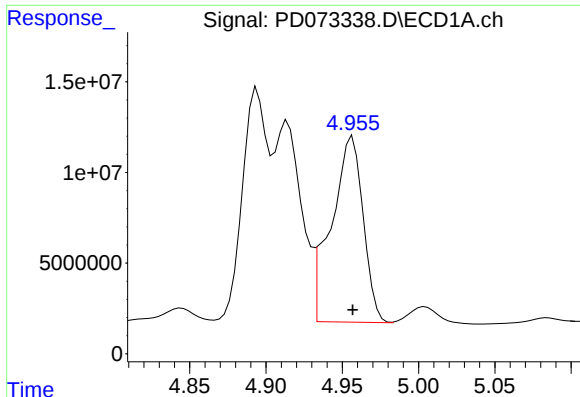

#26 Chlordane-4


R.T.: 4.957 min
Delta R.T.: 0.000 min
Response: 148702060
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

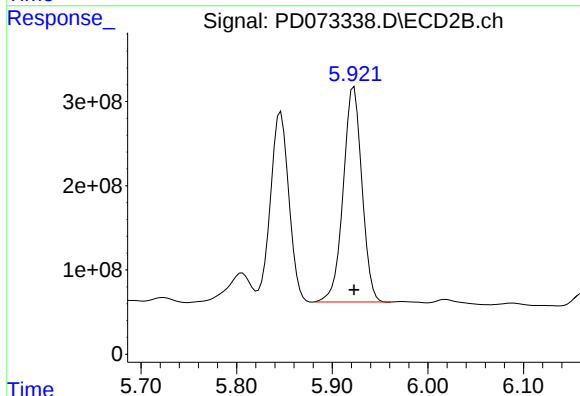


#26 Chlordane-4

R.T.: 5.923 min
Delta R.T.: 0.000 min
Response: 3482362213
Conc: 500.00 ng/ml

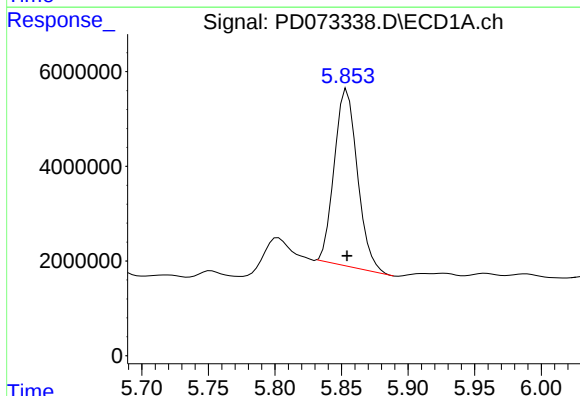


#27 Chlordane-5

R.T.: 5.854 min
Delta R.T.: 0.000 min
Response: 44898869
Conc: 500.00 ng/ml

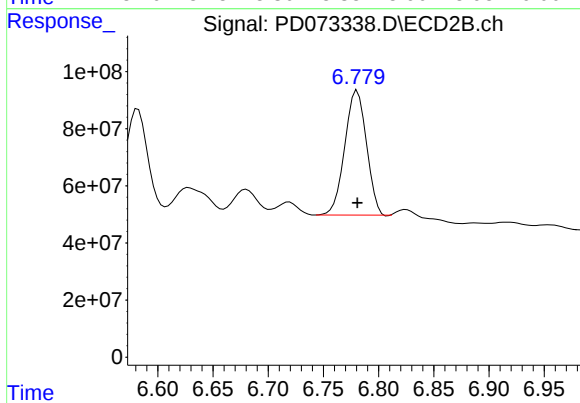

#27 Chlordane-5


R.T.: 6.781 min
Delta R.T.: 0.000 min
Response: 582839473
Conc: 500.00 ng/ml

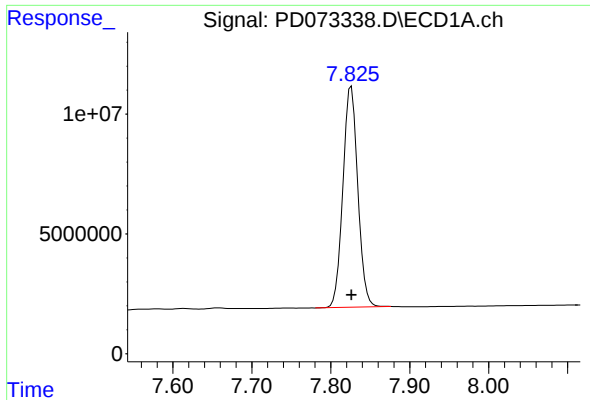

#28 Decachlorobiphenyl

R.T.: 7.826 min
Delta R.T.: 0.000 min
Response: 120922328
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

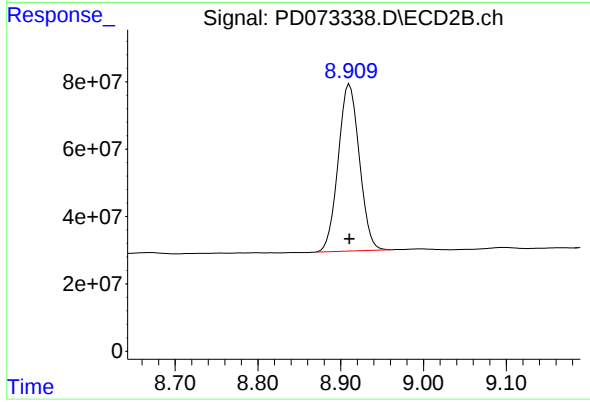

#28 Decachlorobiphenyl

R.T.: 8.911 min
Delta R.T.: 0.000 min
Response: 878590367
Conc: 50.00 ng/ml