

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121622\
 Data File : PD073347.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Dec 2022 15:39
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD121622CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 16 15:50:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121622.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 16 15:44:52 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.697	3.459	124.6E6	4806.2E6	50.023	48.729
28)	SA Decachlor...	7.826	8.910	121.1E6	883.0E6	47.825	48.677
Target Compounds							
23)	Chlordane-1	3.687	4.607	40569217	1221.0E6	498.811	482.243
24)	Chlordane-2	4.264	5.139	48774843	817.5E6	489.414	488.990
25)	Chlordane-3	4.894	5.846	149.4E6	2869.0E6	500.490	494.348
26)	Chlordane-4	4.956	5.923	149.2E6	3604.6E6	493.593	495.199
27)	Chlordane-5	5.854	6.781	45158457	602.2E6	500.503	507.543



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121622\
Data File : PD073347.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Dec 2022 15:39
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD121622CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 15:50:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121622.M
Quant Title : GC Extractables
QLast Update : Fri Dec 16 15:44:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

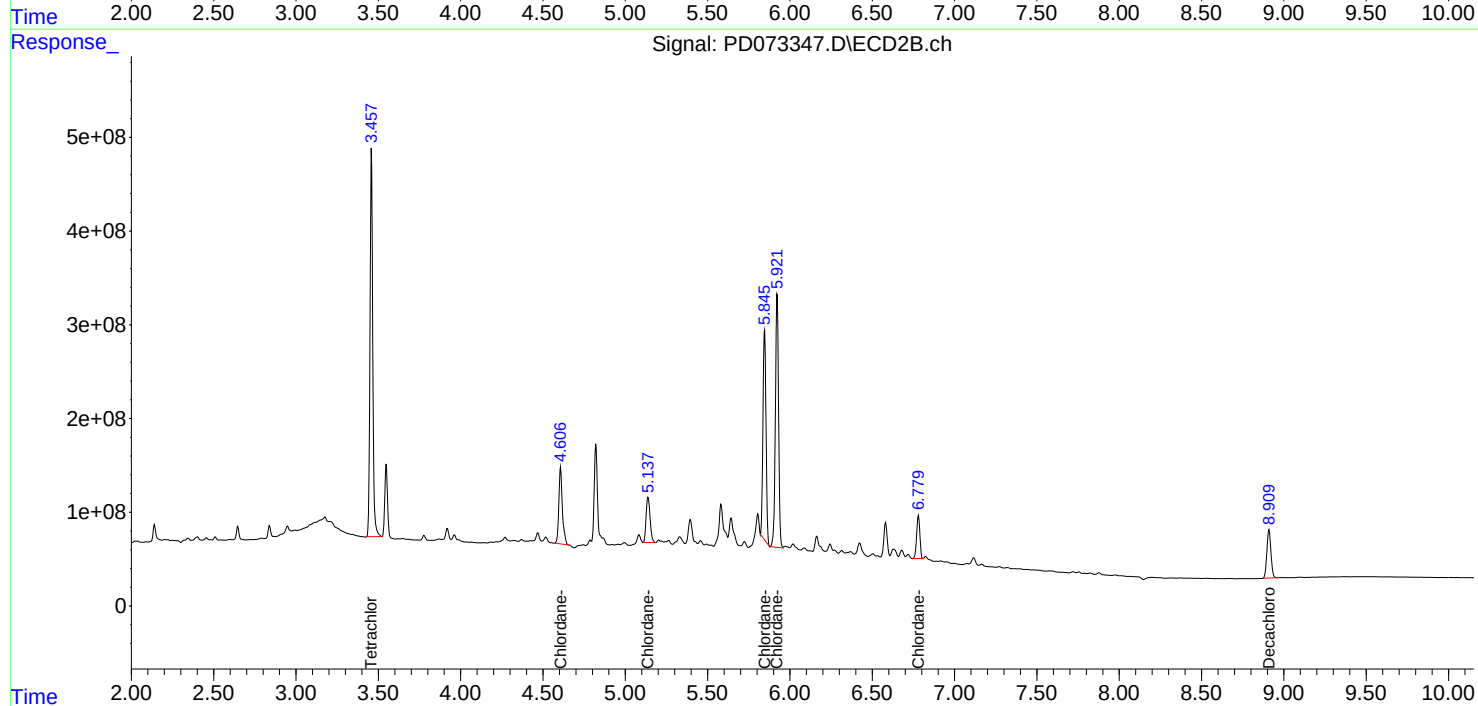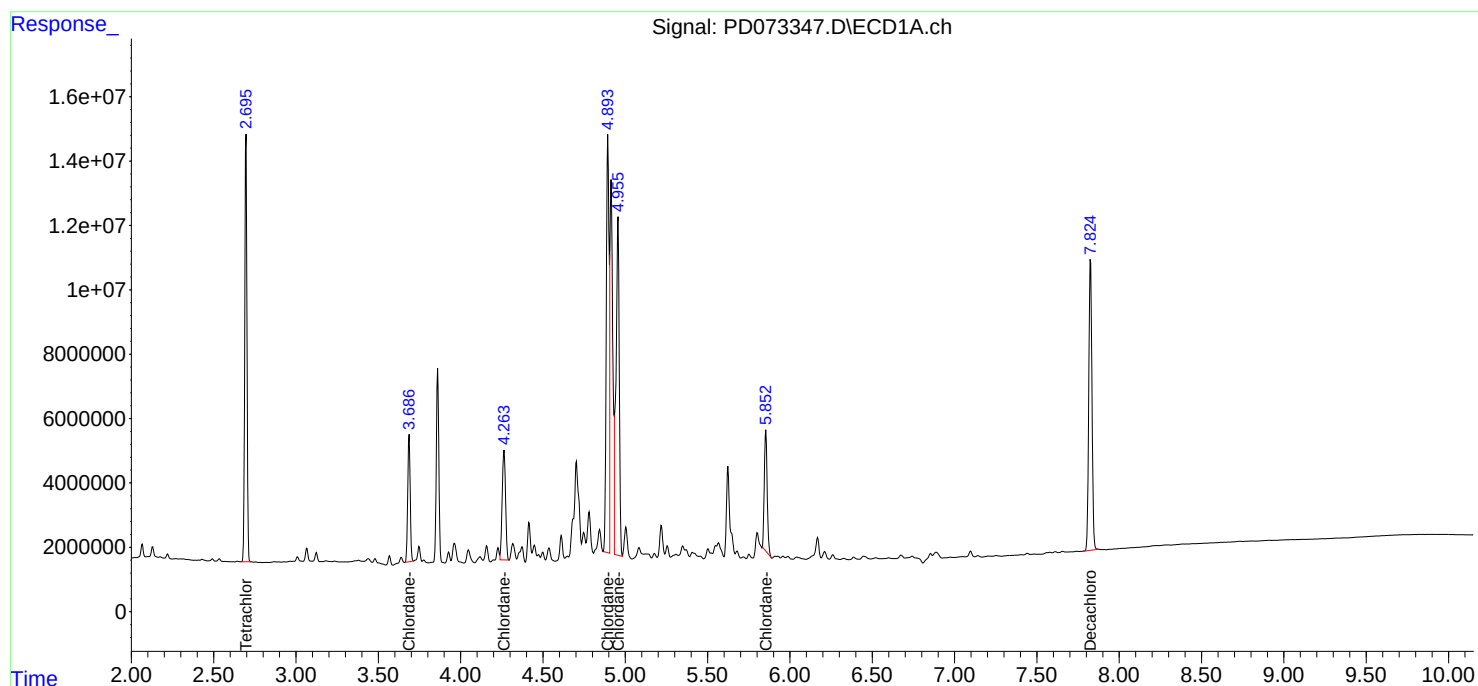


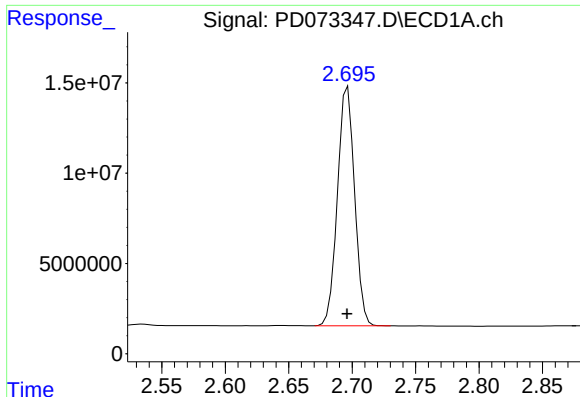

#1 Tetrachloro-m-xylene


R.T.: 2.697 min
Delta R.T.: 0.000 min
Response: 124564932
Conc: 50.02 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD121622CHLOR

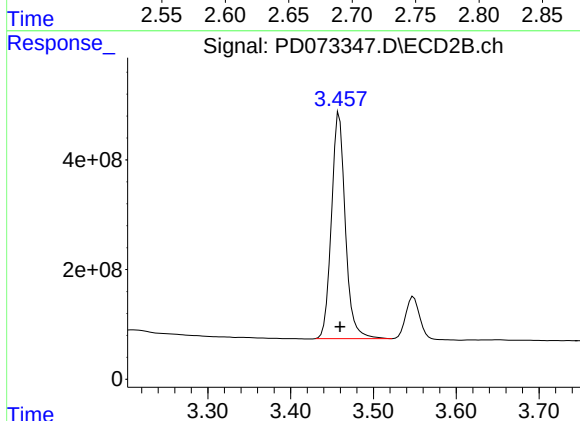


#1 Tetrachloro-m-xylene

R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 4806164808
Conc: 48.73 ng/ml

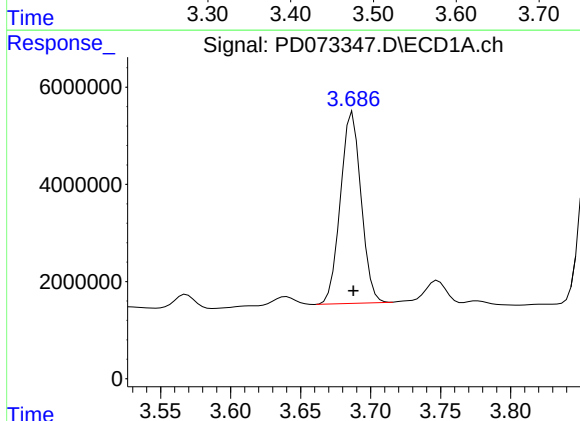


#23 Chlordane-1

R.T.: 3.687 min
Delta R.T.: 0.000 min
Response: 40569217
Conc: 498.81 ng/ml

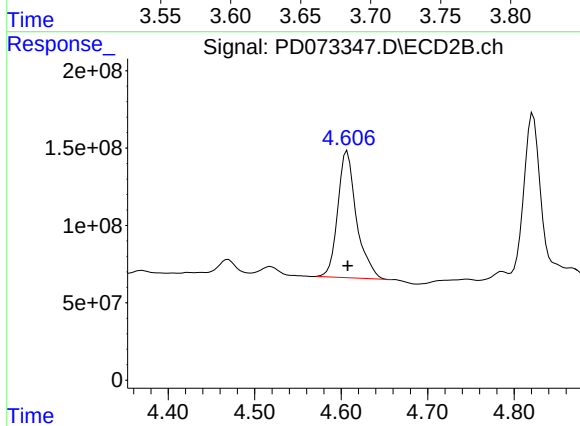

#23 Chlordane-1


R.T.: 4.607 min
Delta R.T.: 0.000 min
Response: 1220974294
Conc: 482.24 ng/ml

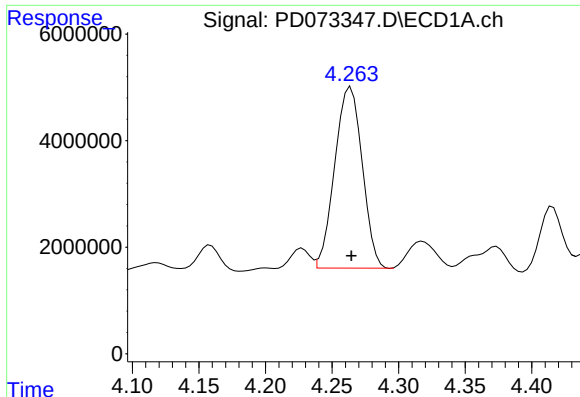

#24 Chlordane-2


R.T.: 4.264 min
Delta R.T.: 0.000 min
Response: 48774843
Conc: 489.41 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD121622CHLOR

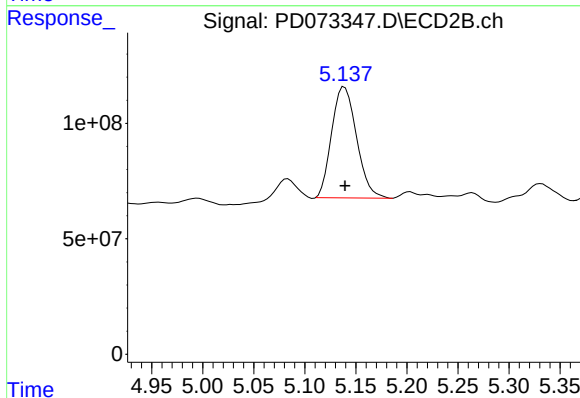


#24 Chlordane-2

R.T.: 5.139 min
Delta R.T.: 0.000 min
Response: 817487972
Conc: 488.99 ng/ml

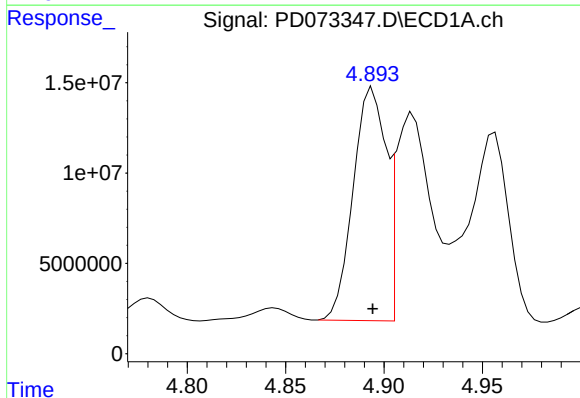


#25 Chlordane-3

R.T.: 4.894 min
Delta R.T.: 0.000 min
Response: 149401345
Conc: 500.49 ng/ml

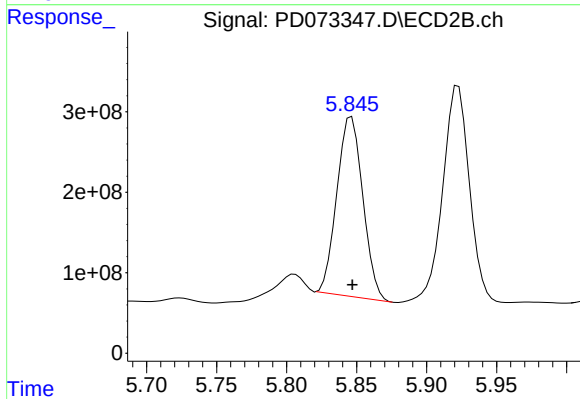

#25 Chlordane-3


R.T.: 5.846 min
Delta R.T.: 0.000 min
Response: 2868980045
Conc: 494.35 ng/ml

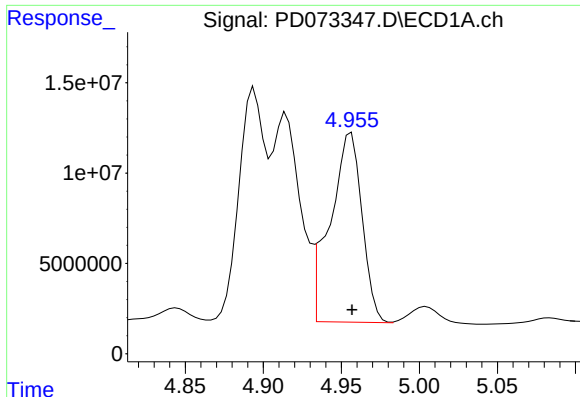

#26 Chlordane-4


R.T.: 4.956 min
Delta R.T.: 0.000 min
Response: 149180225
Conc: 493.59 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD121622CHLOR

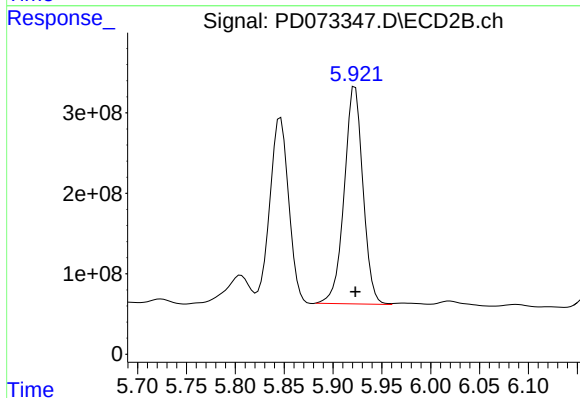


#26 Chlordane-4

R.T.: 5.923 min
Delta R.T.: 0.000 min
Response: 3604554353
Conc: 495.20 ng/ml

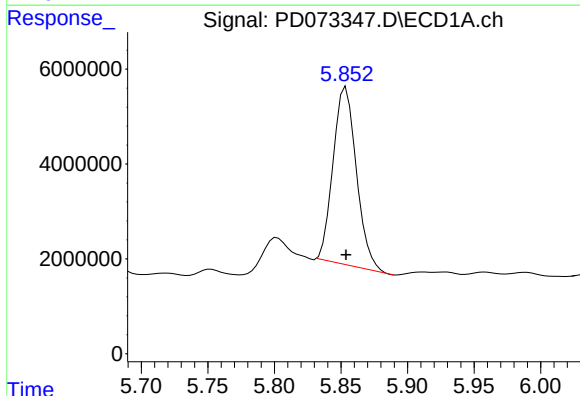


#27 Chlordane-5

R.T.: 5.854 min
Delta R.T.: 0.000 min
Response: 45158457
Conc: 500.50 ng/ml

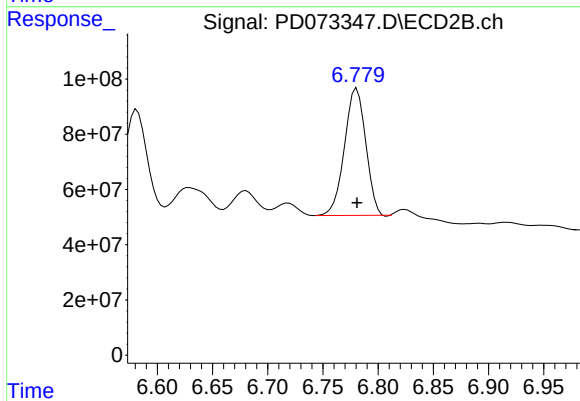

#27 Chlordane-5


R.T.: 6.781 min
Delta R.T.: 0.000 min
Response: 602217496
Conc: 507.54 ng/ml

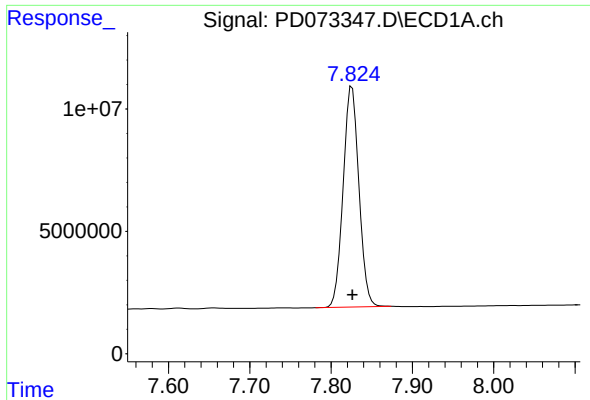

#28 Decachlorobiphenyl

R.T.: 7.826 min
Delta R.T.: 0.000 min
Response: 121086767
Conc: 47.83 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD121622CHLOR

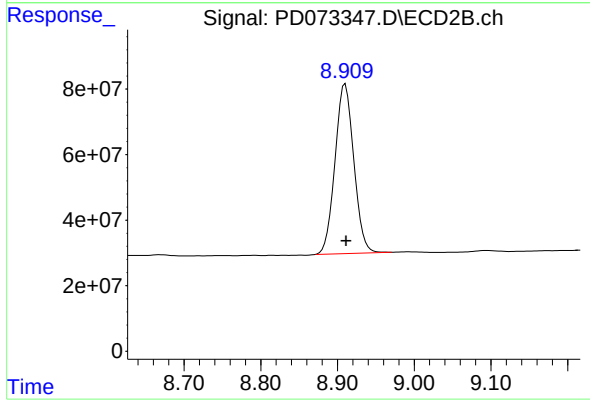

#28 Decachlorobiphenyl

R.T.: 8.910 min
Delta R.T.: -0.001 min
Response: 883030075
Conc: 48.68 ng/ml