

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121623\
 Data File : PD080098.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Dec 2023 17:03
 Operator : AR\AJ
 Sample : TOXAPH301
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 21 13:38:16 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 21 13:37:55 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.567	2.800	28231152	48440295	20.000	20.000
27)	SA Decachlor...	9.111	7.942	44596067	60680811	40.000	40.000
Target Compounds							
22)	Toxaphene-1	5.886	5.031	12437819	34639642	2000.000	2000.000
23)	Toxaphene-2	6.476	5.356	35294990	34644054	2000.000	2000.000
24)	Toxaphene-3	7.096	6.629	104.1E6	123.5E6	2000.000	2000.000
25)	Toxaphene-4	7.187	6.753	77613741	169.9E6	2000.000	2000.000
26)	Toxaphene-5	7.608	7.069	57434084	71501208	2000.000	2000.000

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121623\
Data File : PD080098.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Dec 2023 17:03
Operator : AR\AJ
Sample : TOXAPH301
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 13:38:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
Quant Title : GC Extractables
QLast Update : Thu Dec 21 13:37:55 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

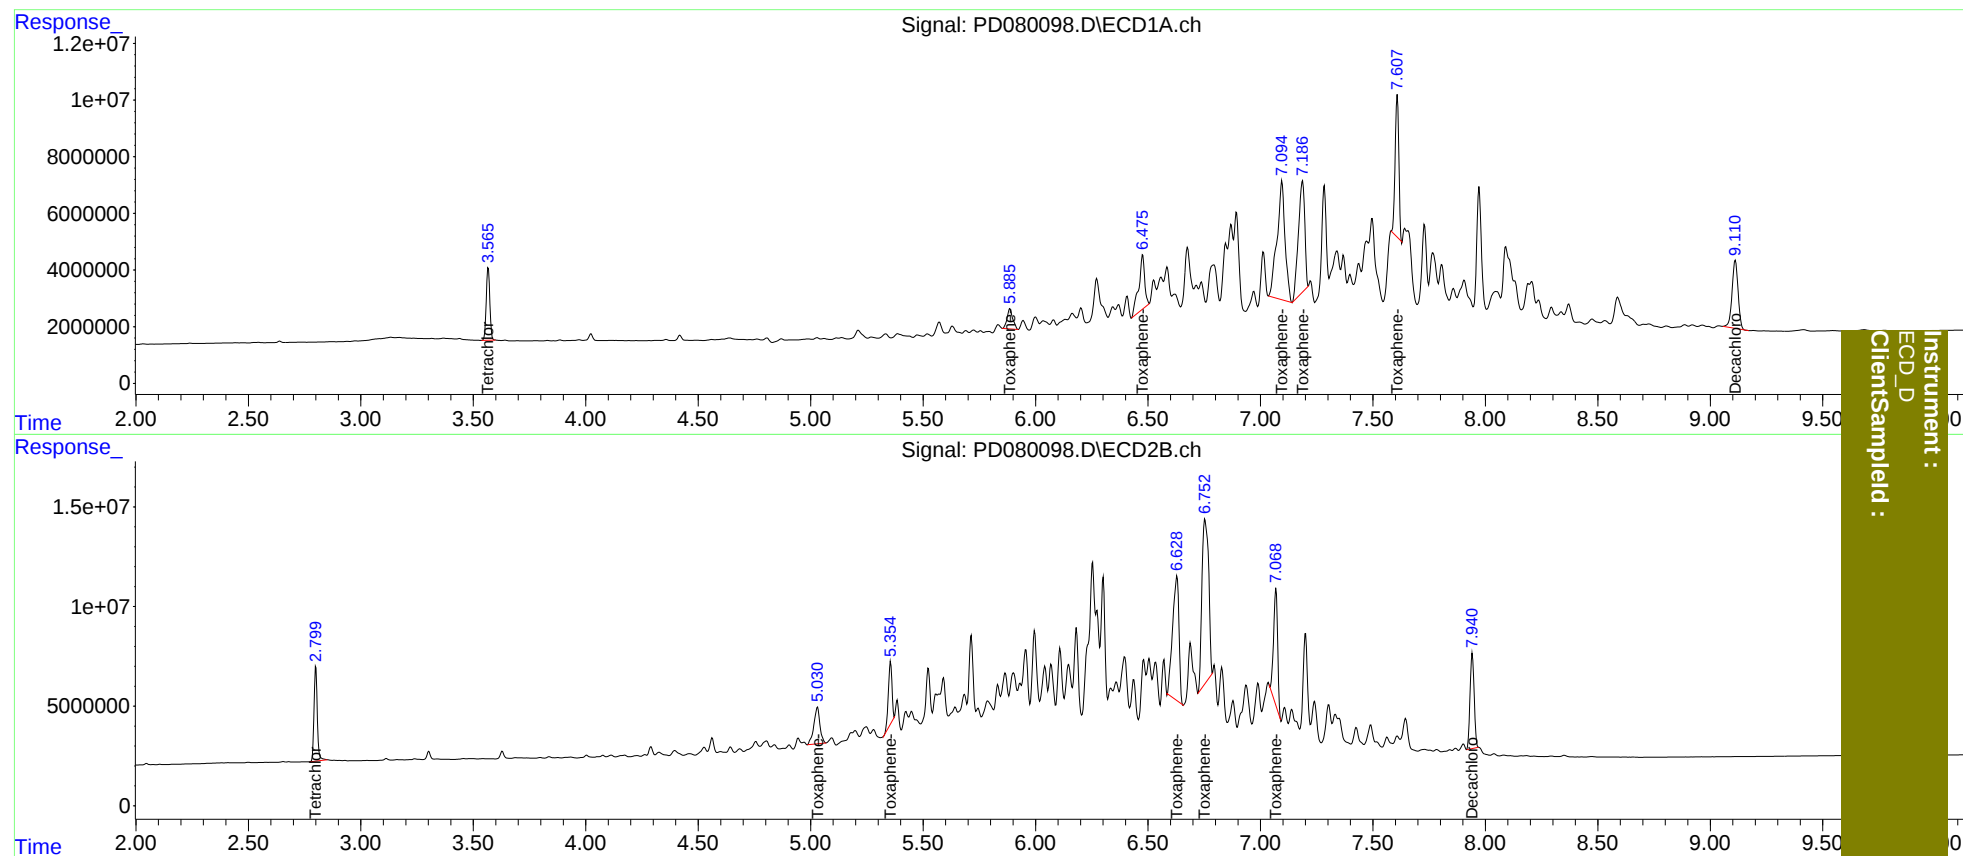

Instrument :
ECD_D
ClientSampled :
0