

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121623\
 Data File : PD080111.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Dec 2023 19:56
 Operator : AR\AJ
 Sample : PIBLK112
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 16 03:13:50 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 16 03:10:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.800	28046469	48003096	21.966	21.588
27)	SA Decachlor...	9.111	7.941	41365030	61253704	25.728	25.520
Target Compounds							
2)	A alpha-BHC	0.000	3.290	0	95731	N.D.	<MDL
3)	MA gamma-BHC...	0.000	3.650	0	64585	N.D.	<MDL
7)	B delta-BHC	0.000	4.182	0	140422	N.D.	<MDL
14)	MA Endrin	0.000	5.682	0	101689	N.D.	<MDL
15)	B Endosulfa...	0.000	5.918f	0	115717	N.D.	<MDL


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121623\
Data File : PD080111.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Dec 2023 19:56
Operator : AR\AJ
Sample : PIBLK112
Misc :
ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 03:13:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Dec 16 03:10:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

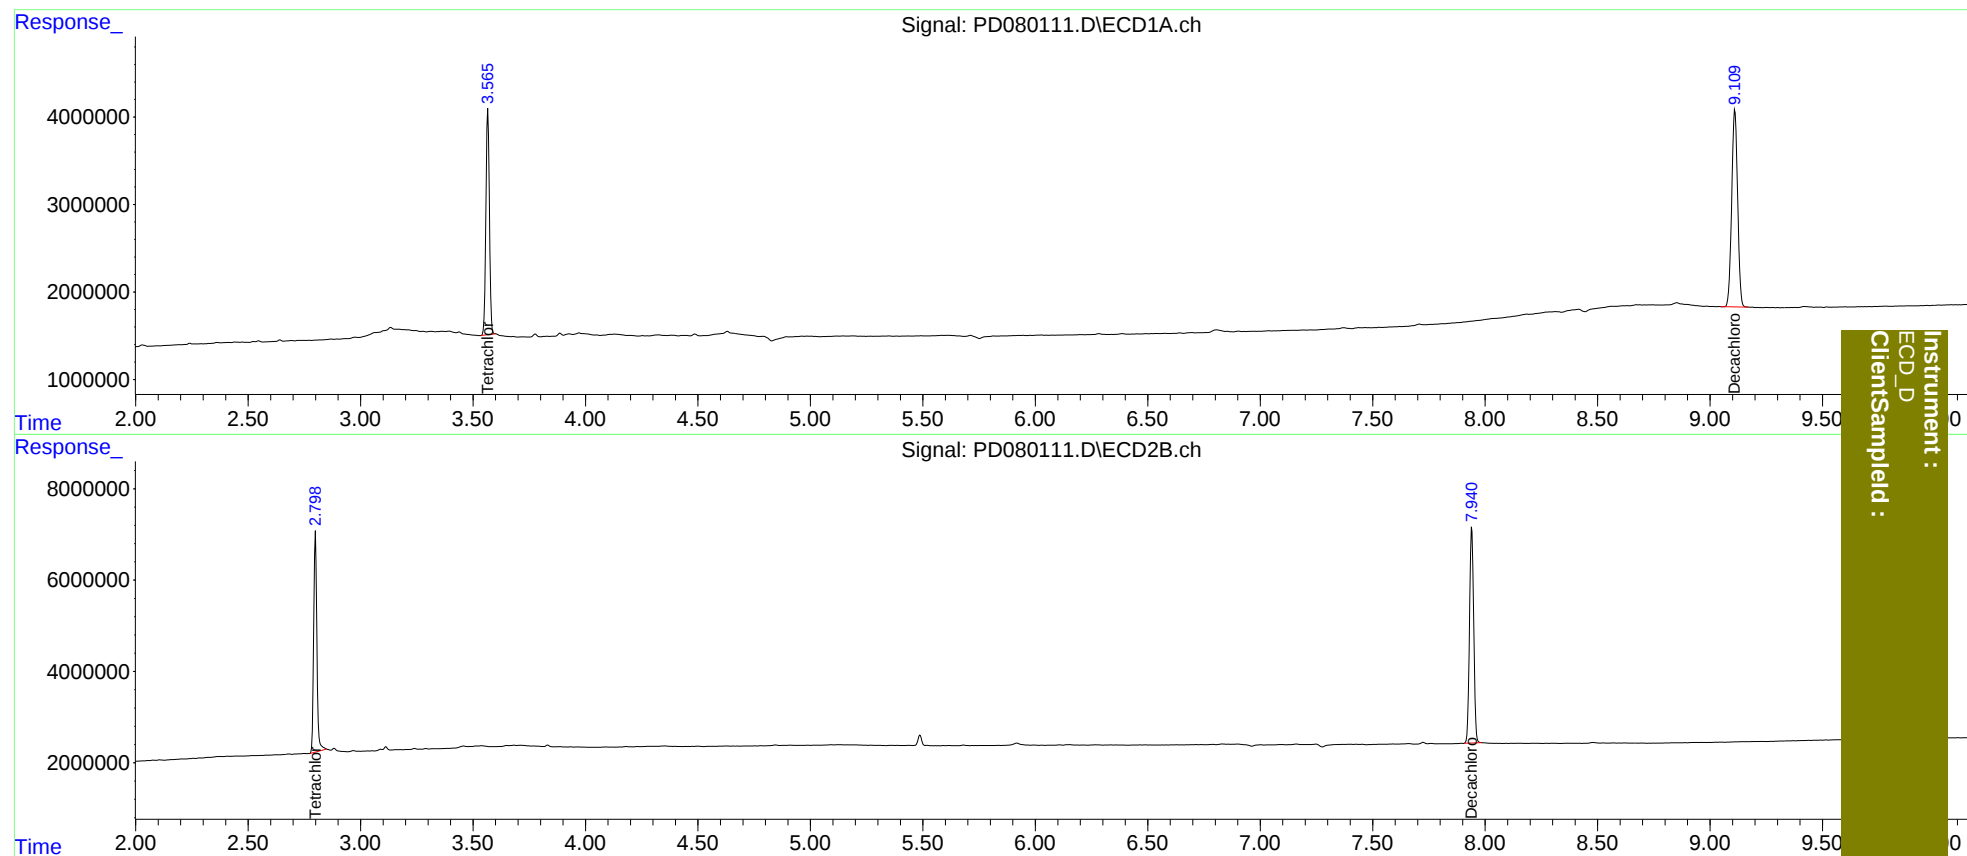


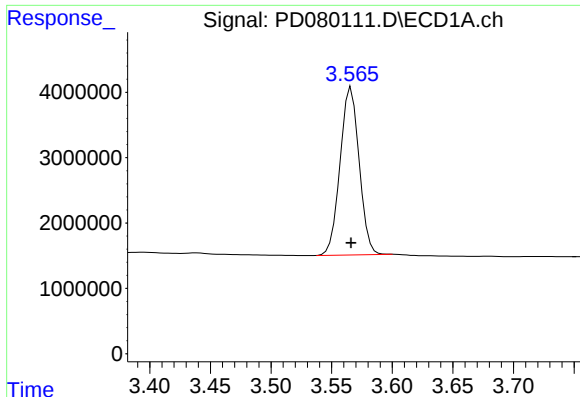

#1 Tetrachloro-m-xylene


R.T.: 3.566 min
Delta R.T.: 0.000 min
Response: 28046469
Conc: 21.97 ng/ml

Instrument :
ECD_D
ClientSampleId :

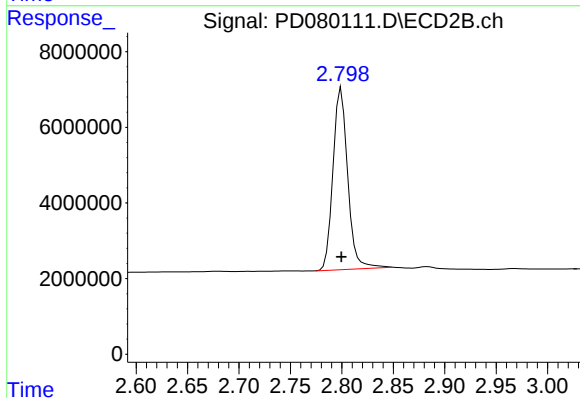


#1 Tetrachloro-m-xylene

R.T.: 2.800 min
Delta R.T.: 0.000 min
Response: 48003096
Conc: 21.59 ng/ml

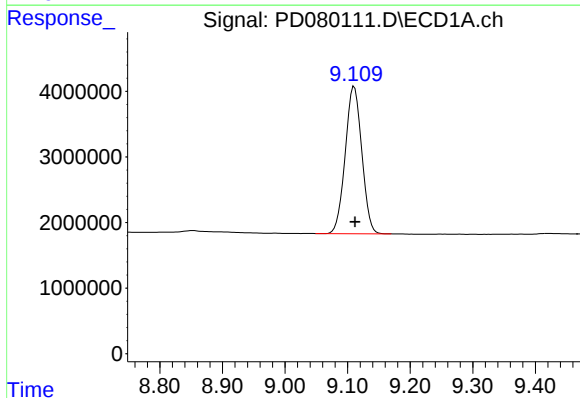

#27 Decachlorobiphenyl

R.T.: 9.111 min
Delta R.T.: -0.001 min
Response: 41365030
Conc: 25.73 ng/ml

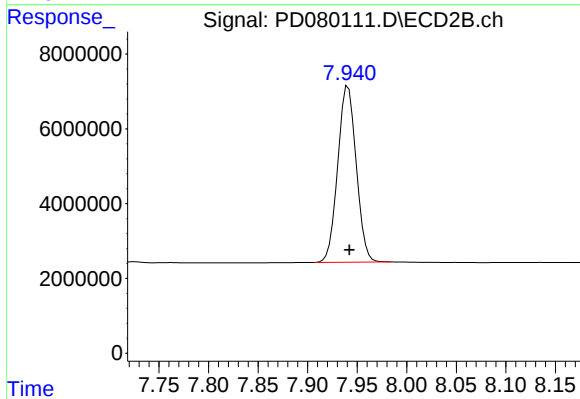

#27 Decachlorobiphenyl

R.T.: 7.941 min
Delta R.T.: -0.001 min
Response: 61253704
Conc: 25.52 ng/ml