

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121623\
 Data File : PD080094.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Dec 2023 16:10
 Operator : AR\AJ
 Sample : RESC015
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC018

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 16 03:18:10 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 16 03:10:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.567	2.800	26815528	46007403	21.002	20.691
27)	SA Decachlor...	9.112	7.942	67657026	98329525	42.081	40.966
Target Compounds							
2)	A alpha-BHC	4.024	3.302	20139145	33959266	9.769	9.960
3)	MA gamma-BHC...	4.357	3.632	19866090	32197823	10.004	10.002
4)	MA Heptachlor	4.950	3.974	21391490	32951691	10.244	10.290
5)	MB Aldrin	5.293	4.254	22859443	35849513	10.220	10.147
6)	B beta-BHC	4.551	3.927	10752178	17587792	10.359	10.299
7)	B delta-BHC	4.800	4.158	22318554	37786261	9.717	9.719
8)	B Heptachlo...	5.720	4.756	21633386	33787452	10.071	9.970
9)	A Endosulfan I	6.106	5.126	18706358	28304503	10.501	10.325
10)	B trans-Chl...	5.976	5.006	20554447	32769753	10.016	9.961
11)	B cis-Chlor...	6.056	5.070	21213946	33448569	10.109	9.973
12)	B 4,4'-DDE	6.226	5.259	37584267	61118873	19.456	19.458
13)	MA Dieldrin	6.382	5.390	37558897	59953584	20.181	20.005
14)	MA Endrin	6.612	5.666	31962427	53268384	20.406	20.246
15)	B Endosulfa...	6.829	5.958	37840127	57574401	20.170	19.858
16)	A 4,4'-DDD	6.743	5.812	27924688	46076330	20.132	20.040
17)	MA 4,4'-DDT	7.058	6.064	30189546	48049989	20.429	19.928
18)	B Endrin al...	6.960	6.138	30455316	47043361	20.417	20.401
19)	B Endosulfa...	7.194	6.360	37234874	56105684	20.303	20.003
20)	A Methoxychlor	7.533	6.638	81716971	133.5E6	103.207	106.059
21)	B Endrin ke...	7.681	6.866	39102583	65050079	20.097	20.328

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121623\
Data File : PD080094.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Dec 2023 16:10
Operator : AR\AJ
Sample : RESC015
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 03:18:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Dec 16 03:10:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

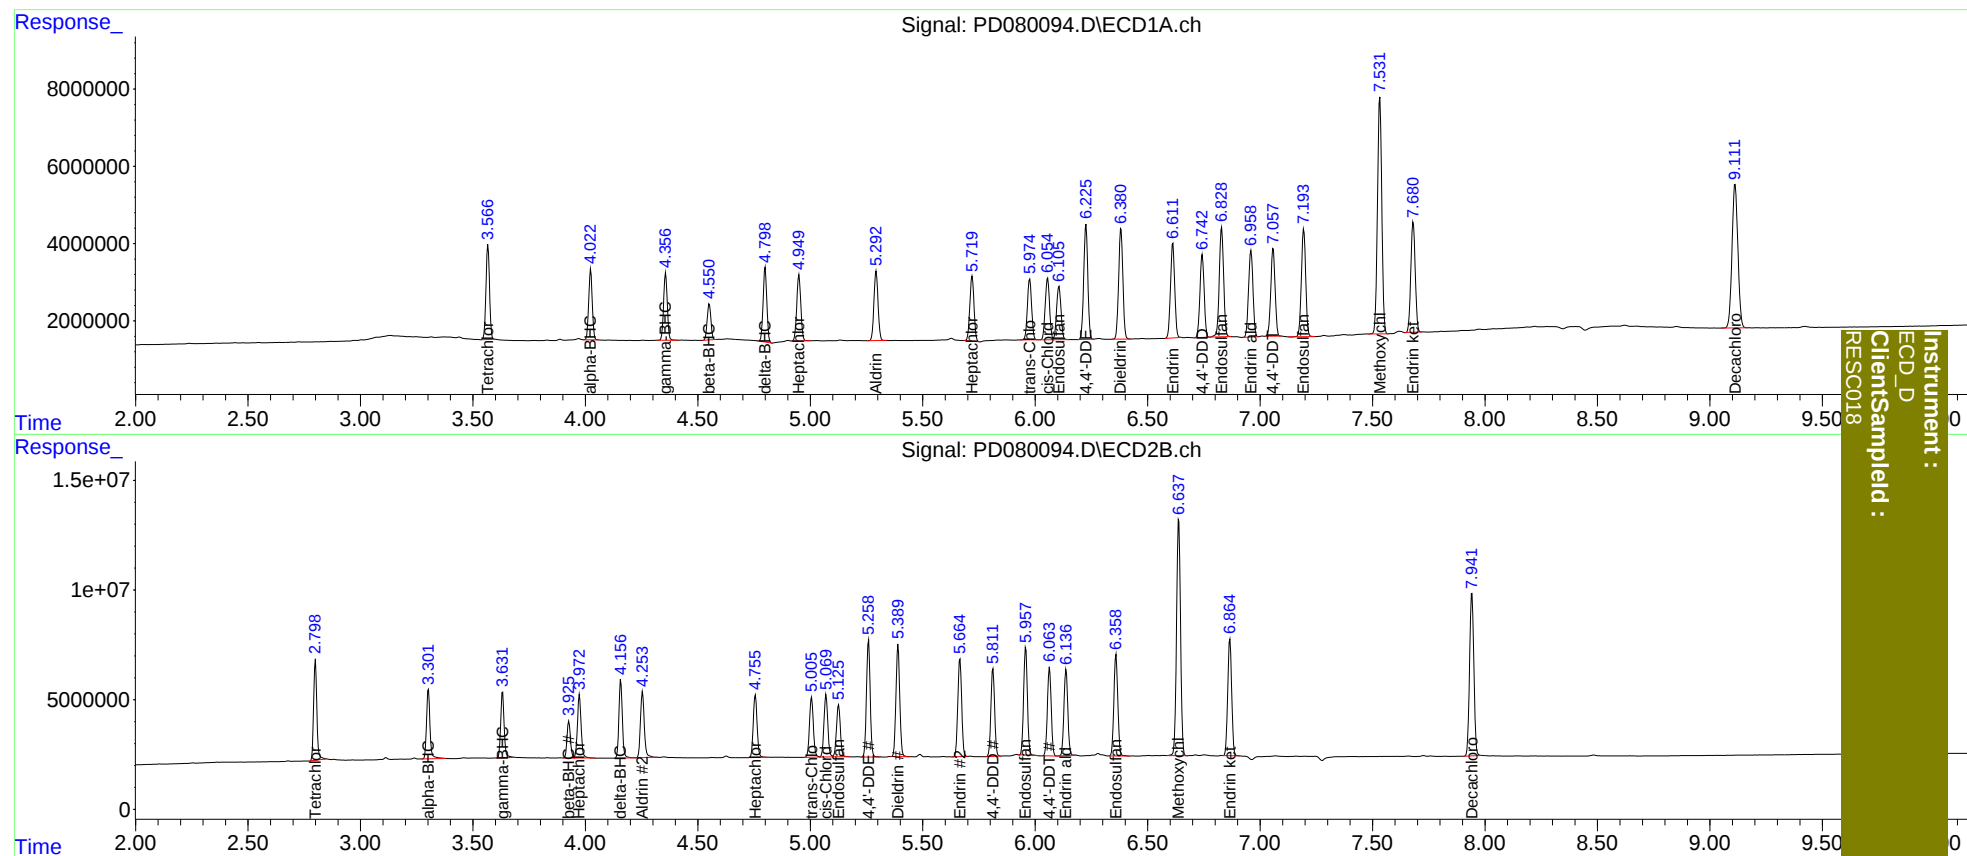

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121623\
Data File : PD080094.D
Acq On : 15 Dec 2023 16:10
Operator : AR\AJ
Sample : RESC015
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC018

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
Title : GC Extractables
Last Update : Sat Dec 16 03:10:23 2023
Integrator: ChemStation

RT#1	RT#2	Resolution
3.567	4.024	100.00%
4.024	4.357	100.00%
4.357	4.551	100.00%
4.551	4.800	100.00%
4.800	4.950	100.00%
4.950	5.293	100.00%
5.293	5.720	100.00%
5.720	5.976	100.00%
5.976	6.056	100.00%
6.056	6.106	97.77%
6.106	6.226	100.00%
6.226	6.382	100.00%
6.382	6.612	100.00%
6.612	6.743	100.00%
6.743	6.829	100.00%
6.829	6.960	100.00%
6.960	7.058	100.00%
7.058	7.194	100.00%
7.194	7.533	100.00%
7.533	7.681	100.00%
7.681	9.112	100.00%

Signal #2


2.800	3.302	100.00%
3.302	3.632	100.00%
3.632	3.927	100.00%
3.927	3.974	98.42%
3.974	4.158	100.00%
4.158	4.254	100.00%
4.254	4.756	100.00%
4.756	5.006	100.00%
5.006	5.070	100.00%
5.070	5.126	99.21%
5.126	5.259	100.00%
5.259	5.390	100.00%
5.390	5.666	100.00%
5.666	5.812	100.00%
5.812	5.958	100.00%
5.958	6.064	100.00%
6.064	6.138	100.00%
6.138	6.360	100.00%
6.360	6.638	100.00%
6.638	6.866	100.00%
6.866	7.942	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121623\
Data File : PD080094.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Dec 2023 16:10
Operator : AR\AJ
Sample : RESC015
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC018

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 03:18:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Dec 16 03:10:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

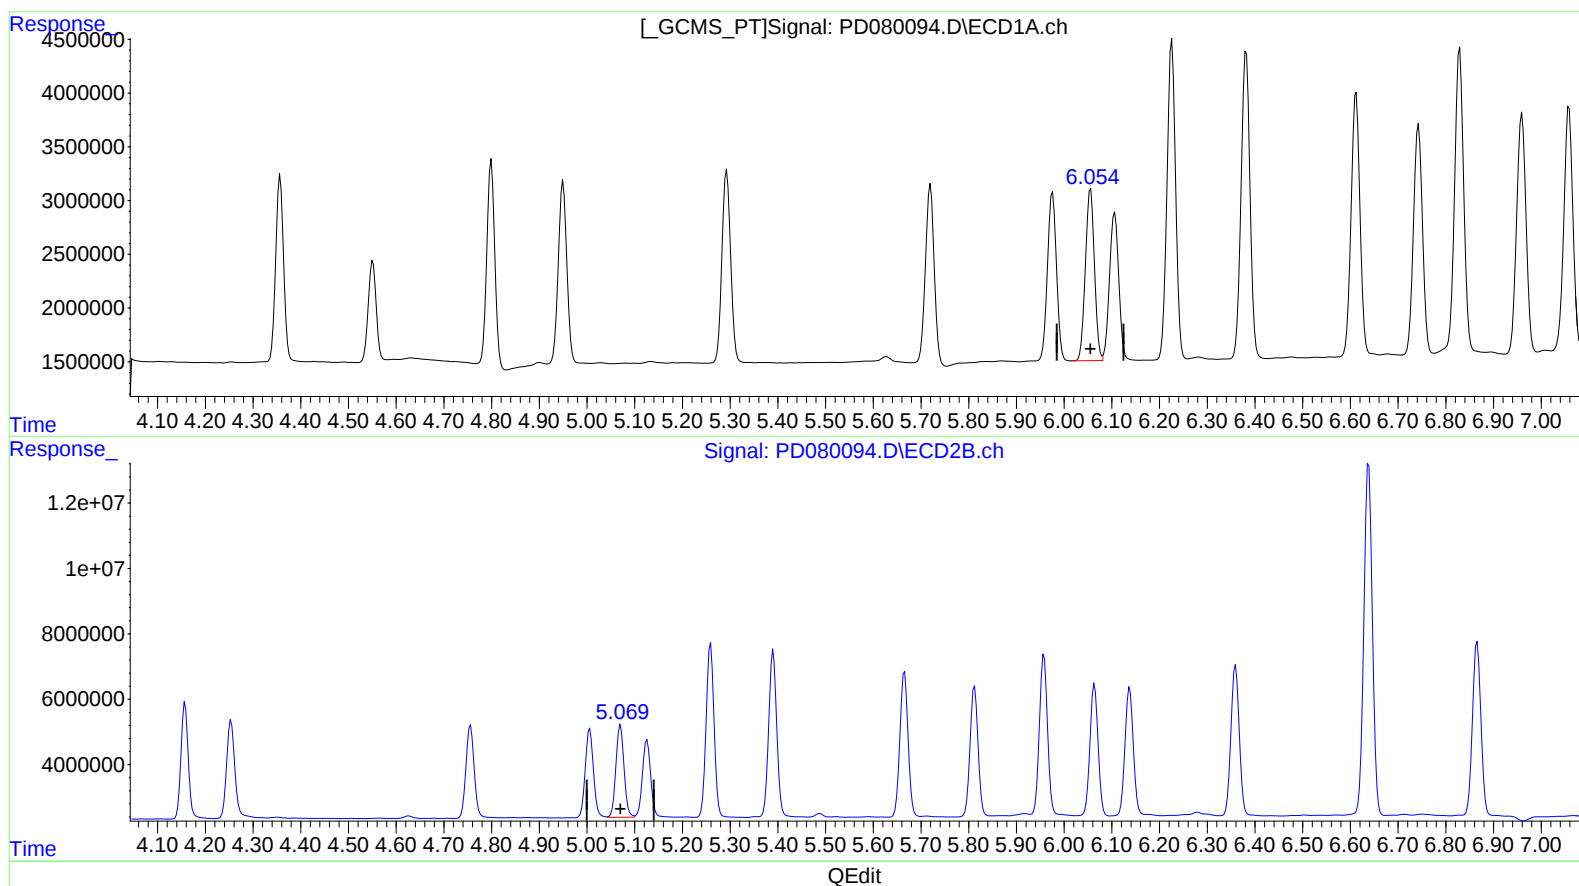

(11) cis-Chlordane (B)

6.056min 10.109 ng/ml

response 21213946

(11) cis-Chlordane #2 (B)

5.070min 9.973 ng/ml


response 33448569

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121623\
Data File : PD080094.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Dec 2023 16:10
Operator : AR\AJ
Sample : RESC015
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC018

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 03:18:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Dec 16 03:10:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

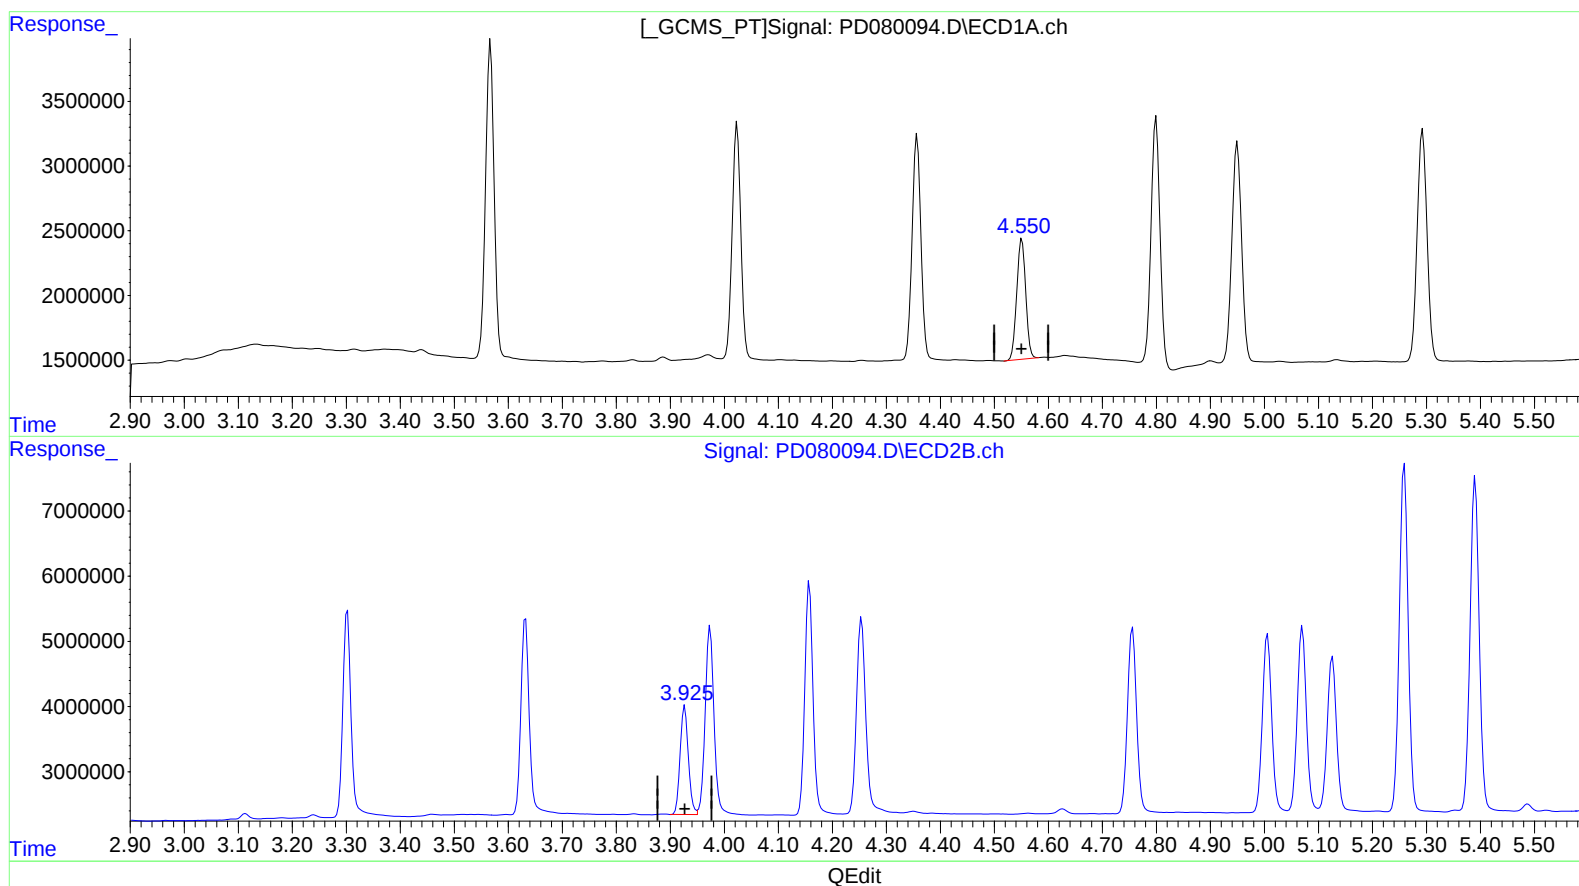

(6) beta-BHC (B)

4.551min 10.359 ng/ml

response 10752178

(6) beta-BHC #2 (B)

3.927min 10.299 ng/ml


response 17587792

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121623\
Data File : PD080094.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Dec 2023 16:10
Operator : AR\AJ
Sample : RESC015
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC018

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 03:18:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD121623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Dec 16 03:10:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

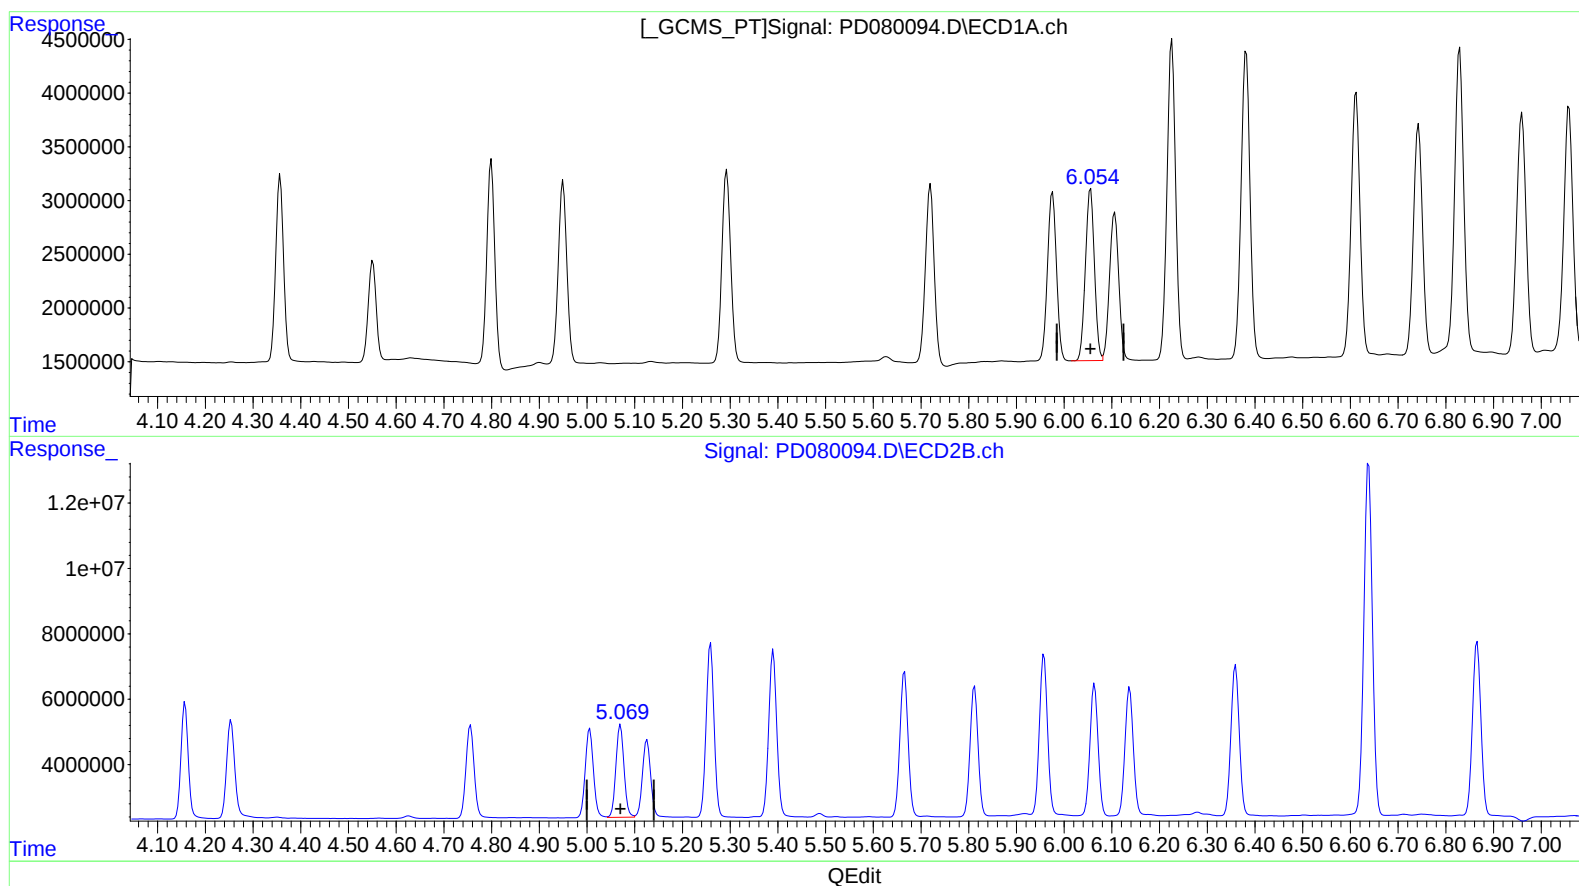

(11) cis-Chlordane (B)

6.056min 10.109 ng/ml

response 21213946

(11) cis-Chlordane #2 (B)

5.070min 9.973 ng/ml

response 33448569