

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121624\
 Data File : PD087130.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Dec 2024 13:41
 Operator : AR\AJ
 Sample : P5157-07MS
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E28W2MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/17/2024
 Supervised By :Ankita Jodhani 12/17/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 00:12:13 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112024CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 20 02:52:29 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.554	2.884	14356541	106.7E6	7.807m	9.245
27)	SA Decachlor...	9.090	8.083	37363419	99151772	14.033m	7.780m#
Target Compounds							
2)	A alpha-BHC	4.005	3.398	209.6E6	566.4E6	59.517	31.626 #
3)	MA gamma-BHC...	4.335	3.735	149.8E6	807.4E6	43.018m	48.409
4)	MA Heptachlor	4.935	4.089	191.9E6	738.8E6	55.214m	42.949
5)	MB Aldrin	5.278	4.376	191.0E6	714.7E6	54.105	41.839
6)	B beta-BHC	4.520	4.029	60173840	318.1E6	37.960	40.270
7)	B delta-BHC	4.767	4.267	136.2E6	525.3E6	37.429m	29.917
8)	B Heptachlo...	5.697	4.880	164.3E6	641.9E6	50.257	40.475
9)	A Endosulfan I	6.080	5.255	164.1E6	565.4E6	55.190	39.062 #
10)	B trans-Chl...	5.950	5.132	161.2E6	647.8E6	50.393m	39.221m
11)	B cis-Chlor...	6.033	5.198	159.0E6	664.4E6	48.865	41.462
12)	B 4,4'-DDE	6.203	5.384	287.2E6	1206.8E6	93.126	79.146
13)	MA Dieldrin	6.352	5.519	343.8E6	1324.6E6	104.892m	86.694m
14)	MA Endrin	6.581	5.797	258.4E6	993.7E6	95.583	71.929
15)	B Endosulfa...	6.791	6.088	255.2E6	1077.5E6	91.983	77.218
16)	A 4,4'-DDD	6.711	5.938	258.1E6	1018.9E6	108.805	84.340
17)	MA 4,4'-DDT	7.026	6.192	179.8E6	730.3E6	72.536m	56.488
18)	B Endrin al...	6.920	6.266	171.2E6	666.4E6	77.886	62.093
19)	B Endosulfa...	7.154	6.490	226.9E6	884.5E6	84.092	65.912
20)	A Methoxychlor	7.497	6.763	484.5E6	1681.7E6	358.949m	290.881m
21)	B Endrin ke...	7.634	7.000	299.7E6	917.2E6	98.241m	61.385 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121624\
Data File : PD087130.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Dec 2024 13:41
Operator : AR\AJ
Sample : P5157-07MS
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 00:12:13 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 20 02:52:29 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

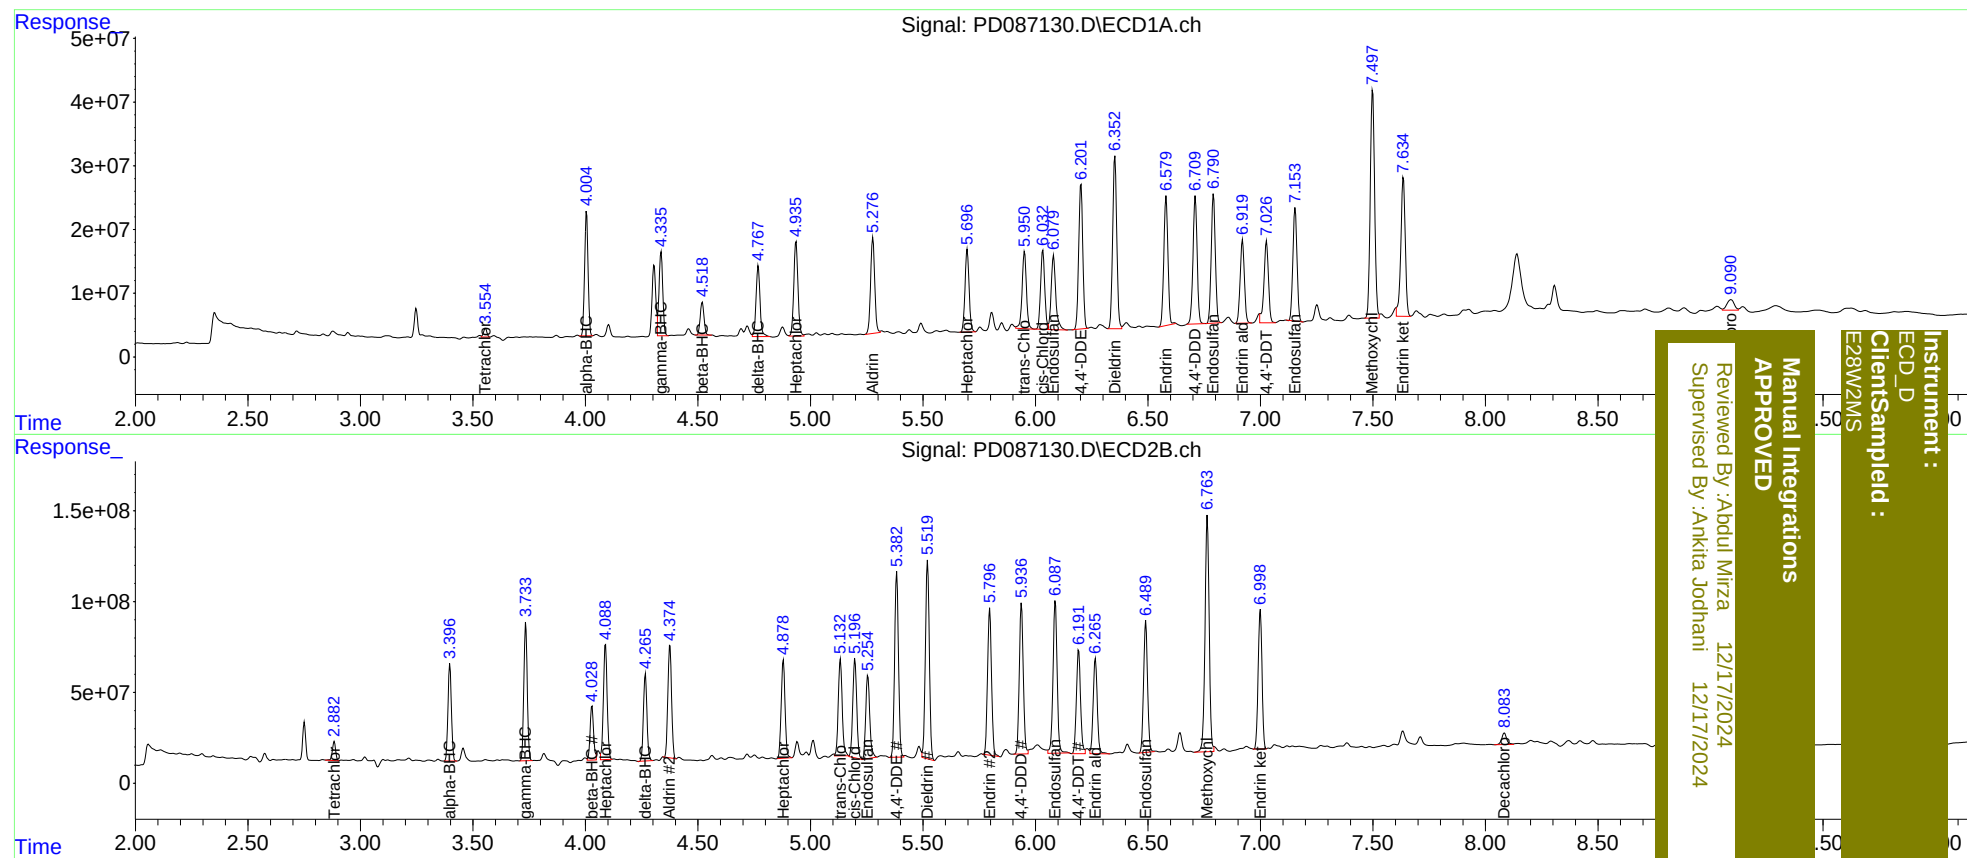

Instrument :
ECD_D
ClientSampled :
E28W2MS

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 12/17/2024
Supervised By: Ankita Jodhani 12/17/2024