

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121624\
 Data File : PD087131.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Dec 2024 13:55
 Operator : AR\AJ
 Sample : P5157-08MSD
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E28W2MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/17/2024
 Supervised By :Ankita Jodhani 12/17/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 00:12:31 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112024CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 20 02:52:29 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.555	2.883	14376426	106.5E6	7.818m	9.227
27)	SA Decachlor...	9.090	8.084	37751328	90036328	14.179m	7.065 #
Target Compounds							
2)	A alpha-BHC	4.004	3.398	213.5E6	562.5E6	60.642m	31.405 #
3)	MA gamma-BHC...	4.336	3.734	147.4E6	807.5E6	42.330m	48.414
4)	MA Heptachlor	4.935	4.089	186.7E6	732.9E6	53.727m	42.604
5)	MB Aldrin	5.278	4.376	190.9E6	714.2E6	54.062	41.807
6)	B beta-BHC	4.520	4.030	59332920	318.2E6	37.430	40.274
7)	B delta-BHC	4.767	4.267	130.9E6	523.6E6	35.971m	29.819
8)	B Heptachlo...	5.697	4.880	164.5E6	639.8E6	50.333	40.341
9)	A Endosulfan I	6.080	5.255	163.9E6	563.7E6	55.128	38.944 #
10)	B trans-Chl...	5.950	5.132	164.1E6	645.1E6	51.298m	39.055m
11)	B cis-Chlor...	6.033	5.198	158.7E6	661.4E6	48.770	41.270
12)	B 4,4'-DDE	6.202	5.383	287.9E6	1203.4E6	93.345	78.925
13)	MA Dieldrin	6.352	5.519	344.5E6	1322.9E6	105.093m	86.584m
14)	MA Endrin	6.581	5.797	257.4E6	989.3E6	95.219	71.611
15)	B Endosulfa...	6.792	6.088	255.6E6	1091.6E6	92.116	78.230
16)	A 4,4'-DDD	6.711	5.938	261.5E6	1030.4E6	110.212	85.287
17)	MA 4,4'-DDT	7.026	6.192	168.2E6	705.1E6	67.873m	54.541
18)	B Endrin al...	6.920	6.266	170.9E6	664.3E6	77.756	61.898
19)	B Endosulfa...	7.155	6.490	227.0E6	883.1E6	84.141	65.813
20)	A Methoxychlor	7.497	6.763	475.1E6	1655.4E6	351.977m	286.325m
21)	B Endrin ke...	7.634	6.999	299.2E6	912.1E6	98.076m	61.039 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD121624\
Data File : PD087131.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Dec 2024 13:55
Operator : AR\AJ
Sample : P5157-08MSD
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 00:12:31 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 20 02:52:29 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

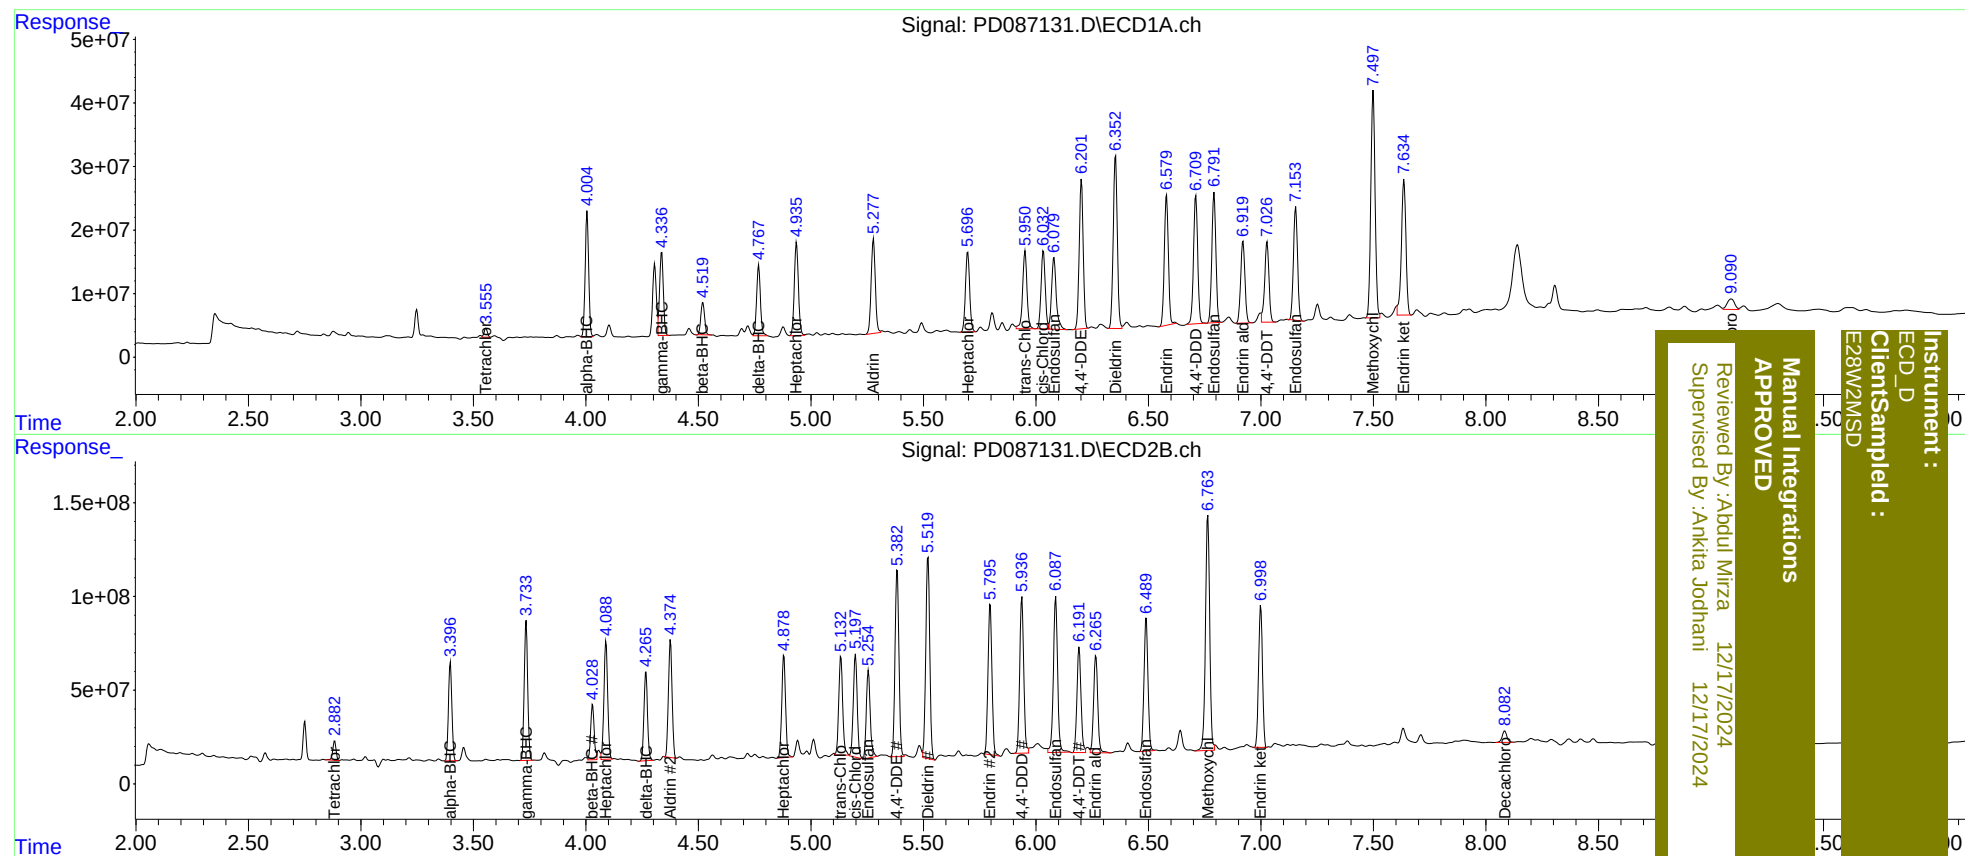

Instrument :
ECD_D
ClientSampled :
E28W2MSD

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 12/17/2024
Supervised By: Ankita Jodhani 12/17/2024